

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101821\
 Data File : BF125883.D
 Acq On : 18 Oct 2021 18:20
 Operator : JU/CG
 Sample : M4243-22
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 T4-COMP-(1-4)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125883.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.763	105	115	122	rVB	261648	356095	7.32%	1.253%
2	4.622	424	431	438	rBV	427240	443030	9.11%	1.559%
3	5.045	500	503	505	rBV	194329	238195	4.90%	0.838%
4	5.069	505	507	511	rVB	283496	248590	5.11%	0.875%
5	5.445	566	571	575	rBV	3427384	3658565	75.22%	12.877%
6	6.451	737	742	745	rBV	3356766	3331274	68.49%	11.725%
7	6.822	802	805	809	rBV	1132802	875836	18.01%	3.083%
8	7.386	895	901	904	rBV	2631898	2551193	52.46%	8.980%
9	8.104	1019	1023	1026	rBV	1455120	1234491	25.38%	4.345%
10	9.180	1201	1206	1209	rBV	5223679	4863543	100.00%	17.119%
11	9.851	1317	1320	1324	rBV	1488578	1371494	28.20%	4.827%
12	10.639	1450	1454	1457	rBV	2929374	2675739	55.02%	9.418%
13	11.333	1569	1572	1576	rBV	1329435	1162832	23.91%	4.093%
14	12.921	1838	1842	1845	rBV	4187773	3598565	73.99%	12.666%
15	13.968	2016	2020	2024	rBV	1118216	937780	19.28%	3.301%
16	15.415	2261	2266	2271	rBV	719878	863739	17.76%	3.040%




Sum of corrected areas: 28410961

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101821\
Data File : BF125883.D
Acq On : 18 Oct 2021 18:20
Operator : JU/CG
Sample : M4243-22
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T4-COMP-(1-4)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

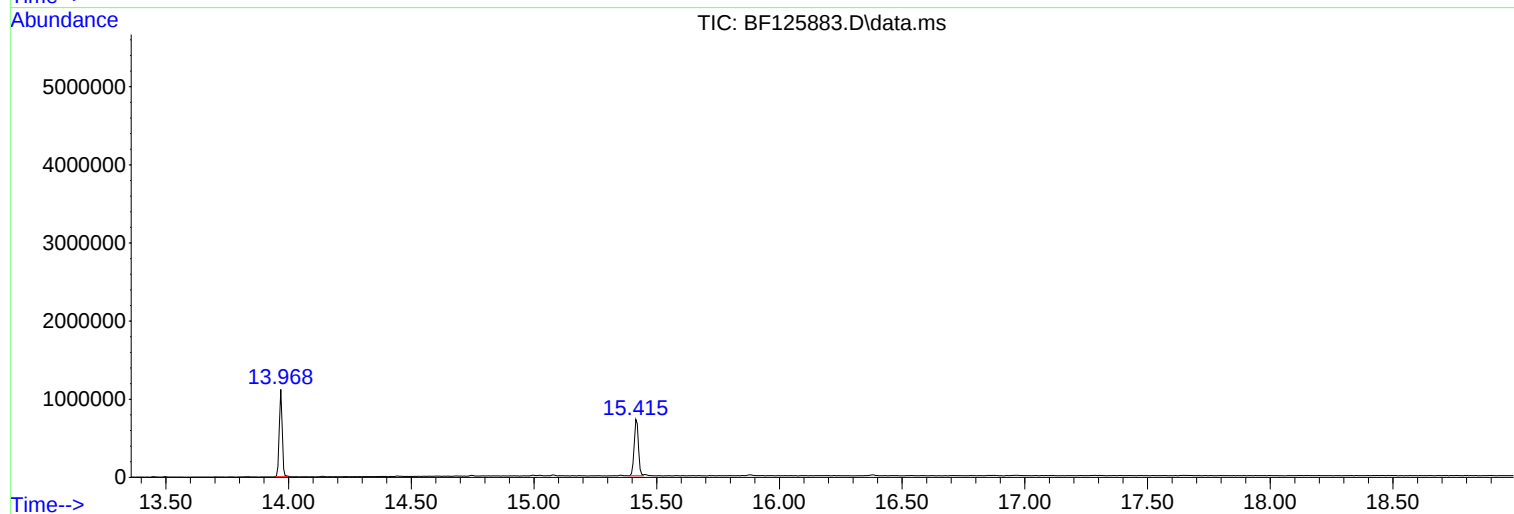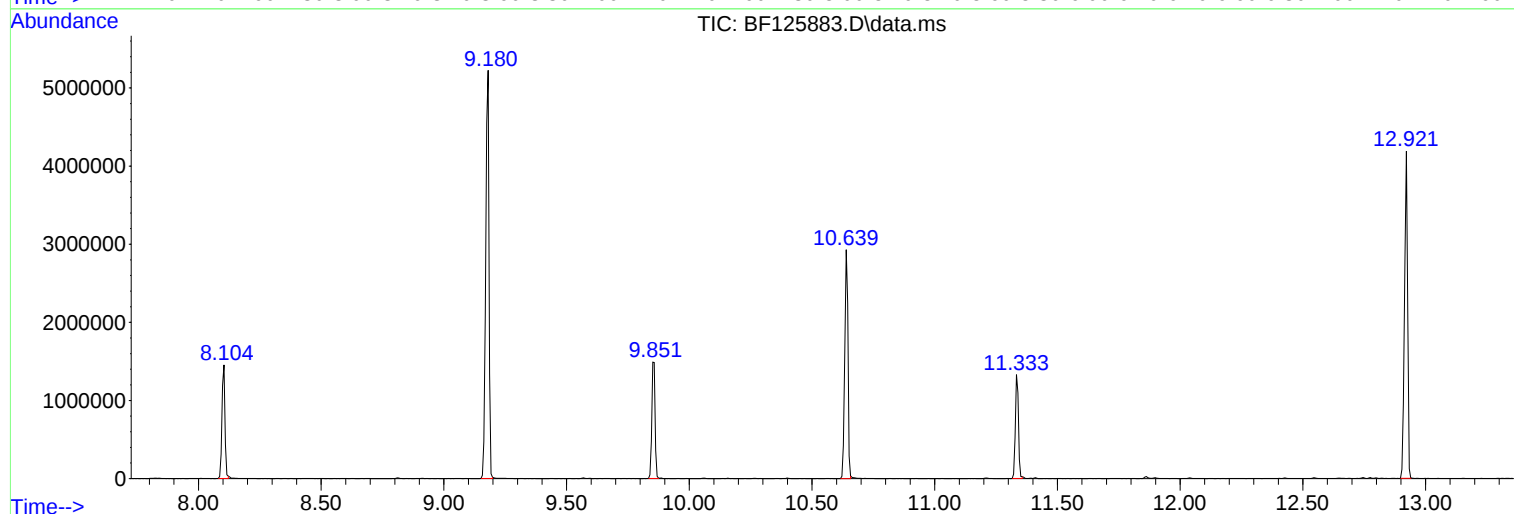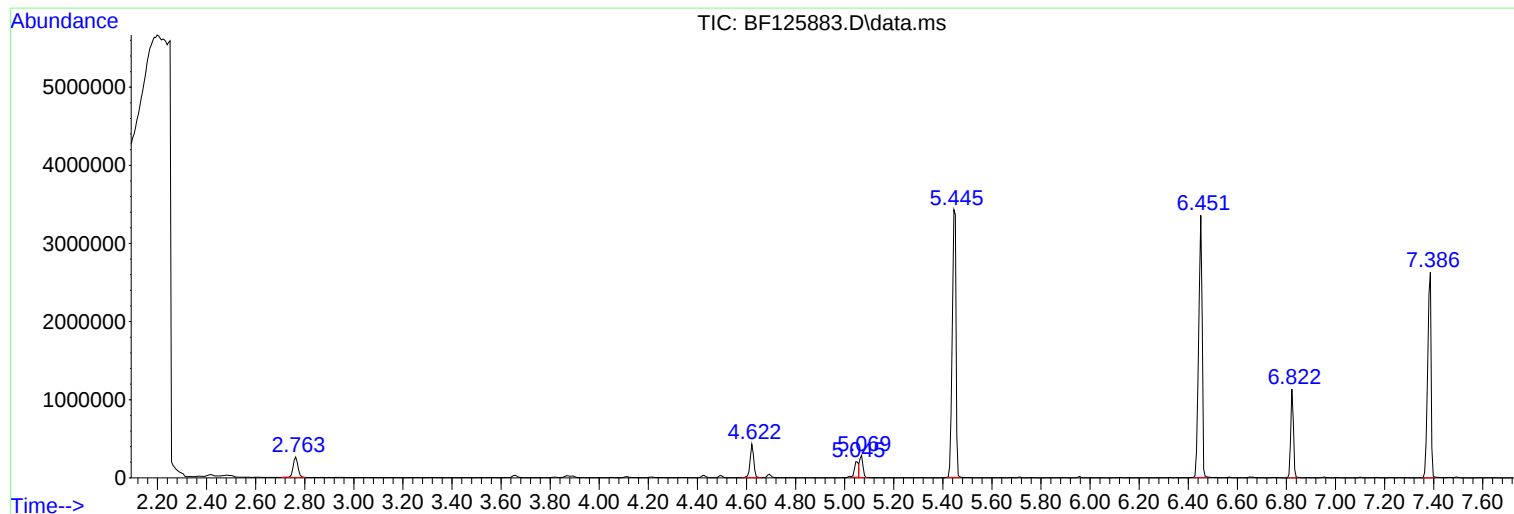

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101821\
Data File : BF125883.D
Acq On : 18 Oct 2021 18:20
Operator : JU/CG
Sample : M4243-22
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T4-COMP-(1-4)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101821\
Data File : BF125883.D
Acq On : 18 Oct 2021 18:20
Operator : JU/CG
Sample : M4243-22
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T4-COMP-(1-4)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------