


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101822\
 Data File : BF130693.D
 Acq On : 18 Oct 2022 10:52
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 18 03:15:54 2022

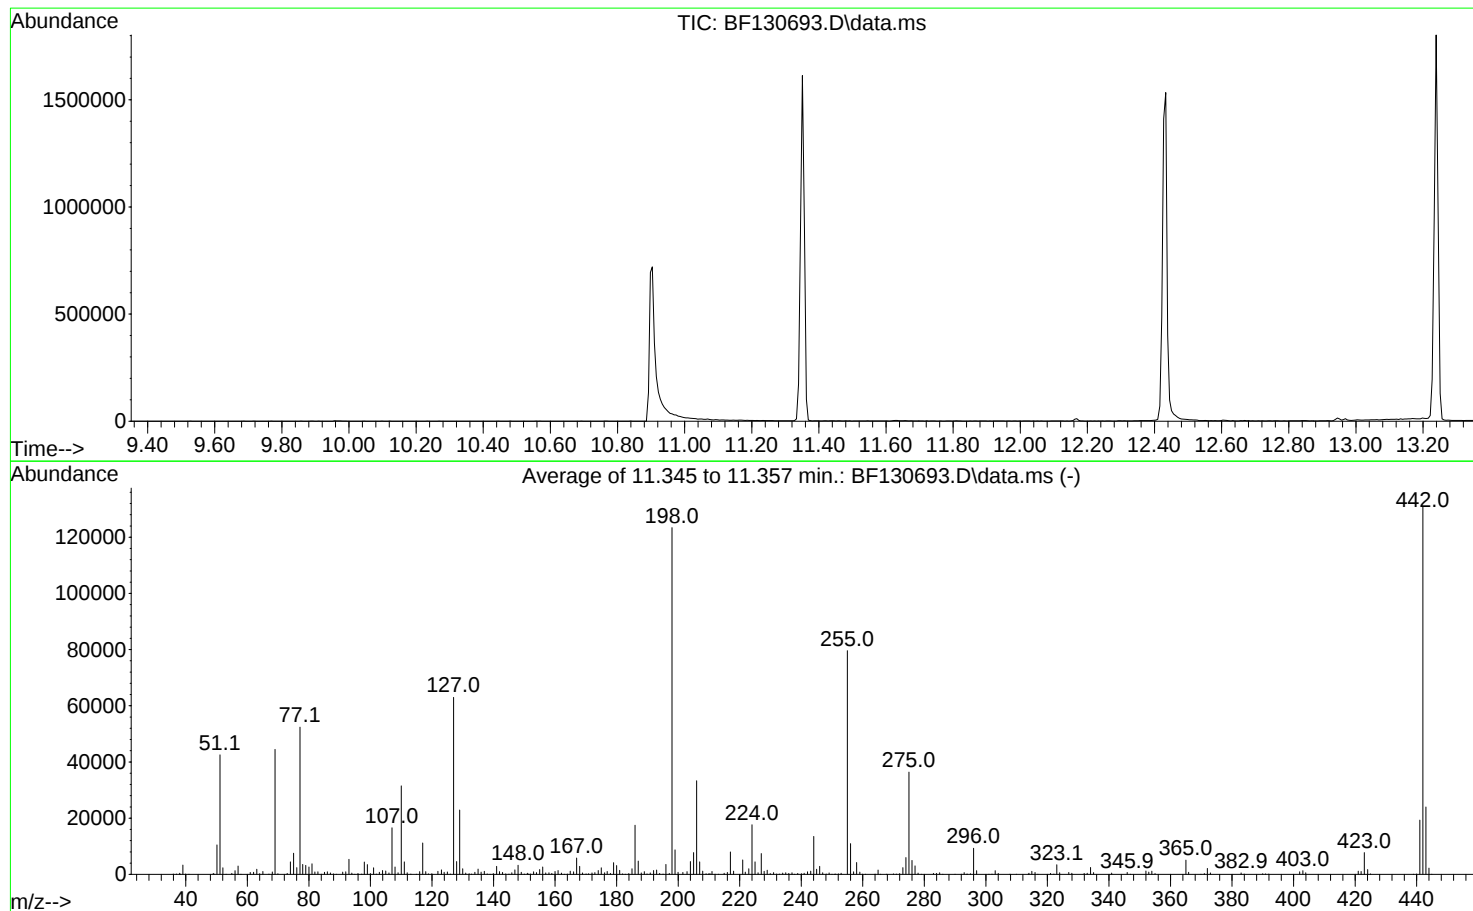




AutoFind: Scans 1574, 1575, 1576; Background Corrected with Scan 1569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	42541	PASS
68	69	0.00	2	1.9	867	PASS
69	198	0.00	100	36.0	44464	PASS
70	69	0.00	2	0.5	234	PASS
127	198	10	80	51.0	62997	PASS
197	198	0.00	2	0.3	344	PASS
198	198	100	100	100.0	123424	PASS
199	198	5	9	7.1	8736	PASS
275	198	10	60	29.5	36371	PASS
365	198	1	100	4.1	5075	PASS
441	198	0.01	100	15.7	19324	PASS
442	442	50	100	100.0	130931	PASS
443	442	15	24	18.3	23976	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101822\
 Data File : BF130693.D
 Acq On : 18 Oct 2022 10:52
 Operator : CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 18 17:20:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 18 03:15:54 2022
 Response via : Initial Calibration

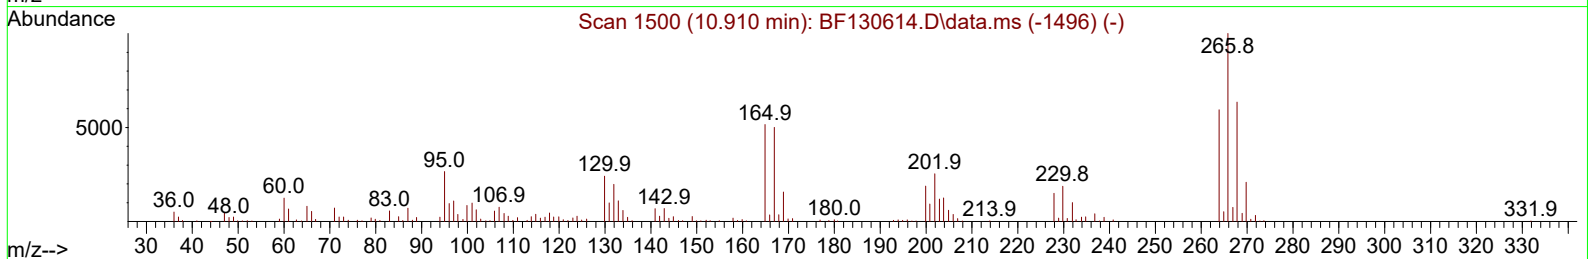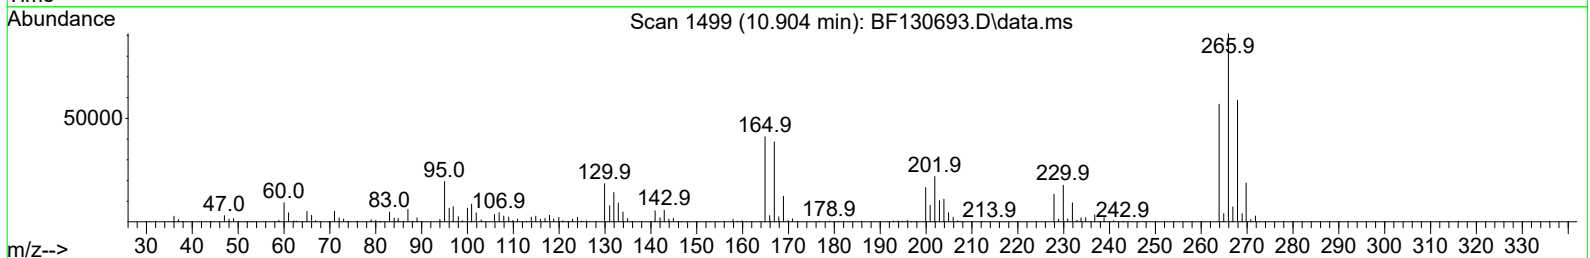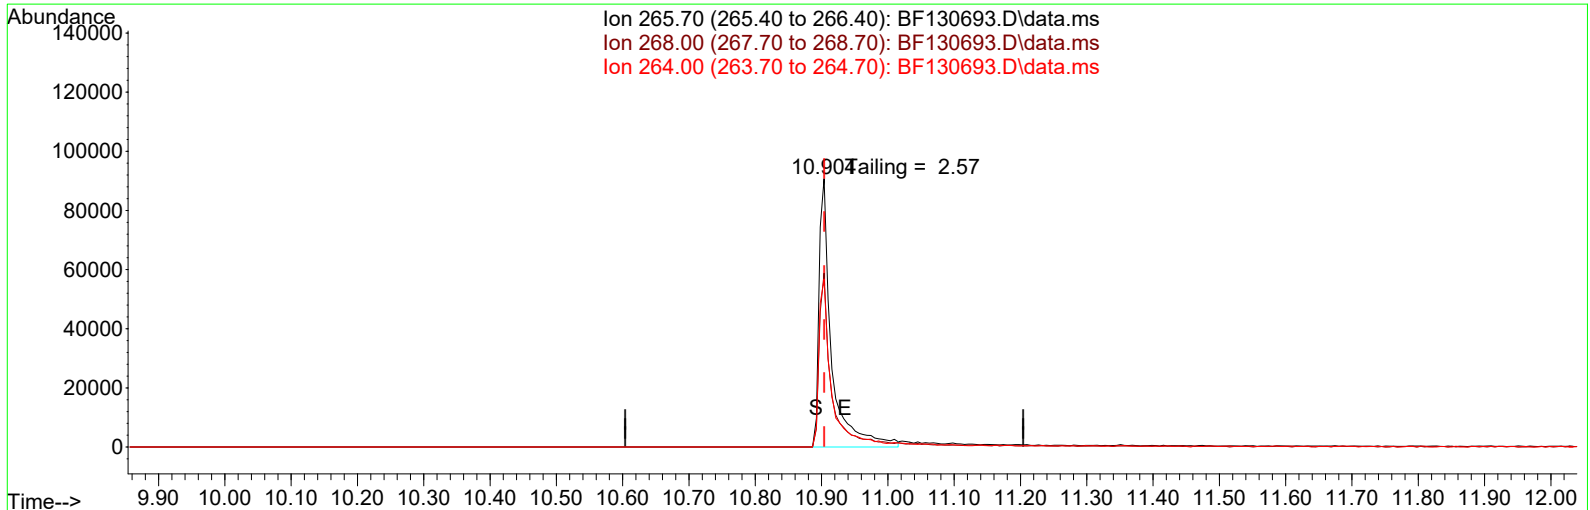

TIC: BF130693.D\data.ms

(70) Pentachlorophenol (C)

10.904min (-0.000) 45893.25 ng




response 123598

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	64.76
264.00	59.40	62.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101822\
 Data File : BF130693.D
 Acq On : 18 Oct 2022 10:52
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 18 17:20:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 18 03:15:54 2022
 Response via : Initial Calibration

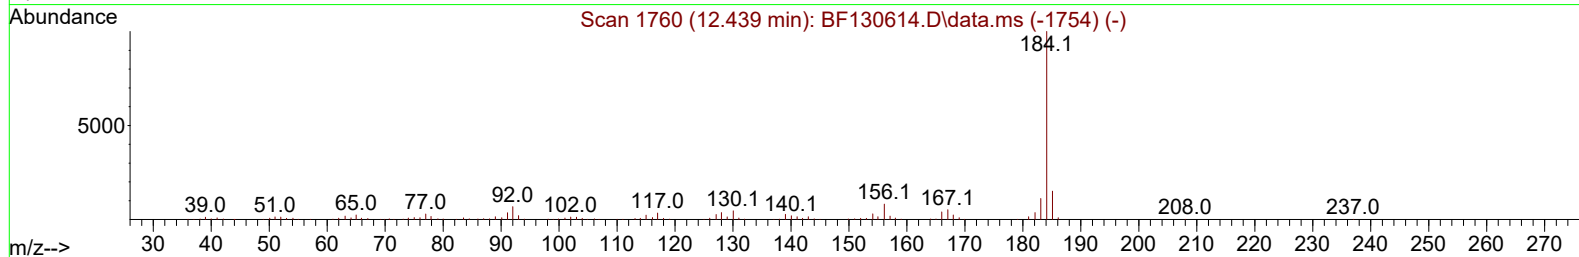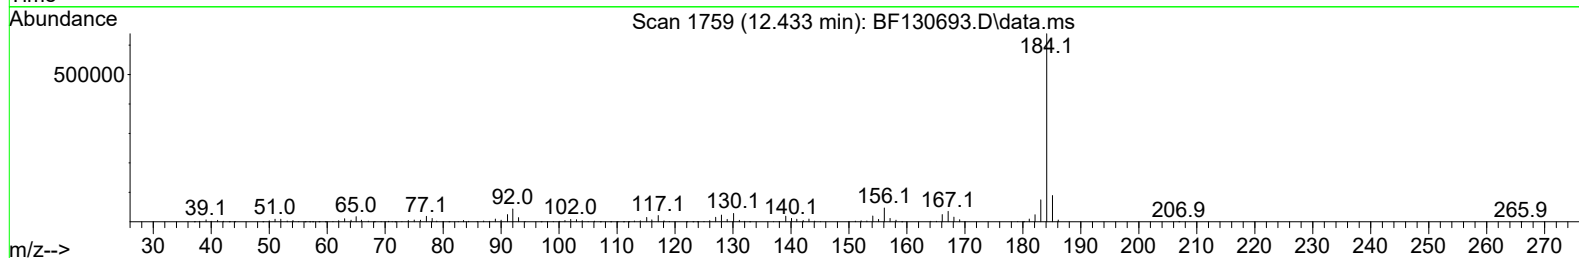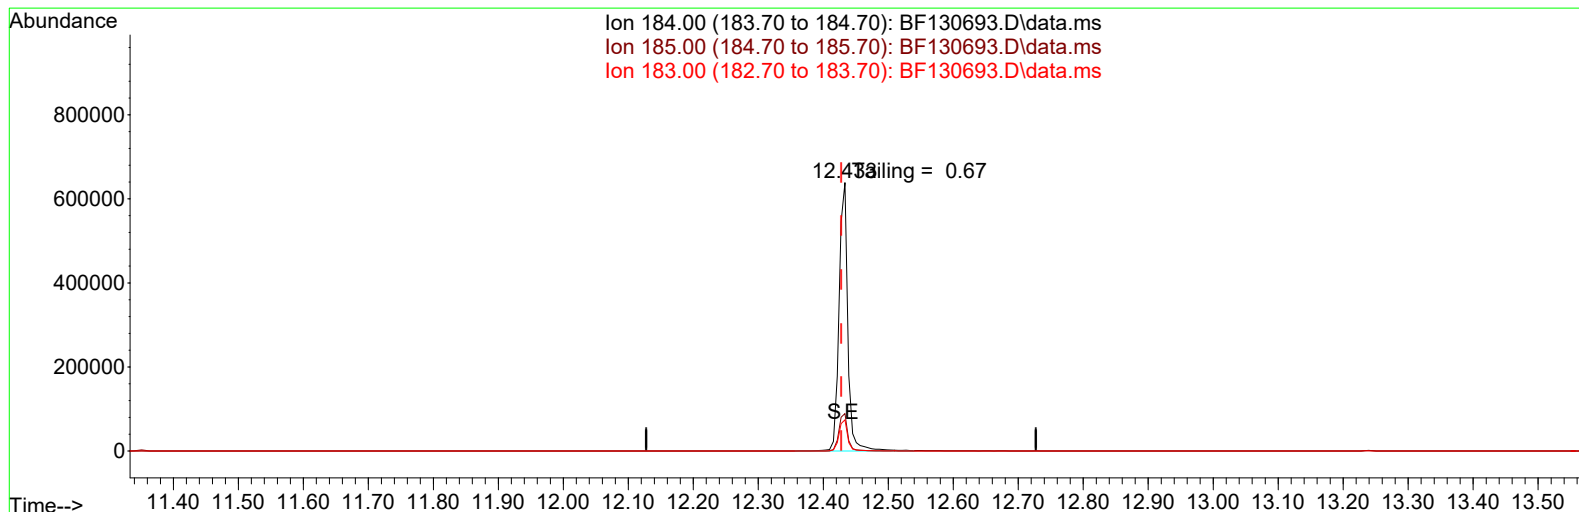

TIC: BF130693.D\data.ms

(77) Benzidine

12.433min (+ 0.006) 0.00 ng

response 602230

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.95
183.00	11.20	11.66
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/18/2022	BNA_F	<u>BF130693.D</u>
Compound Name	Response	Retention Time
DDT	279740	13.239
DDD	4737	12.945
DDE	651	12.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5388	285128	1.89

Instrument :
BNA_F
ClientSampleId :
DFTPP