

Data Path : U:\HPCHEM1\BNA F\DATA\BF101915\
 Data File : BF082357.D
 Acq On : 19 Oct 2015 15:59
 Operator : UM/IZ
 Sample : PB86144BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB86144BL

Quant Time: Oct 20 02:18:44 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 01:57:16 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.80	152	106489	20.00	ng	0.00
21) Naphthalene-d8	8.09	136	411033	20.00	ng	0.00
38) Acenaphthene-d10	9.85	164	209250	20.00	ng	0.00
63) Phenanthrene-d10	11.34	188	424603	20.00	ng	-0.01
75) Chrysene-d12	14.06	240	365882	20.00	ng	-0.03
86) Perylene-d12	15.62	264	285758	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.41	112	640594	121.41	ng	0.01
7) Phenol-d6	6.45	99	860285	125.29	ng	0.00
23) Nitrobenzene-d5	7.37	82	495003	80.87	ng	-0.01
41) 2,4,6-Tribromophenol	10.64	330	188039	95.82	ng	-0.01
44) 2-Fluorobiphenyl	9.18	172	1073103	85.05	ng	0.00
78) Terphenyl-d14	12.95	244	1148683	83.19	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA F\DATA\BF101915\
Data File : BF082357.D
Acq On : 19 Oct 2015 15:59
Operator : UM/IZ
Sample : PB86144BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB86144BL

Quant Time: Oct 20 02:18:44 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 20 01:57:16 2015
Response via : Initial Calibration

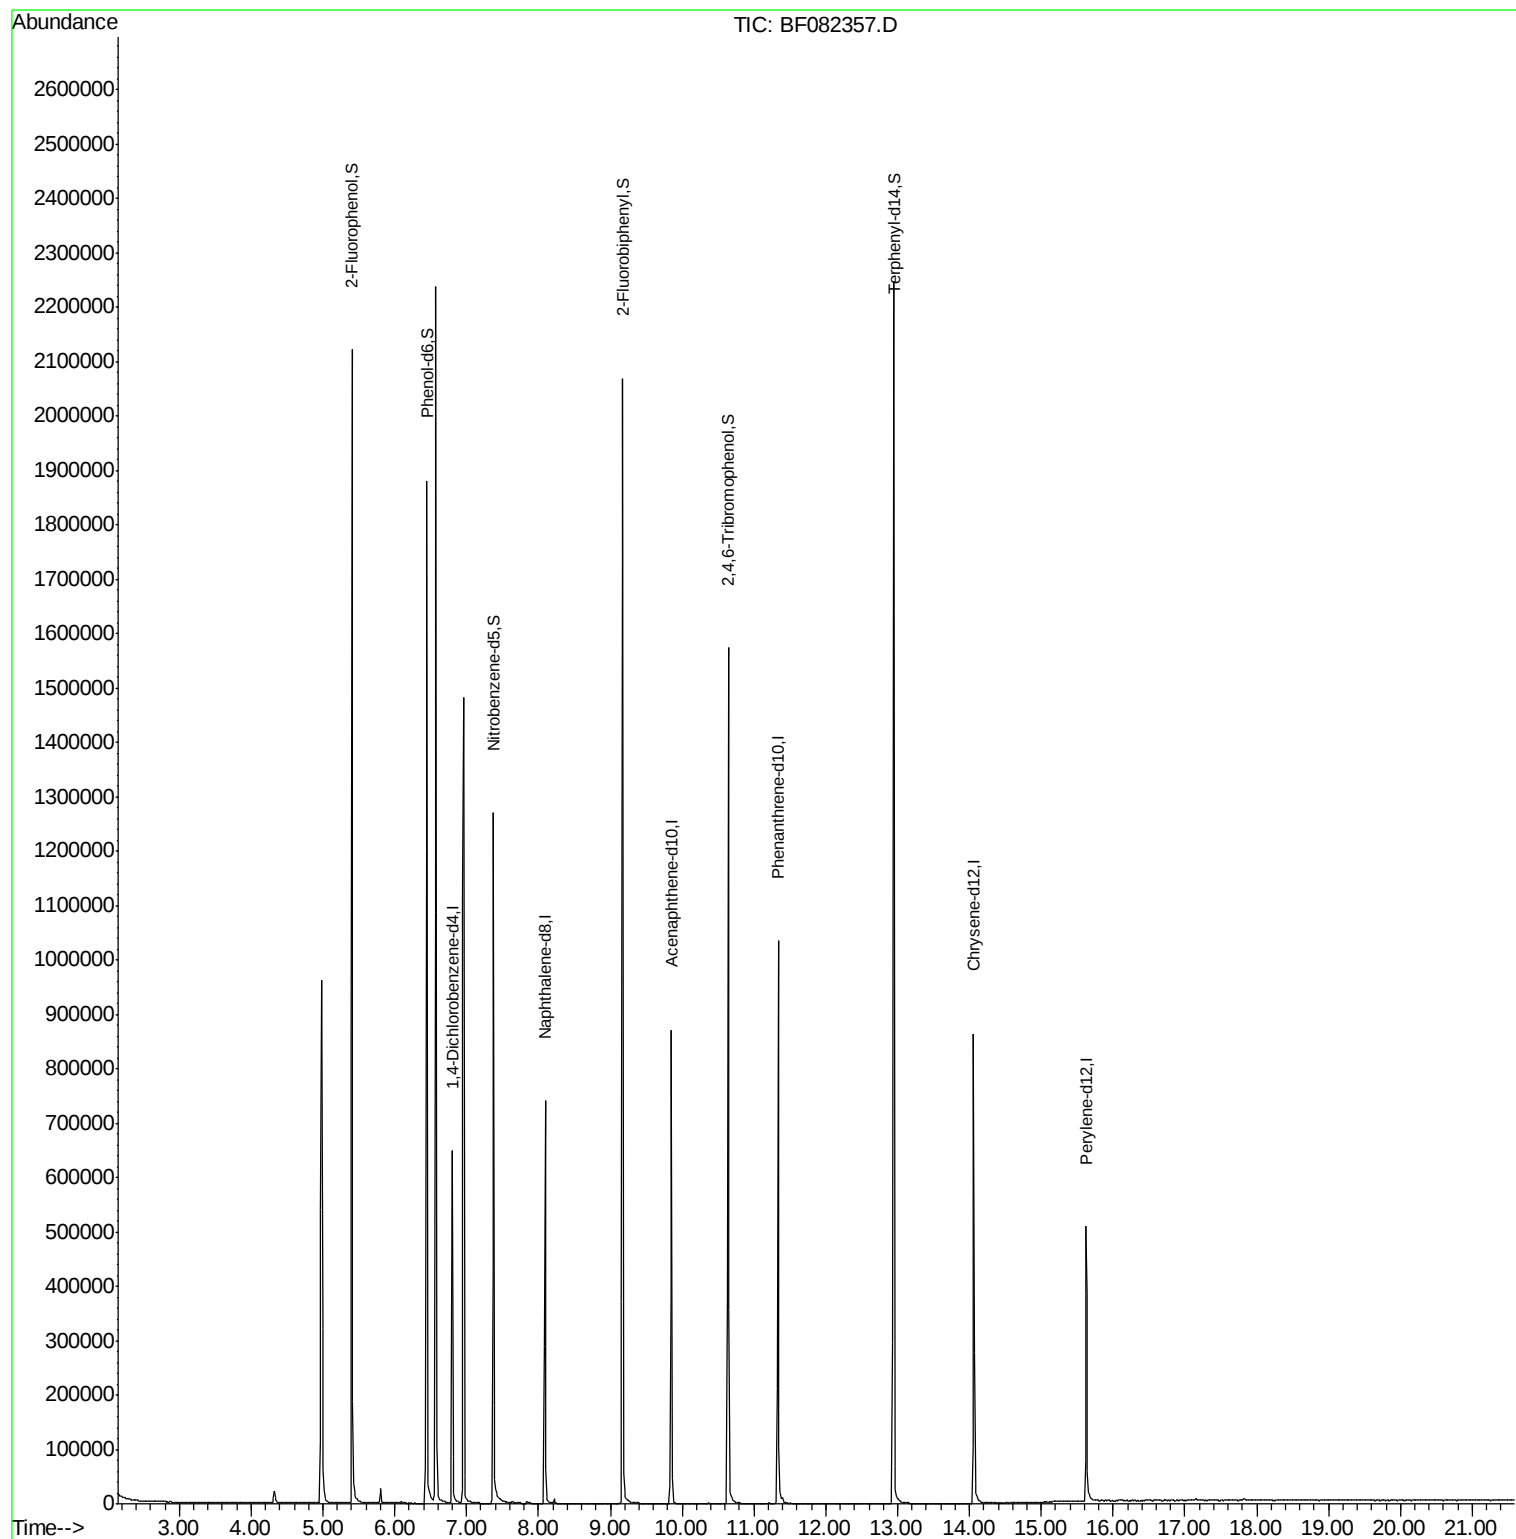

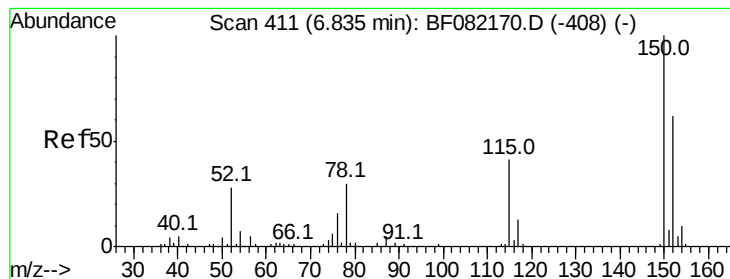

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.80 min Scan# 408

Delta R.T. 0.00 min

Lab File: BF082357.D

Acq: 19 Oct 2015 15:59

Instrument :

BNA_F

ClientSampleId :

PB86144BL


Tot Ion:152 Resp: 106489

Ion Ratio Lower Upper

152 100

150 153.8 129.0 193.4




115 55.5 52.1 78.1

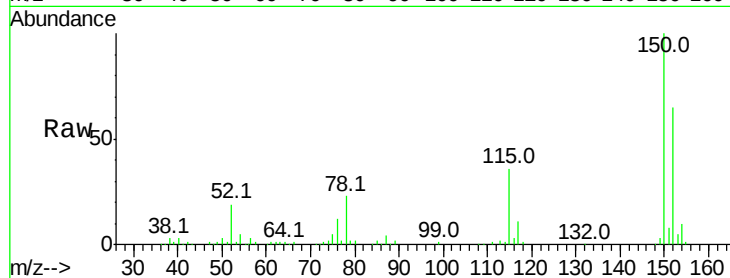

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

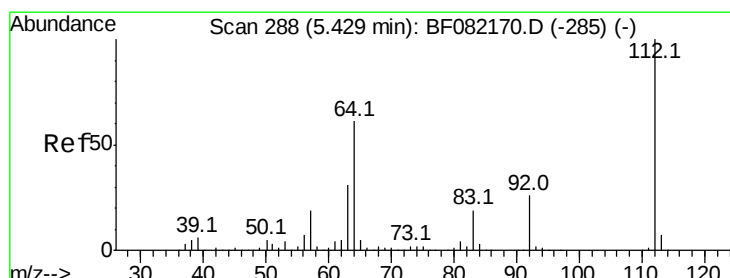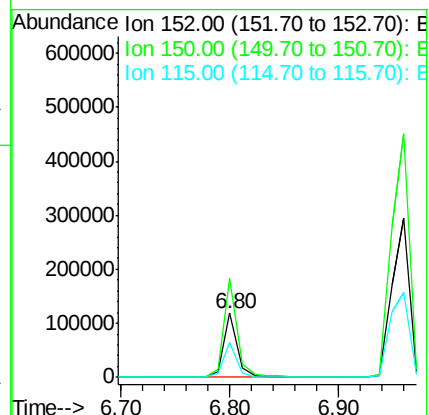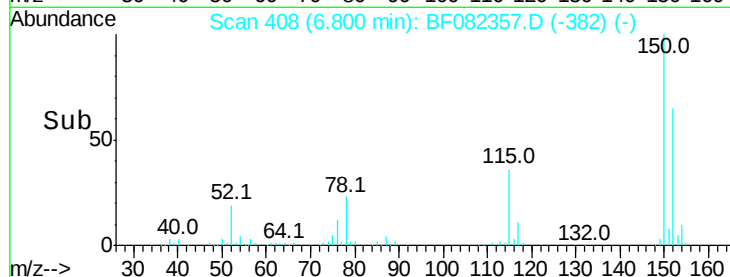

#5

2-Fluorophenol

Concen: 121.41 ng

RT: 5.41 min Scan# 286

Delta R.T. 0.01 min

Lab File: BF082357.D

Acq: 19 Oct 2015 15:59


Tgt Ion:112 Resp: 640594

Ion Ratio Lower Upper

112 100

64 60.1 48.6 73.0



63 31.8 25.1 37.7

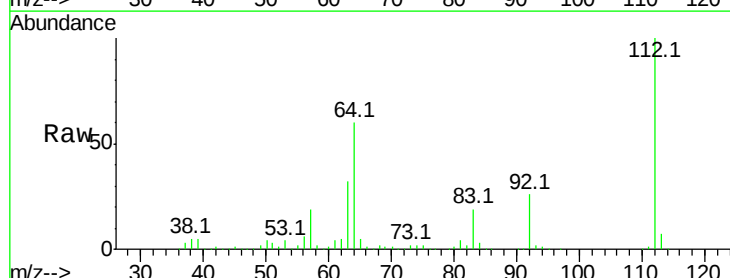

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

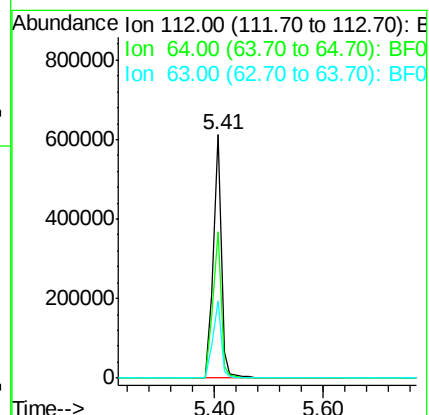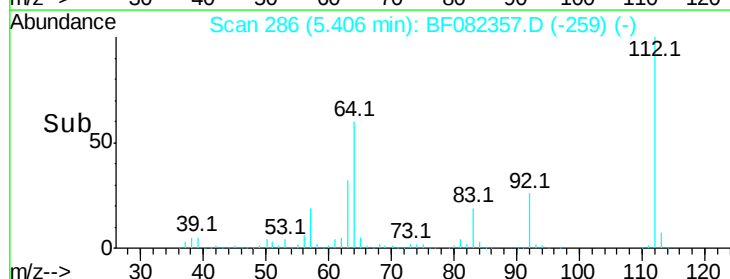



#7

Phenol-d6

Concen: 125.29 ng

RT: 6.45 min Scan# 377

Delta R.T. 0.00 min

Lab File: BF082357.D

Acq: 19 Oct 2015 15:59

Instrument :

BNA_F

ClientSampleId :

PB86144BL




Tot Ion: 99 Resp: 860285

Ion Ratio Lower Upper

99 100

42 15.8 13.2 19.8

71 32.4 25.6 38.4

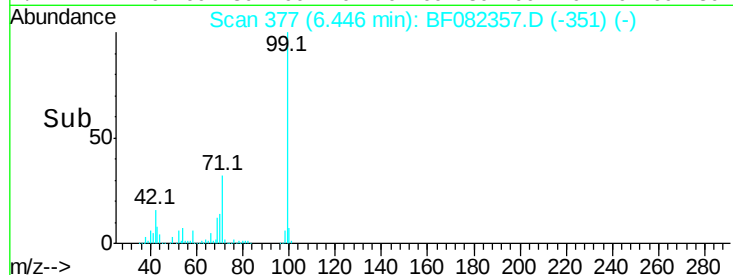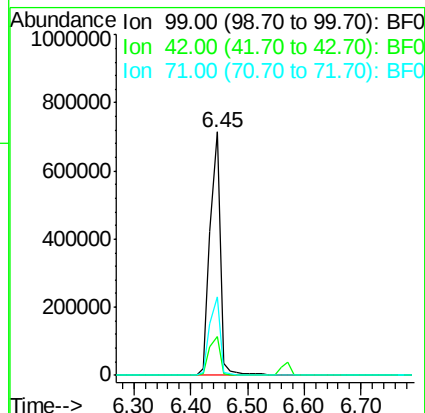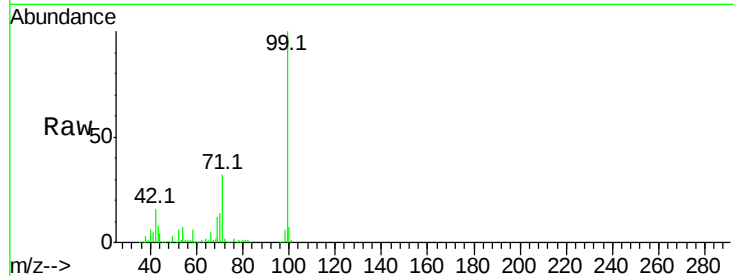

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.09 min Scan# 521

Delta R.T. 0.00 min

Lab File: BF082357.D

Acq: 19 Oct 2015 15:59

Tgt Ion: 136 Resp: 411033




Ion Ratio Lower Upper


136 100

137 10.7 9.0 13.6

54 7.1 7.5 11.3#

68 4.6 4.6 7.0


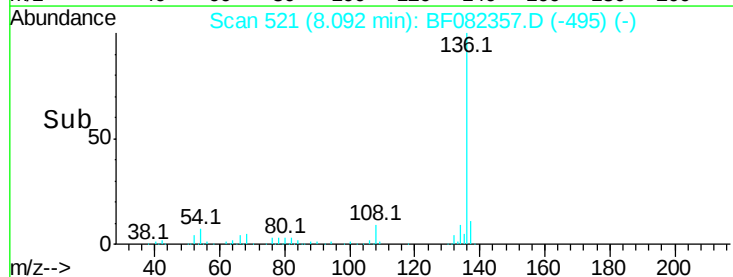
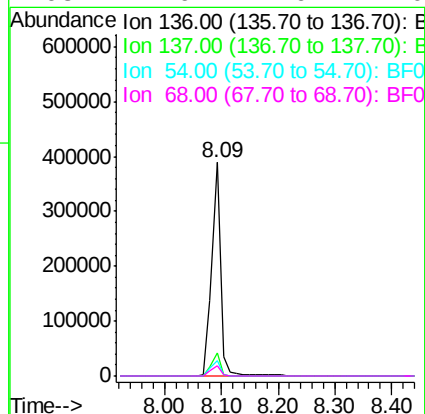
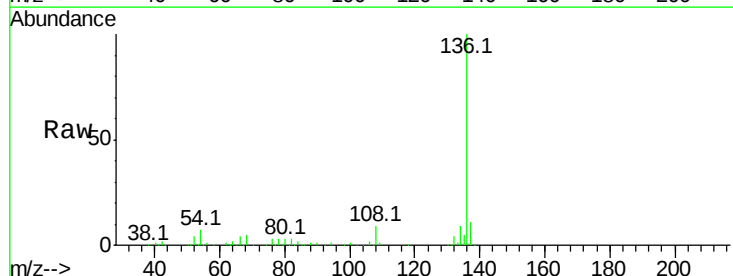


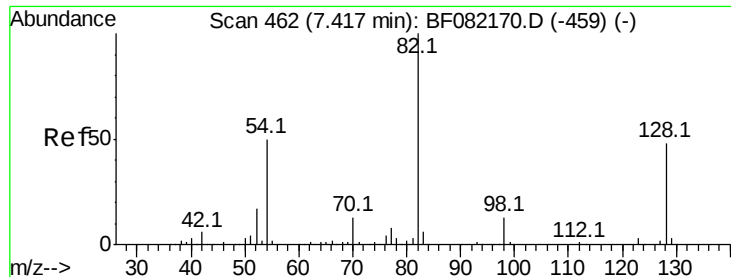

#23
 Nitrobenzene-d5
 Concen: 80.87 ng
 RT: 7.37 min Scan# 458
 Delta R.T. -0.01 min
 Lab File: BF082357.D
 Acq: 19 Oct 2015 15:59




Instrument :
 BNA_F
 ClientSampleId :
 PB86144BL


Tot Ion	82	Resp	495003
Ion Ratio	100		
Lower		38.7	58.1
Upper		40.1	60.1

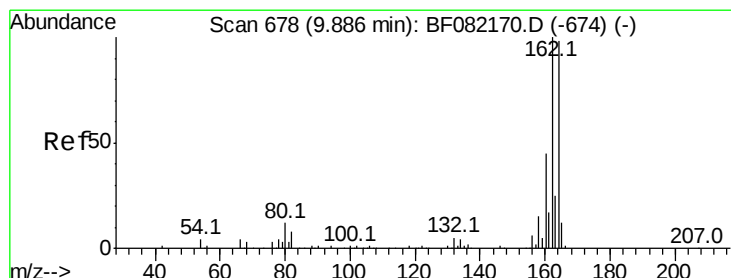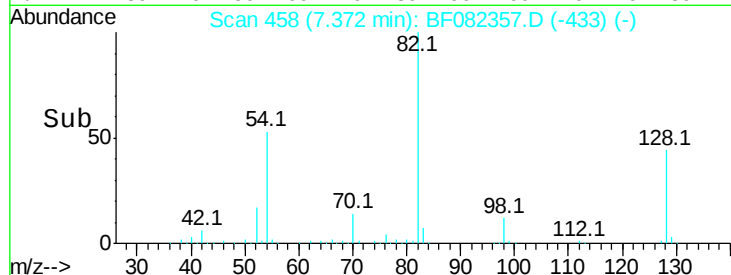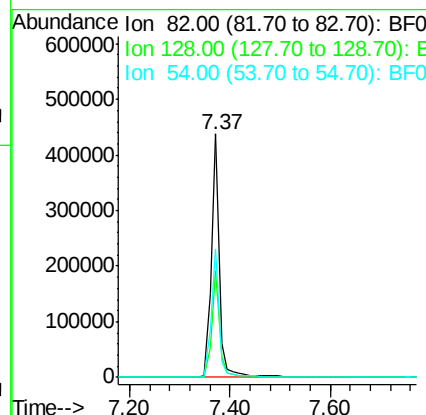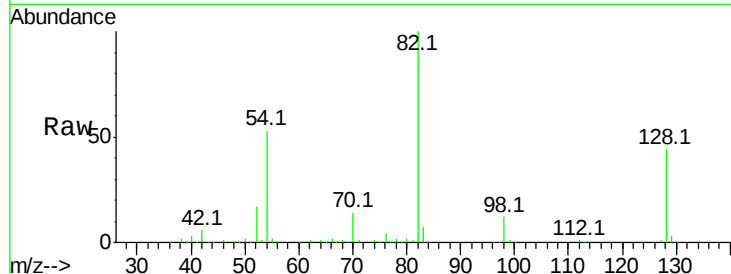

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.85 min Scan# 675
 Delta R.T. 0.00 min
 Lab File: BF082357.D
 Acq: 19 Oct 2015 15:59

Tgt Ion	164	Resp	209250
Ion Ratio	100		
Lower		81.6	122.4
Upper		36.4	54.6

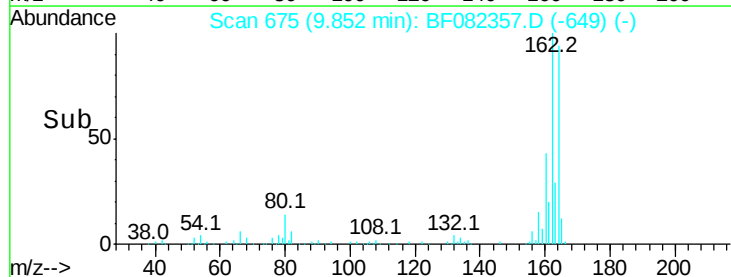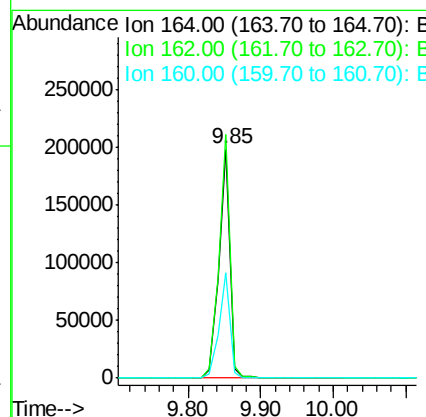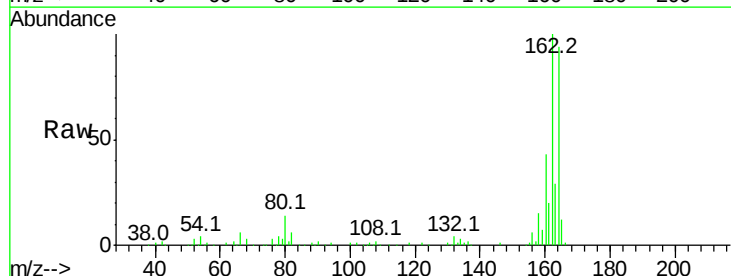


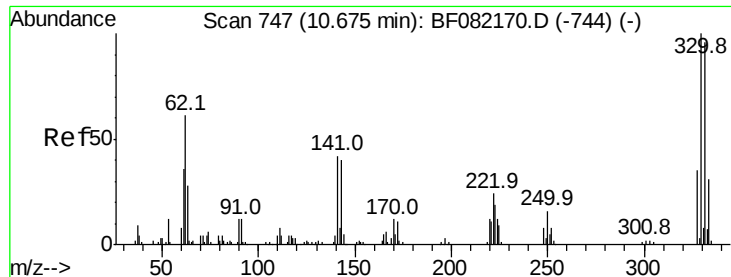




#41
 2,4,6-Tribromophenol
 Concen: 95.82 ng
 RT: 10.64 min Scan# 744
 Delta R.T. -0.01 min
 Lab File: BF082357.D
 Acq: 19 Oct 2015 15:59

Instrument :
 BNA_F
 ClientSampleId :
 PB86144BL

Tot Ion:330 Resp: 188039
 Ion Ratio Lower Upper
 330 100
 332 98.3 77.1 115.7
 141 44.4 29.8 44.8

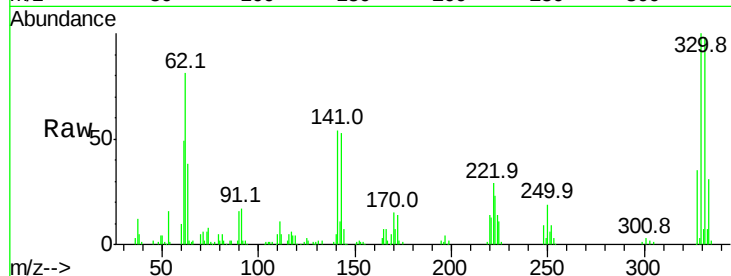


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

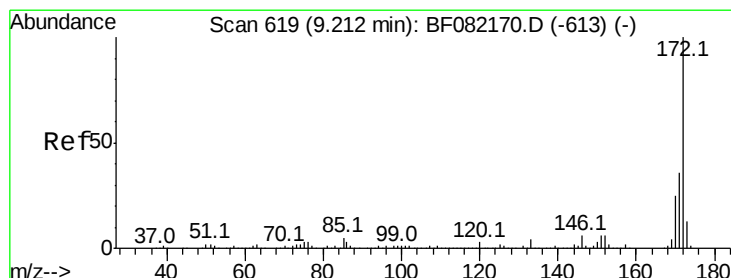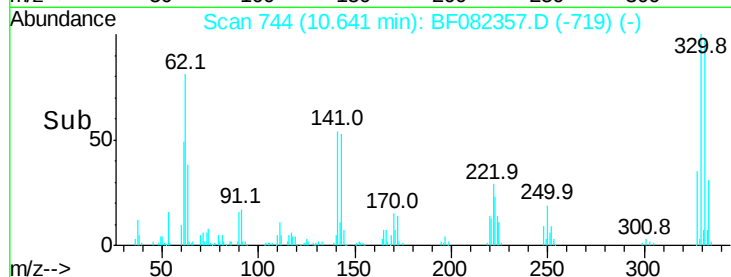
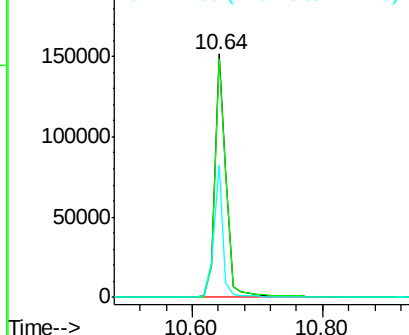



#44
 2-Fluorobiphenyl
 Concen: 85.05 ng
 RT: 9.18 min Scan# 616
 Delta R.T. 0.00 min
 Lab File: BF082357.D
 Acq: 19 Oct 2015 15:59

Tgt Ion:172 Resp: 1073103
 Ion Ratio Lower Upper
 172 100
 171 35.5 28.6 42.8
 170 24.0 19.7 29.5

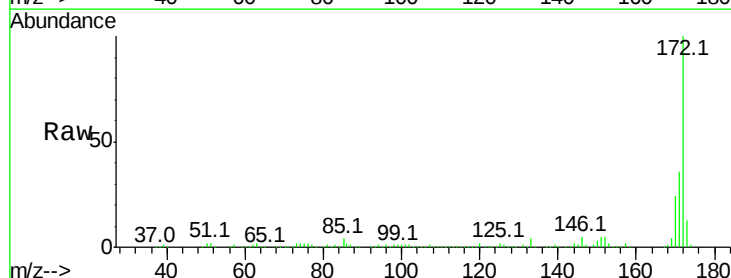

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

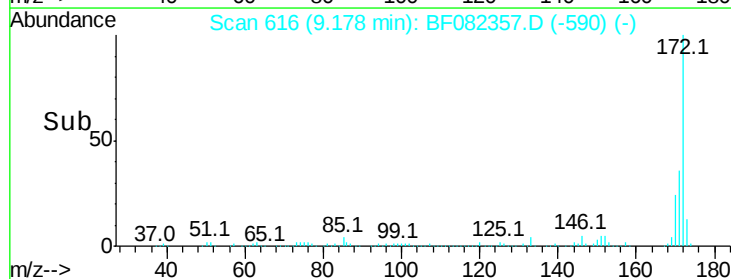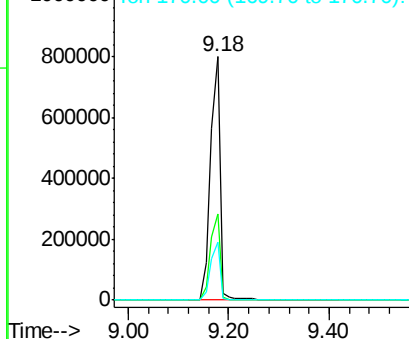

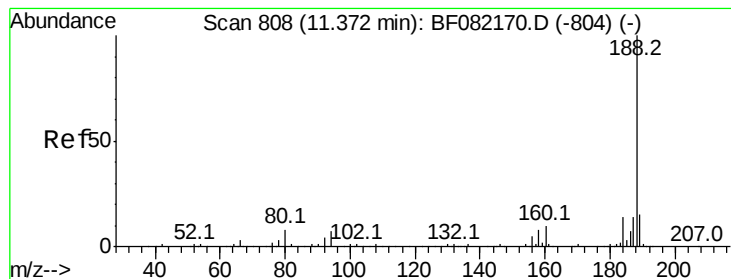

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.34 min Scan# 805

Delta R.T. -0.01 min

Lab File: BF082357.D

Acq: 19 Oct 2015 15:59

Instrument :

BNA_F

ClientSampleId :

PB86144BL



Tot Ion:188 Resp: 424603

Ion Ratio Lower Upper

188 100

94 7.5 5.8 8.6



80 7.8 6.4 9.6

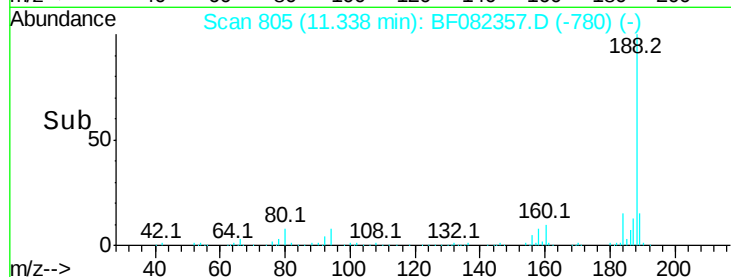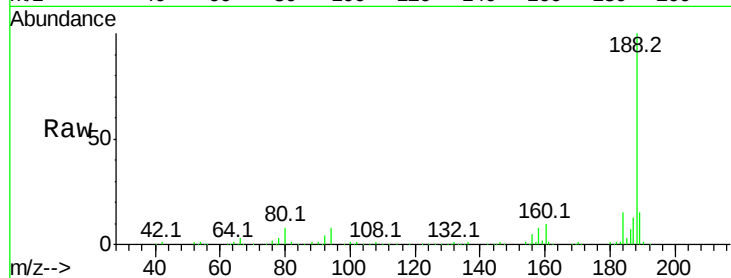

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

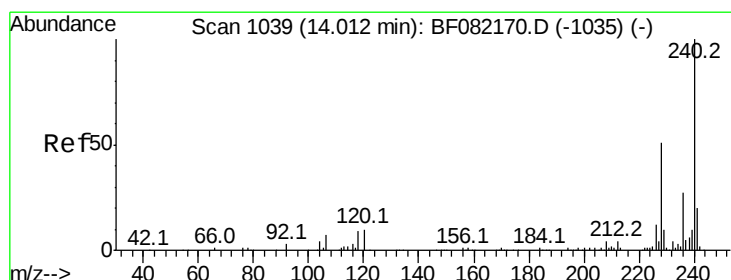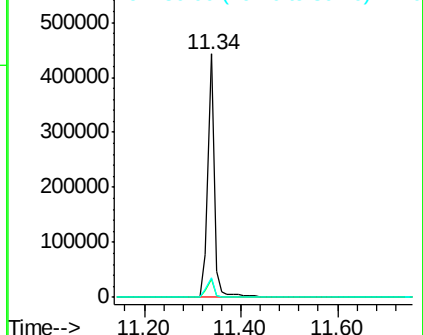

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.06 min Scan# 1043

Delta R.T. -0.03 min

Lab File: BF082357.D

Acq: 19 Oct 2015 15:59



Tgt Ion:240 Resp: 365882

Ion Ratio Lower Upper

240 100

120 10.8 8.1 12.1


236 26.2 21.3 31.9

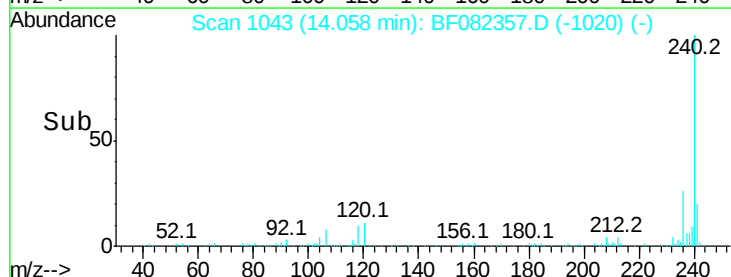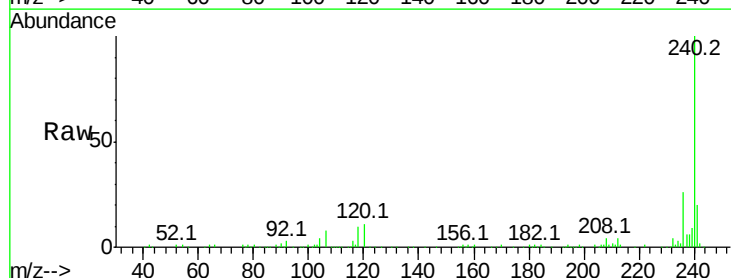


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

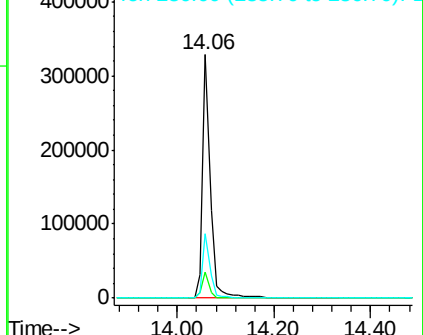

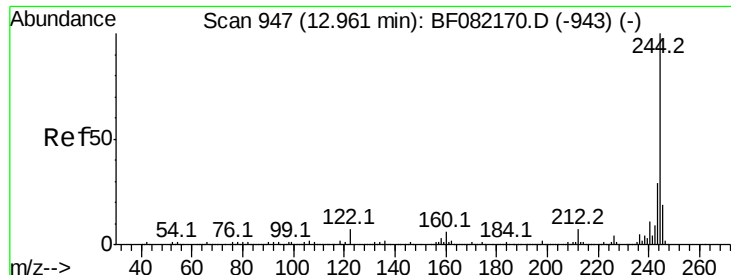

#78

Terphenyl-d14

Concen: 83.19 ng

RT: 12.95 min Scan# 946

Delta R.T. 0.00 min

Lab File: BF082357.D

Acq: 19 Oct 2015 15:59

Instrument :

BNA_F

ClientSampleId :

PB86144BL


Tot Ion:244 Resp: 1148683

Ion Ratio Lower Upper

244 100

212 7.1 5.8 8.6




122 6.1 5.9 8.9

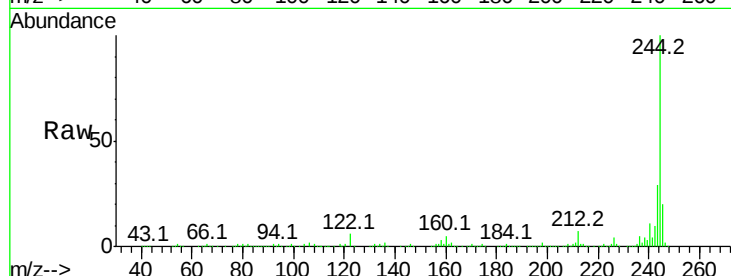

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

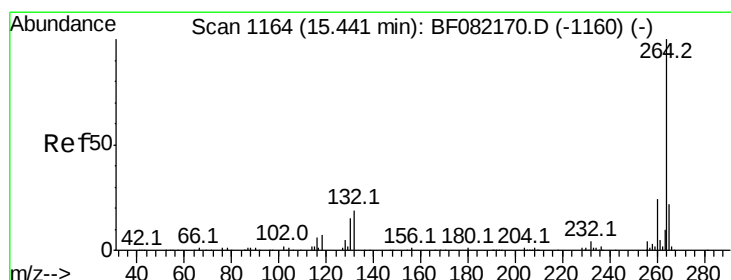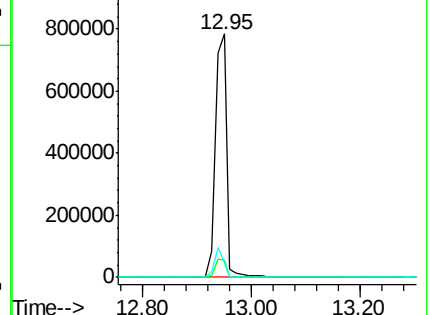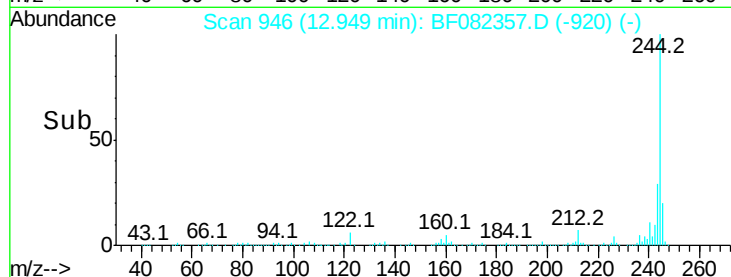

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.62 min Scan# 1180

Delta R.T. -0.05 min

Lab File: BF082357.D

Acq: 19 Oct 2015 15:59


Tgt Ion:264 Resp: 285758

Ion Ratio Lower Upper

264 100

260 23.9 19.0 28.6

265 22.0 17.3 25.9

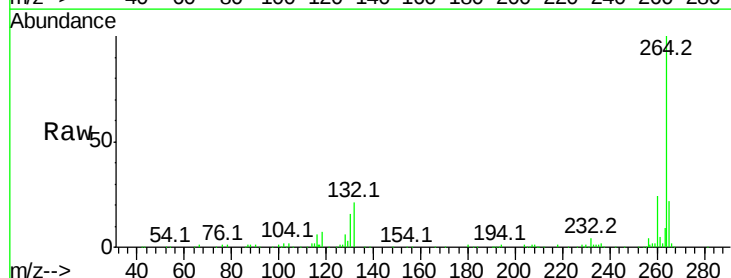

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

