


Data Path : U:\HPCHEM1\BNA F\Data\BF101915\
 Data File : BF082351.D
 Acq On : 19 Oct 2015 12:50
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 12 01:46:21 2015

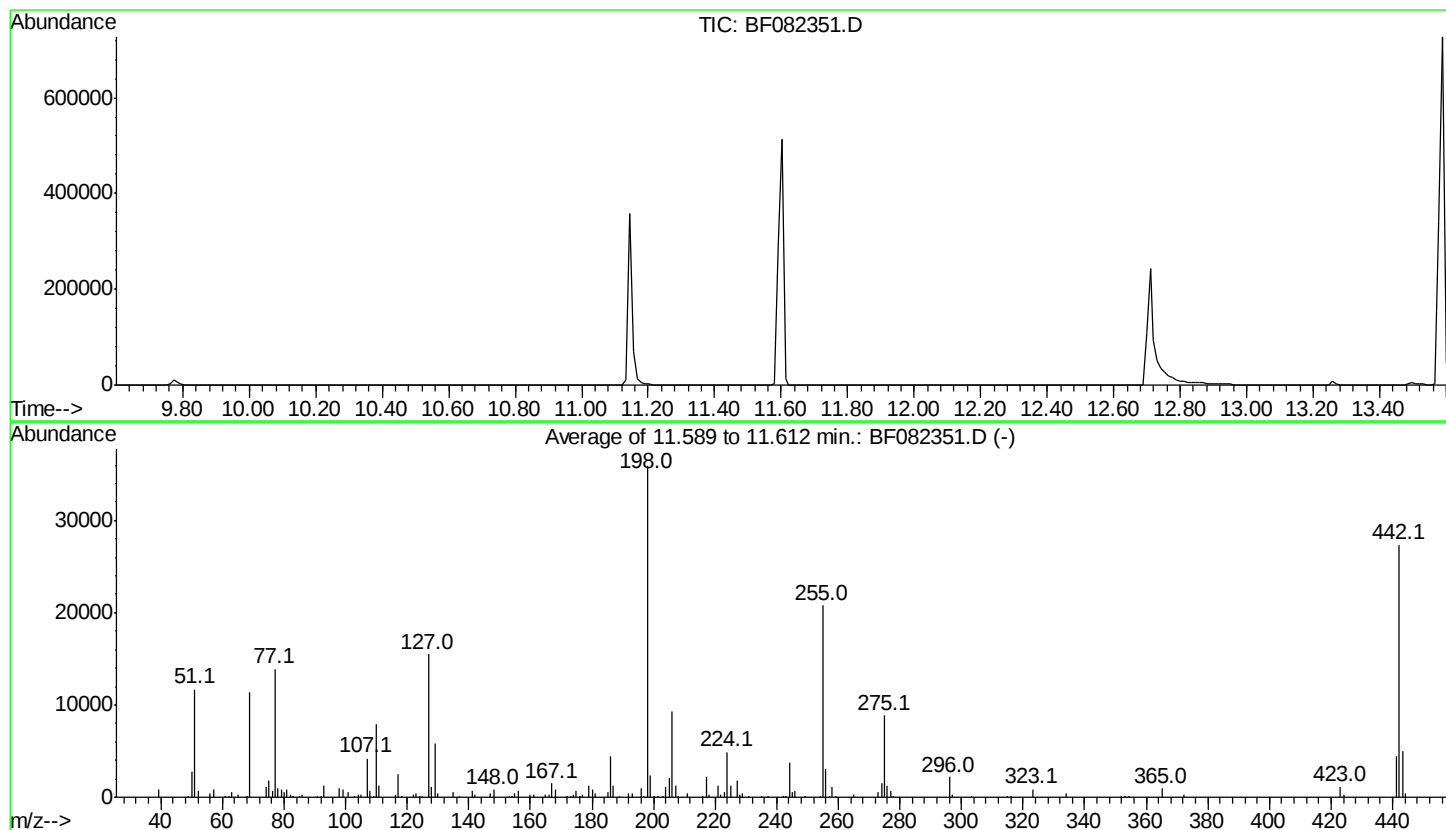

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	11710	PASS
68	69	0.00	2	1.0	118	PASS
69	198	0.00	100	31.8	11424	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.1	15485	PASS
197	198	0.00	2	0.3	123	PASS
198	198	100	100	100.0	35946	PASS
199	198	5	9	6.7	2391	PASS
275	198	10	60	24.7	8870	PASS
365	198	1	100	2.6	926	PASS
441	442	0.01	24	16.5	4498	PASS
442	198	50	100	76.1	27339	PASS
443	442	15	24	18.4	5028	PASS