


Data Path : U:\HPCHEM1\BNA_F\DATA\BF101915\
Data File : BF082373.D
Acq On : 20 Oct 2015 00:44
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 12 01:46:21 2015

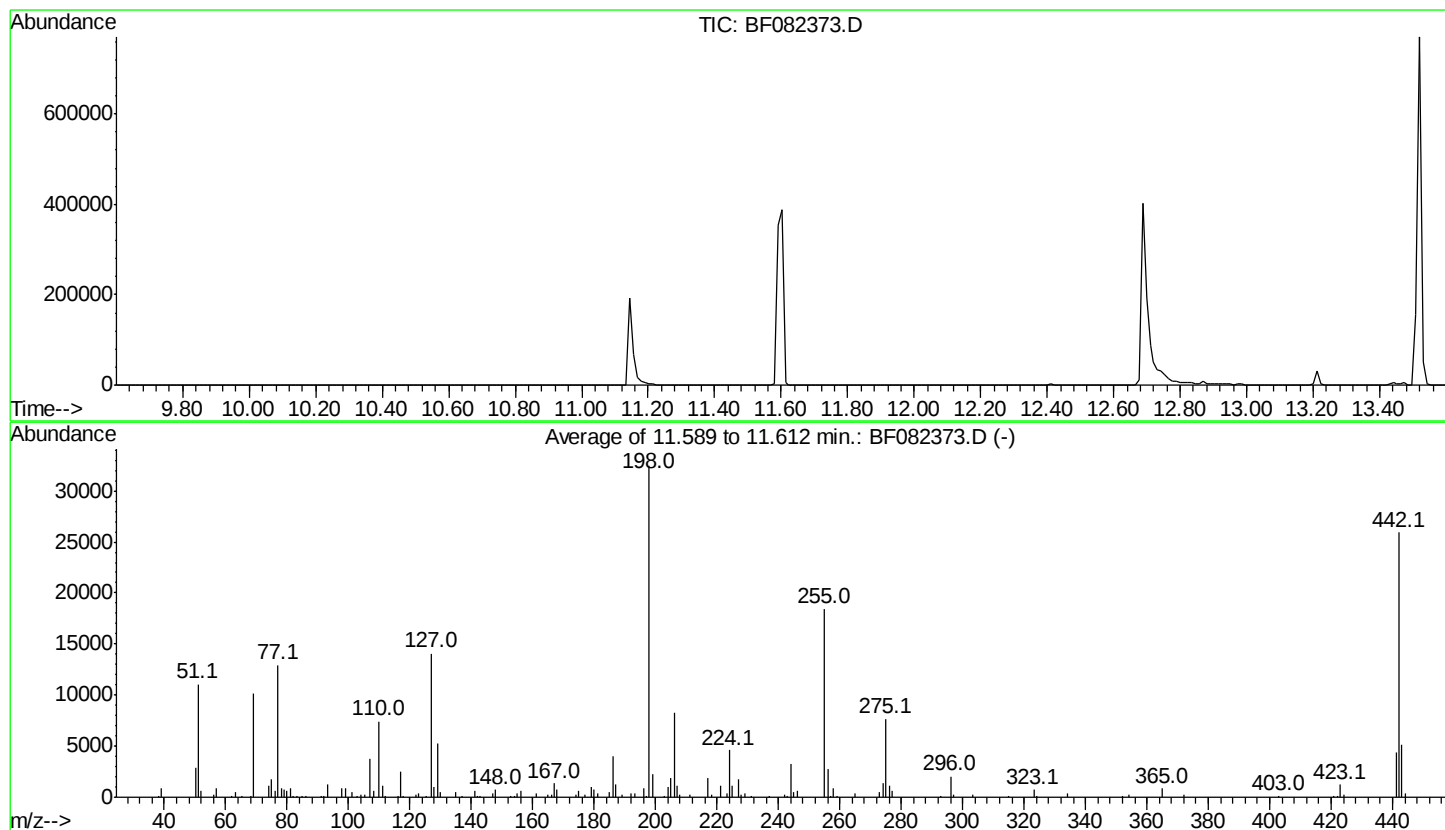

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	11064	PASS
68	69	0.00	2	1.2	126	PASS
69	198	0.00	100	31.5	10215	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.2	14039	PASS
197	198	0.00	2	0.3	101	PASS
198	198	100	100	100.0	32468	PASS
199	198	5	9	6.9	2234	PASS
275	198	10	60	23.6	7649	PASS
365	198	1	100	2.6	828	PASS
441	442	0.01	24	17.1	4444	PASS
442	198	50	100	79.9	25928	PASS
443	442	15	24	19.7	5106	PASS