
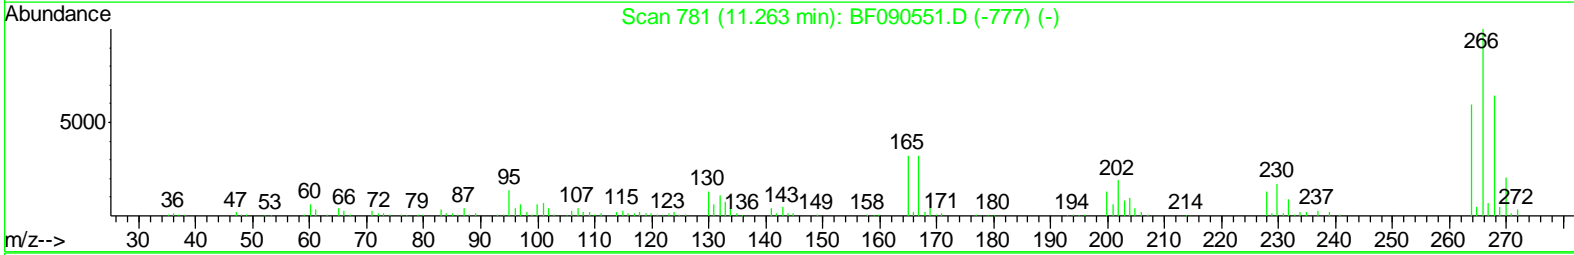
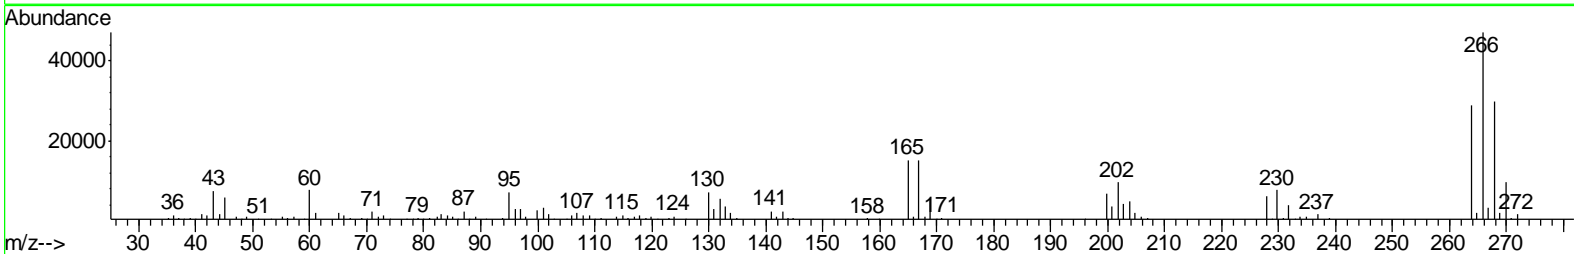


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101916\
 Data File : BF090639.D
 Acq On : 19 Oct 2016 10:16
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 20 07:20:33 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 15:13:23 2016
 Response via : Initial Calibration

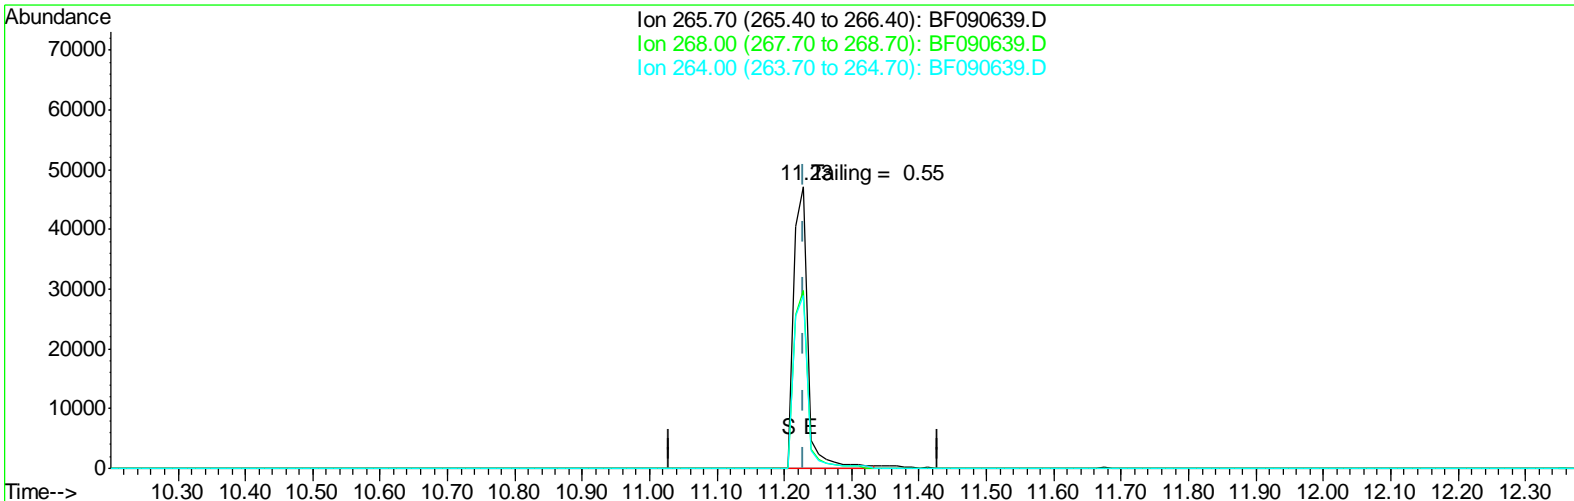

TIC: BF090639.D

(69) Pentachlorophenol (C)




11.229min (-0.000) 0.00ng

response 69702

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	63.36
264.00	59.90	61.54
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101916\
 Data File : BF090639.D
 Acq On : 19 Oct 2016 10:16
 Operator : UM/SJ
 Sample : DF7PP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 20 07:20:33 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 15:13:23 2016
 Response via : Initial Calibration

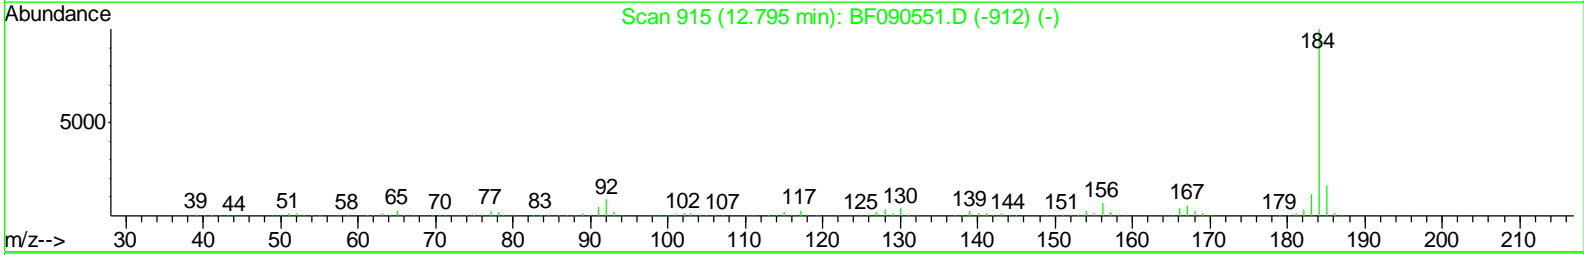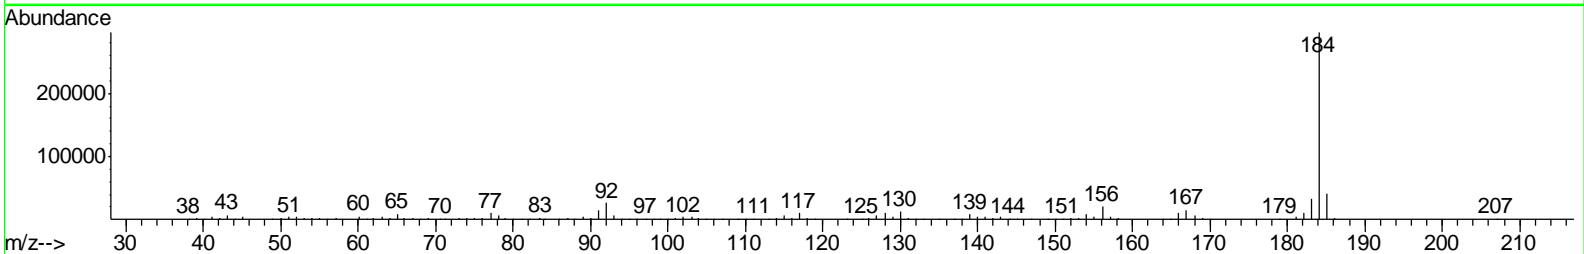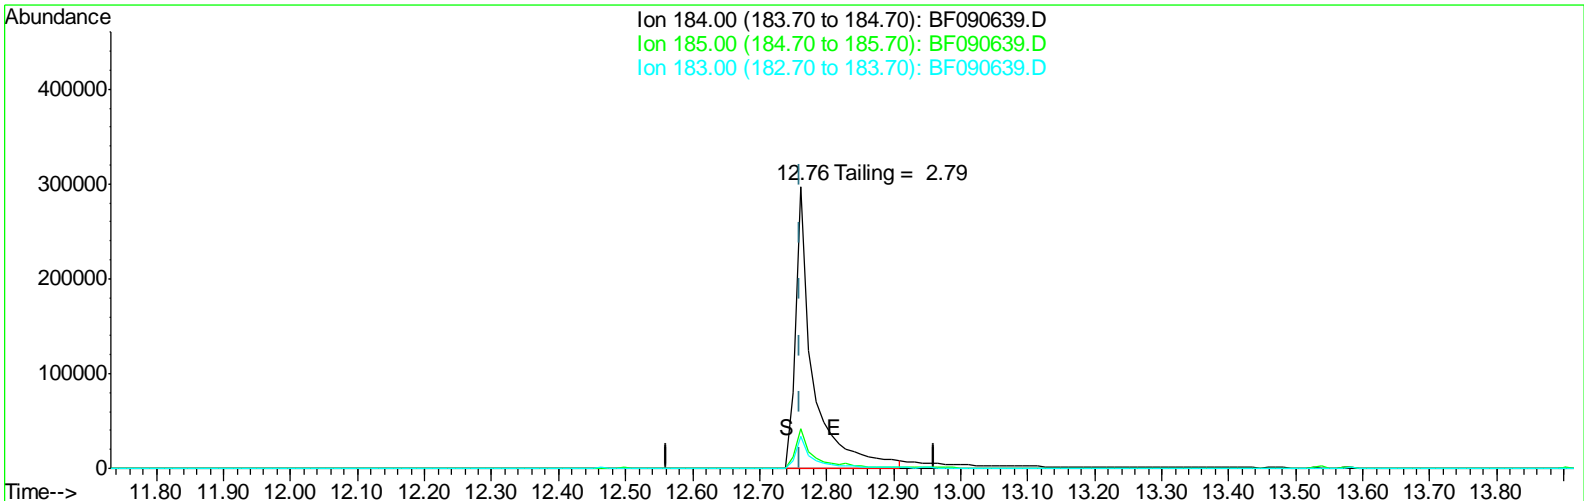

TIC: BF090639.D

(76) Benzidine

12.761min (-0.000) 0.00ng

response 540881

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.10
183.00	11.70	11.33
0.00	0.00	0.00