
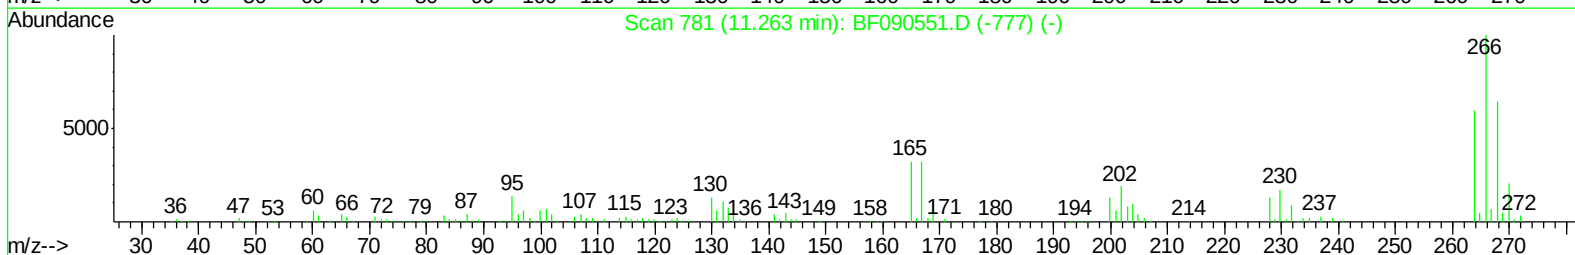
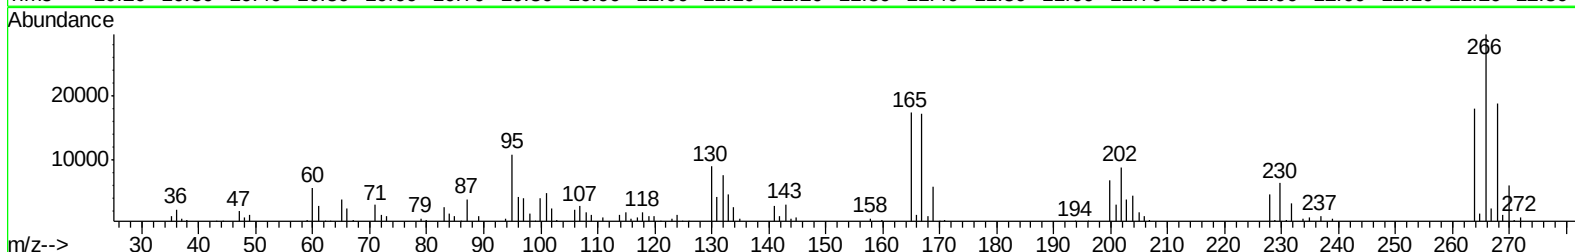


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101916\
Data File : BF090670.D
Acq On : 20 Oct 2016 2:31
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 20 07:49:14 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 15:13:23 2016
Response via : Initial Calibration

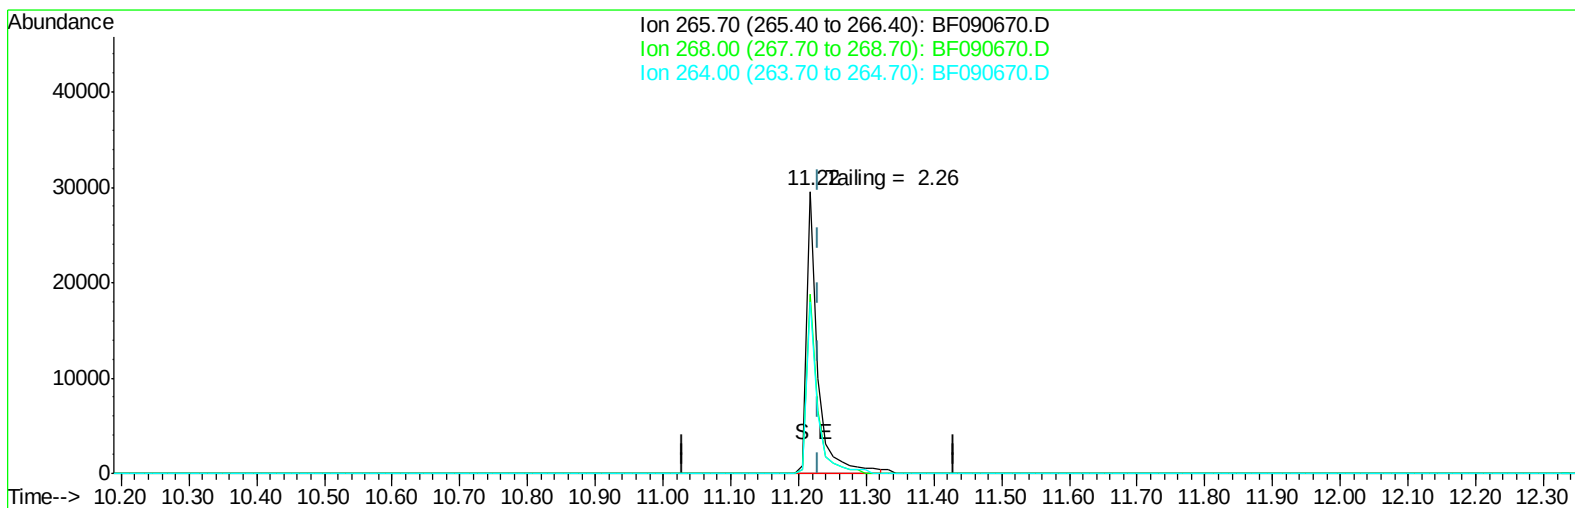

TIC: BF090670.D

(69) Pentachlorophenol (C)




11.218min (-0.011) 7480.80ng

response 33994

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	63.46
264.00	59.90	61.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101916\
Data File : BF090670.D
Acq On : 20 Oct 2016 2:31
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 20 07:49:14 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 15:13:23 2016
Response via : Initial Calibration

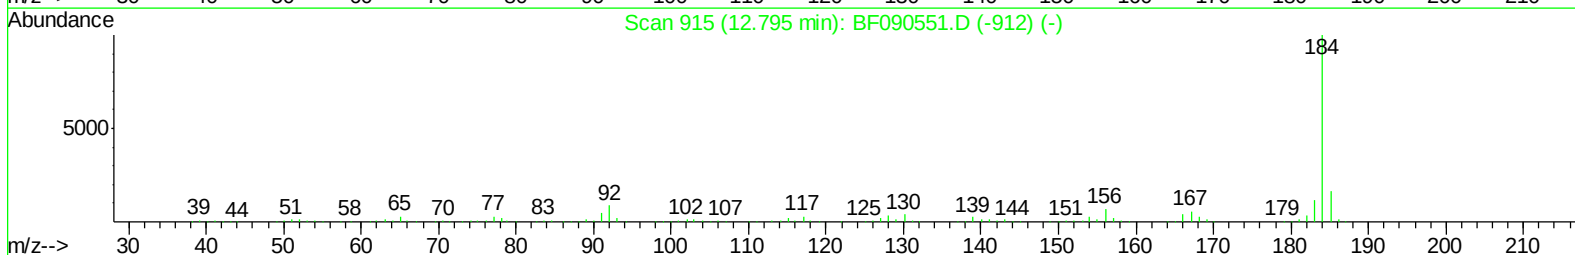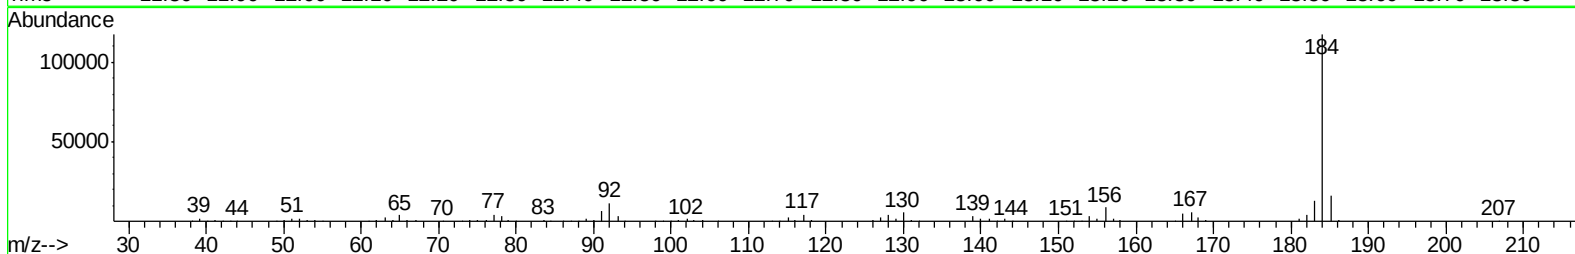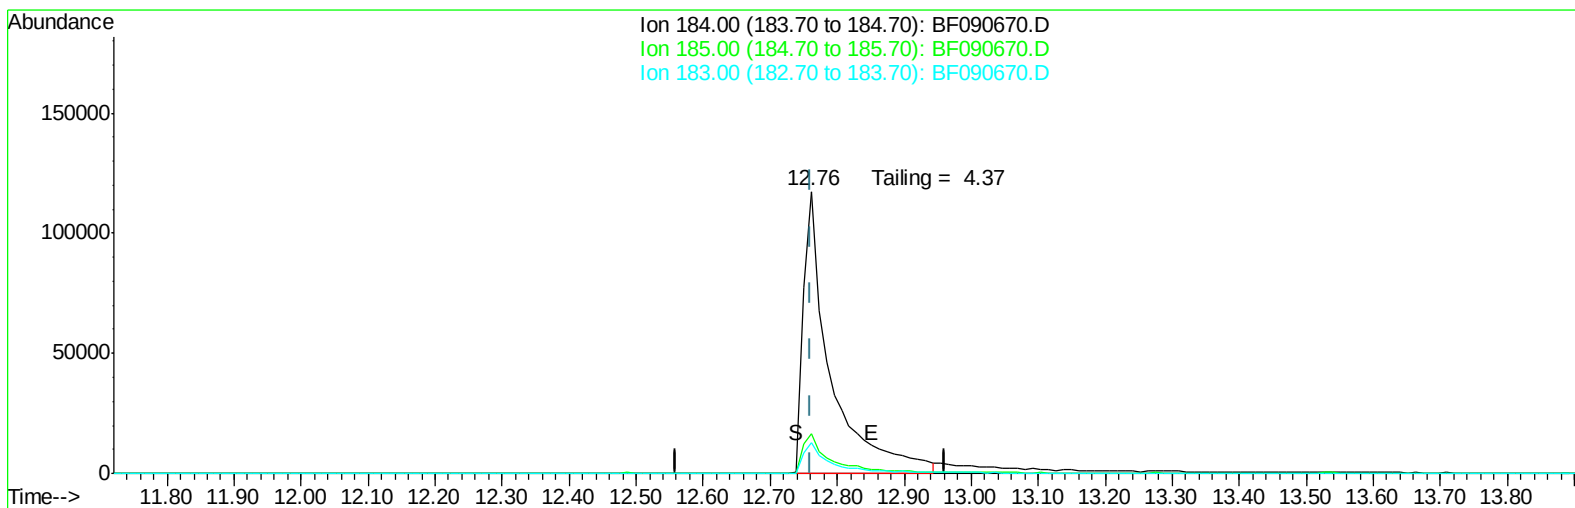

TIC: BF090670.D

(76) Benzidine

12.761min (-0.000) 45424.37ng

response 322113

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.27
183.00	11.70	10.97
0.00	0.00	0.00