


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101916\
 Data File : BF090639.D
 Acq On : 19 Oct 2016 10:16
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 19 15:13:23 2016

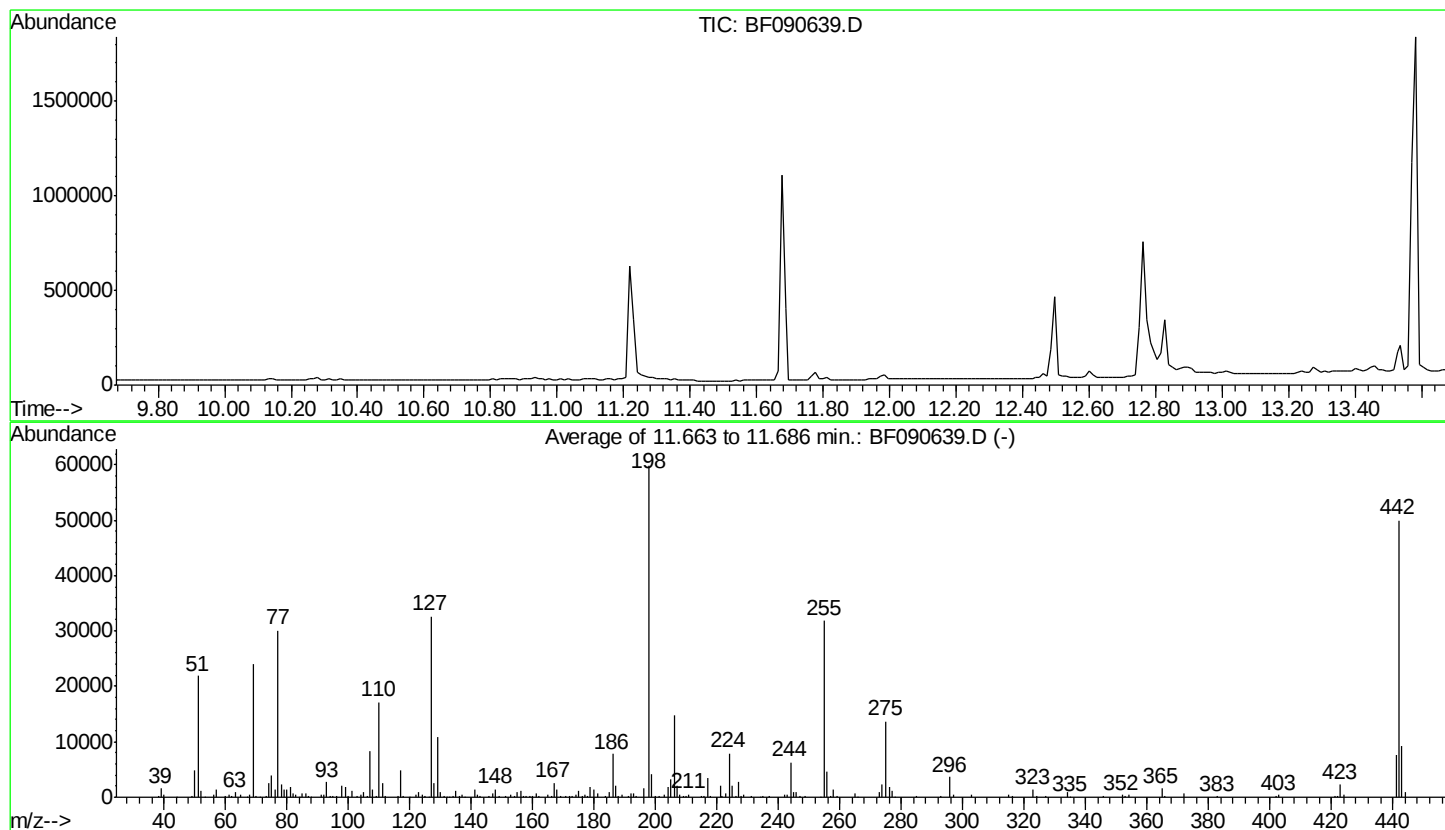

AutoFind: Scans 816, 817, 818; Background Corrected with Scan 813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	21886	PASS
68	69	0.00	2	1.9	453	PASS
69	198	0.00	100	40.1	24000	PASS
70	69	0.00	2	0.8	198	PASS
127	198	10	80	54.5	32626	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59832	PASS
199	198	5	9	7.0	4193	PASS
275	198	10	60	22.8	13667	PASS
365	198	1	100	2.6	1582	PASS
441	442	0.01	24	15.3	7624	PASS
442	198	50	100	83.4	49928	PASS
443	442	15	24	18.5	9261	PASS