


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101916\
 Data File : BF090642.D
 Acq On : 19 Oct 2016 12:47
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 19 15:13:23 2016

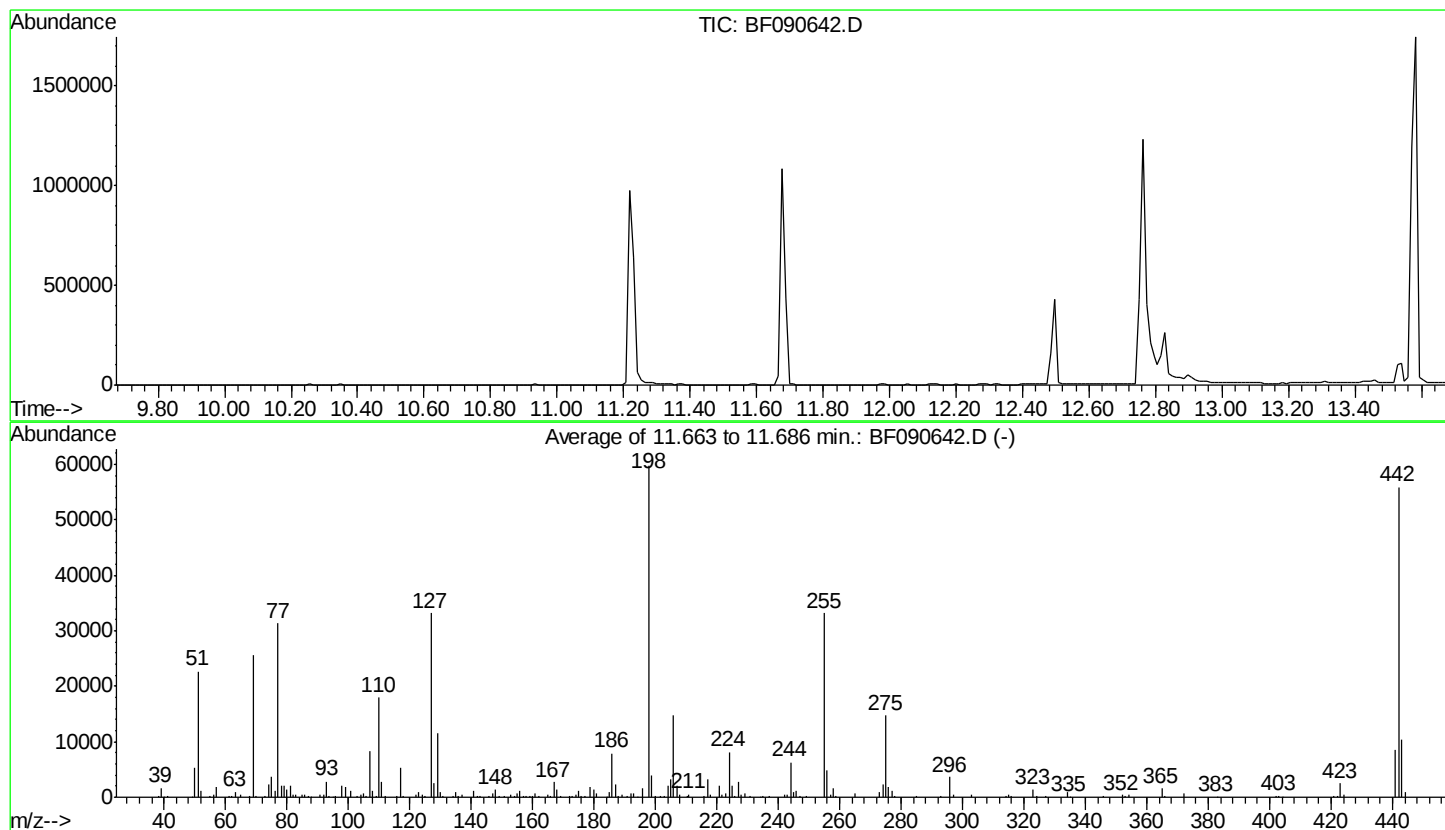

AutoFind: Scans 816, 817, 818; Background Corrected with Scan 813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	22712	PASS
68	69	0.00	2	1.2	315	PASS
69	198	0.00	100	42.9	25624	PASS
70	69	0.00	2	0.5	124	PASS
127	198	10	80	55.6	33202	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59753	PASS
199	198	5	9	6.5	3895	PASS
275	198	10	60	24.6	14708	PASS
365	198	1	100	2.6	1542	PASS
441	442	0.01	24	15.2	8509	PASS
442	198	50	100	93.5	55878	PASS
443	442	15	24	18.6	10374	PASS