


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101916\
 Data File : BF090670.D
 Acq On : 20 Oct 2016 2:31
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 19 15:13:23 2016

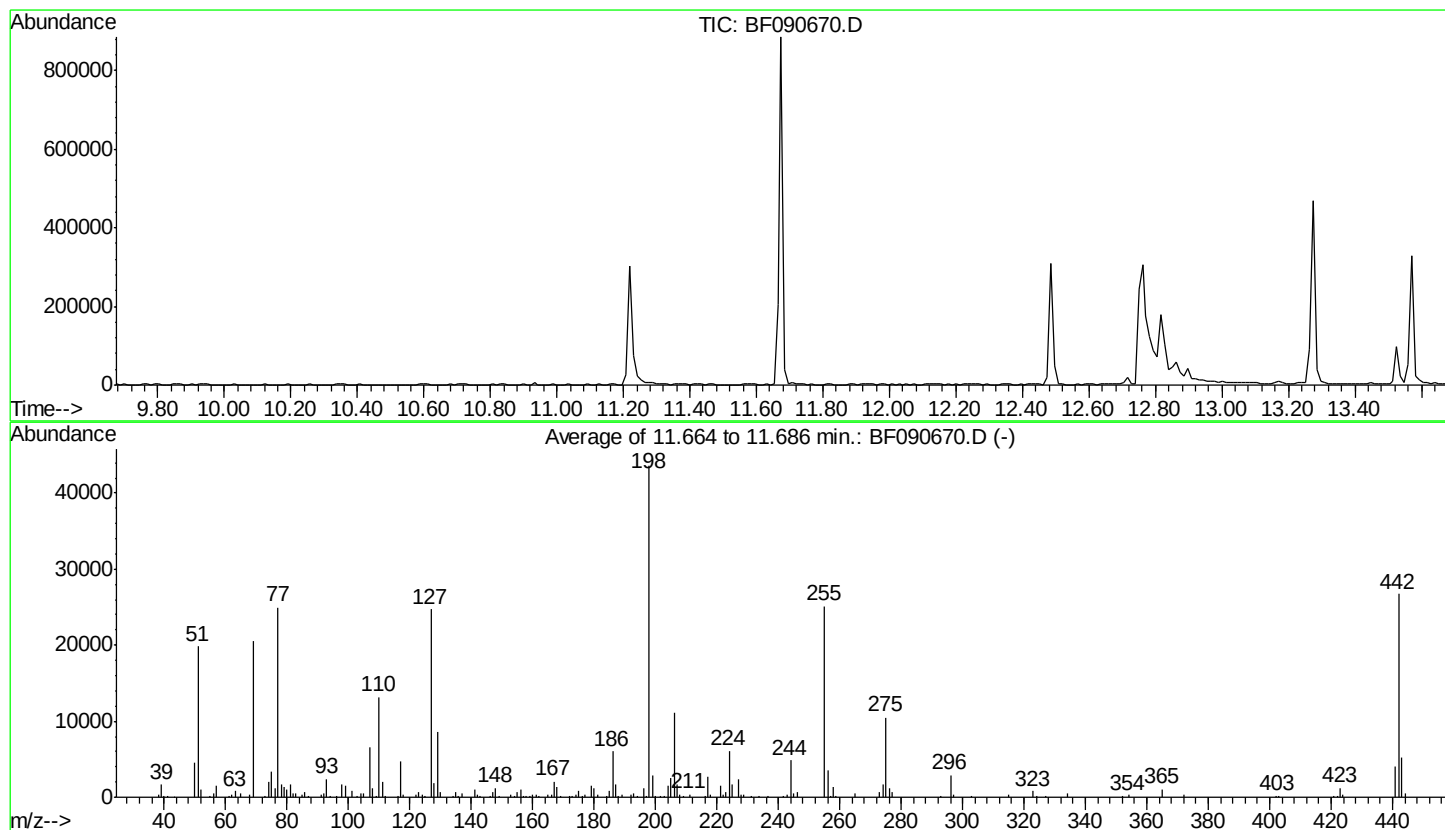

AutoFind: Scans 816, 817, 818; Background Corrected with Scan 813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.4	19813	PASS
68	69	0.00	2	1.7	346	PASS
69	198	0.00	100	47.1	20557	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.7	24725	PASS
197	198	0.00	2	0.3	113	PASS
198	198	100	100	100.0	43606	PASS
199	198	5	9	6.7	2929	PASS
275	198	10	60	24.0	10449	PASS
365	198	1	100	2.4	1026	PASS
441	442	0.01	24	15.2	4068	PASS
442	198	50	100	61.2	26688	PASS
443	442	15	24	19.4	5174	PASS