

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101917\
 Data File : BF099673.D
 Acq On : 19 Oct 2017 22:47
 Operator : SJ/JU
 Sample : I5884-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 101217-TIFR-E-D-B

Quant Time: Oct 20 13:39:28 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 20 13:11:43 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	93888	20.00	ng	0.00
21) Naphthalene-d8	8.10	136	382468	20.00	ng	0.00
38) Acenaphthene-d10	9.85	164	158926	20.00	ng	0.00
63) Phenanthrene-d10	11.34	188	222091	20.00	ng	0.00
75) Chrysene-d12	13.99	240	158947	20.00	ng	0.00
86) Perylene-d12	15.44	264	177981	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	329676	55.90	ng	0.00
7) Phenol-d6	6.46	99	248415	34.14	ng	0.00
23) Nitrobenzene-d5	7.39	82	618827	103.76	ng	0.00
41) 2,4,6-Tribromophenol	10.65	330	121752	93.62	ng	0.00
44) 2-Fluorobiphenyl	9.17	172	1116853	117.32	ng	0.00
78) Terphenyl-d14	12.92	244	674481	96.50	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	9.57	163	28979	2.416	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101917\
Data File : BF099673.D
Acq On : 19 Oct 2017 22:47
Operator : SJ/JU
Sample : I5884-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
101217-TIFR-E-D-B

Quant Time: Oct 20 13:39:28 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 20 13:11:43 2017
Response via : Initial Calibration

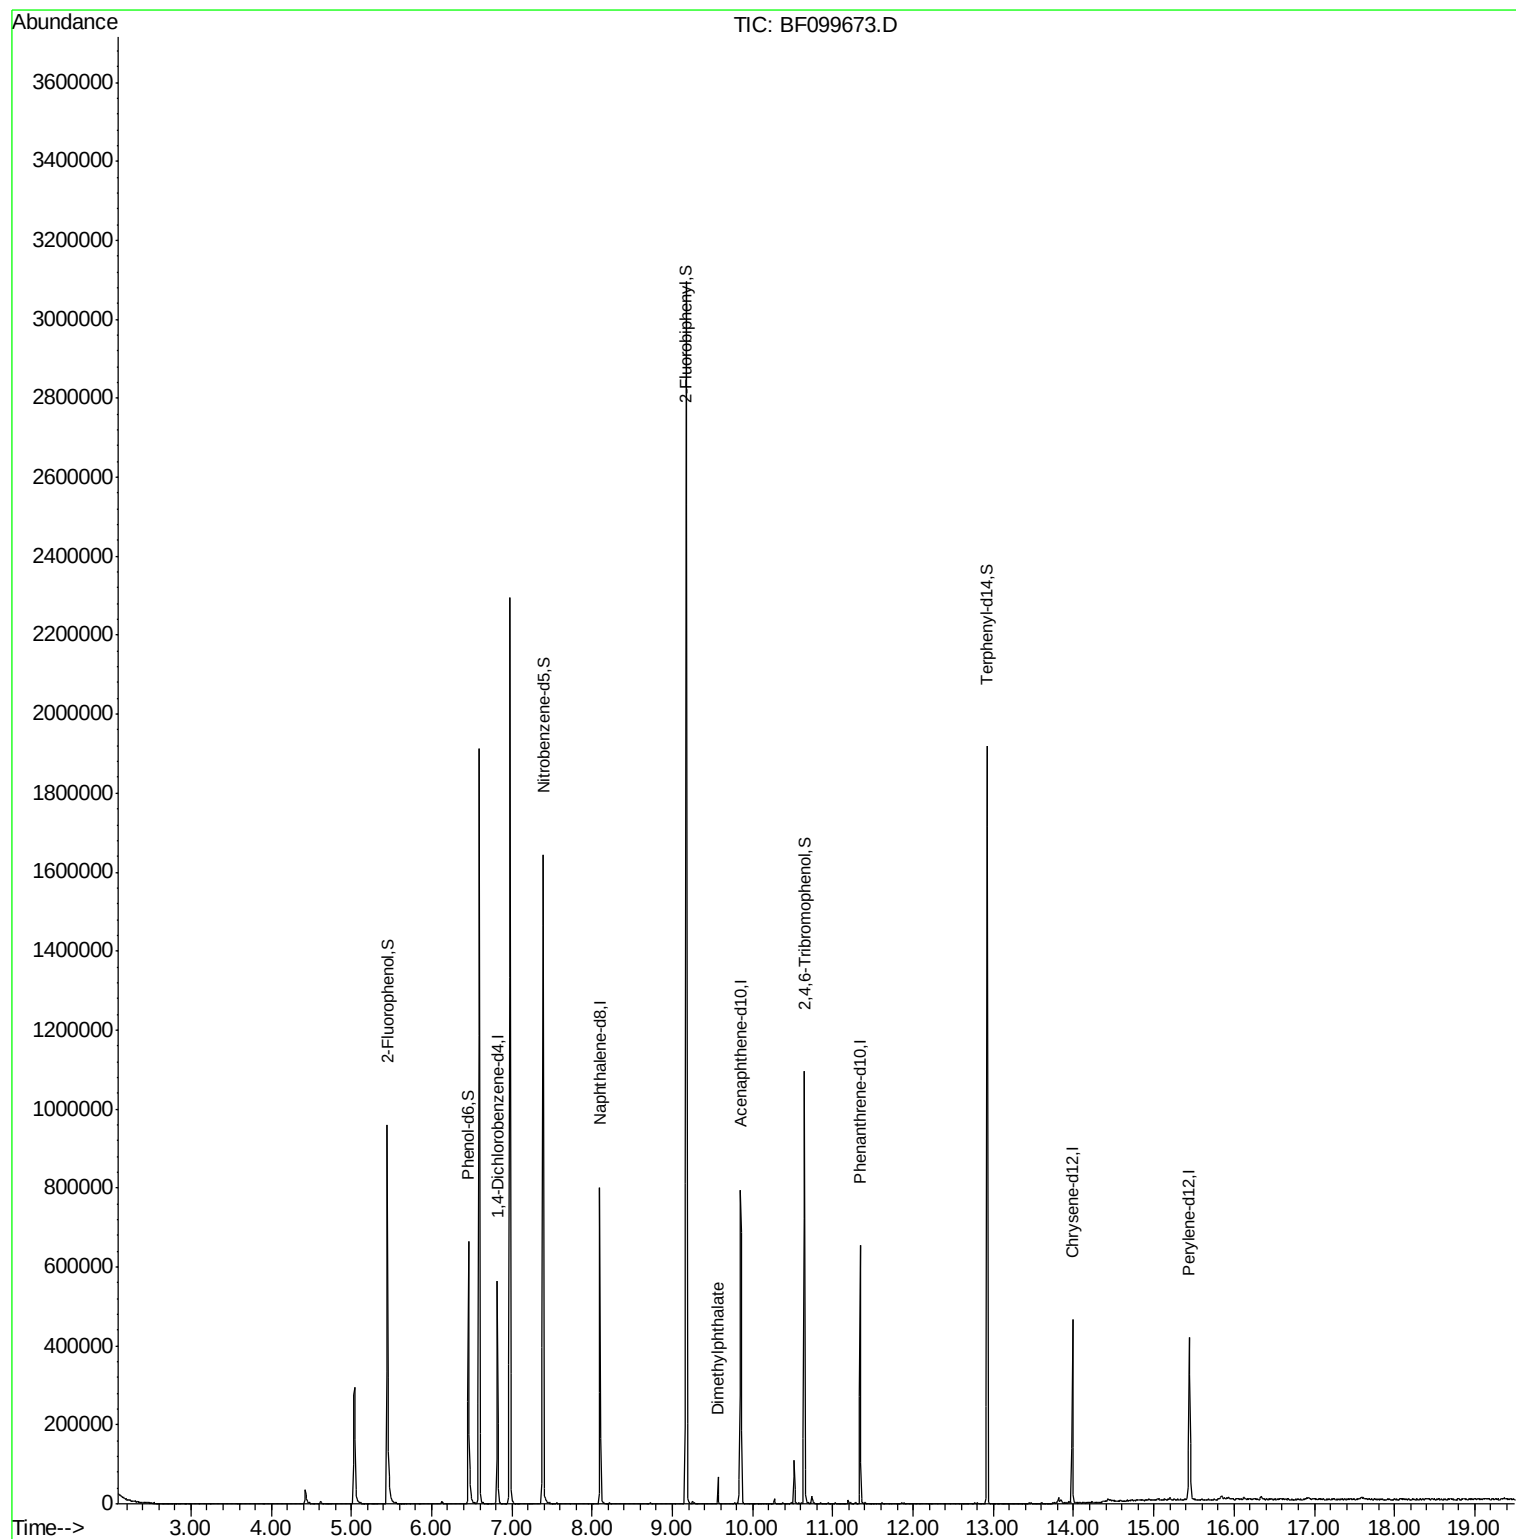

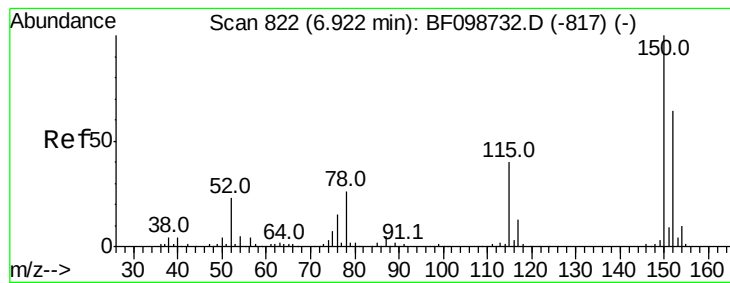


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.82 min Scan# 805
Delta R.T. -0.00 min
Lab File: BF099673.D
Acq: 19 Oct 2017 22:47

Instrument :
BNA_F
ClientSampleId :
101217-TIFR-E-D-B

Tot Ion:152 Resp: 93888
Ion Ratio Lower Upper
152 100
150 156.6 124.6 186.8
115 57.0 50.1 75.1

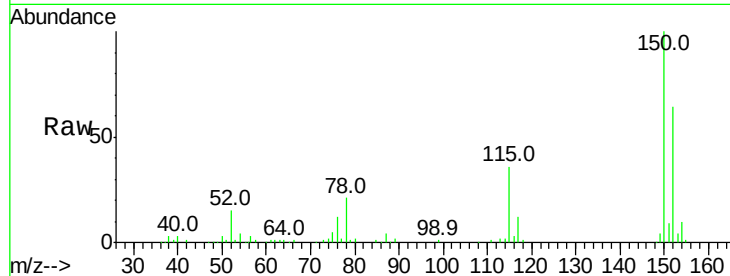


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

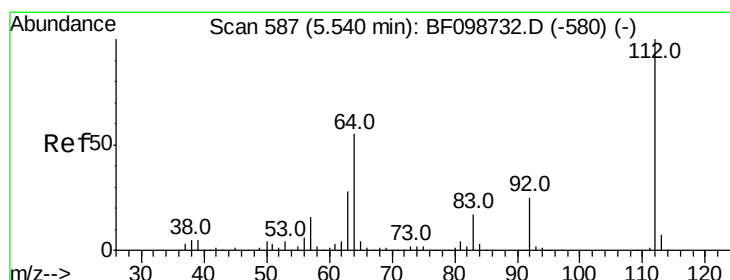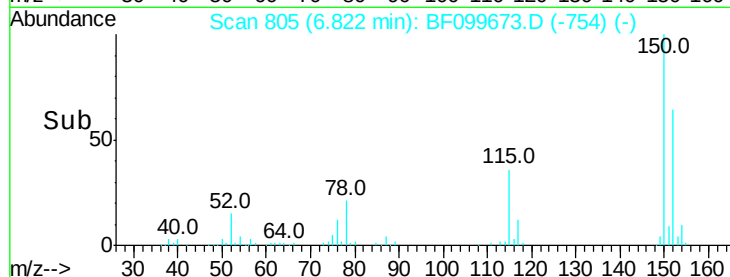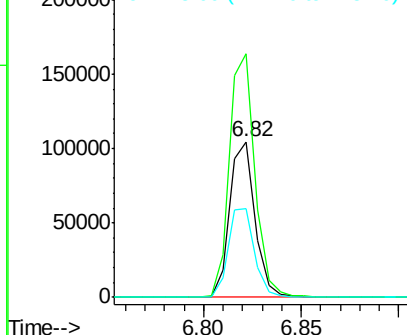



#5


2-Fluorophenol
Concen: 55.898 ng
RT: 5.45 min Scan# 571
Delta R.T. 0.01 min
Lab File: BF099673.D
Acq: 19 Oct 2017 22:47

Tgt Ion:112 Resp: 329676
Ion Ratio Lower Upper
112 100
64 53.7 47.9 71.9
63 26.2 23.7 35.5

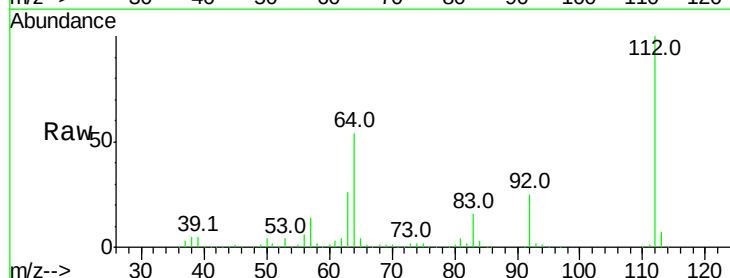

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

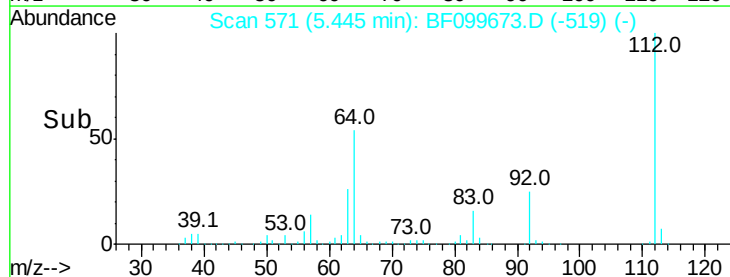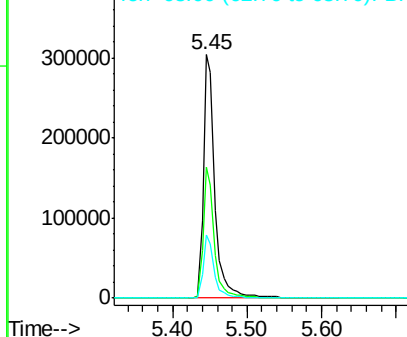

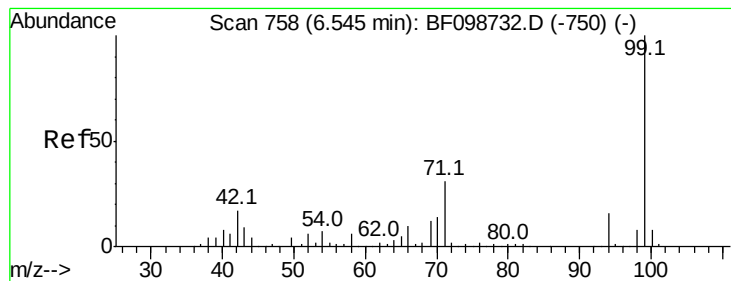

#7

Phenol-d6

Concen: 34.143 ng

RT: 6.46 min Scan# 743

Delta R.T. -0.01 min

Lab File: BF099673.D

Acq: 19 Oct 2017 22:47

Instrument :

BNA_F

ClientSampleId :

101217-TIFR-E-D-B


Tot Ion: 99 Resp: 248415

Ion Ratio Lower Upper

99 100

42 14.6 14.5 21.7




71 29.6 25.4 38.0

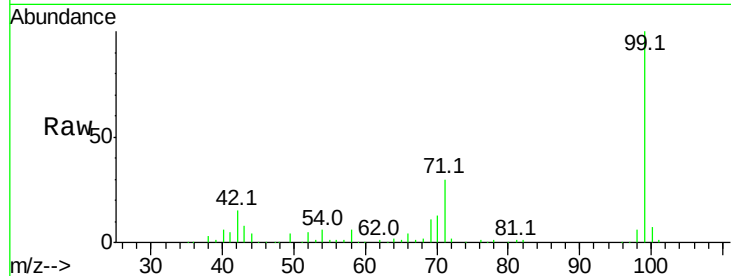

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

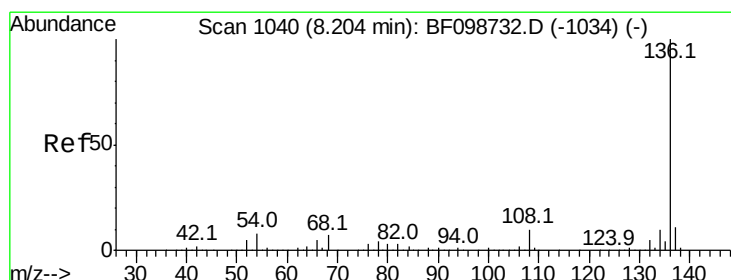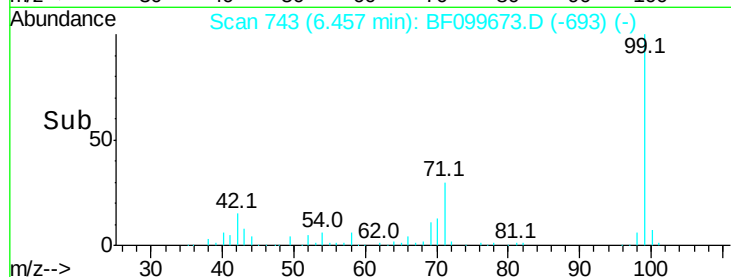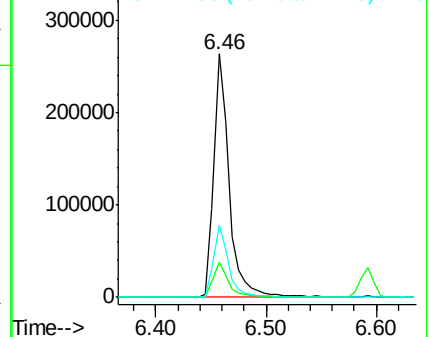

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.10 min Scan# 1022

Delta R.T. -0.01 min

Lab File: BF099673.D

Acq: 19 Oct 2017 22:47

Tgt Ion: 136 Resp: 382468


Ion Ratio Lower Upper

136 100

137 10.8 8.9 13.3

54 7.3 6.6 9.8

68 6.1 5.0 7.4


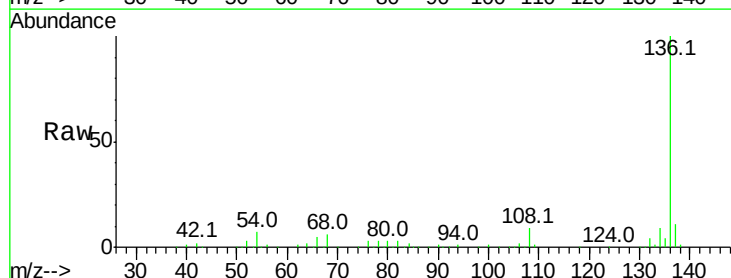



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



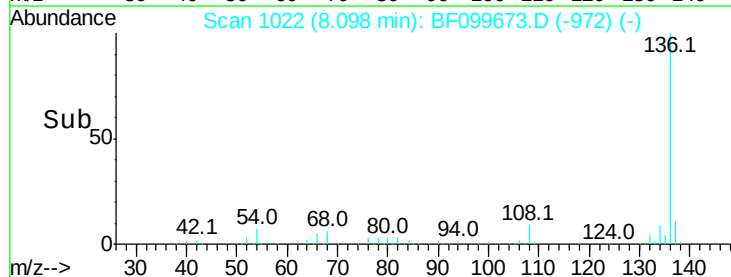
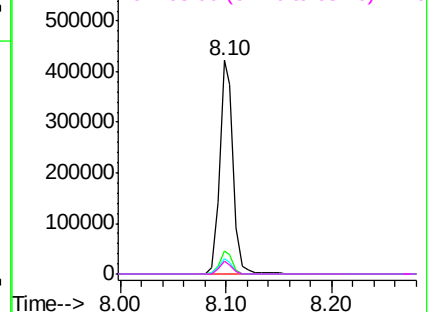


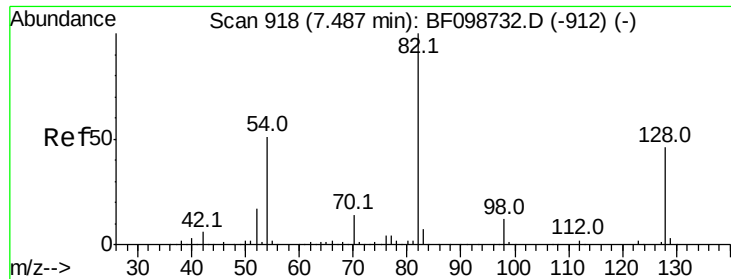

#23
Nitrobenzene-d5
Concen: 103.762 ng
RT: 7.39 min Scan# 902
Delta R.T. -0.00 min
Lab File: BF099673.D
Acq: 19 Oct 2017 22:47




Instrument :
BNA_F
ClientSampleId :
101217-TIFR-E-D-B


Tot Ion: 82 Resp: 618827
Ion Ratio Lower Upper
82 100
128 51.5 36.1 54.1
54 43.3 41.4 62.2

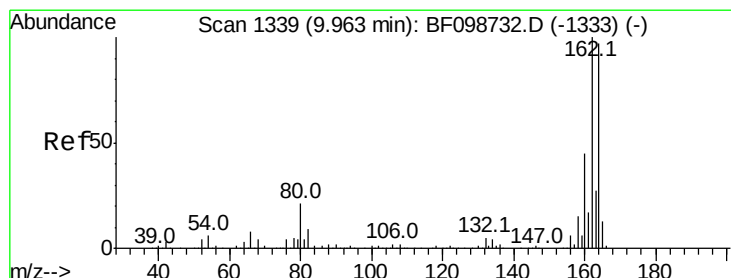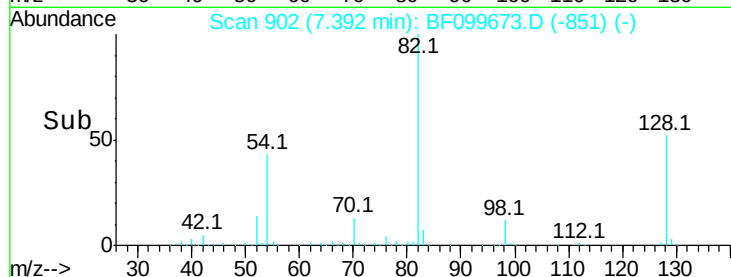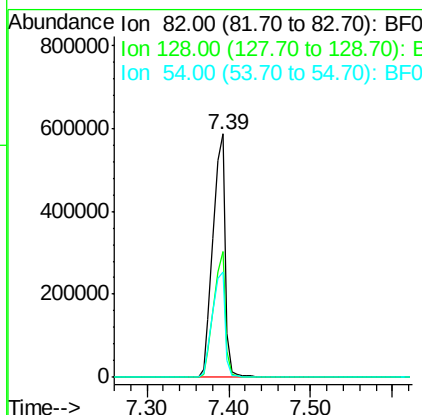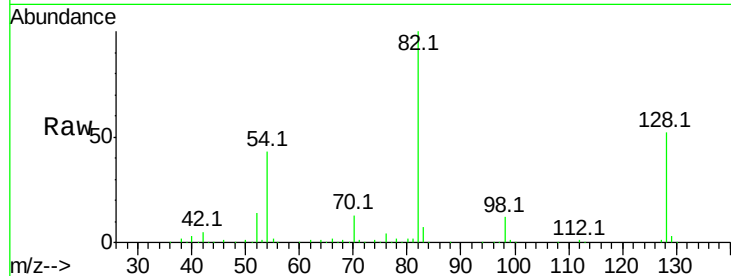

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.85 min Scan# 1320
Delta R.T. -0.01 min
Lab File: BF099673.D
Acq: 19 Oct 2017 22:47

Tgt Ion:164 Resp: 158926
Ion Ratio Lower Upper
164 100
162 101.5 86.1 129.1
160 44.1 38.3 57.5

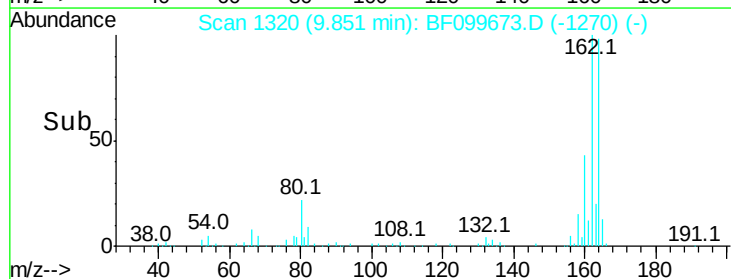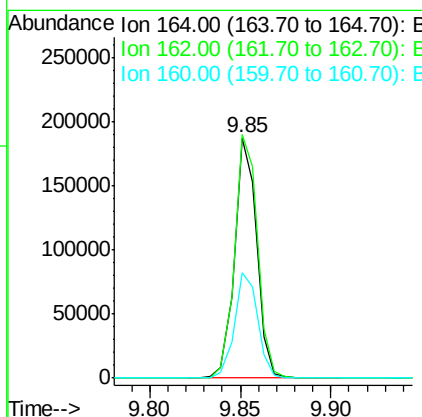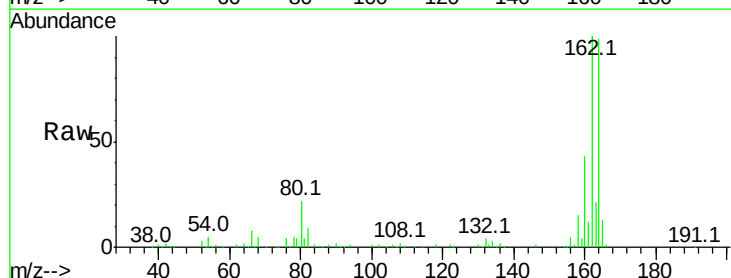


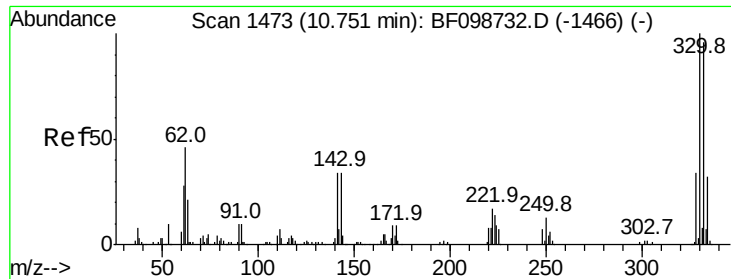




#41
 2,4,6-Tribromophenol
 Concen: 93.623 ng
 RT: 10.65 min Scan# 1455
 Delta R.T. -0.01 min
 Lab File: BF099673.D
 Acq: 19 Oct 2017 22:47

Instrument :
 BNA_F
 ClientSampleId :
 101217-TIFR-E-D-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.1	77.0	115.6
141	36.3	29.9	44.9

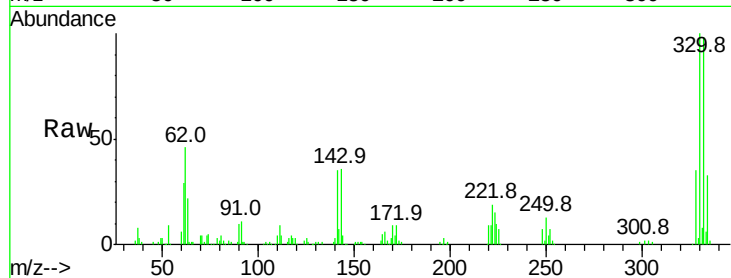


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

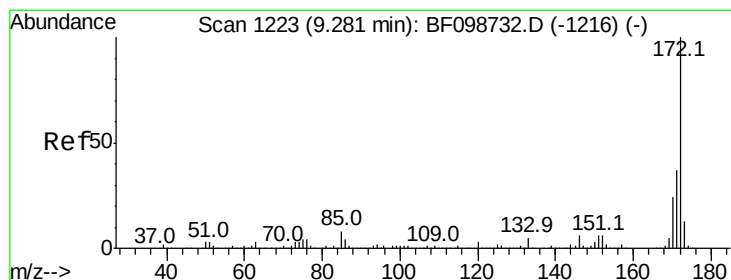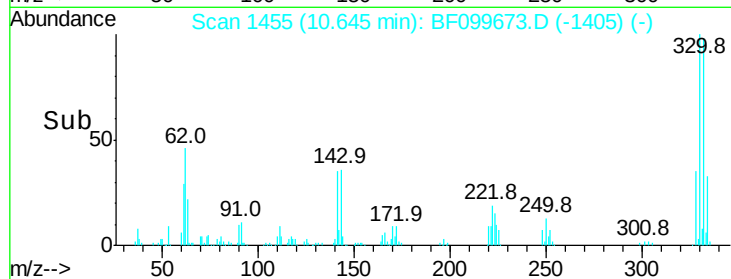
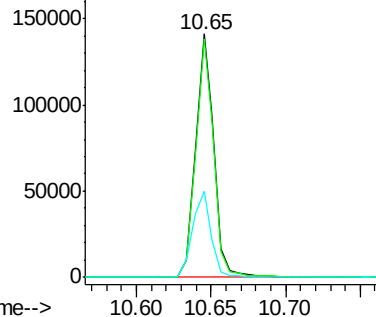



#44
 2-Fluorobiphenyl
 Concen: 117.318 ng
 RT: 9.17 min Scan# 1205
 Delta R.T. -0.00 min
 Lab File: BF099673.D
 Acq: 19 Oct 2017 22:47

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.8	29.7	44.5
170	23.6	19.6	29.4

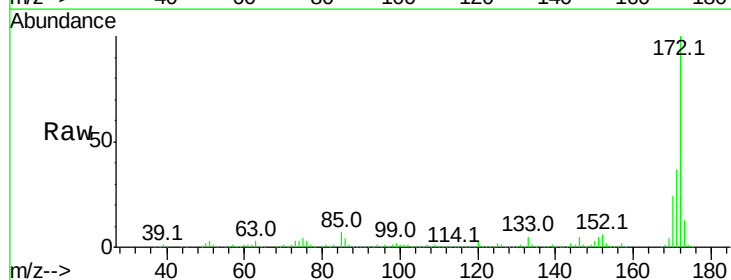

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

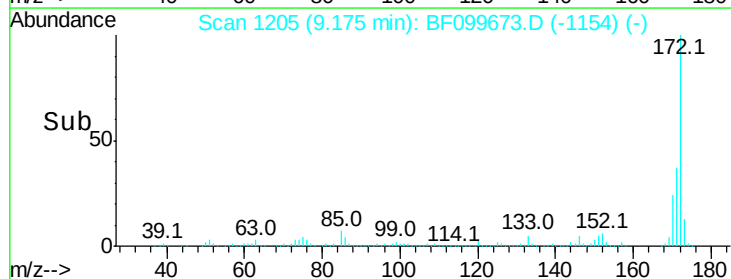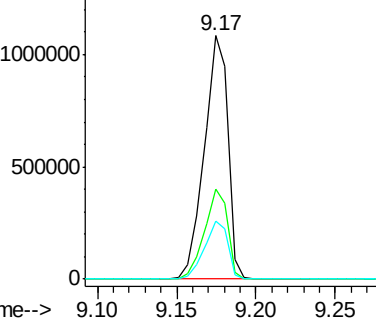


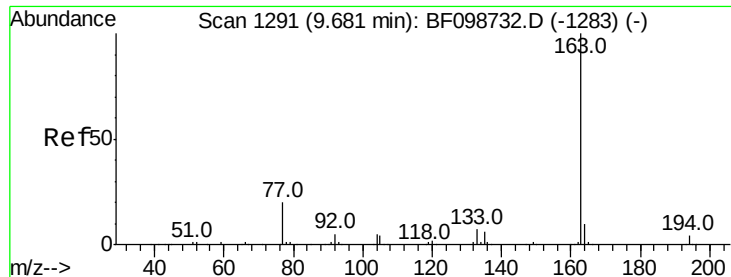




#49
Dimethylphthalate
Concen: 2.416 ng
RT: 9.57 min Scan# 1272
Delta R.T. -0.01 min
Lab File: BF099673.D
Acq: 19 Oct 2017 22:47

Instrument :
BNA_F
ClientSampleId :
101217-TIFR-E-D-B

Tot Ion:163 Resp: 28979
Ion Ratio Lower Upper
163 100
194 3.6 2.7 4.1
164 9.3 8.2 12.2

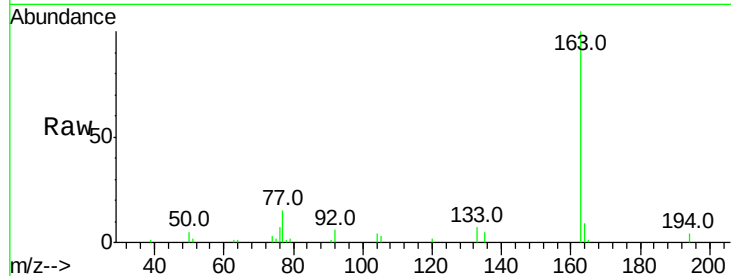


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

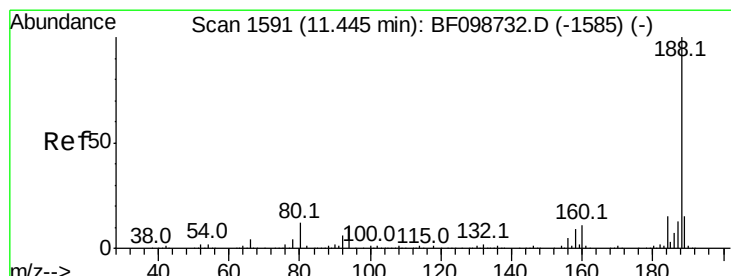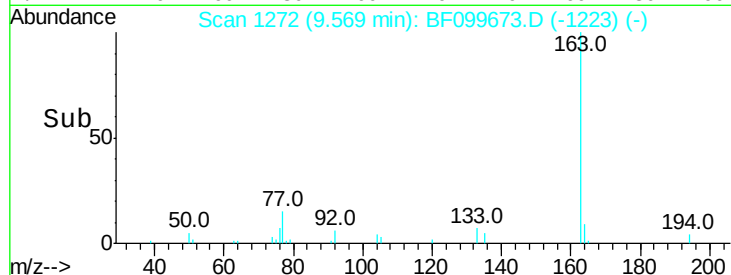
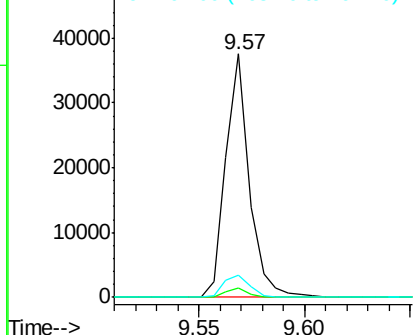



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.34 min Scan# 1573
Delta R.T. -0.01 min
Lab File: BF099673.D
Acq: 19 Oct 2017 22:47

Tgt Ion:188 Resp: 222091
Ion Ratio Lower Upper
188 100
94 10.7 8.5 12.7
80 12.1 9.2 13.8

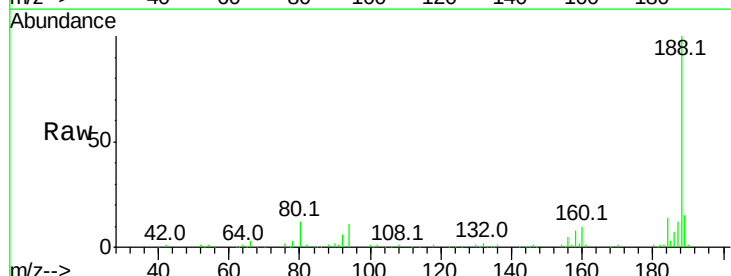

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

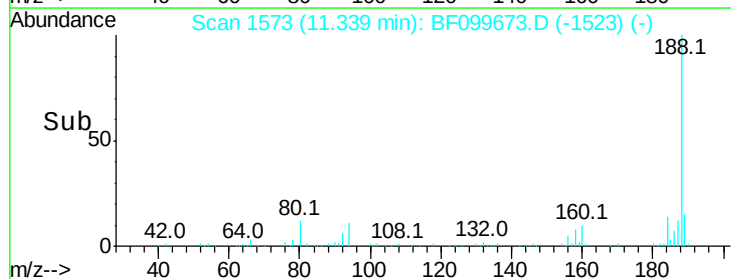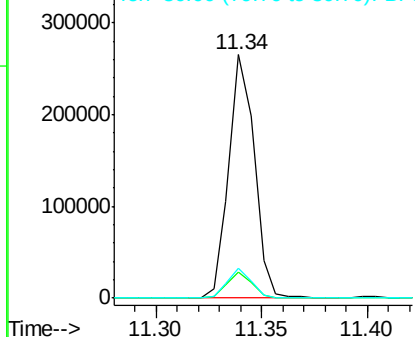

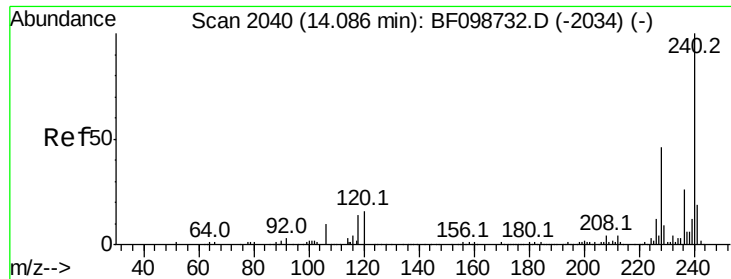

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.99 min Scan# 2023

Delta R.T. -0.00 min

Lab File: BF099673.D

Acq: 19 Oct 2017 22:47

Instrument :

BNA_F

ClientSampleId :

101217-TIFR-E-D-B


Tot Ion:240 Resp: 158947

Ion Ratio Lower Upper

240 100

120 12.5 9.5 14.3




236 25.4 20.7 31.1

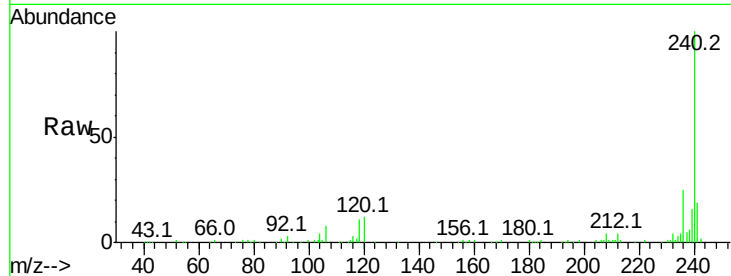

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

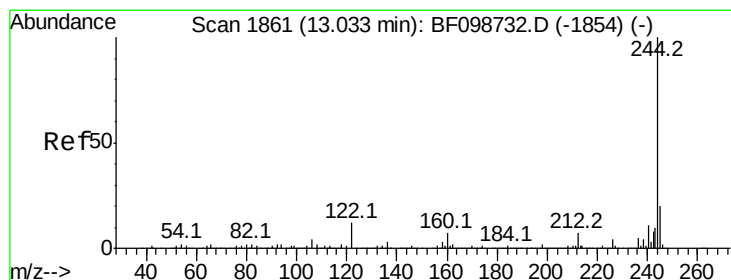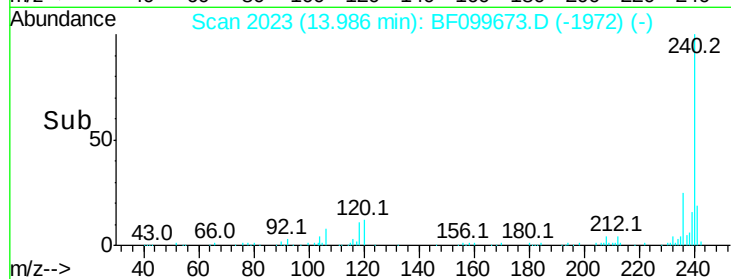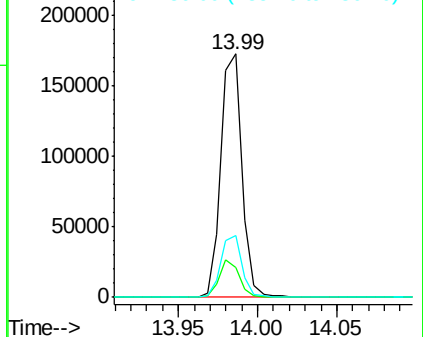

#78

Terphenyl-d14

Concen: 96.504 ng

RT: 12.92 min Scan# 1842

Delta R.T. -0.00 min

Lab File: BF099673.D

Acq: 19 Oct 2017 22:47


Tgt Ion:244 Resp: 674481

Ion Ratio Lower Upper

244 100

212 6.9 5.4 8.0



122 14.5 11.0 16.4

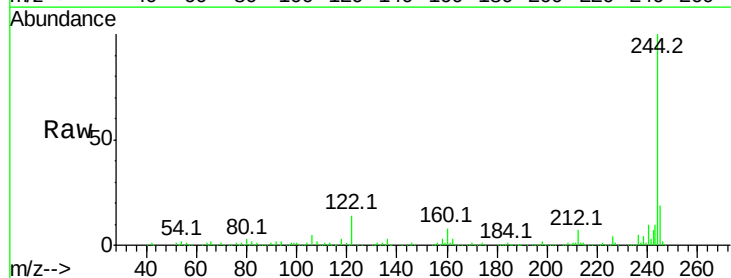


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

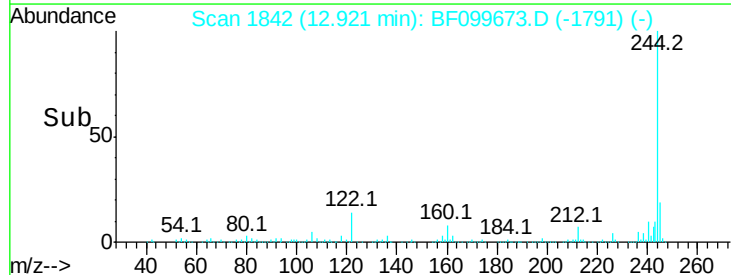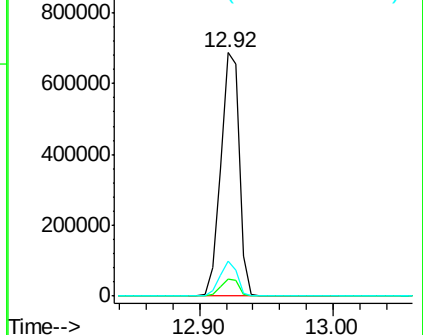


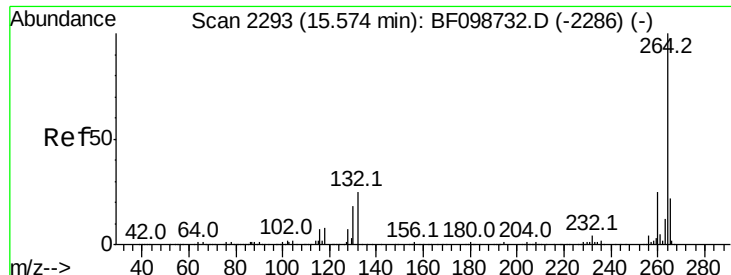

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.44 min Scan# 2271
 Delta R.T. 0.01 min
 Lab File: BF099673.D
 Acq: 19 Oct 2017 22:47

Instrument :
 BNA_F
 ClientSampleId :
 101217-TIFR-E-D-B

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.5	19.2	28.8
265	21.0	17.5	26.3

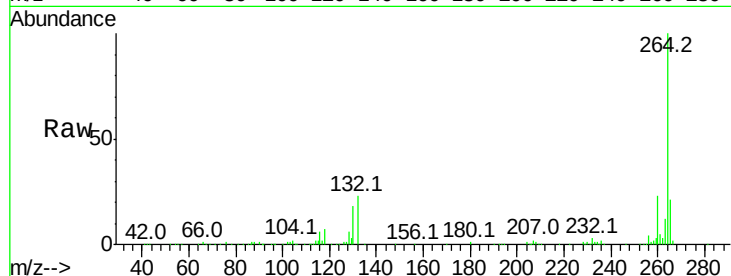

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

