

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101917\
 Data File : BF099674.D
 Acq On : 19 Oct 2017 23:15
 Operator : SJ/JU
 Sample : I5884-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 101217-TIFR-E-D-M

Quant Time: Oct 20 13:40:38 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 20 13:11:43 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	88907	20.00	ng	0.00
21) Naphthalene-d8	8.10	136	354973	20.00	ng	0.00
38) Acenaphthene-d10	9.85	164	150338	20.00	ng	0.00
63) Phenanthrene-d10	11.34	188	217080	20.00	ng	0.00
75) Chrysene-d12	13.99	240	149326	20.00	ng	0.00
86) Perylene-d12	15.44	264	170739	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	278995	49.95	ng	0.00
7) Phenol-d6	6.46	99	212665	30.87	ng	0.00
23) Nitrobenzene-d5	7.39	82	551375	99.61	ng	0.00
41) 2,4,6-Tribromophenol	10.65	330	105901	86.09	ng	0.00
44) 2-Fluorobiphenyl	9.17	172	997637	110.78	ng	0.00
78) Terphenyl-d14	12.92	244	603821	91.96	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101917\
Data File : BF099674.D
Acq On : 19 Oct 2017 23:15
Operator : SJ/JU
Sample : I5884-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
101217-TIFR-E-D-M

Quant Time: Oct 20 13:40:38 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 20 13:11:43 2017
Response via : Initial Calibration

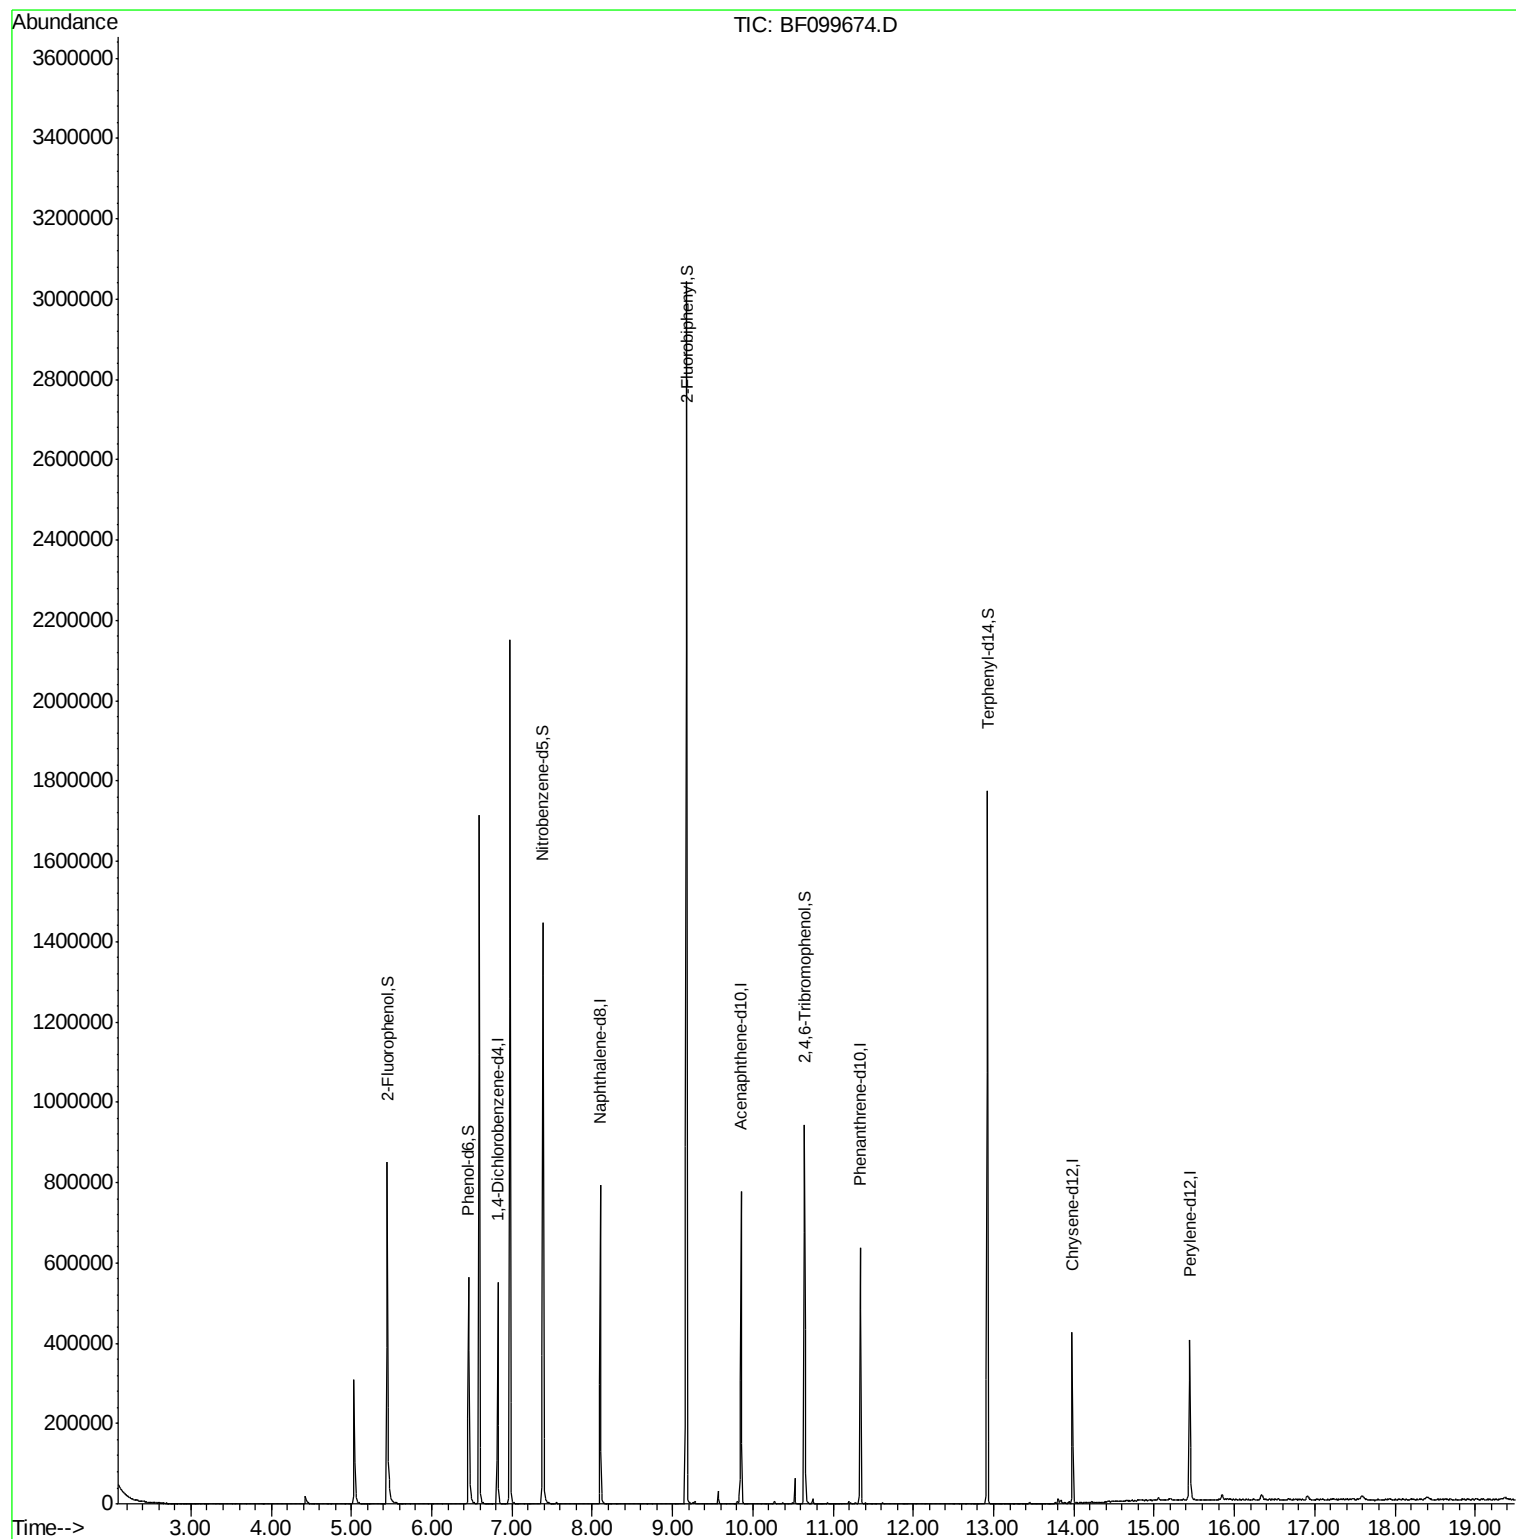




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.82 min Scan# 805
 Delta R.T. -0.00 min
 Lab File: BF099674.D
 Acq: 19 Oct 2017 23:15

Instrument :
 BNA_F
 ClientSampleId :
 101217-TIFR-E-D-M

Tot Ion:152 Resp: 88907
 Ion Ratio Lower Upper
 152 100
 150 155.1 124.6 186.8
 115 57.5 50.1 75.1

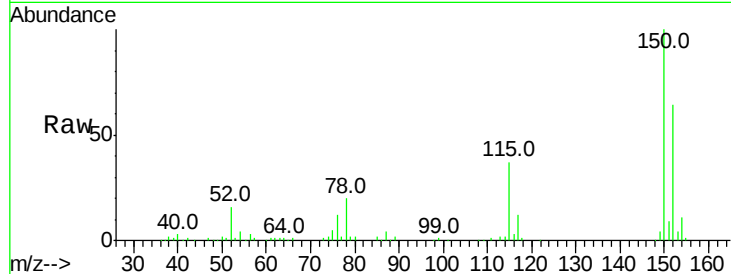


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

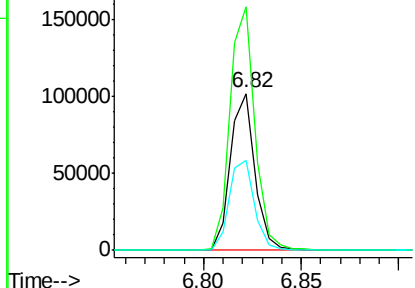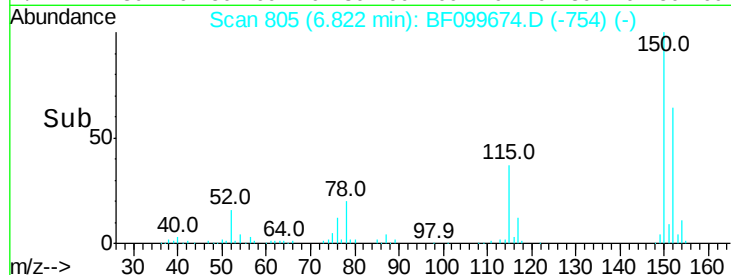



#5

2-Fluorophenol
 Concen: 49.955 ng
 RT: 5.45 min Scan# 571
 Delta R.T. 0.01 min
 Lab File: BF099674.D
 Acq: 19 Oct 2017 23:15

Tgt Ion:112 Resp: 278995
 Ion Ratio Lower Upper
 112 100
 64 54.4 47.9 71.9
 63 26.1 23.7 35.5

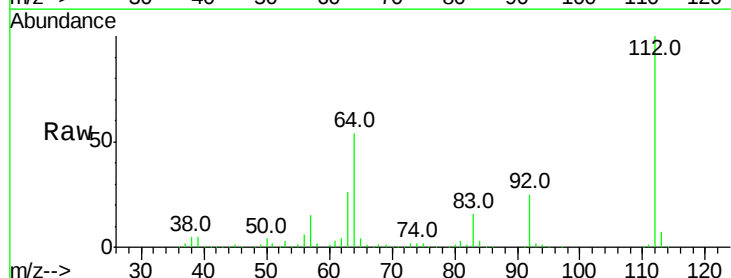

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

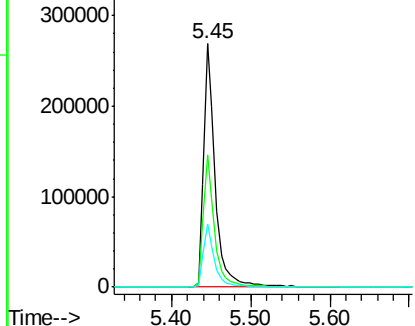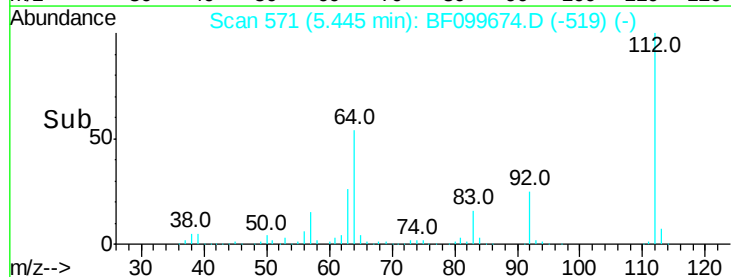



#7

Phenol-d6

Concen: 30.867 ng

RT: 6.46 min Scan# 743

Delta R.T. -0.01 min

Lab File: BF099674.D

Acq: 19 Oct 2017 23:15

Instrument :

BNA_F

ClientSampleId :

101217-TIFR-E-D-M


Tot Ion: 99 Resp: 212665

Ion Ratio Lower Upper

99 100

42 14.5 14.5 21.7




71 29.1 25.4 38.0

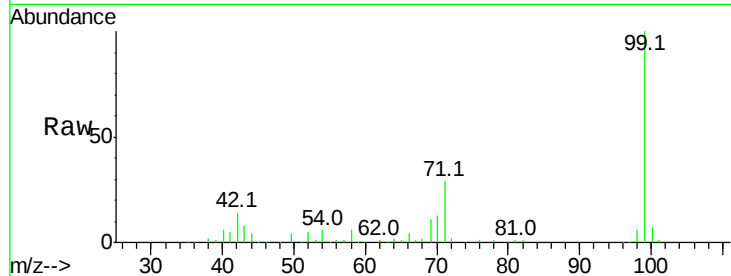

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

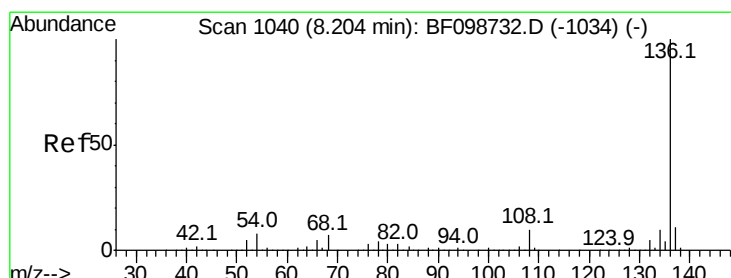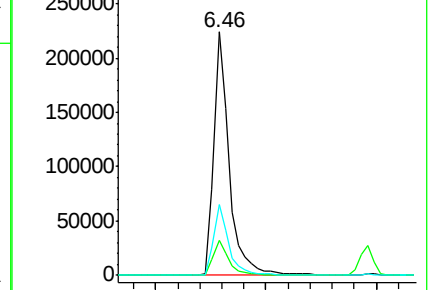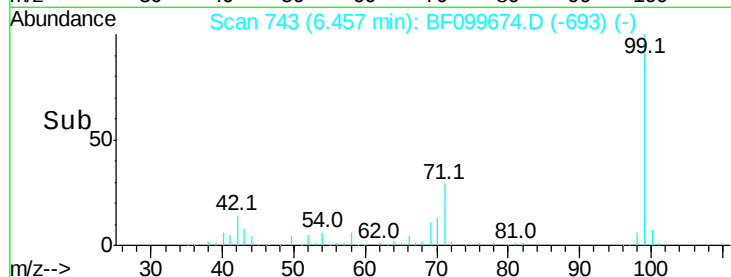

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.10 min Scan# 1022

Delta R.T. -0.01 min

Lab File: BF099674.D

Acq: 19 Oct 2017 23:15

Tgt Ion: 136 Resp: 354973


Ion Ratio Lower Upper

136 100

137 11.1 8.9 13.3

54 7.0 6.6 9.8

68 5.7 5.0 7.4


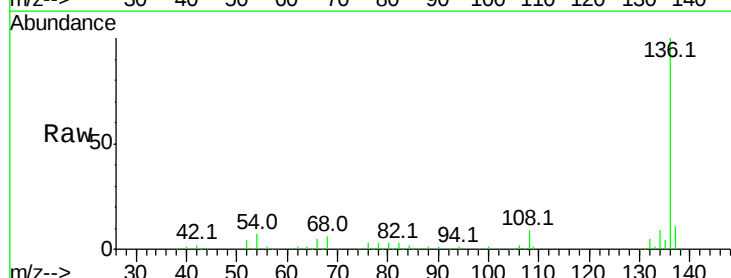


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



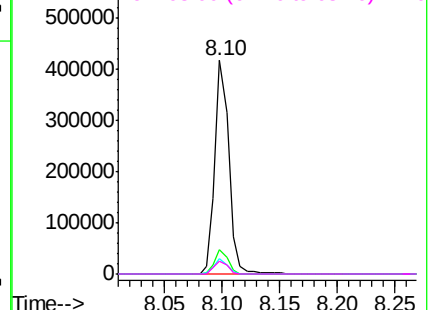
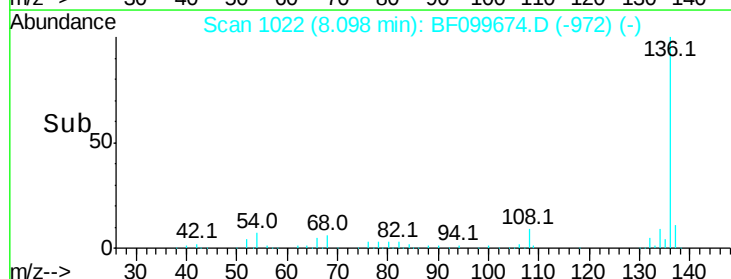




#23
Nitrobenzene-d5
Concen: 99.613 ng
RT: 7.39 min Scan# 901
Delta R.T. -0.01 min
Lab File: BF099674.D
Acq: 19 Oct 2017 23:15




Instrument :
BNA_F
ClientSampleId :
101217-TIFR-E-D-M

Tot Ion: 82 Resp: 551375
Ion Ratio Lower Upper
82 100
128 48.6 36.1 54.1
54 44.6 41.4 62.2

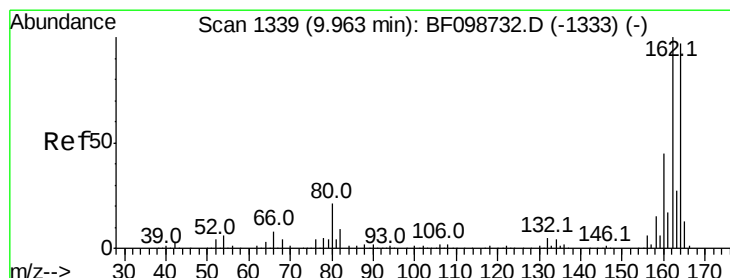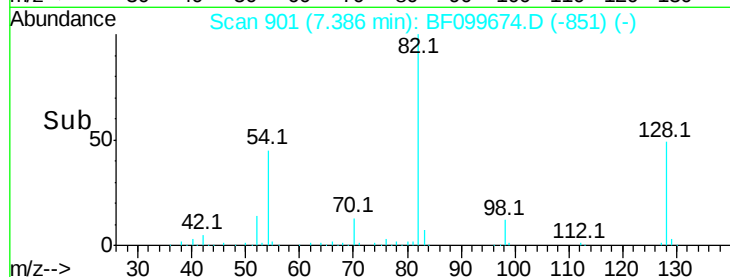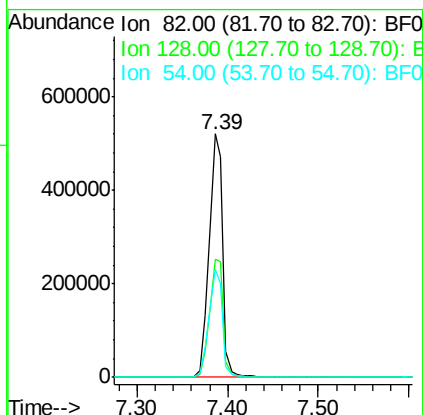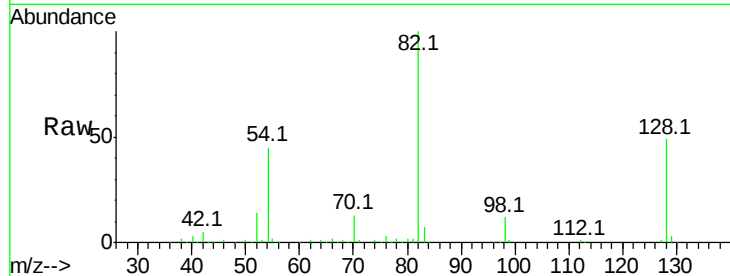

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.85 min Scan# 1320
Delta R.T. -0.01 min
Lab File: BF099674.D
Acq: 19 Oct 2017 23:15

Tgt Ion:164 Resp: 150338
Ion Ratio Lower Upper
164 100
162 103.7 86.1 129.1
160 44.3 38.3 57.5

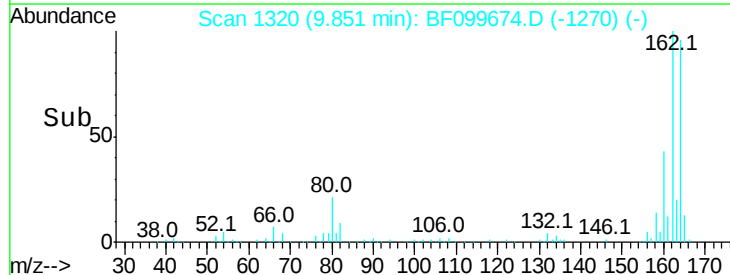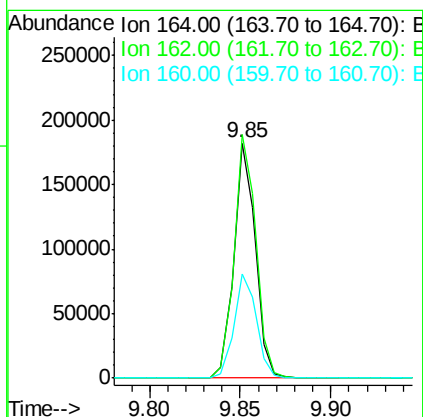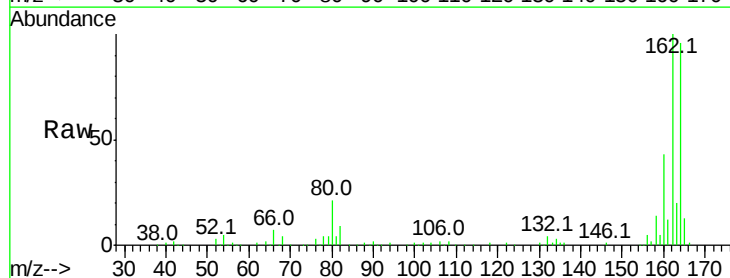






#41
 2,4,6-Tribromophenol
 Concen: 86.086 ng
 RT: 10.65 min Scan# 1455
 Delta R.T. -0.01 min
 Lab File: BF099674.D
 Acq: 19 Oct 2017 23:15

Instrument :
 BNA_F
 ClientSampleId :
 101217-TIFR-E-D-M

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.0	77.0	115.6
141	36.2	29.9	44.9

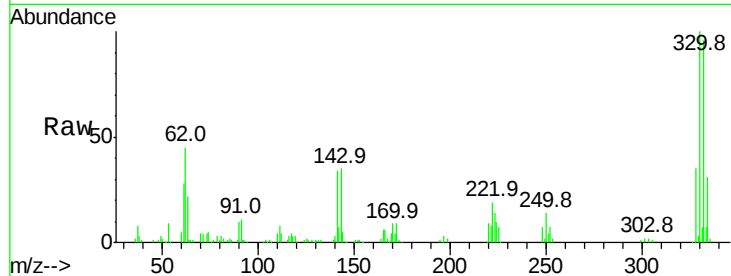


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

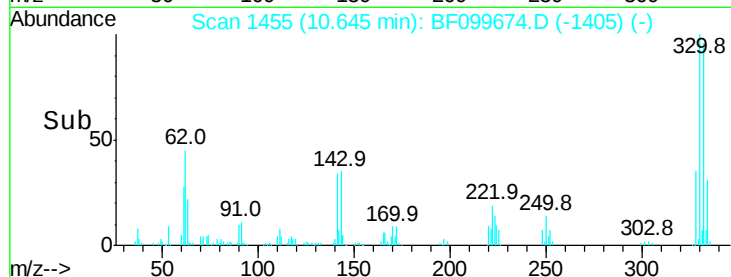
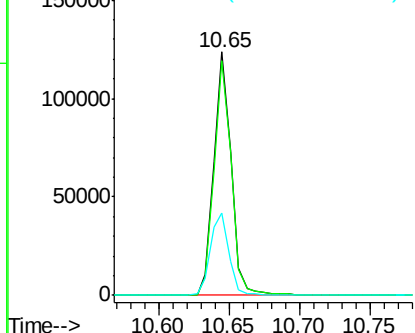



#44
 2-Fluorobiphenyl
 Concen: 110.782 ng
 RT: 9.17 min Scan# 1205
 Delta R.T. -0.00 min
 Lab File: BF099674.D
 Acq: 19 Oct 2017 23:15

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.5	29.7	44.5
170	23.9	19.6	29.4

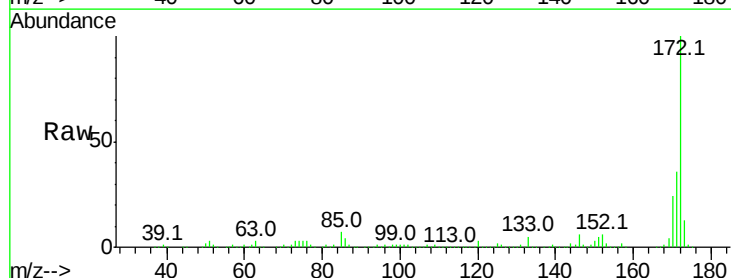

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



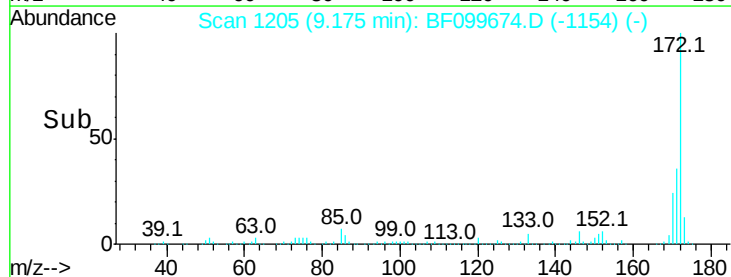
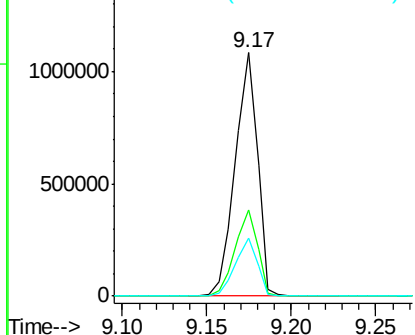


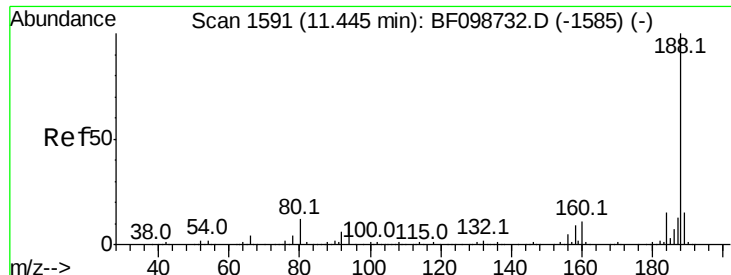

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.34 min Scan# 1573
Delta R.T. -0.01 min
Lab File: BF099674.D
Acq: 19 Oct 2017 23:15




Instrument :
BNA_F
ClientSampleId :
101217-TIFR-E-D-M

Tot Ion:188 Resp: 217080
Ion Ratio Lower Upper
188 100
94 10.9 8.5 12.7
80 12.0 9.2 13.8

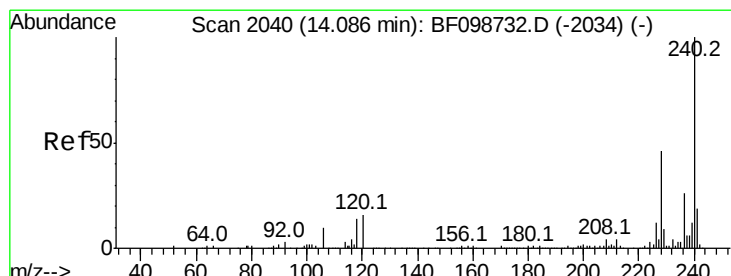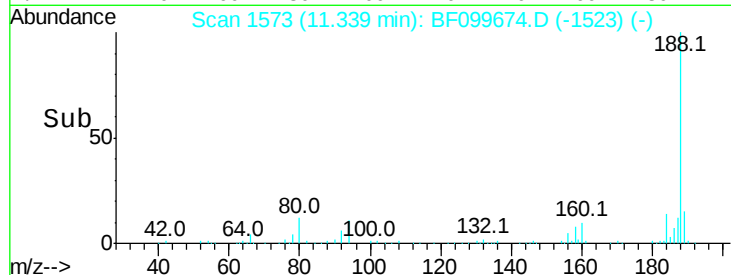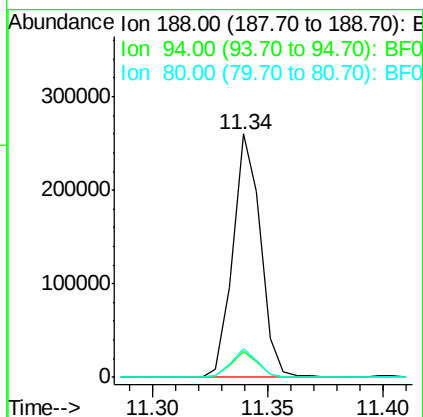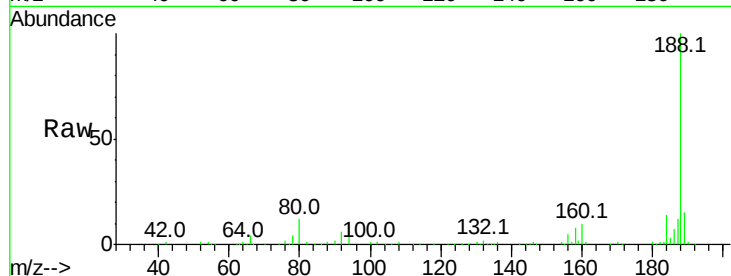

#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.99 min Scan# 2023
Delta R.T. -0.00 min
Lab File: BF099674.D
Acq: 19 Oct 2017 23:15

Tgt Ion:240 Resp: 149326
Ion Ratio Lower Upper
240 100
120 12.1 9.5 14.3
236 26.0 20.7 31.1

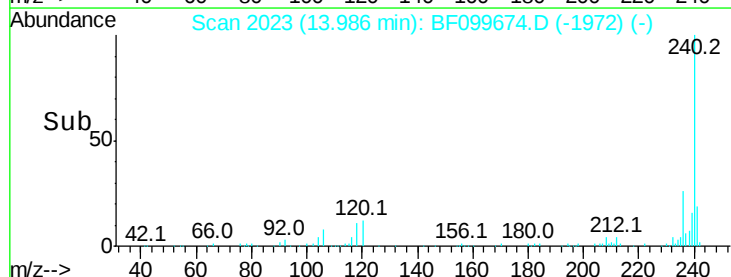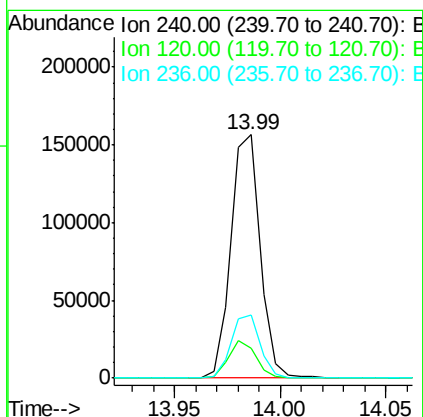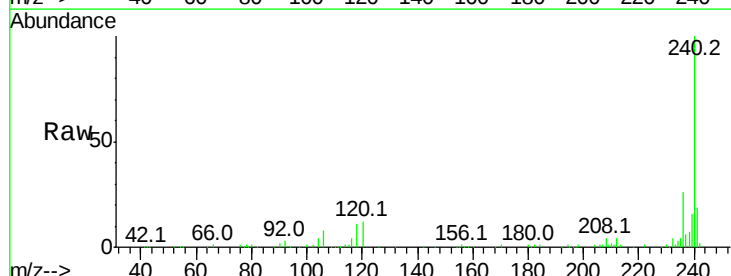



#78

Terphenyl-d14

Concen: 91.961 ng

RT: 12.92 min Scan# 1842

Delta R.T. -0.00 min

Lab File: BF099674.D

Acq: 19 Oct 2017 23:15

Instrument :

BNA_F

ClientSampleId :

101217-TIFR-E-D-M


Tot Ion:244 Resp: 603821

Ion Ratio Lower Upper

244 100

212 6.7 5.4 8.0




122 14.6 11.0 16.4

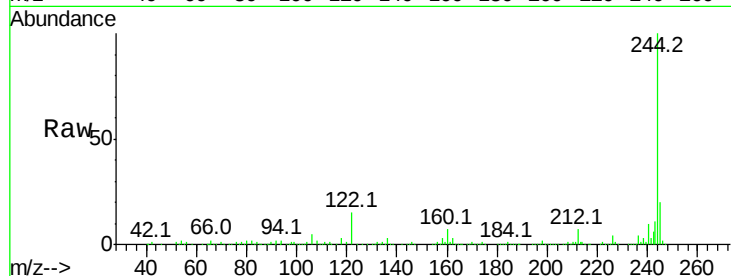

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

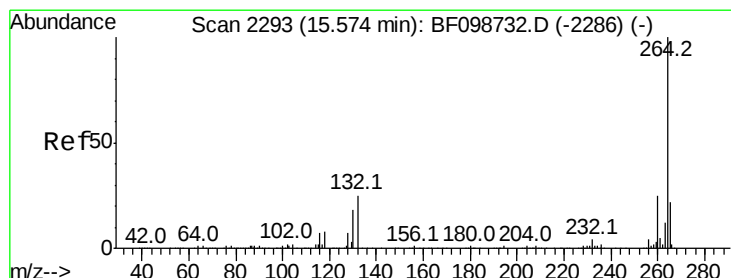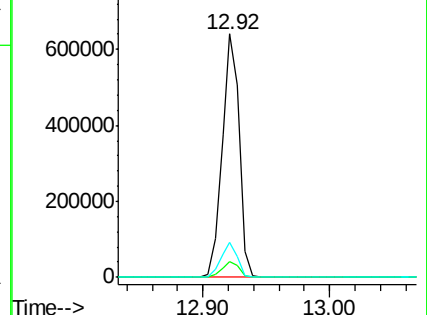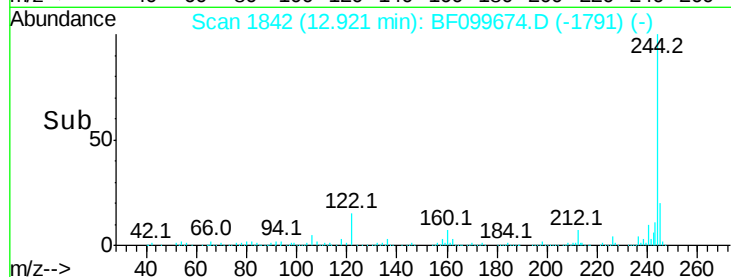

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.44 min Scan# 2271

Delta R.T. 0.01 min

Lab File: BF099674.D

Acq: 19 Oct 2017 23:15


Tgt Ion:264 Resp: 170739

Ion Ratio Lower Upper

264 100

260 23.5 19.2 28.8

265 21.1 17.5 26.3

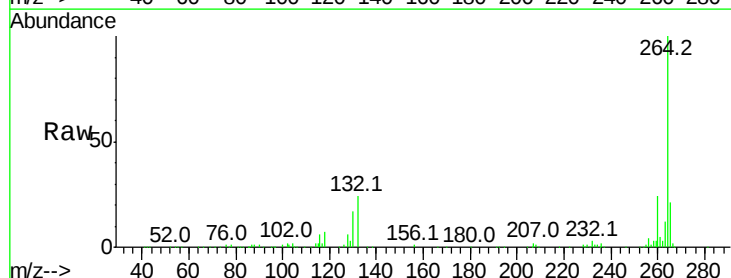

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

