

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101917\
 Data File : BF099681.D
 Acq On : 20 Oct 2017 2:29
 Operator : SJ/JU
 Sample : I5968-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 101717-TIDO-F-U-B

Quant Time: Oct 20 13:50:30 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 20 13:11:43 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	90499	20.00	ng	0.00
21) Naphthalene-d8	8.10	136	372731	20.00	ng	0.00
38) Acenaphthene-d10	9.85	164	163401	20.00	ng	0.00
63) Phenanthrene-d10	11.34	188	244537	20.00	ng	0.00
75) Chrysene-d12	13.98	240	158860	20.00	ng	0.00
86) Perylene-d12	15.44	264	169143	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	284302	50.01	ng	0.00
7) Phenol-d6	6.46	99	214756	30.62	ng	0.00
23) Nitrobenzene-d5	7.39	82	568766	97.86	ng	0.00
41) 2,4,6-Tribromophenol	10.65	330	122763	91.82	ng	0.00
44) 2-Fluorobiphenyl	9.17	172	1057036	107.99	ng	0.00
78) Terphenyl-d14	12.92	244	694748	99.46	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.57	163	48682	3.947	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101917\
Data File : BF099681.D
Acq On : 20 Oct 2017 2:29
Operator : SJ/JU
Sample : I5968-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
101717-TIDO-F-U-B

Quant Time: Oct 20 13:50:30 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 20 13:11:43 2017
Response via : Initial Calibration

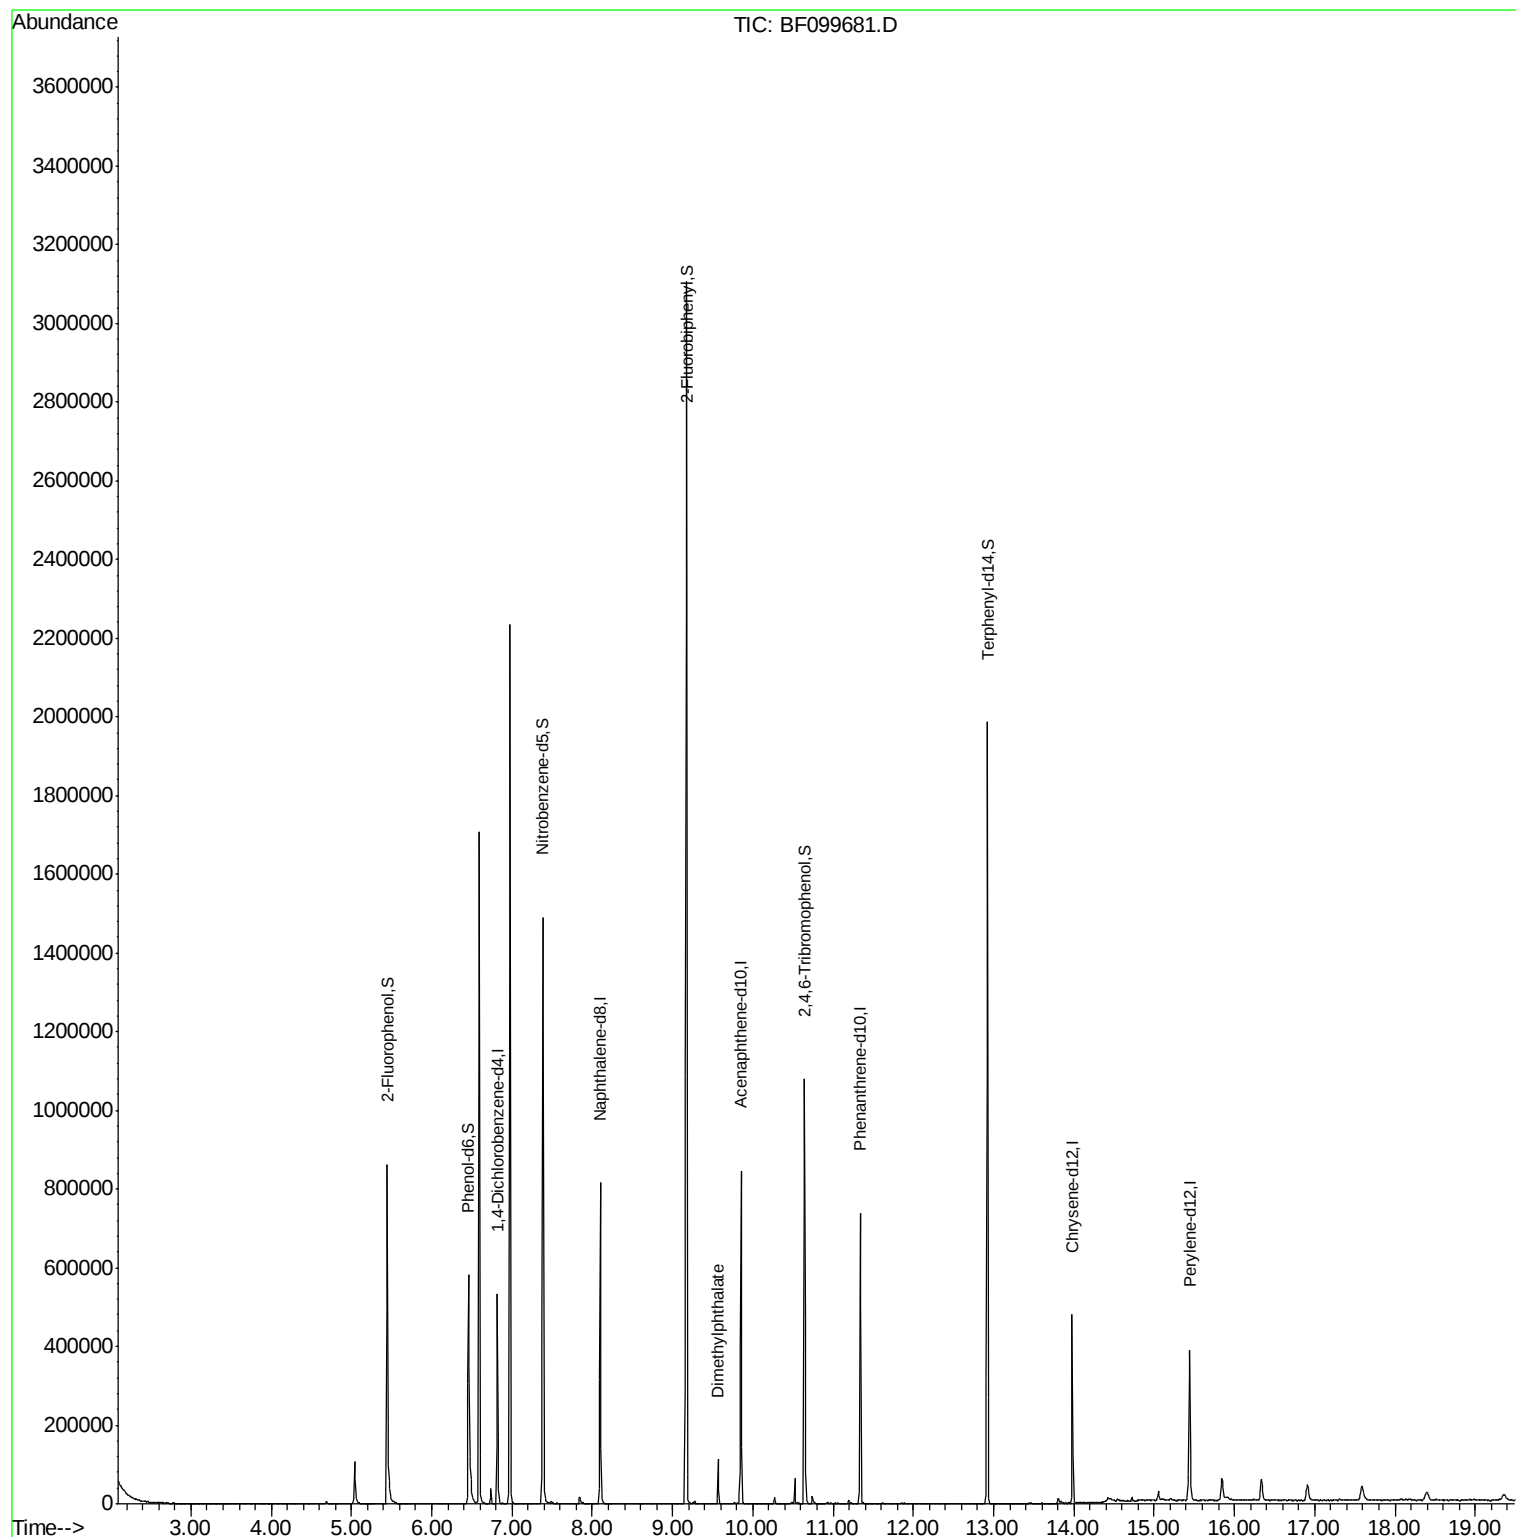




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.82 min Scan# 805
 Delta R.T. -0.00 min
 Lab File: BF099681.D
 Acq: 20 Oct 2017 2:29

Instrument :
 BNA_F
 ClientSampleId :
 101717-TIDO-F-U-B

Tot Ion:152 Resp: 90499
 Ion Ratio Lower Upper
 152 100
 150 152.7 124.6 186.8
 115 57.0 50.1 75.1

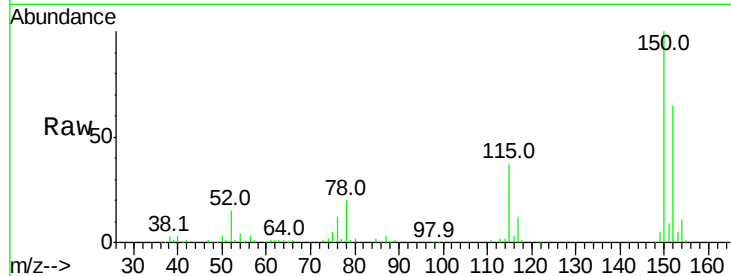


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

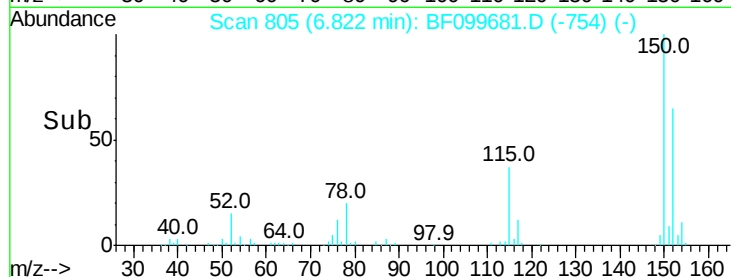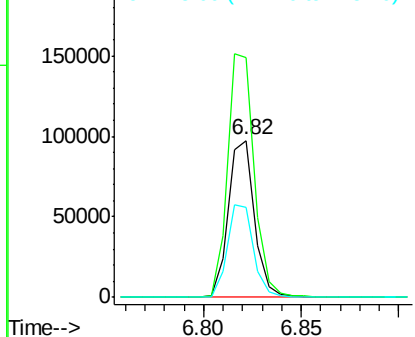



#5

2-Fluorophenol
 Concen: 50.009 ng
 RT: 5.45 min Scan# 571
 Delta R.T. 0.01 min
 Lab File: BF099681.D
 Acq: 20 Oct 2017 2:29

Tgt Ion:112 Resp: 284302
 Ion Ratio Lower Upper
 112 100
 64 52.3 47.9 71.9
 63 25.1 23.7 35.5

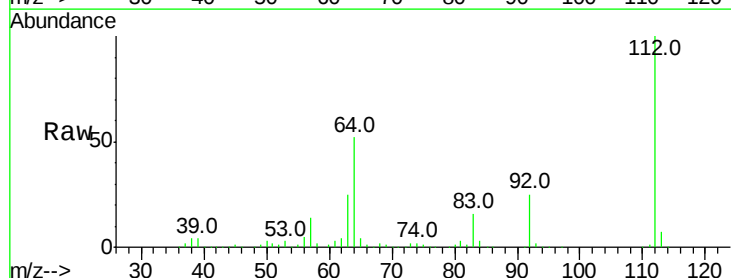

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

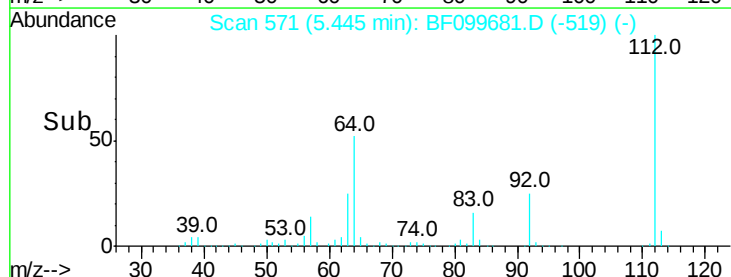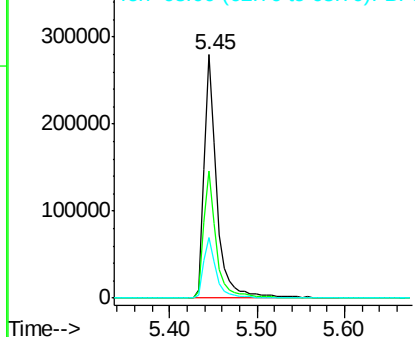



#7

Phenol-d6

Concen: 30.622 ng

RT: 6.46 min Scan# 743

Delta R.T. -0.01 min

Lab File: BF099681.D

Acq: 20 Oct 2017 2:29

Instrument :

BNA_F

ClientSampleId :

101717-TIDO-F-U-B


Tot Ion: 99 Resp: 214756

Ion Ratio Lower Upper

99 100

42 14.0 14.5 21.7#



71 29.5 25.4 38.0

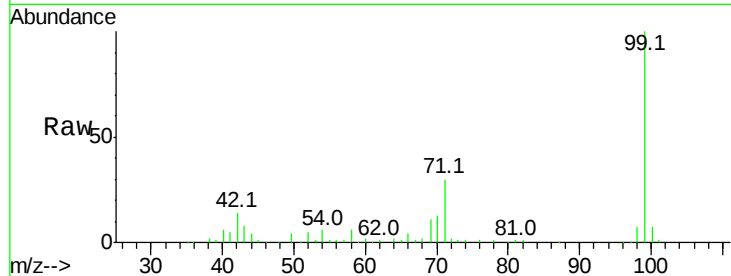

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

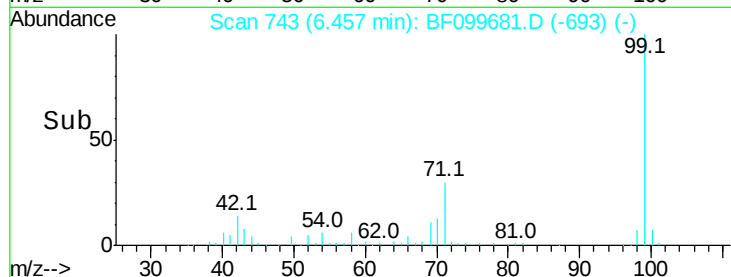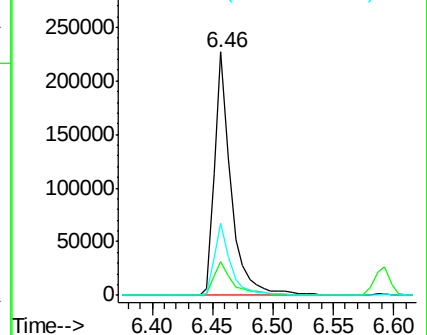

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.10 min Scan# 1022

Delta R.T. -0.01 min

Lab File: BF099681.D

Acq: 20 Oct 2017 2:29

Tgt Ion: 136 Resp: 372731


Ion Ratio Lower Upper

136 100

137 11.4 8.9 13.3

54 6.8 6.6 9.8

68 6.1 5.0 7.4


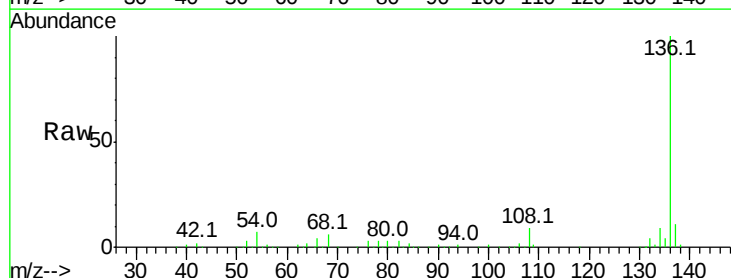


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



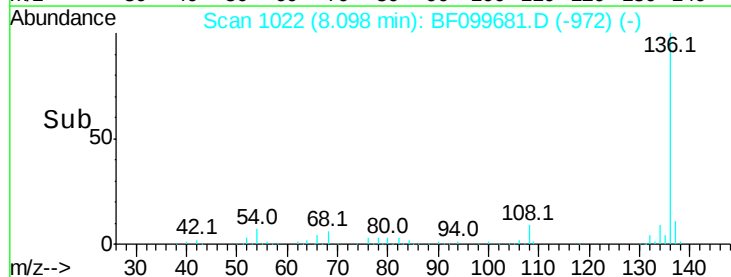
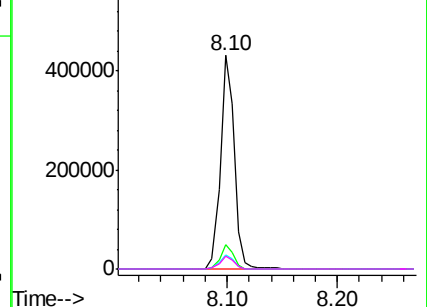




#23
Nitrobenzene-d5
Concen: 97.859 ng
RT: 7.39 min Scan# 901
Delta R.T. -0.01 min
Lab File: BF099681.D
Acq: 20 Oct 2017 2:29




Instrument :
BNA_F
ClientSampleId :
101717-TIDO-F-U-B

Tot Ion: 82 Resp: 568766
Ion Ratio Lower Upper
82 100
128 48.1 36.1 54.1
54 45.0 41.4 62.2

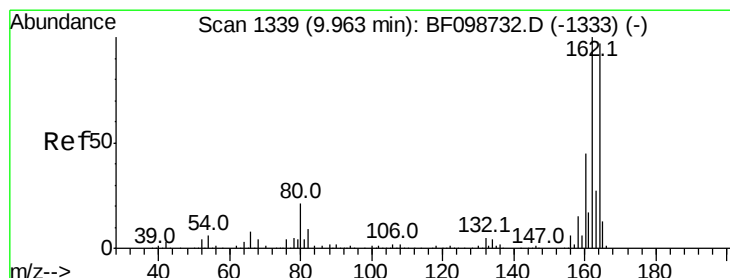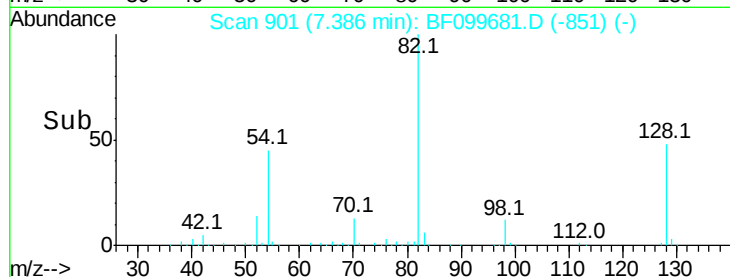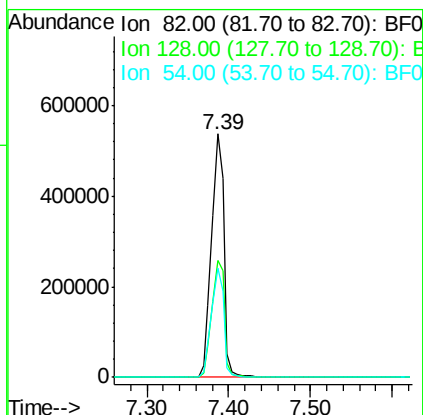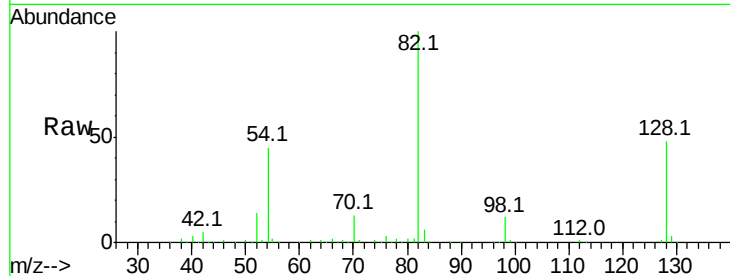

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.85 min Scan# 1320
Delta R.T. -0.01 min
Lab File: BF099681.D
Acq: 20 Oct 2017 2:29

Tgt Ion:164 Resp: 163401
Ion Ratio Lower Upper
164 100
162 102.1 86.1 129.1
160 45.2 38.3 57.5

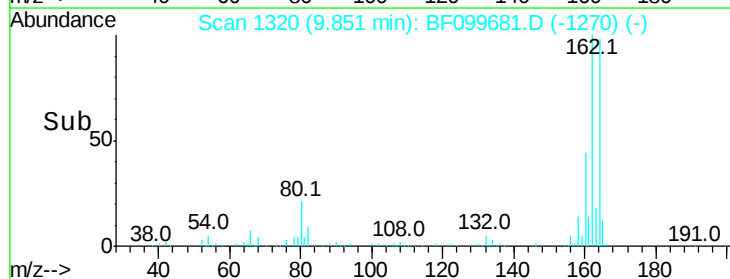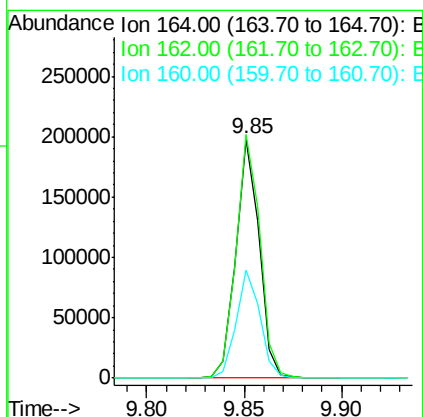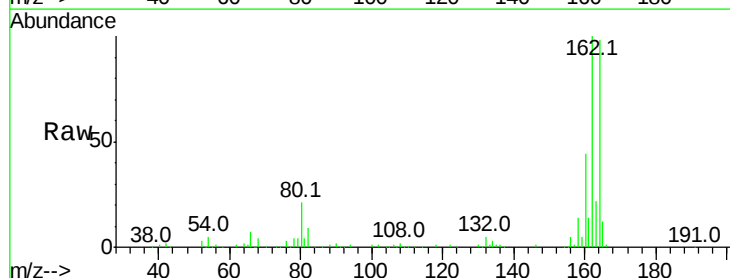







#41
 2,4,6-Tribromophenol
 Concen: 91.815 ng
 RT: 10.65 min Scan# 1455
 Delta R.T. -0.01 min
 Lab File: BF099681.D
 Acq: 20 Oct 2017 2:29

Instrument :
 BNA_F
 ClientSampleId :
 101717-TIDO-F-U-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.3	77.0	115.6
141	36.6	29.9	44.9

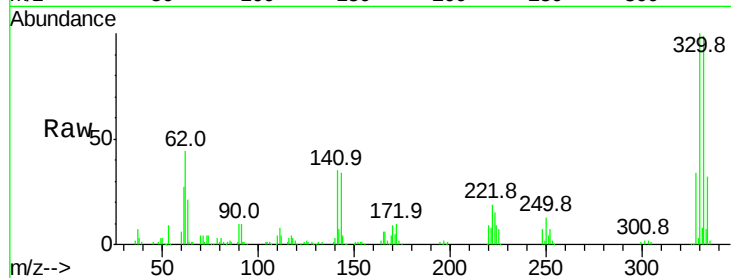


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

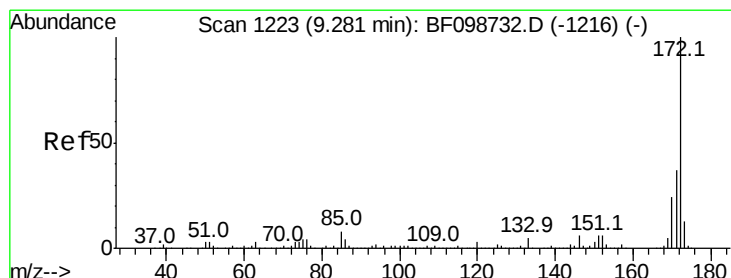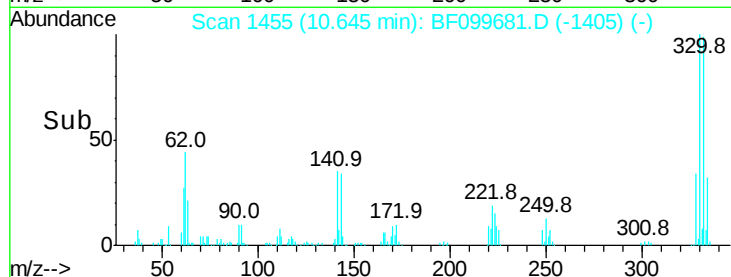
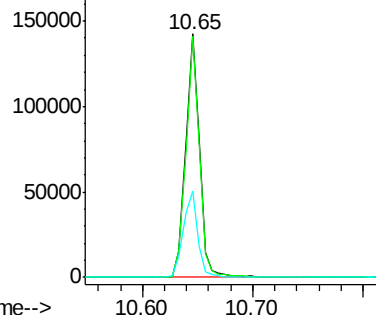



#44
 2-Fluorobiphenyl
 Concen: 107.994 ng
 RT: 9.17 min Scan# 1205
 Delta R.T. -0.00 min
 Lab File: BF099681.D
 Acq: 20 Oct 2017 2:29

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.0	29.7	44.5
170	24.2	19.6	29.4

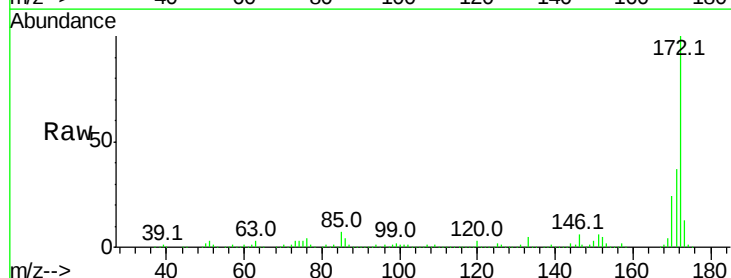

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

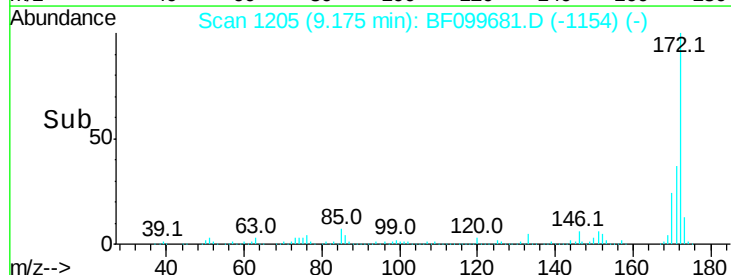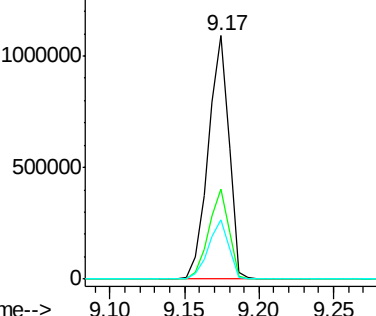

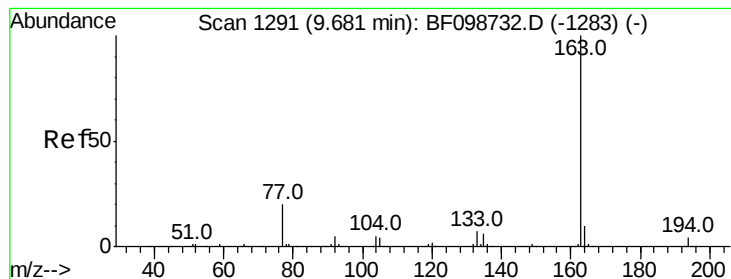

#49

Dimethylphthalate

Concen: 3.947 ng

RT: 9.57 min Scan# 1272

Delta R.T. -0.01 min

Lab File: BF099681.D

Acq: 20 Oct 2017 2:29

Instrument :

BNA_F

ClientSampleId :

101717-TIDO-F-U-B


Tot Ion:163 Resp: 48682

Ion Ratio Lower Upper

163 100

194 3.3 2.7 4.1




164 9.9 8.2 12.2

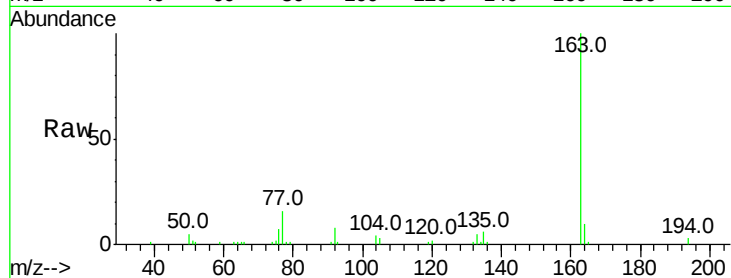

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

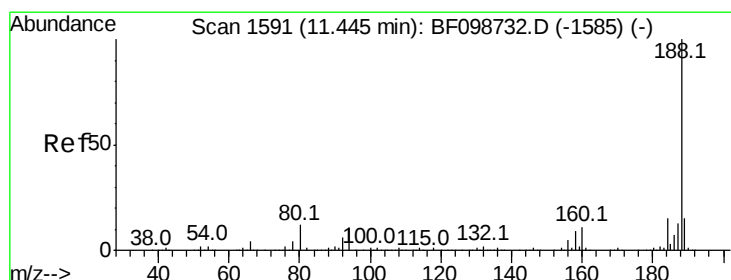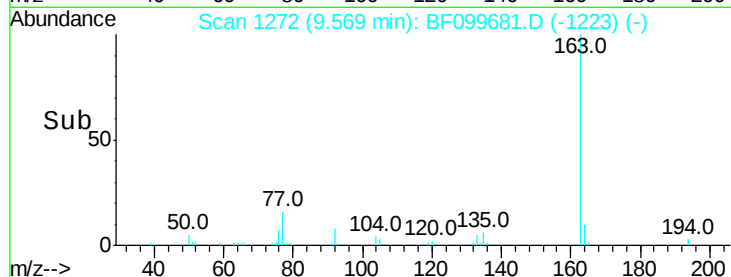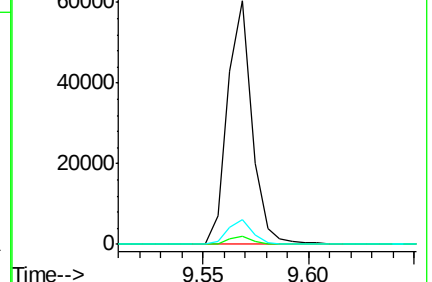

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.34 min Scan# 1573

Delta R.T. -0.01 min

Lab File: BF099681.D

Acq: 20 Oct 2017 2:29


Tgt Ion:188 Resp: 244537

Ion Ratio Lower Upper

188 100

94 10.9 8.5 12.7



80 12.0 9.2 13.8

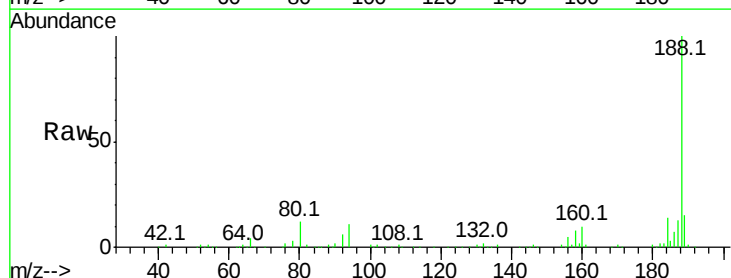


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

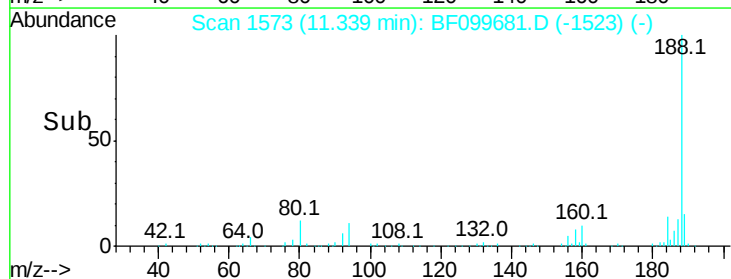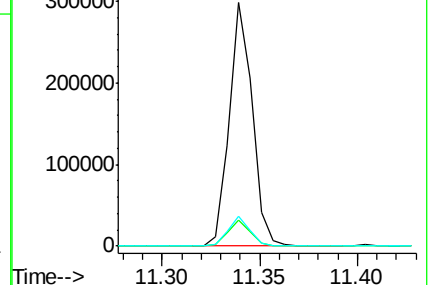

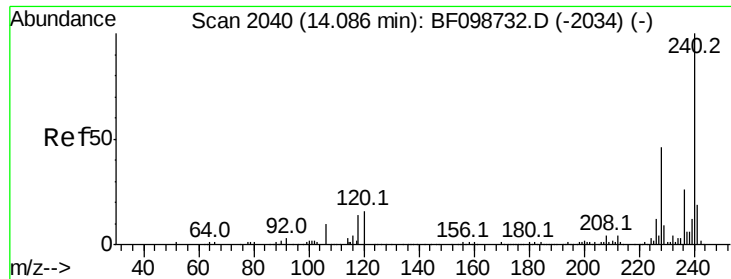

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.98 min Scan# 2022

Delta R.T. -0.01 min

Lab File: BF099681.D

Acq: 20 Oct 2017 2:29

Instrument :

BNA_F

ClientSampleId :

101717-TIDO-F-U-B


Tot Ion:240 Resp: 158860

Ion Ratio Lower Upper

240 100

120 15.7 9.5 14.3#



236 25.3 20.7 31.1

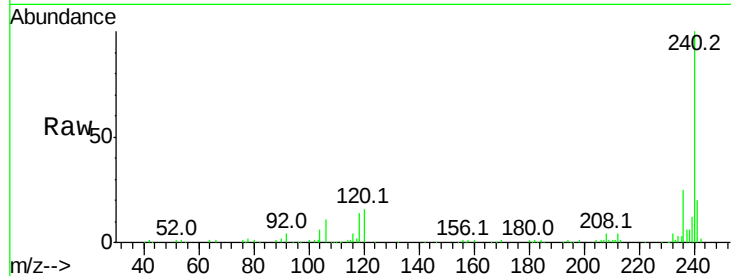

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

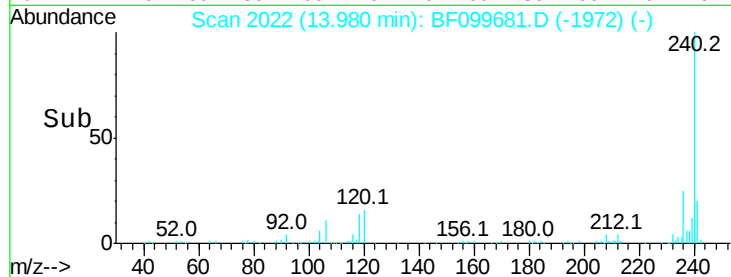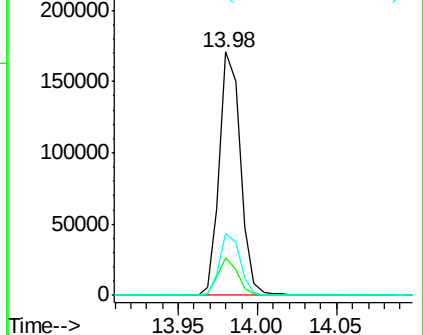

#78

Terphenyl-d14

Concen: 99.458 ng

RT: 12.92 min Scan# 1842

Delta R.T. -0.00 min

Lab File: BF099681.D

Acq: 20 Oct 2017 2:29


Tgt Ion:244 Resp: 694748

Ion Ratio Lower Upper

244 100

212 7.0 5.4 8.0



122 14.7 11.0 16.4

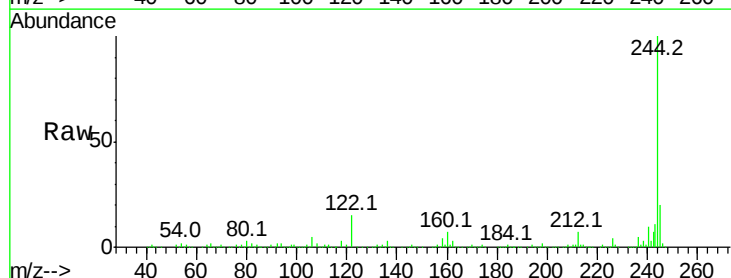

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

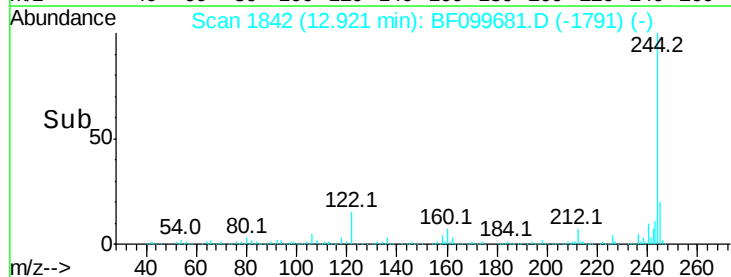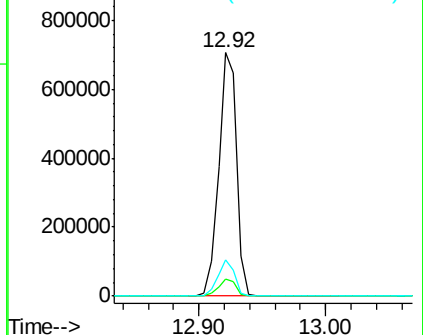




#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.44 min Scan# 2271
 Delta R.T. 0.01 min
 Lab File: BF099681.D
 Acq: 20 Oct 2017 2:29

Instrument :
 BNA_F
 ClientSampleId :
 101717-TIDO-F-U-B

Tot Ion:	264	Resp:	169143
Ion	Ratio	Lower	Upper
264	100		
260	22.8	19.2	28.8
265	21.3	17.5	26.3

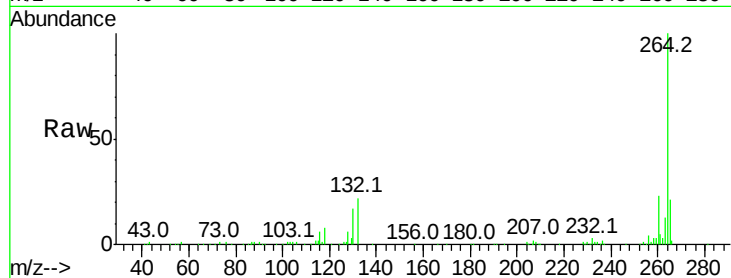

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

