

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101917\
 Data File : BF099662.D
 Acq On : 19 Oct 2017 17:39
 Operator : SJ/JU
 Sample : I5901-06
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S-6-20170693

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.046	499	503	513	rBV	222880	301325	16.00%	1.346%
2	5.451	568	572	590	rVB	1859357	1786311	94.85%	7.979%
3	6.463	740	744	762	rBV	1677355	1851691	98.32%	8.271%
4	6.592	762	766	770	rBV	2066120	1883275	100.00%	8.412%
5	6.816	801	804	808	rBV	568081	479030	25.44%	2.140%
6	6.975	827	831	834	rBV	1384276	1272718	67.58%	5.685%
7	7.387	896	901	904	rBV	1117032	1145324	60.82%	5.116%
8	8.098	1018	1022	1026	rBV	800731	672245	35.70%	3.003%
9	8.798	1138	1141	1150	rBV	26299	33104	1.76%	0.148%
10	9.169	1199	1204	1208	rBV	1786853	1627901	86.44%	7.271%
11	9.563	1268	1271	1275	rBV	82454	70459	3.74%	0.315%
12	9.851	1316	1320	1324	rVB	887951	773778	41.09%	3.456%
13	10.051	1350	1354	1360	rVB3	22329	24822	1.32%	0.111%
14	10.569	1431	1442	1450	rBV2	29158	76001	4.04%	0.339%
15	10.645	1450	1455	1458	rVV	1286982	1164010	61.81%	5.199%
16	10.692	1461	1463	1469	rVB6	19050	19682	1.05%	0.088%
17	10.998	1512	1515	1518	rBV4	26026	27650	1.47%	0.124%
18	11.339	1569	1573	1576	rBV	933812	763065	40.52%	3.408%
19	11.863	1659	1662	1666	rBV3	124580	136997	7.27%	0.612%
20	12.639	1791	1794	1798	rVB2	44658	48508	2.58%	0.217%
21	12.921	1837	1842	1845	rBV	1664195	1457092	77.37%	6.508%
22	12.963	1845	1849	1858	rVB7	13721	27984	1.49%	0.125%
23	13.133	1872	1878	1884	rVB3	61156	81575	4.33%	0.364%
24	13.257	1891	1899	1911	rBV2	131332	330138	17.53%	1.475%
25	13.386	1917	1921	1925	rBV3	23234	37133	1.97%	0.166%
26	13.492	1937	1939	1943	rVB	88552	80271	4.26%	0.359%
27	13.733	1975	1980	1988	rBV2	214202	262369	13.93%	1.172%
28	13.798	1988	1991	1995	rBV	165543	191731	10.18%	0.856%
29	13.874	2001	2004	2008	rVB4	39966	42064	2.23%	0.188%
30	13.980	2013	2022	2029	rVV	767538	861531	45.75%	3.848%
31	14.245	2064	2067	2072	rVB	85213	67759	3.60%	0.303%
32	14.339	2080	2083	2090	rVB5	82941	79574	4.23%	0.355%
33	14.427	2094	2098	2106	rBV3	75988	130709	6.94%	0.584%
34	14.533	2111	2116	2122	rBV	148626	239264	12.70%	1.069%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101917\
Data File : BF099662.D
Acq On : 19 Oct 2017 17:39
Operator : SJ/JU
Sample : I5901-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S-6-20170693

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	14.580	2122	2124	2131	rVB2	35318	47083	2.50%	0.210%
36	14.868	2169	2173	2176	rBV	172225	217322	11.54%	0.971%
37	15.051	2201	2204	2206	rBV2	62526	77998	4.14%	0.348%
38	15.080	2206	2209	2214	rVB	132037	195258	10.37%	0.872%
39	15.439	2263	2270	2280	rVB	370389	491430	26.09%	2.195%
40	15.621	2296	2301	2307	rVB	85288	111526	5.92%	0.498%
41	15.698	2309	2314	2321	rVV	73467	141041	7.49%	0.630%
42	15.839	2334	2338	2343	rVB2	55898	83795	4.45%	0.374%
43	15.898	2344	2348	2356	rVB3	40850	72050	3.83%	0.322%
44	16.127	2382	2387	2388	rBV5	18022	31458	1.67%	0.141%
45	16.333	2418	2422	2428	rVB2	53497	88655	4.71%	0.396%
46	16.415	2429	2436	2443	rVB2	45398	109737	5.83%	0.490%
47	16.621	2467	2471	2477	rVB5	34350	65406	3.47%	0.292%
48	16.704	2481	2485	2495	rVB8	42472	74679	3.97%	0.334%
49	16.904	2515	2519	2527	rVB	68284	139175	7.39%	0.622%
50	16.998	2528	2535	2547	rBV3	162883	405220	21.52%	1.810%
51	17.256	2573	2579	2588	rVB3	32486	90885	4.83%	0.406%
52	17.415	2600	2606	2609	rBV5	106659	232645	12.35%	1.039%
53	17.962	2692	2699	2713	rBV8	109741	323702	17.19%	1.446%
54	18.215	2733	2742	2744	rBV6	89215	215596	11.45%	0.963%
55	18.403	2768	2774	2788	rVB6	49266	195414	10.38%	0.873%
56	18.880	2846	2855	2863	rVB4	134143	351362	18.66%	1.569%
57	19.227	2902	2914	2926	rBV9	151529	579406	30.77%	2.588%


Sum of corrected areas: 22387933

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101917\
Data File : BF099662.D
Acq On : 19 Oct 2017 17:39
Operator : SJ/JU
Sample : I5901-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S-6-20170693

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

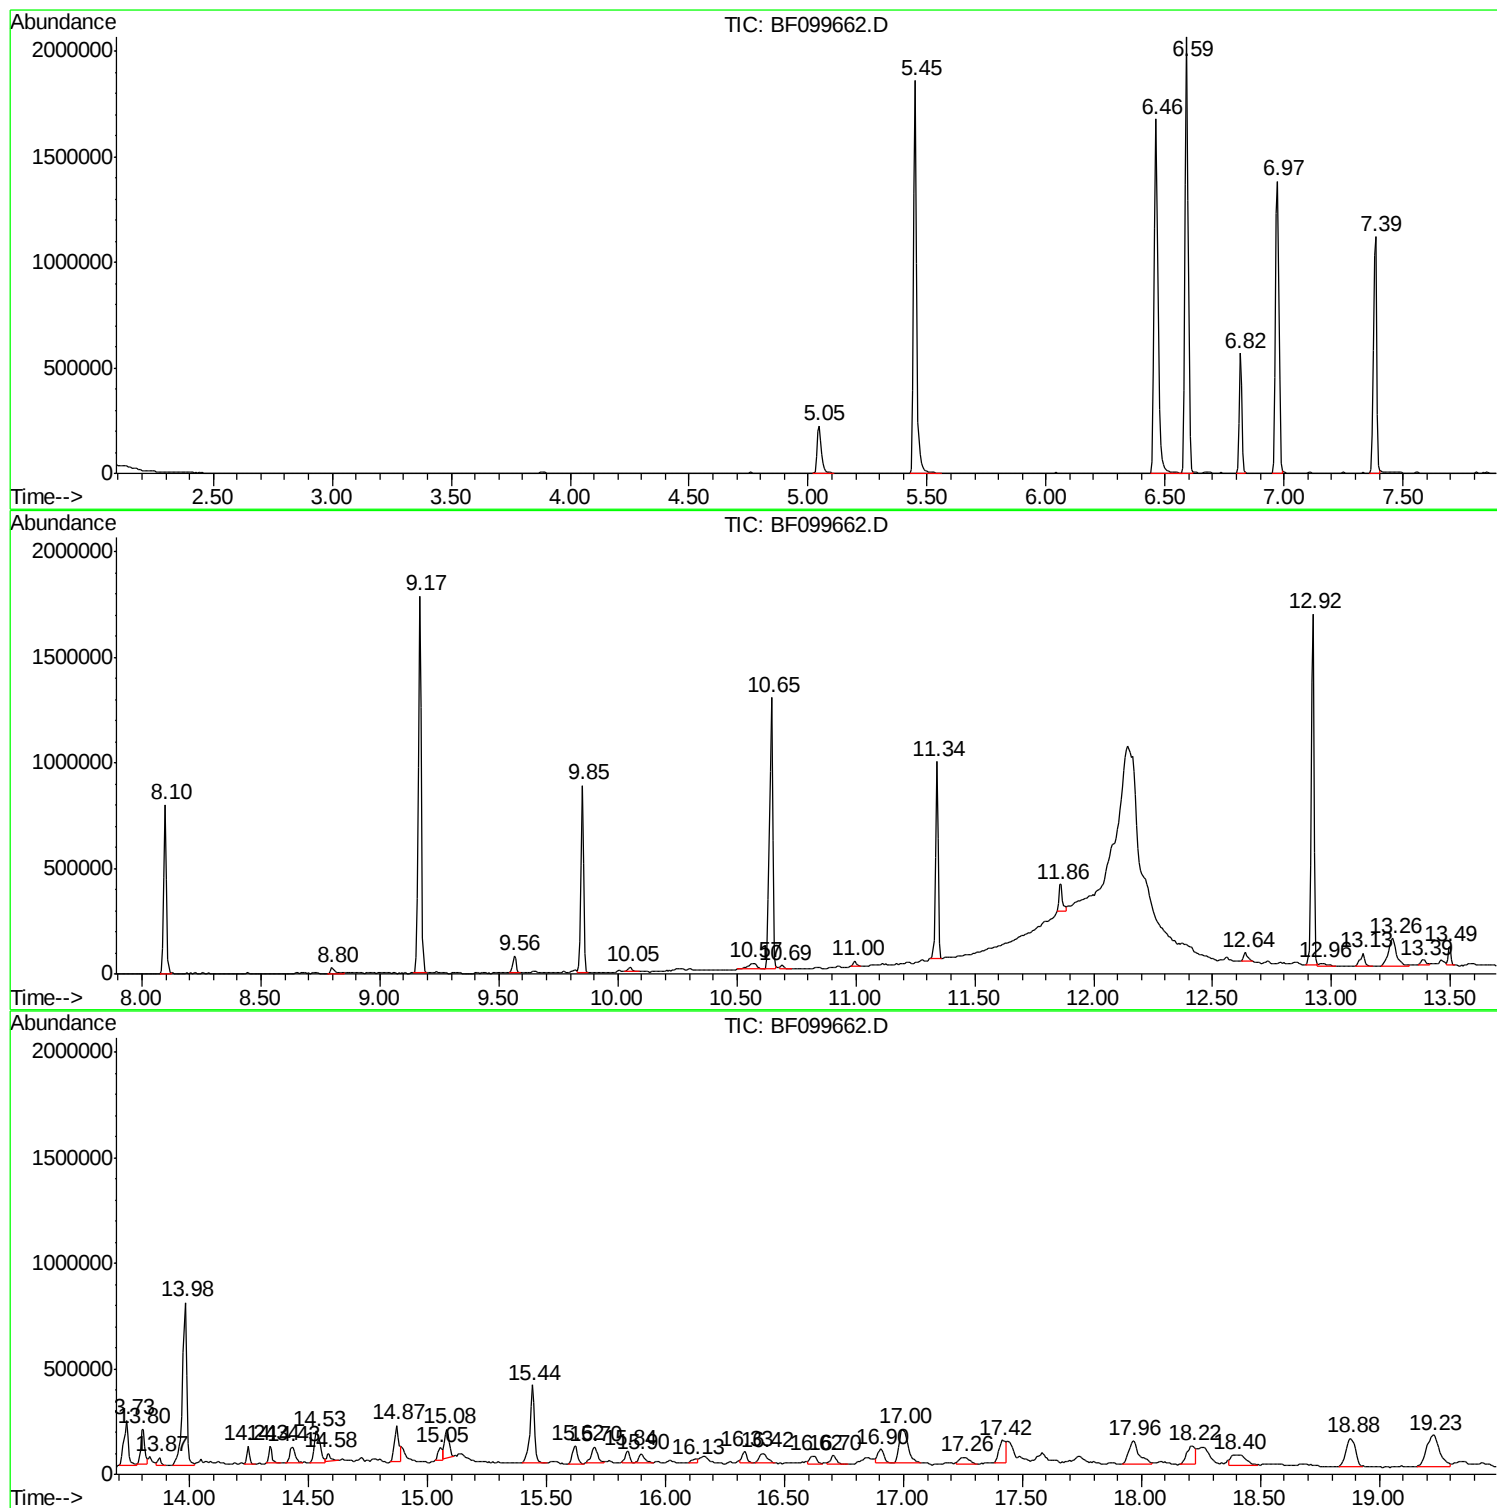

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF101917\
Data_File : BF099662.D
Acq_On : 19_Oct_2017. 17:399
Operator : SJ/JUU
Sample : I5901-066
Misc :
ALS_Vial : 3 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
S-6-20170693

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
