


Data Path : Z:\HPCHEM1\BNA F\Data\BF101917\
 Data File : BF099660.D
 Acq On : 19 Oct 2017 16:30
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 20 13:11:43 2017

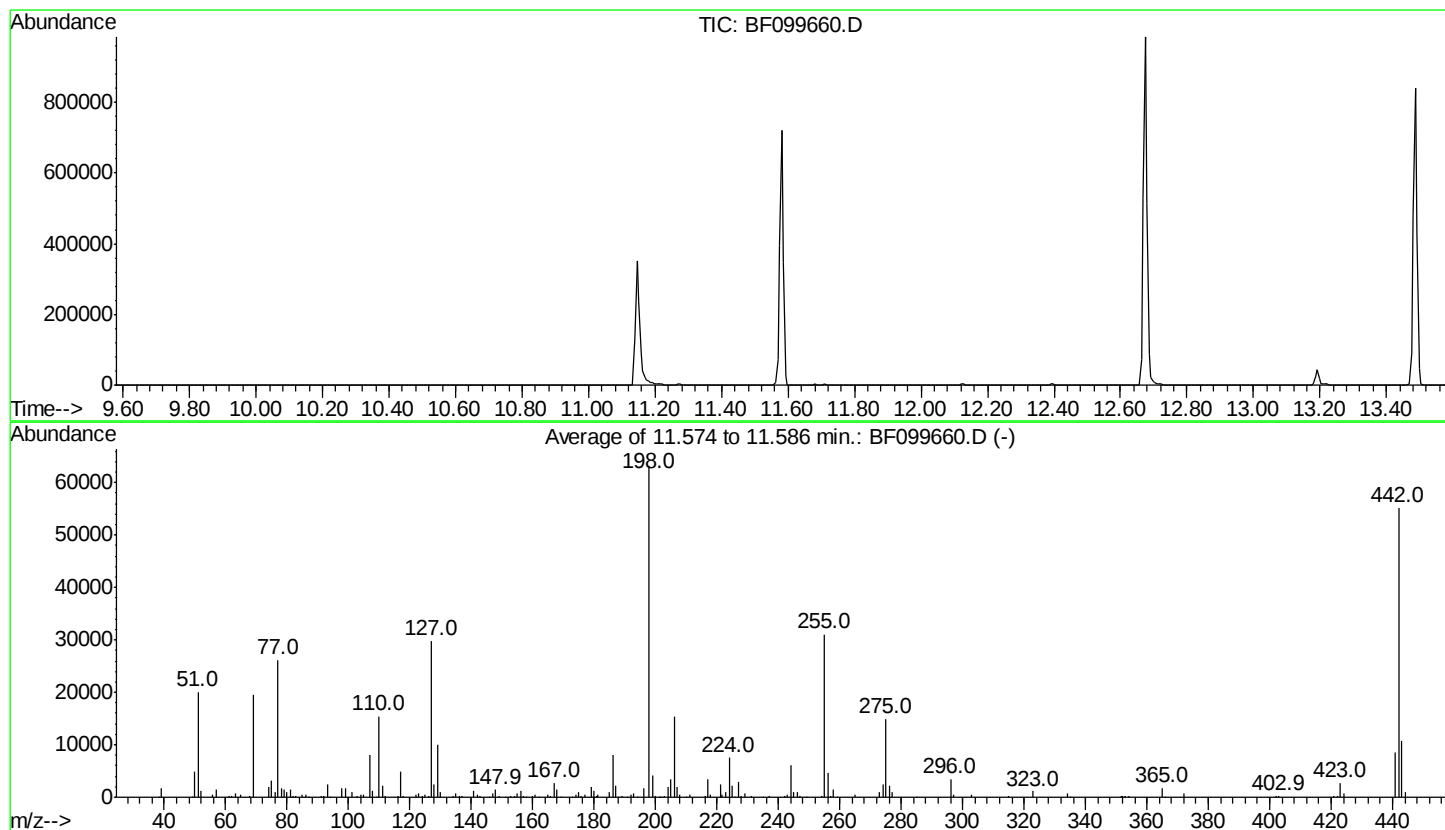

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	20145	PASS
68	69	0.00	2	1.4	274	PASS
69	198	0.00	100	30.8	19459	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.1	29792	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63240	PASS
199	198	5	9	6.5	4136	PASS
275	198	10	60	23.8	15022	PASS
365	198	1	100	2.8	1763	PASS
441	442	0.01	24	15.7	8674	PASS
442	198	50	100	87.4	55258	PASS
443	442	15	24	19.4	10716	PASS