


Data Path : Z:\HPCHEM1\BNA_F\Data\BF101917\
 Data File : BF099685.D
 Acq On : 20 Oct 2017 5:15
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 20 13:11:43 2017

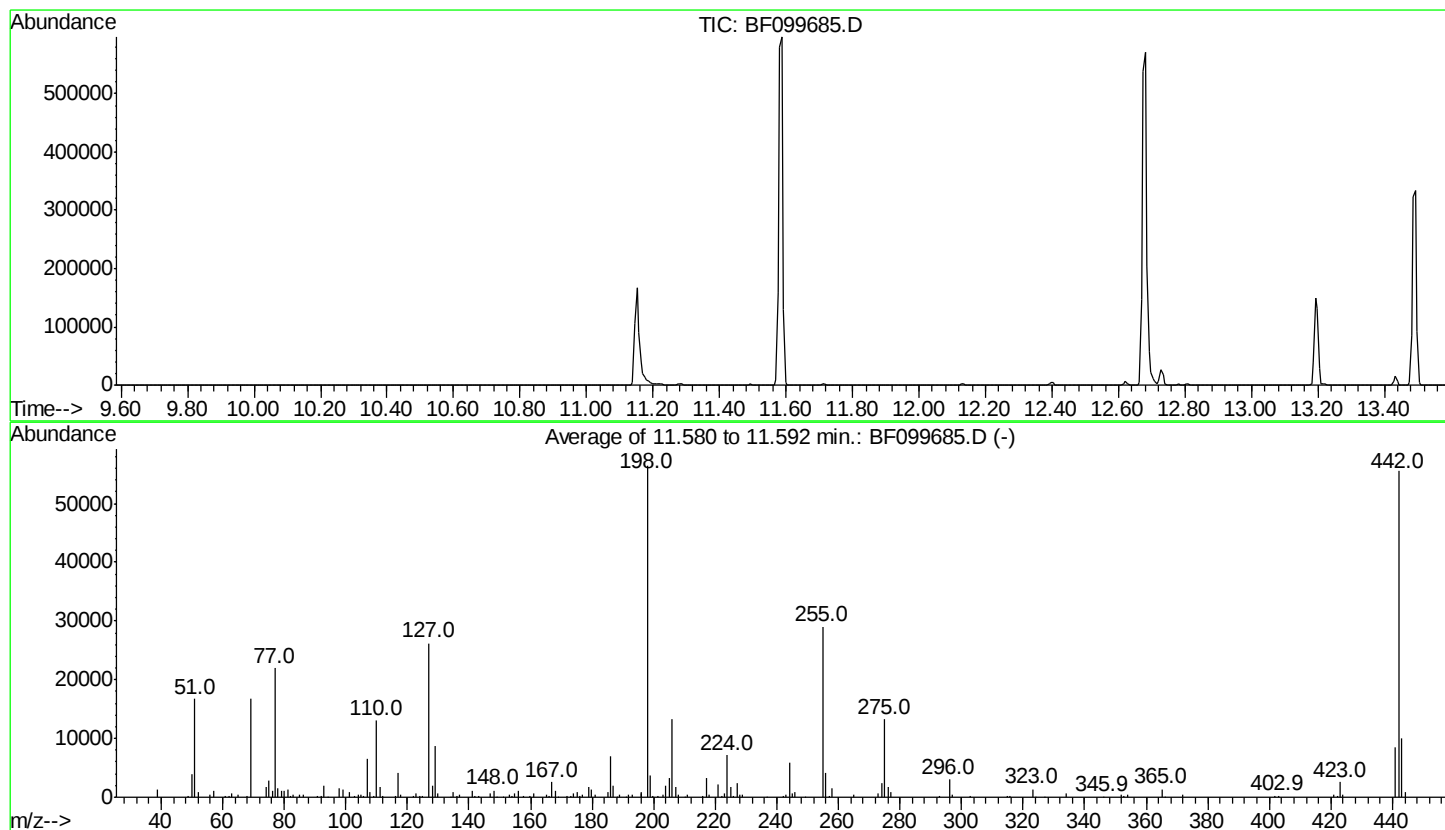

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.6	16703	PASS
68	69	0.00	2	0.9	157	PASS
69	198	0.00	100	29.9	16850	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.4	26194	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56440	PASS
199	198	5	9	6.5	3681	PASS
275	198	10	60	23.5	13251	PASS
365	198	1	100	2.5	1413	PASS
441	442	0.01	24	15.2	8431	PASS
442	198	50	100	98.4	55557	PASS
443	442	15	24	17.9	9966	PASS