

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101921\
 Data File : BF125897.D
 Acq On : 19 Oct 2021 13:39
 Operator : JU/CG
 Sample : M4248-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CHVB-0513

Quant Time: Oct 19 16:45:26 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 18 12:43:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.822	152	153512	20.000	ng	0.00
21) Naphthalene-d8	8.104	136	631966	20.000	ng	# 0.00
39) Acenaphthene-d10	9.857	164	315757	20.000	ng	0.00
64) Phenanthrene-d10	11.339	188	535389	20.000	ng	# 0.00
76) Chrysene-d12	13.974	240	389525	20.000	ng	0.00
86) Perylene-d12	15.421	264	332816	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.439	112	929834	98.950	ng	0.00
7) Phenol-d6	6.451	99	1103243	91.199	ng	0.00
23) Nitrobenzene-d5	7.381	82	640898	63.039	ng	-0.01
42) 2,4,6-Tribromophenol	10.645	330	255324	81.900	ng	0.00
45) 2-Fluorobiphenyl	9.180	172	1194307	65.239	ng	0.00
79) Terphenyl-d14	12.927	244	1173422	45.887	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propyla...	7.381	70	78896	12.355	ng	# 51
25) Isophorone	7.381	82	638348	35.441	ng	# 59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101921\
Data File : BF125897.D
Acq On : 19 Oct 2021 13:39
Operator : JU/CG
Sample : M4248-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CHVB-0513

Quant Time: Oct 19 16:45:26 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 18 12:43:03 2021
Response via : Initial Calibration




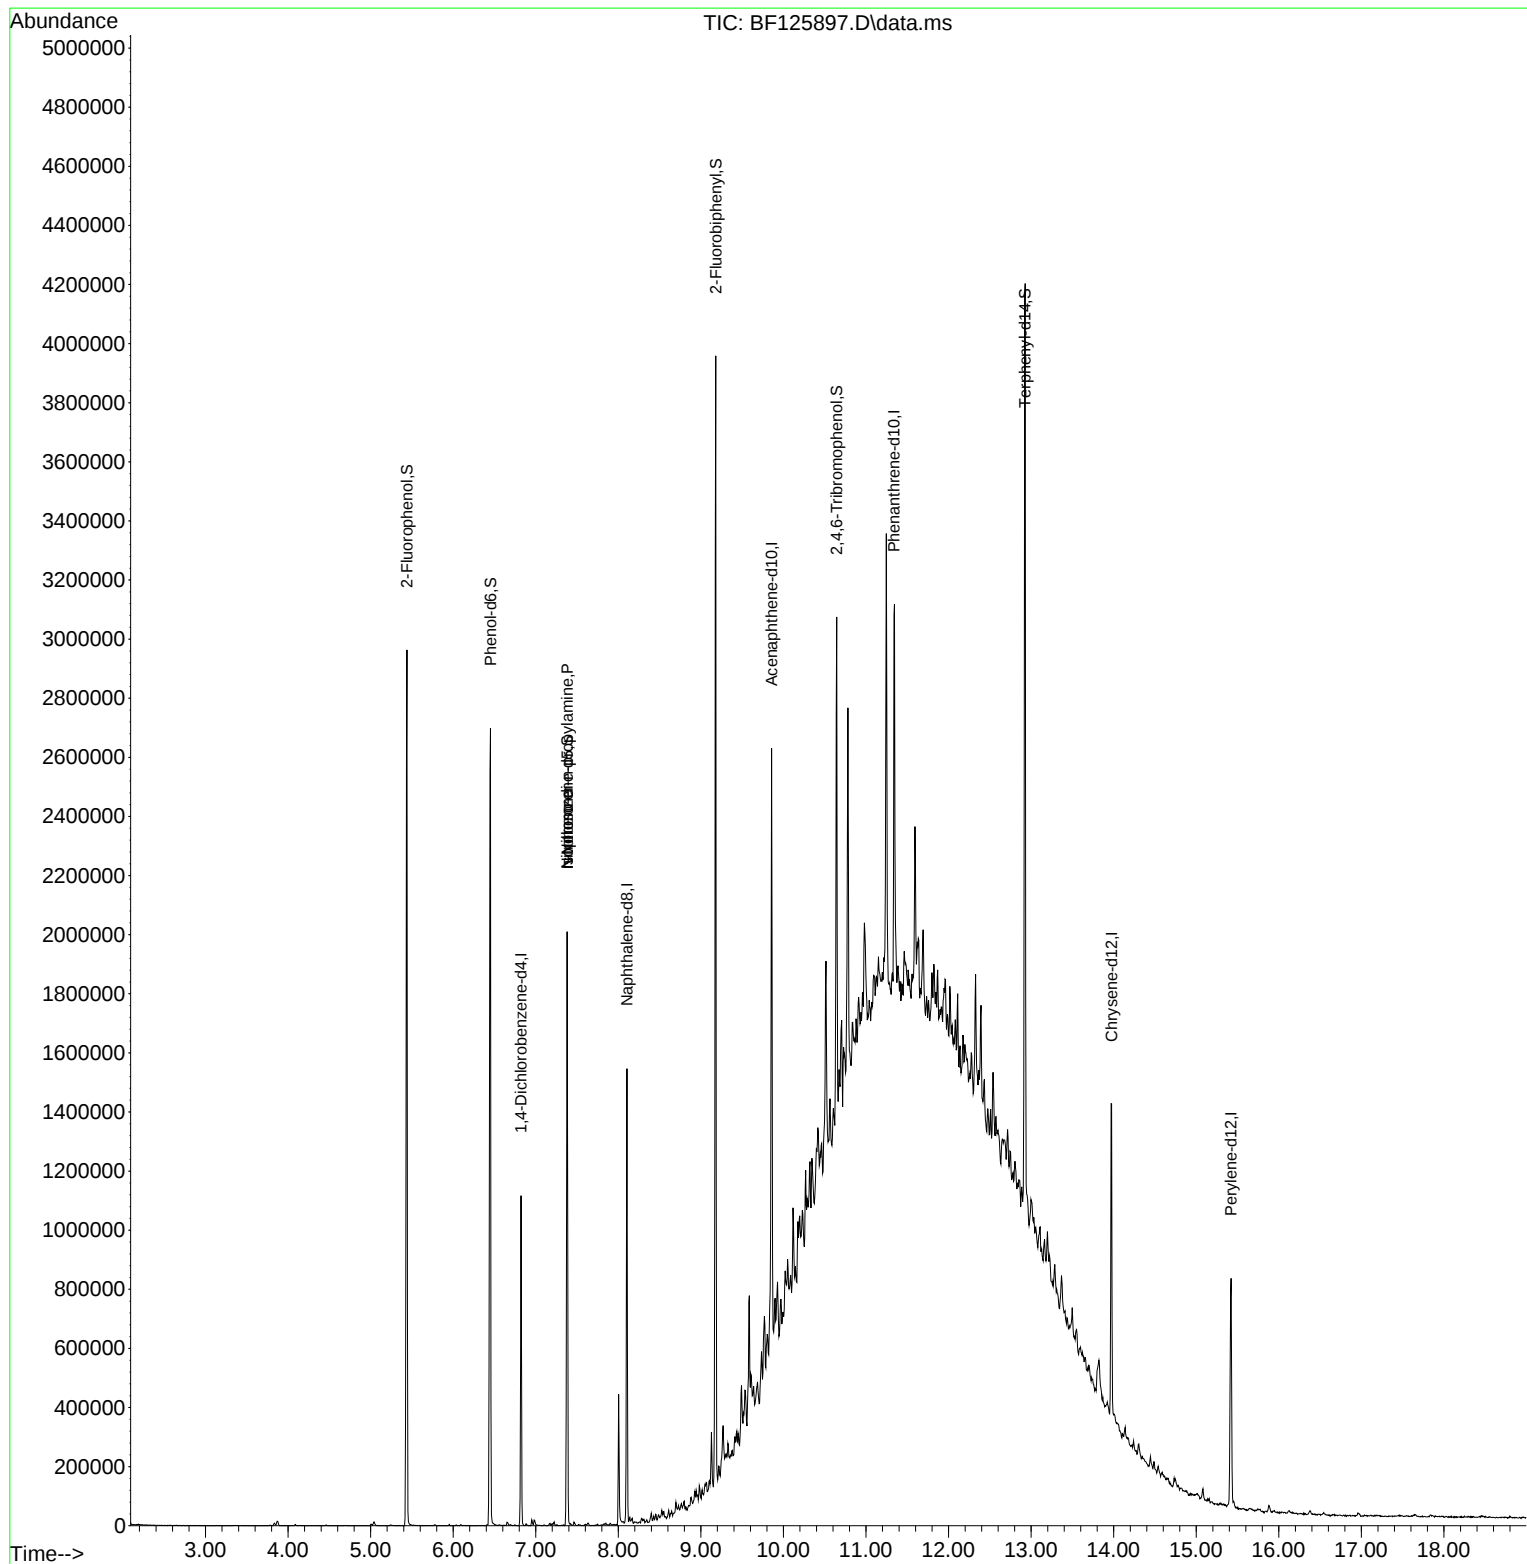


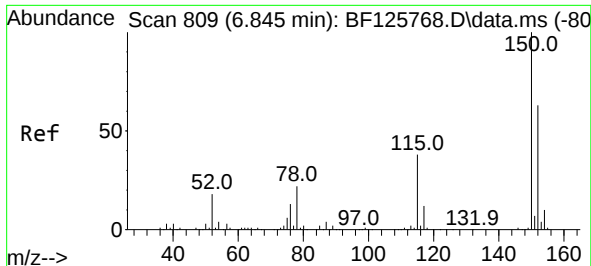

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.822 min Scan# 805
Delta R.T. -0.006 min
Lab File: BF125897.D
Acq: 19 Oct 2021 13:39




Instrument :
BNA_F
ClientSampleId :
CHVB-0513


Tgt Ion:152 Resp: 153512
Ion Ratio Lower Upper
152 100
150 157.5 117.6 176.4
115 60.2 47.1 70.7

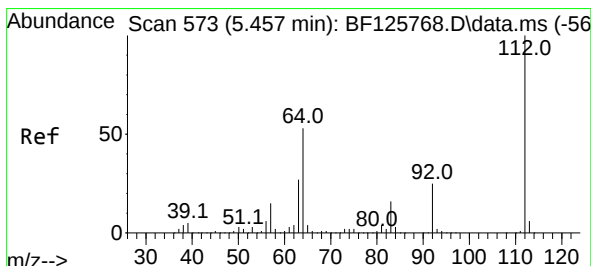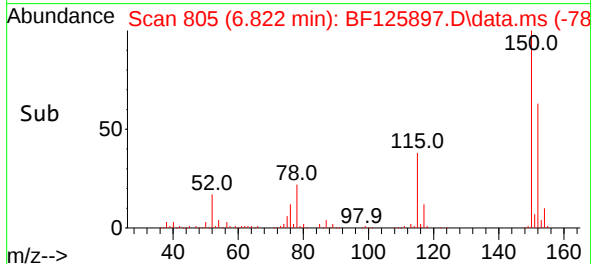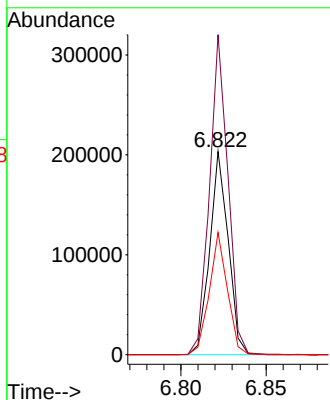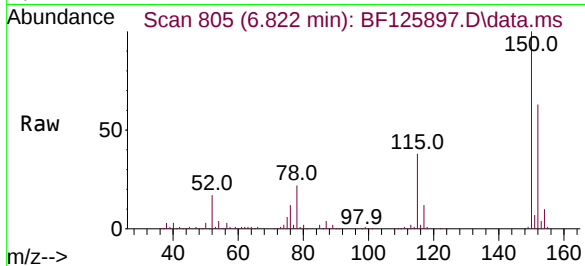

#5
2-Fluorophenol
Concen: 98.950 ng
RT: 5.439 min Scan# 570
Delta R.T. -0.000 min
Lab File: BF125897.D
Acq: 19 Oct 2021 13:39

Tgt Ion:112 Resp: 929834
Ion Ratio Lower Upper
112 100
64 50.4 44.2 66.2
63 24.4 26.2 39.2#


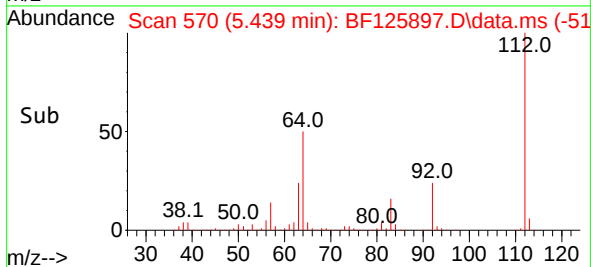
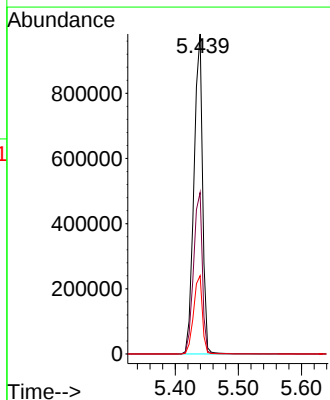
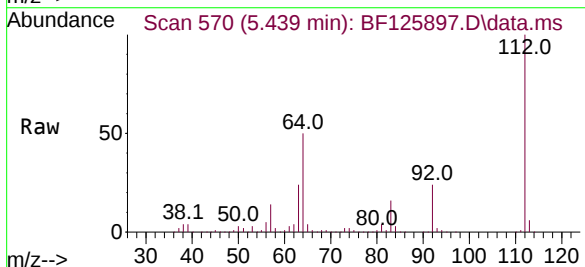


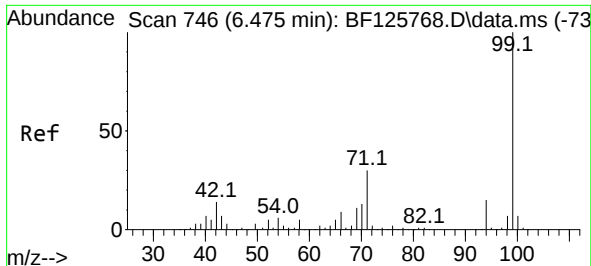

#7
Phenol-d6
Concen: 91.199 ng
RT: 6.451 min Scan# 742
Delta R.T. -0.006 min
Lab File: BF125897.D
Acq: 19 Oct 2021 13:39




Instrument :
BNA_F
ClientSampleId :
CHVB-0513


Tgt Ion: 99 Resp: 1103243
Ion Ratio Lower Upper
99 100
42 13.1 23.5 35.3#
71 28.6 25.6 38.4

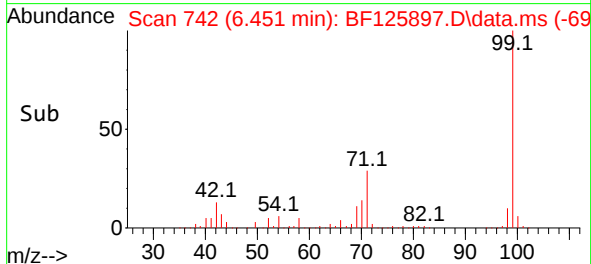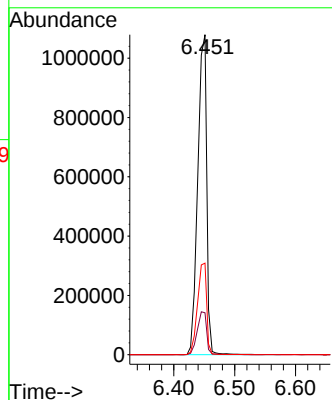

#19
n-Nitroso-di-n-propylamine
Concen: 12.355 ng
RT: 7.381 min Scan# 900
Delta R.T. 0.141 min
Lab File: BF125897.D
Acq: 19 Oct 2021 13:39

Tgt Ion: 70 Resp: 78896
Ion Ratio Lower Upper
70 100
42 41.2 72.2 108.2#
101 0.0 7.8 11.8#
130 2.6 21.8 32.6#


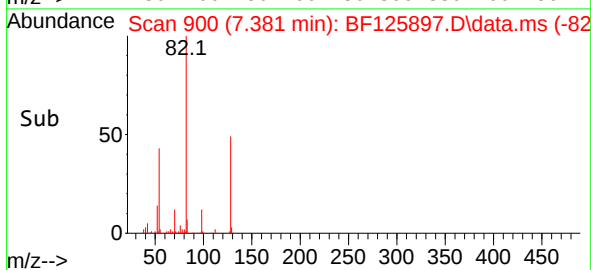
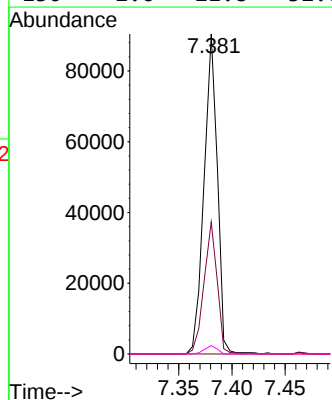
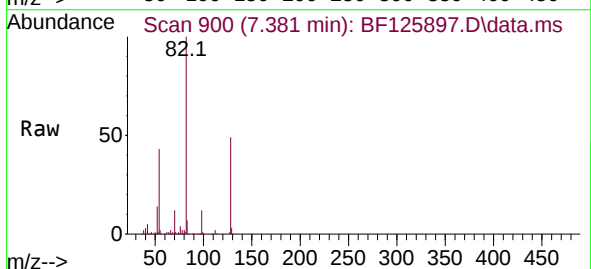


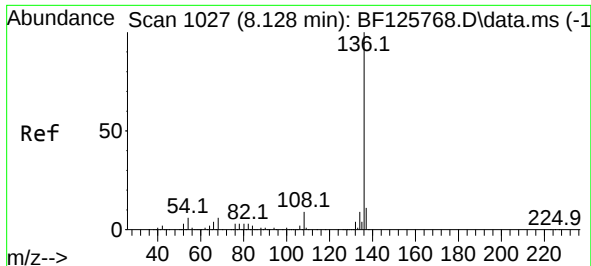

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.104 min Scan# 1023
Delta R.T. -0.006 min
Lab File: BF125897.D
Acq: 19 Oct 2021 13:39




Instrument :
BNA_F
ClientSampleId :
CHVB-0513


Tgt Ion:136	Resp: 631966
Ion Ratio	Lower Upper
136	100
137	10.6 9.8 14.6
54	6.2 6.4 9.6#
68	6.0 3.3 4.9#

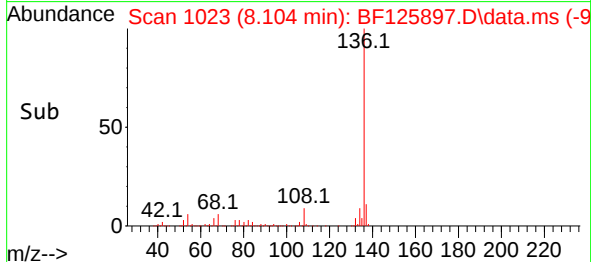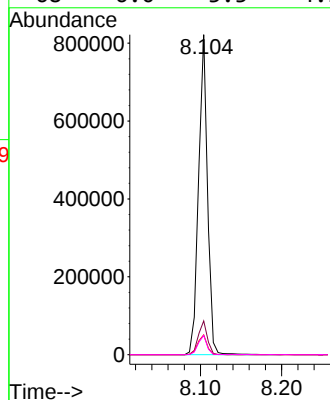

#23
Nitrobenzene-d5
Concen: 63.039 ng
RT: 7.381 min Scan# 900
Delta R.T. -0.012 min
Lab File: BF125897.D
Acq: 19 Oct 2021 13:39

Tgt Ion: 82	Resp: 640898
Ion Ratio	Lower Upper
82	100
128	48.5 40.6 60.8
54	42.7 49.6 74.4#


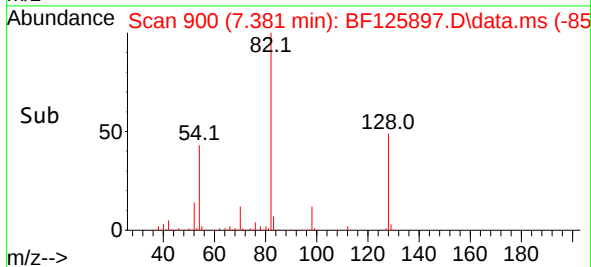
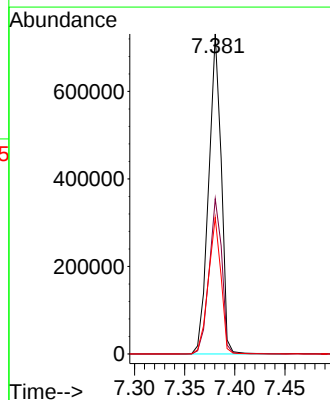
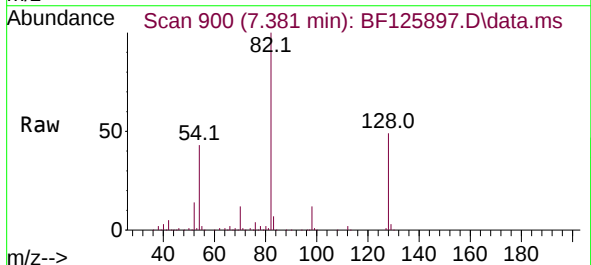


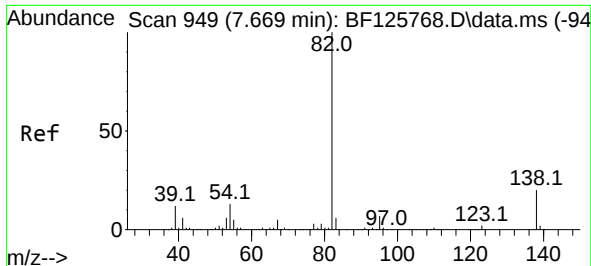

#25
Isophorone
Concen: 35.441 ng
RT: 7.381 min Scan# 900
Delta R.T. -0.271 min
Lab File: BF125897.D
Acq: 19 Oct 2021 13:39




Instrument :
BNA_F
ClientSampleId :
CHVB-0513


Tgt Ion: 82 Resp: 638348
Ion Ratio Lower Upper
82 100
95 0.0 6.5 9.7#
138 0.0 18.4 27.6#

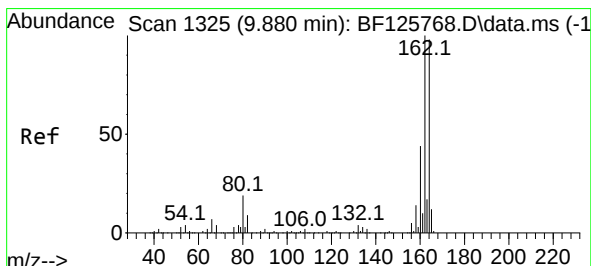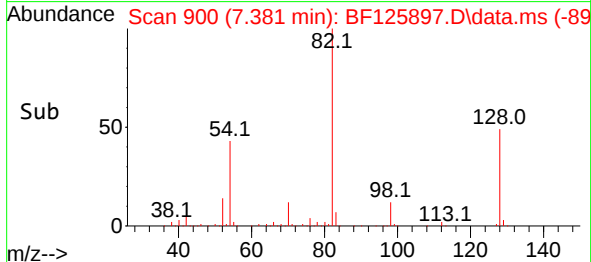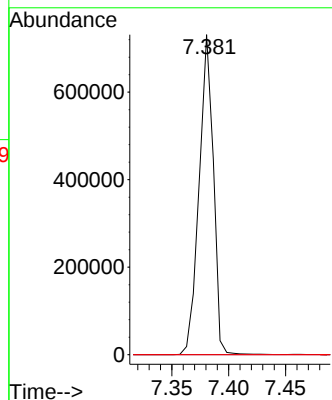

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.857 min Scan# 1321
Delta R.T. -0.006 min
Lab File: BF125897.D
Acq: 19 Oct 2021 13:39

Tgt Ion:164 Resp: 315757
Ion Ratio Lower Upper
164 100
162 100.0 81.3 121.9
160 42.7 38.0 57.0


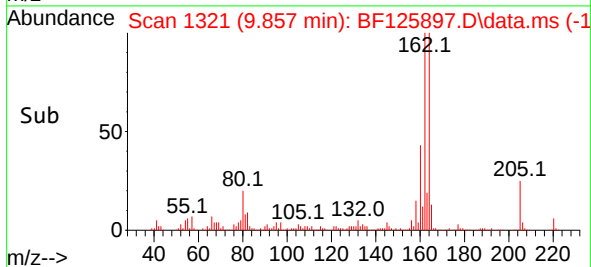
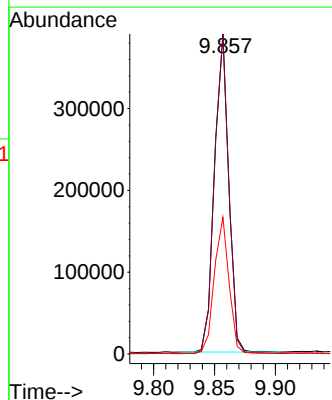
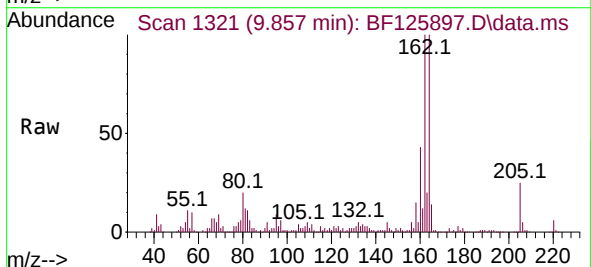


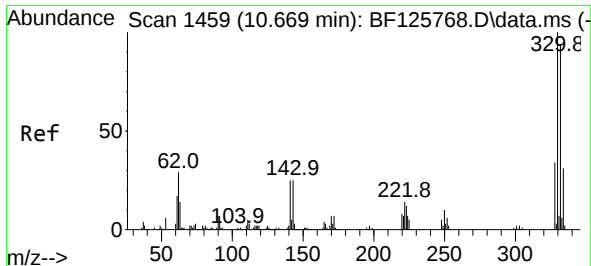

#42
2,4,6-Tribromophenol
Concen: 81.900 ng
RT: 10.645 min Scan# 1455
Delta R.T. -0.000 min
Lab File: BF125897.D
Acq: 19 Oct 2021 13:39




Instrument :
BNA_F
ClientSampleId :
CHVB-0513


Tgt Ion: 330 Resp: 255324
Ion Ratio Lower Upper
330 100
332 95.9 76.2 114.4
141 31.6 44.6 66.8#

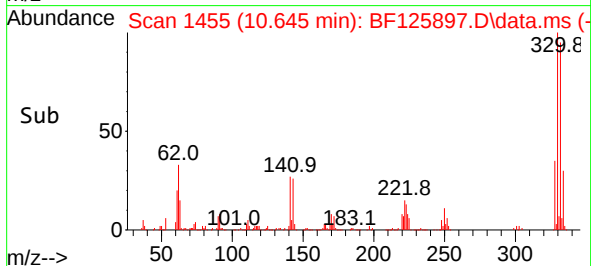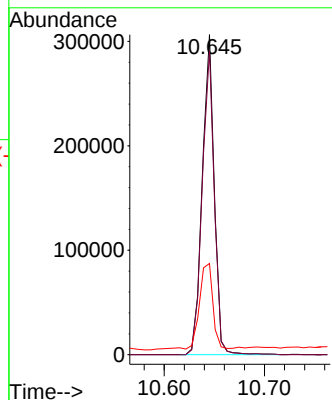

#45
2-Fluorobiphenyl
Concen: 65.239 ng
RT: 9.180 min Scan# 1206
Delta R.T. -0.000 min
Lab File: BF125897.D
Acq: 19 Oct 2021 13:39

Tgt Ion: 172 Resp: 1194307
Ion Ratio Lower Upper
172 100
171 35.1 26.5 39.7
170 23.6 18.8 28.2



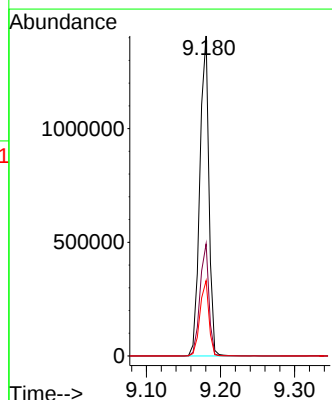
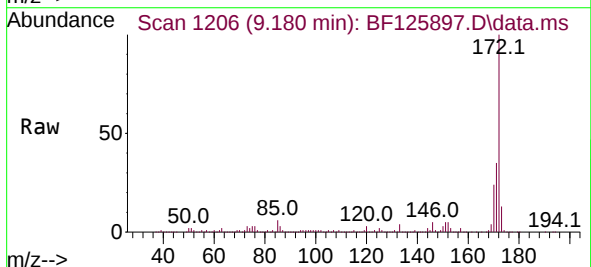




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.339 min Scan# 1573
Delta R.T. -0.000 min
Lab File: BF125897.D
Acq: 19 Oct 2021 13:39




Instrument :
BNA_F
ClientSampleId :
CHVB-0513


Tgt Ion:188 Resp: 535389
Ion Ratio Lower Upper
188 100
94 12.3 6.7 10.1#
80 12.2 7.5 11.3#

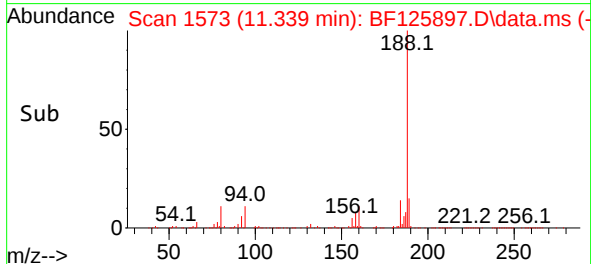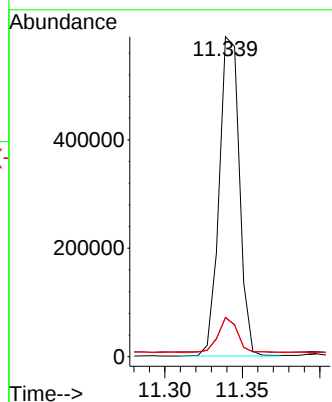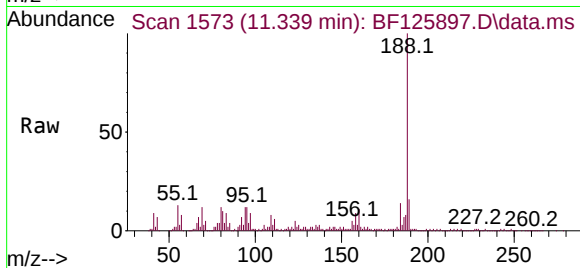

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.974 min Scan# 2021
Delta R.T. -0.000 min
Lab File: BF125897.D
Acq: 19 Oct 2021 13:39

Tgt Ion:240 Resp: 389525
Ion Ratio Lower Upper
240 100
120 11.7 10.8 16.2
236 25.1 21.6 32.4


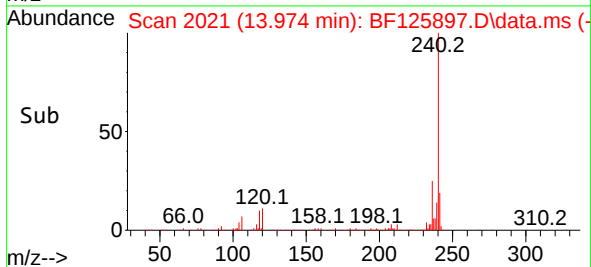
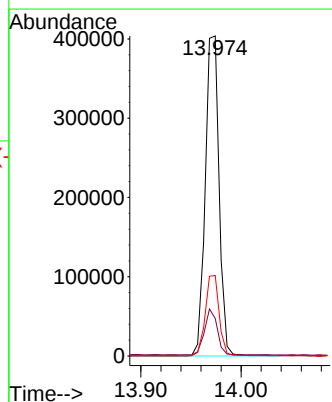
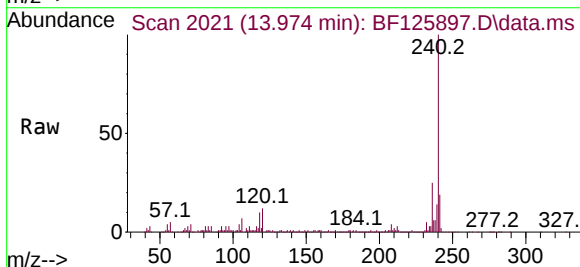




#79
 Terphenyl-d14
 Concen: 45.887 ng
 RT: 12.927 min Scan# 1843
 Delta R.T. 0.006 min
 Lab File: BF125897.D
 Acq: 19 Oct 2021 13:39

Instrument :
 BNA_F
 ClientSampleId :
 CHVB-0513

Tgt Ion:244 Resp: 1173422
 Ion Ratio Lower Upper
 244 100
 212 6.5 5.9 8.9
 122 10.7 9.0 13.4

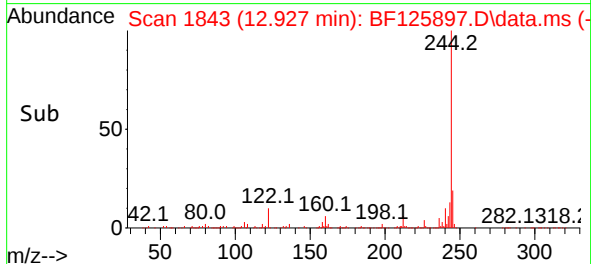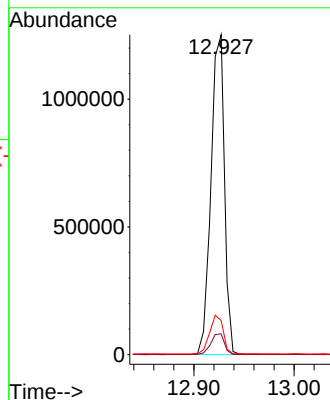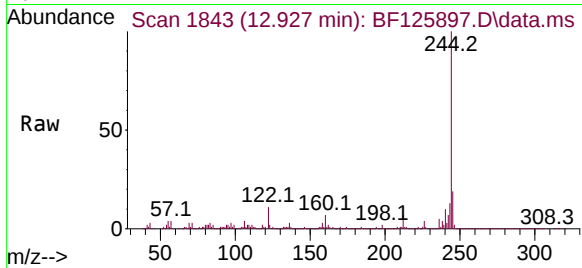

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.421 min Scan# 2267
 Delta R.T. -0.000 min
 Lab File: BF125897.D
 Acq: 19 Oct 2021 13:39

Tgt Ion:264 Resp: 332816
 Ion Ratio Lower Upper
 264 100
 260 24.4 19.6 29.4
 265 21.2 17.2 25.8

