
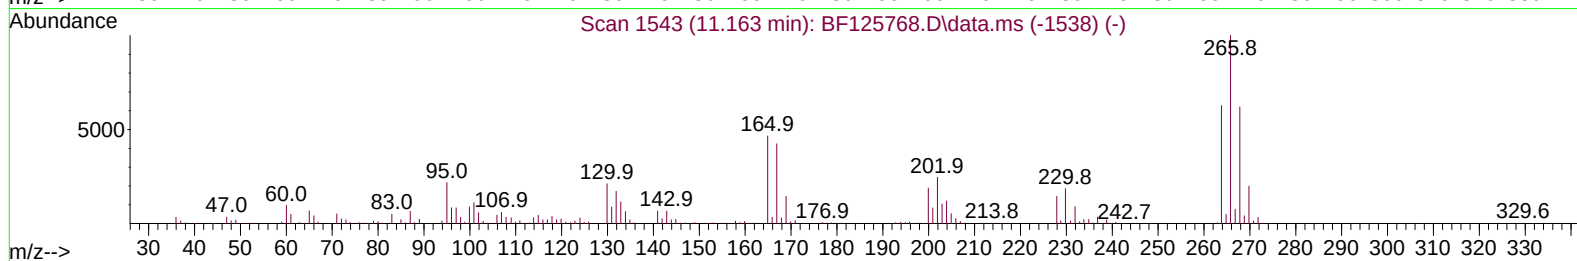
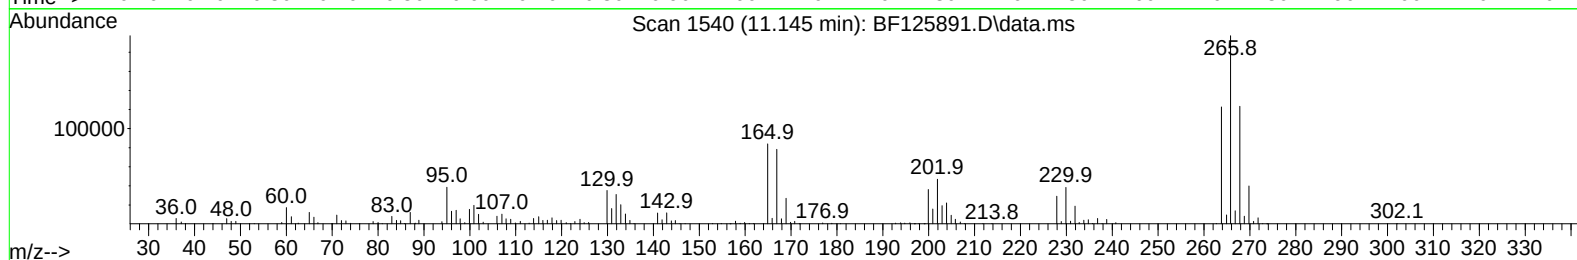


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101921\
 Data File : BF125891.D
 Acq On : 19 Oct 2021 10:07
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 19 13:04:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 18 12:43:03 2021
 Response via : Initial Calibration

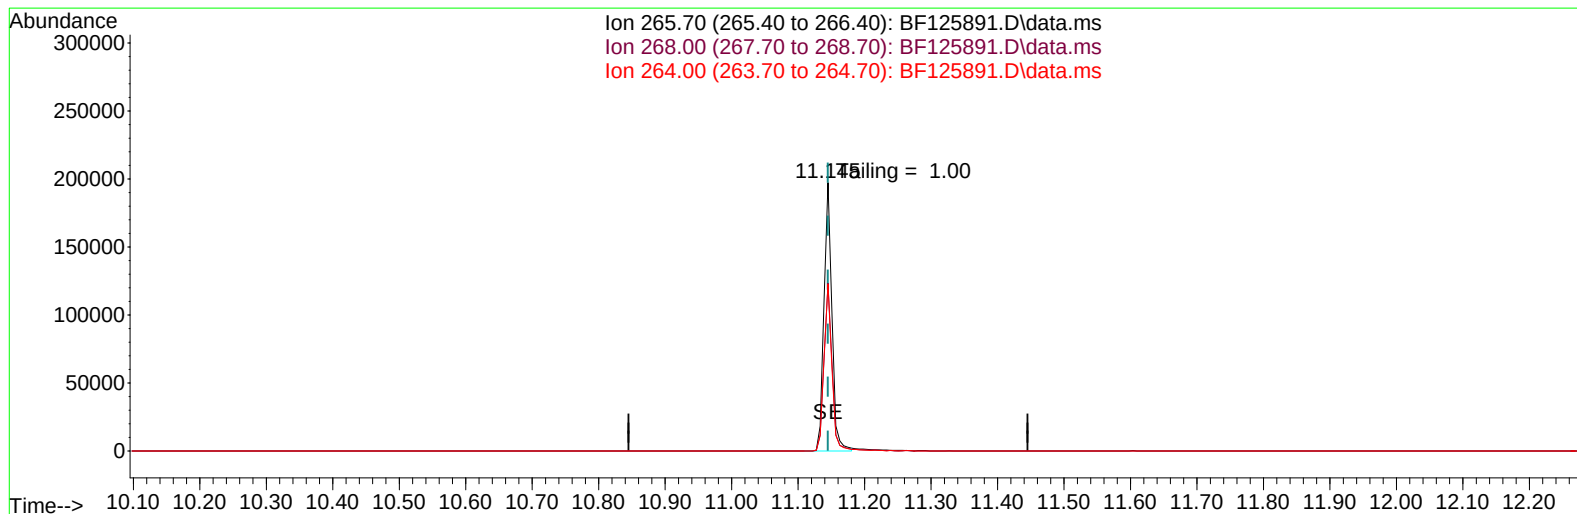

TIC: BF125891.D\data.ms

(70) Pentachlorophenol (C)




11.145min (-0.000) 46031.52 ng

response 168311

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.52
264.00	69.90	62.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101921\
 Data File : BF125891.D
 Acq On : 19 Oct 2021 10:07
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 19 13:04:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 18 12:43:03 2021
 Response via : Initial Calibration

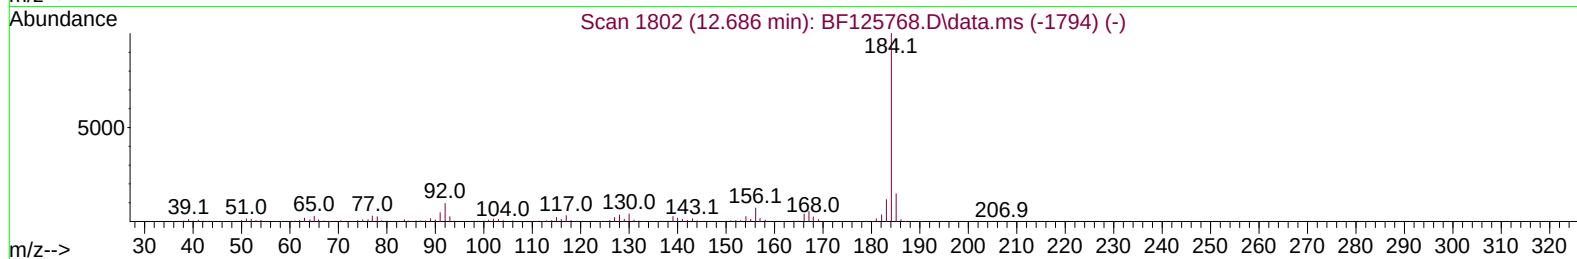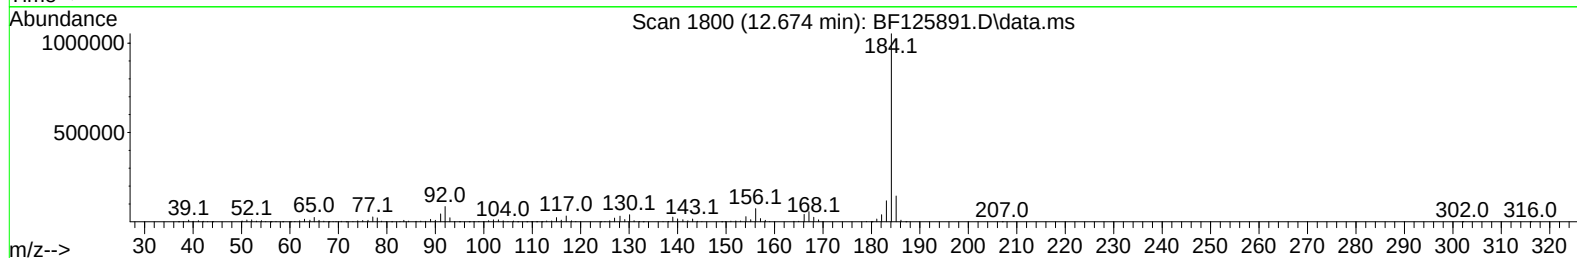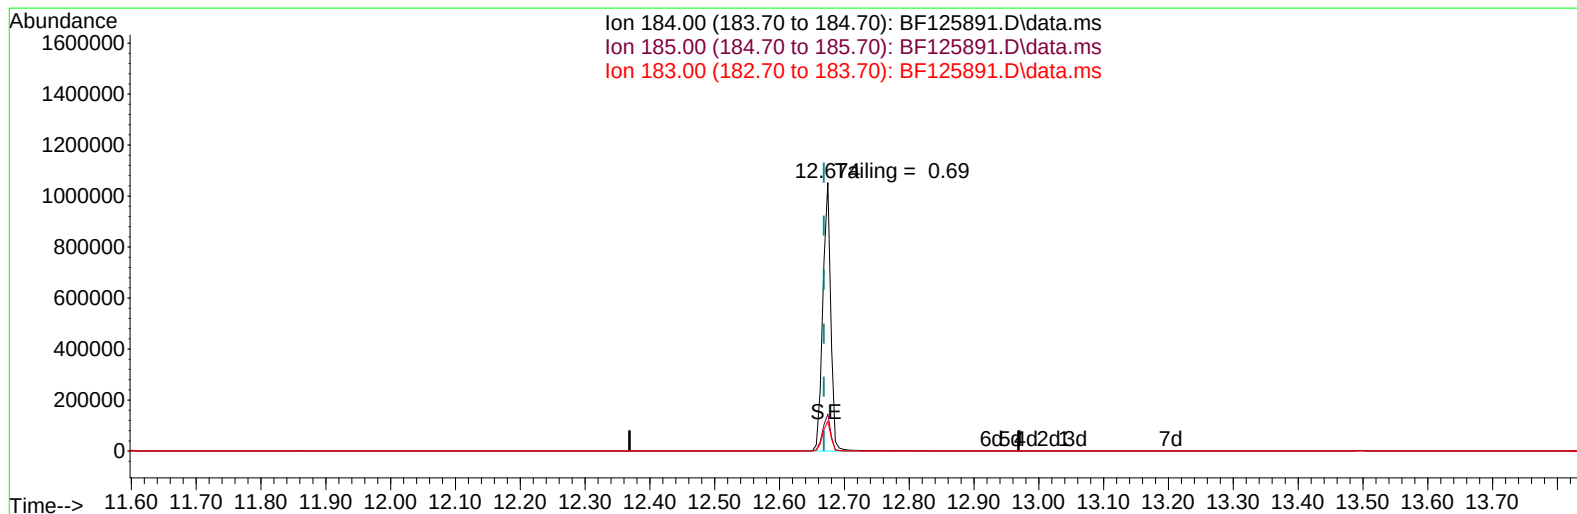

TIC: BF125891.D\data.ms

(77) Benzidine

12.674min (+ 0.006) 204169.40 ng m

response 889109

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.70
183.00	10.10	11.15
0.00	0.00	0.00