
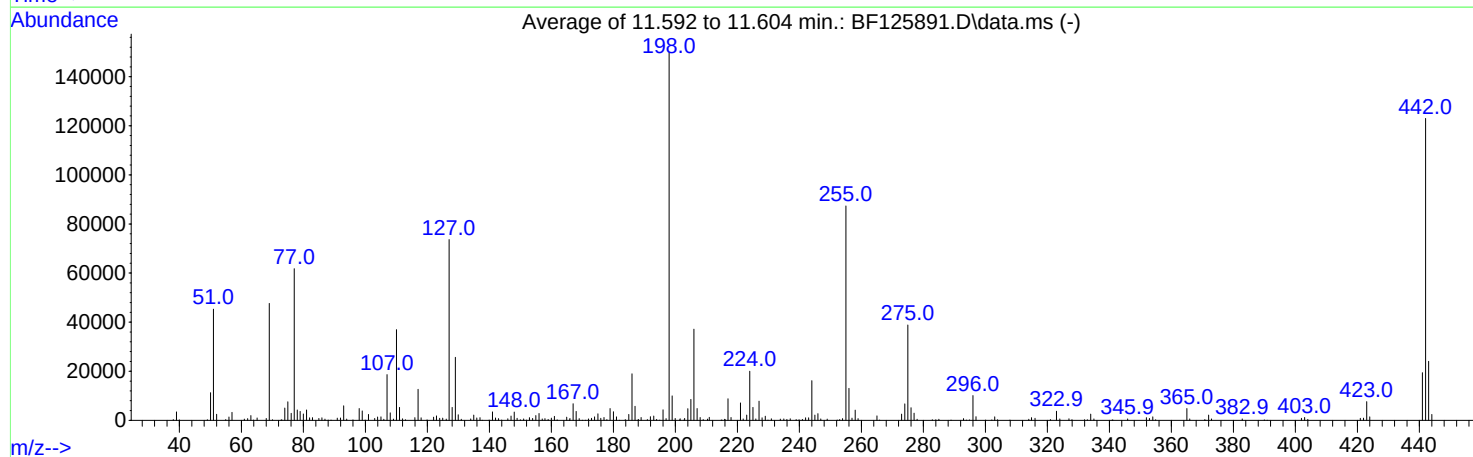


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101921\
 Data File : BF125891.D
 Acq On : 19 Oct 2021 10:07
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 18 12:43:03 2021

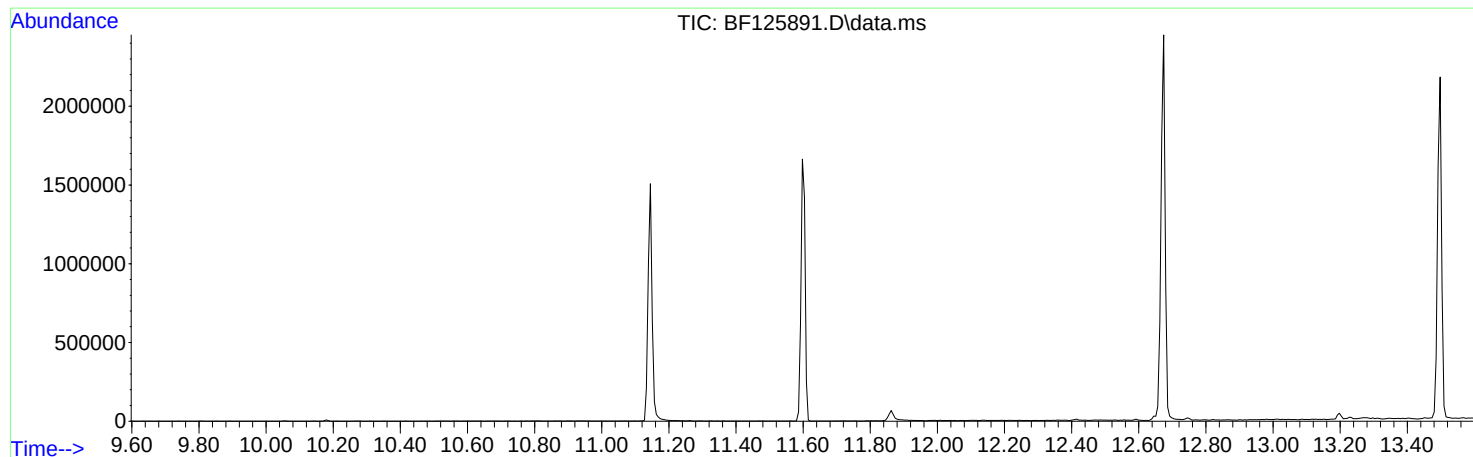




AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	45275	PASS
68	69	0.00	2	1.7	793	PASS
69	198	0.00	100	31.8	47632	PASS
70	69	0.00	2	0.6	292	PASS
127	198	10	80	49.2	73648	PASS
197	198	0.00	2	0.5	737	PASS
198	198	100	100	100.0	149843	PASS
199	198	5	9	6.7	10001	PASS
275	198	10	60	25.9	38818	PASS
365	198	1	100	3.2	4809	PASS
441	198	0.01	100	13.0	19462	PASS
442	442	50	100	100.0	122955	PASS
443	442	15	24	19.6	24040	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101921\
Data File : BF125891.D
Acq On : 19 Oct 2021 10:07
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 19 13:04:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 18 12:43:03 2021
Response via : Initial Calibration

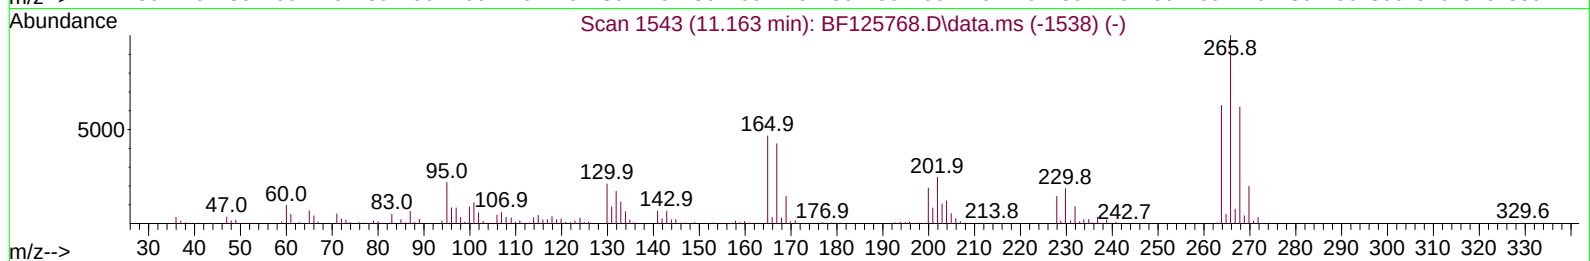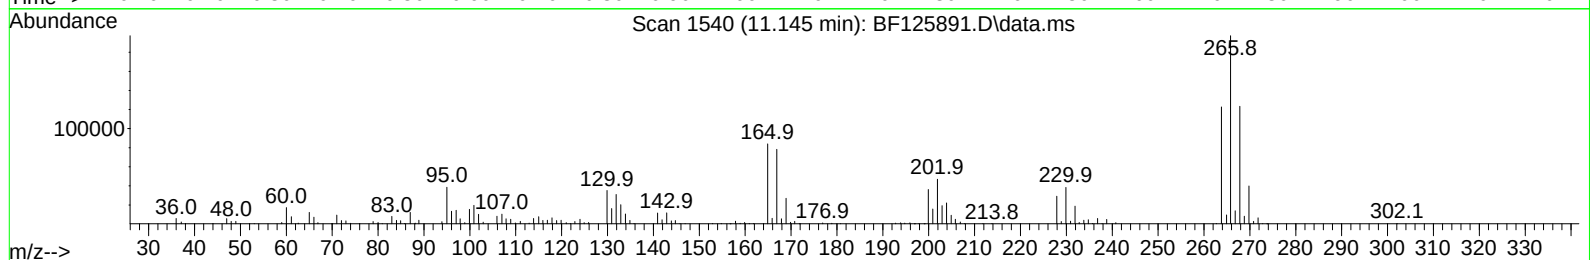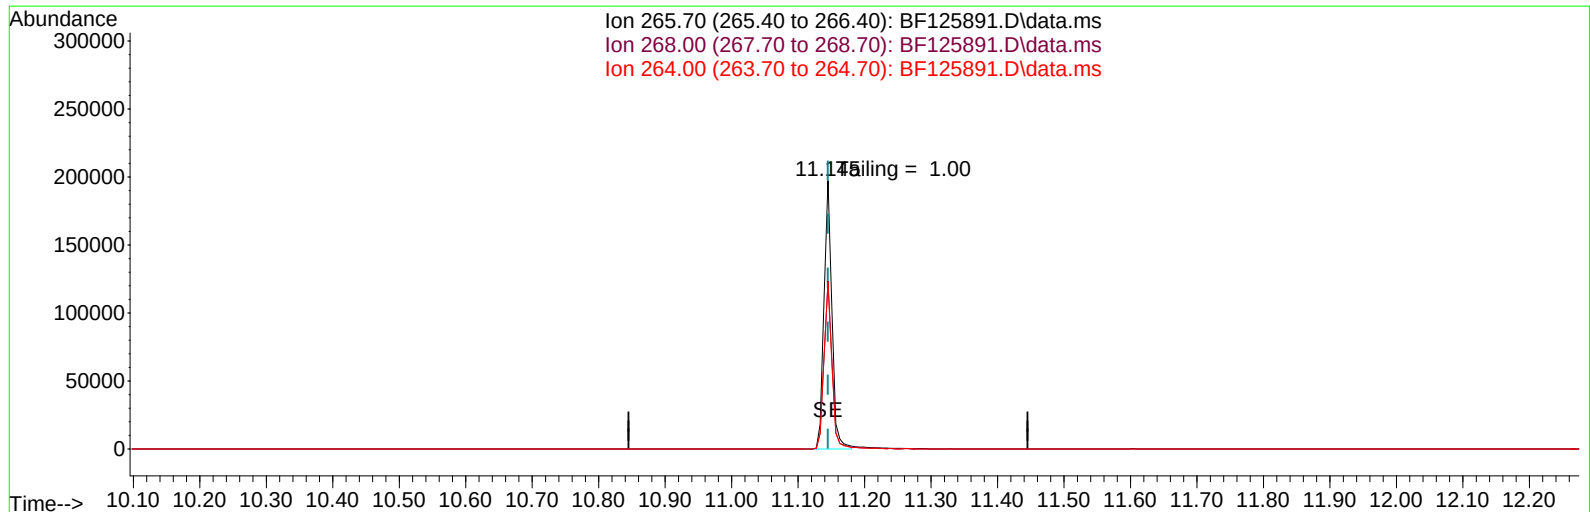

TIC: BF125891.D\data.ms

(70) Pentachlorophenol (C)

11.145min (-0.000) 46031.52 ng




response 168311

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.52
264.00	69.90	62.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101921\
 Data File : BF125891.D
 Acq On : 19 Oct 2021 10:07
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 19 13:04:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 18 12:43:03 2021
 Response via : Initial Calibration

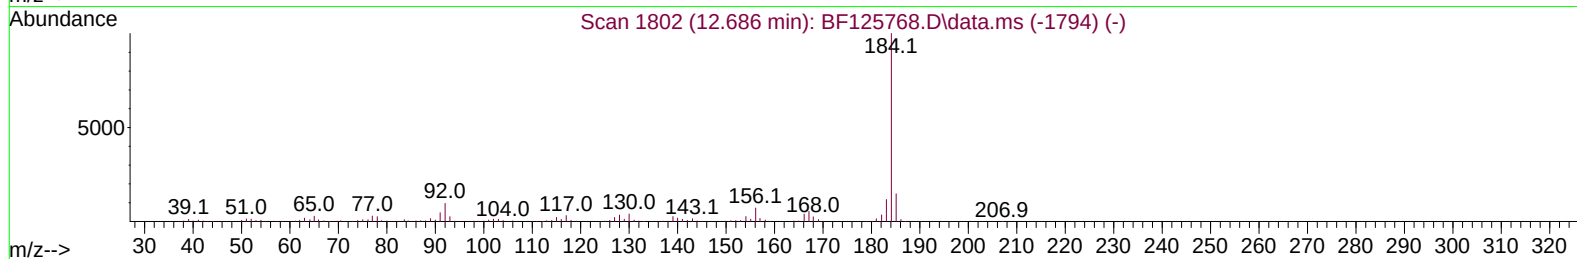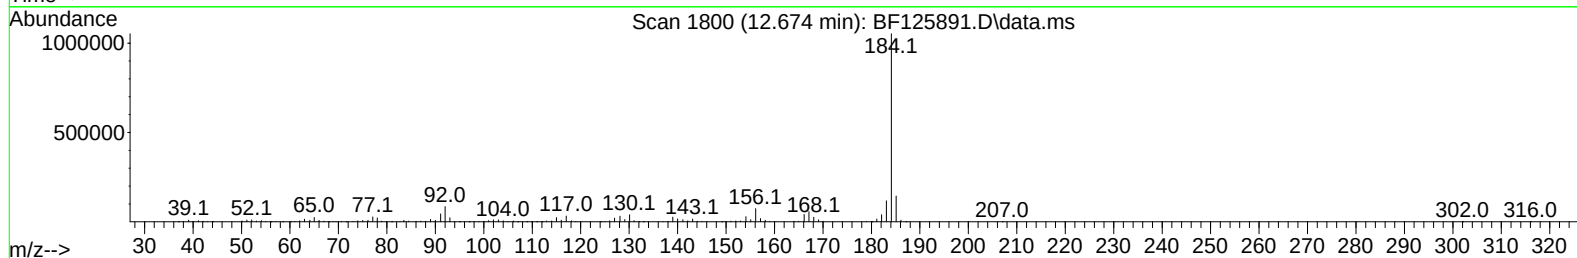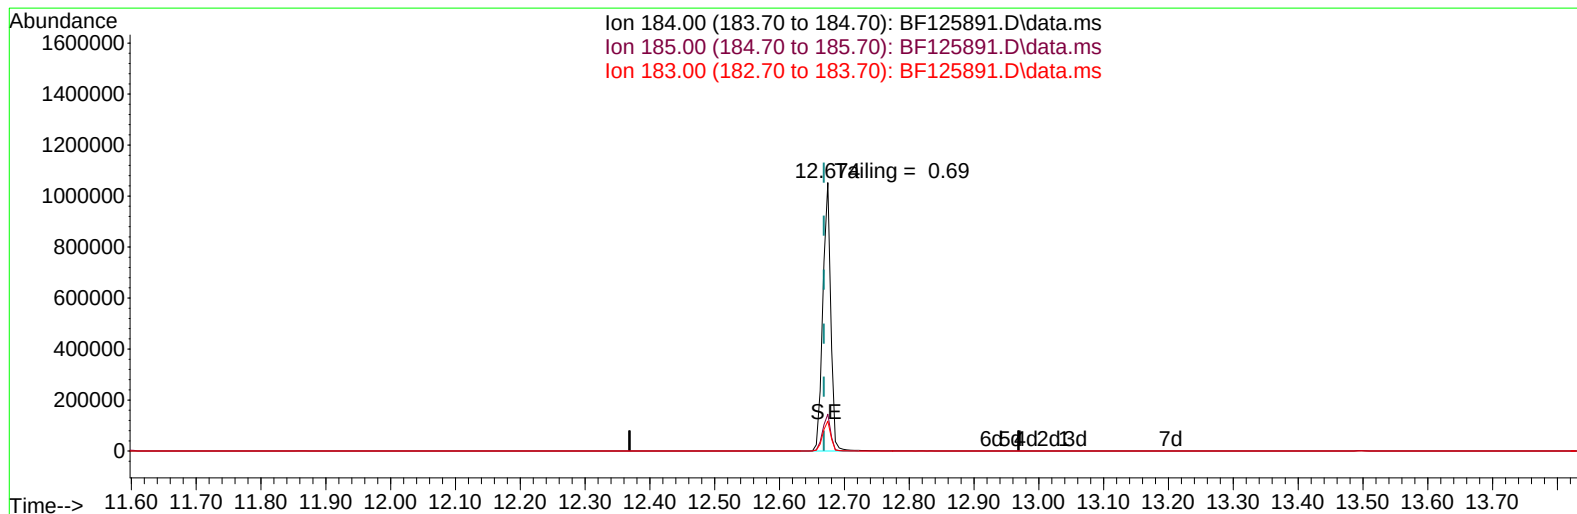

TIC: BF125891.D\data.ms

(77) Benzidine

12.674min (+ 0.006) 204169.40 ng m

response 889109

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.70
183.00	10.10	11.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/19/2021	BNA_F	<u>BF125891.D</u>
Compound Name	Response	Retention Time
DDT	370146	13.49
DDD	7935	13.19
DDE	535	12.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8470	378616	2.24

Instrument :
BNA_F
ClientSampleId :
DFTPP