

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101922\
 Data File : BF130713.D
 Acq On : 19 Oct 2022 16:23
 Operator : CG\JU
 Sample : PB148429BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB148429BL

Quant Time: Oct 19 16:58:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 18 03:15:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.569	152	94009	20.000	ng	0.00
21) Naphthalene-d8	7.851	136	327513	20.000	ng	0.00
39) Acenaphthene-d10	9.598	164	179899	20.000	ng	-0.01
64) Phenanthrene-d10	11.080	188	327017	20.000	ng	0.00
76) Chrysene-d12	13.710	240	221736	20.000	ng	-0.01
86) Perylene-d12	15.086	264	183001	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.187	112	812740	155.836	ng	0.02
7) Phenol-d6	6.228	99	974488	148.615	ng	0.00
23) Nitrobenzene-d5	7.139	82	703831	117.316	ng	-0.01
42) 2,4,6-Tribromophenol	10.392	330	308724	175.381	ng	0.00
45) 2-Fluorobiphenyl	8.927	172	1347752	113.481	ng	-0.01
79) Terphenyl-d14	12.668	244	1411336	105.641	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propyla...	7.139	70	92944	21.970	ng	# 76
25) Isophorone	7.139	82	703822	70.487	ng	# 64
50) Dimethylphthalate	9.598	163	32958	2.647	ng	# 1
51) 2,6-Dinitrotoluene	9.598	165	23447	8.583	ng	# 24
57) 2,4-Dinitrotoluene	9.598	165	23447	6.679	ng	# 14
67) 4-Bromophenyl-phenylether	10.392	248	17864	4.828	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101922\
Data File : BF130713.D
Acq On : 19 Oct 2022 16:23
Operator : CG\JU
Sample : PB148429BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148429BL

Quant Time: Oct 19 16:58:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 18 03:15:54 2022
Response via : Initial Calibration




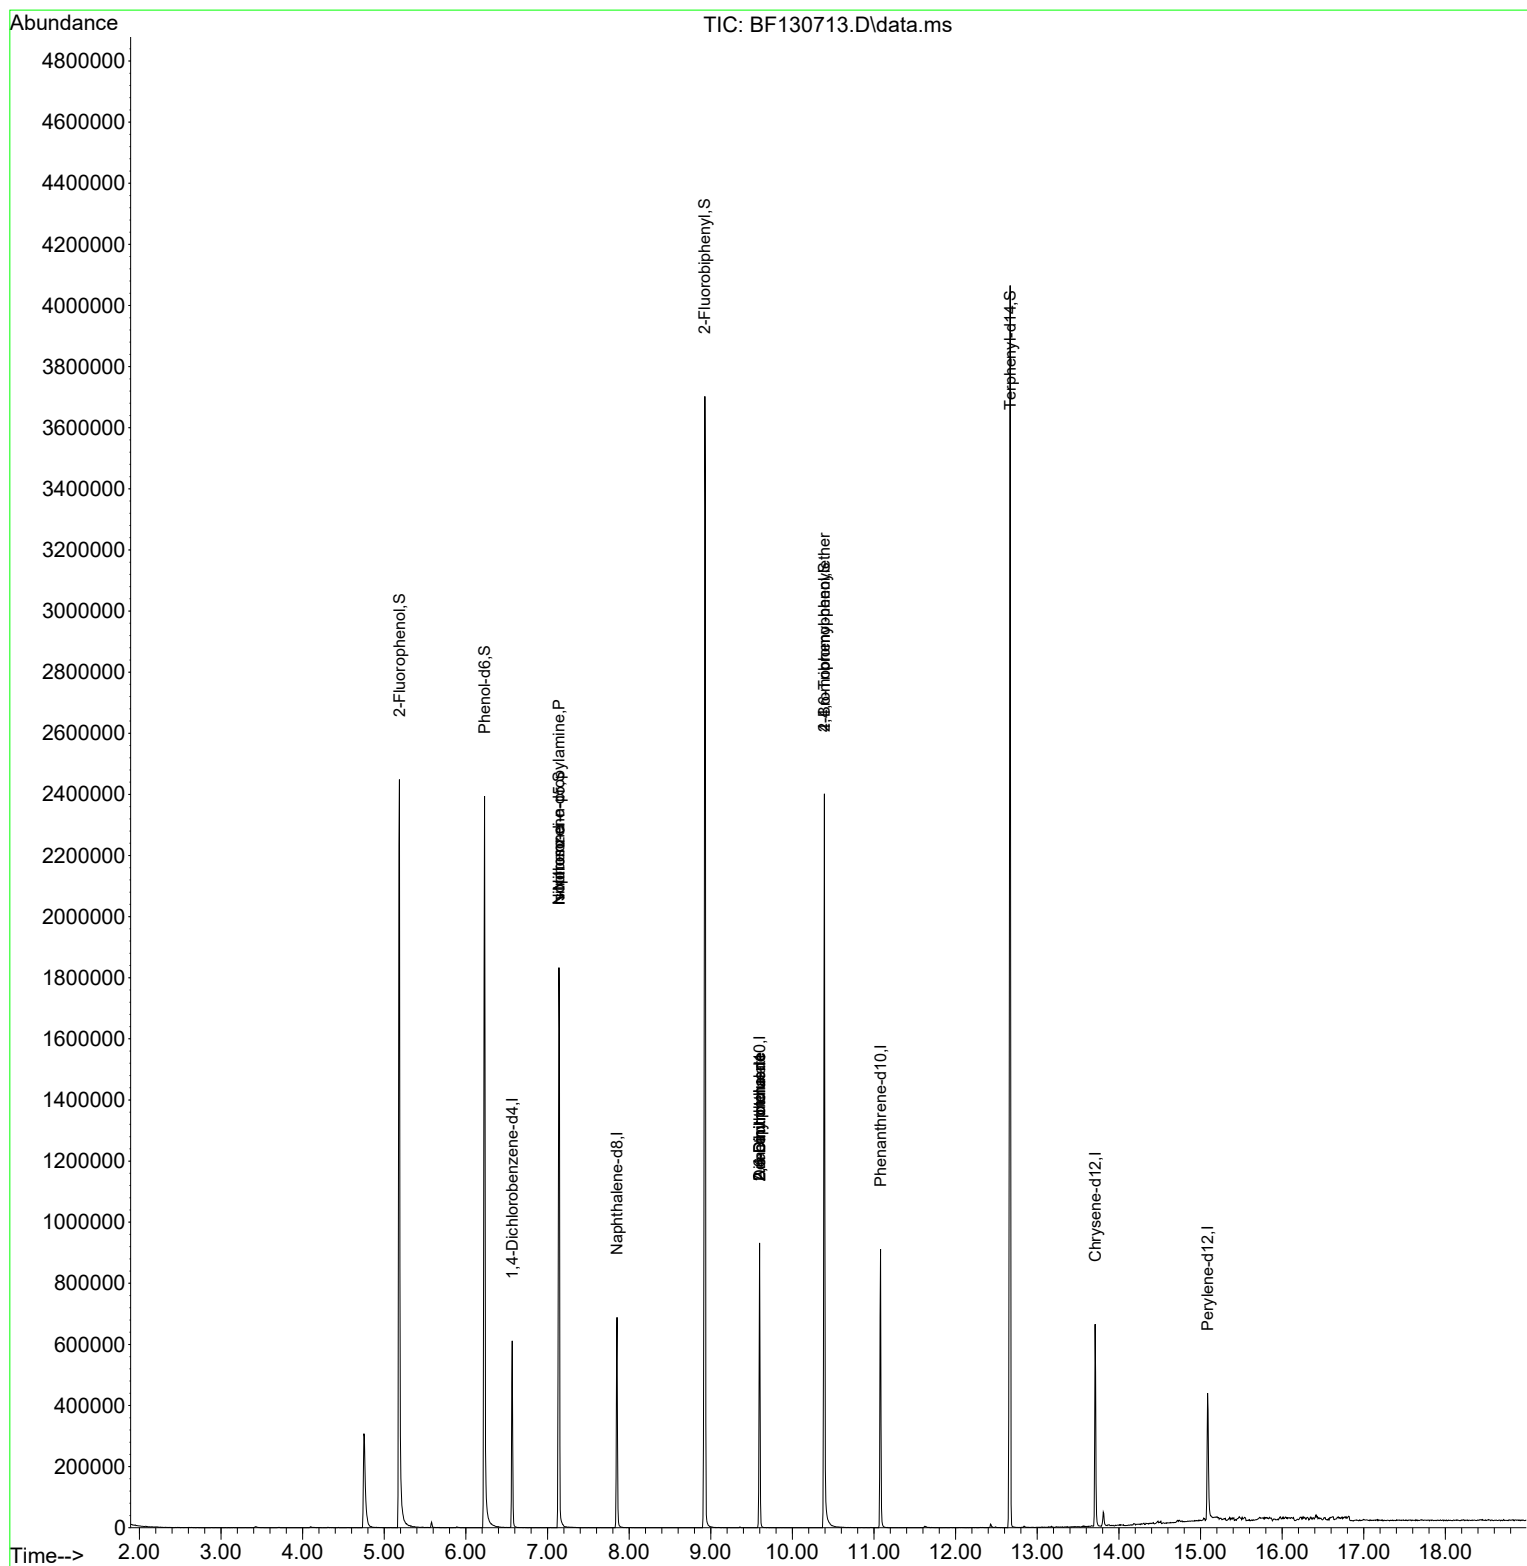


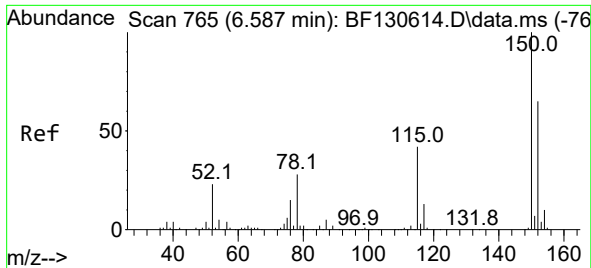

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.569 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF130713.D
Acq: 19 Oct 2022 16:23




Instrument :
BNA_F
ClientSampleId :
PB148429BL


Tgt Ion:152 Resp: 94009
Ion Ratio Lower Upper
152 100
150 155.0 123.8 185.6
115 61.7 52.2 78.4

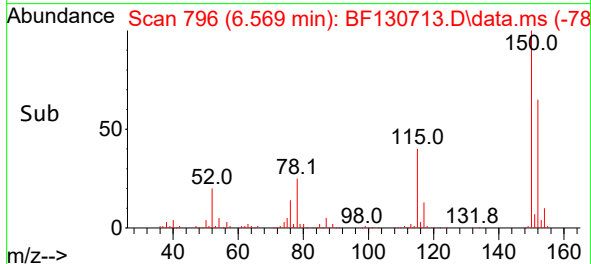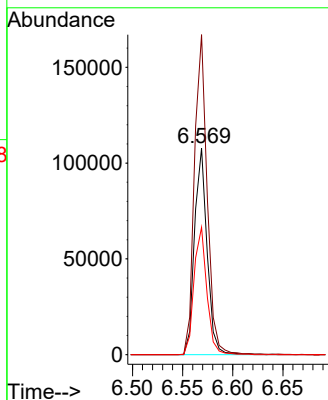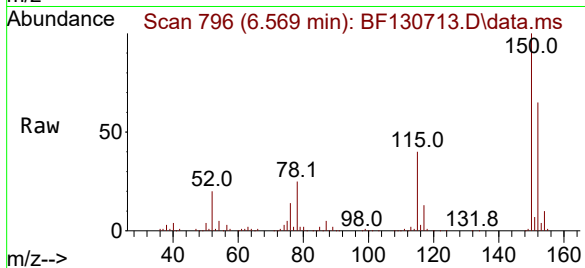

#5
2-Fluorophenol
Concen: 155.836 ng
RT: 5.187 min Scan# 561
Delta R.T. 0.017 min
Lab File: BF130713.D
Acq: 19 Oct 2022 16:23

Tgt Ion:112 Resp: 812740
Ion Ratio Lower Upper
112 100
64 54.5 43.5 65.3
63 29.0 22.6 34.0


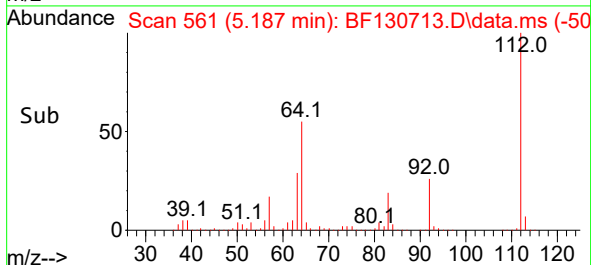
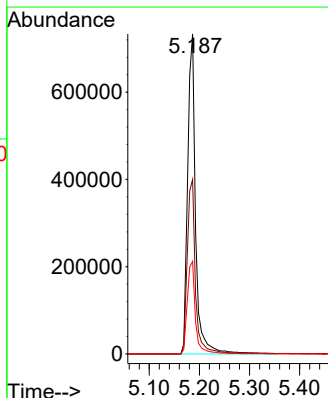
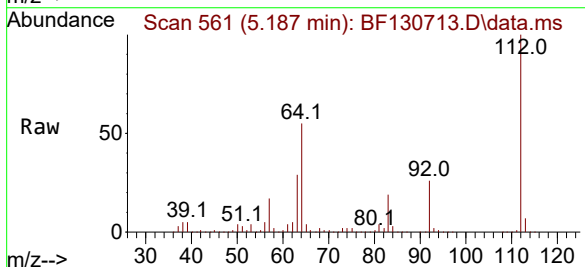


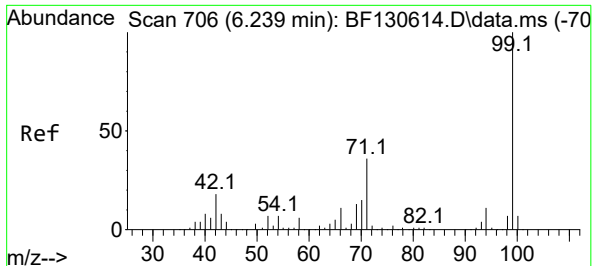

#7
Phenol-d6
Concen: 148.615 ng
RT: 6.228 min Scan# 713
Delta R.T. -0.000 min
Lab File: BF130713.D
Acq: 19 Oct 2022 16:23




Instrument :
BNA_F
ClientSampleId :
PB148429BL


Tgt Ion: 99 Resp: 974488
Ion Ratio Lower Upper
99 100
42 17.0 14.0 21.0
71 36.1 28.8 43.2

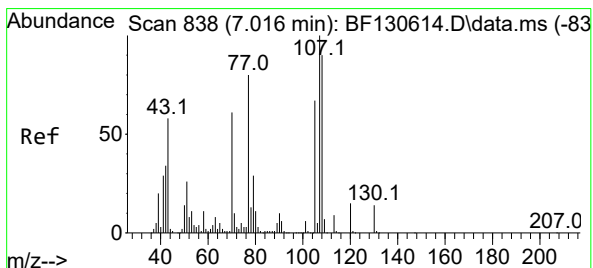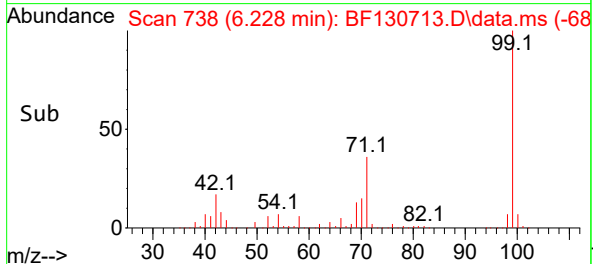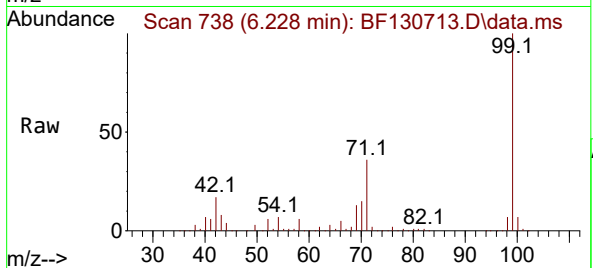

#19
n-Nitroso-di-n-propylamine
Concen: 21.970 ng
RT: 7.139 min Scan# 893
Delta R.T. 0.135 min
Lab File: BF130713.D
Acq: 19 Oct 2022 16:23


Tgt Ion: 70 Resp: 92944
Ion Ratio Lower Upper
70 100
42 44.2 44.3 66.5#
101 0.0 7.9 11.9#
130 1.8 18.1 27.1#

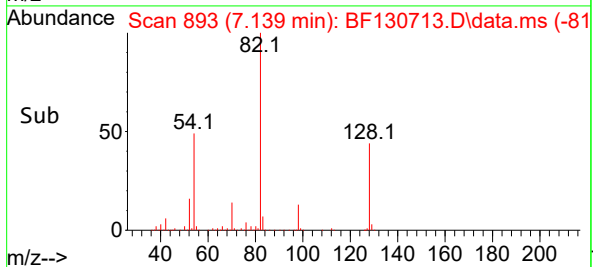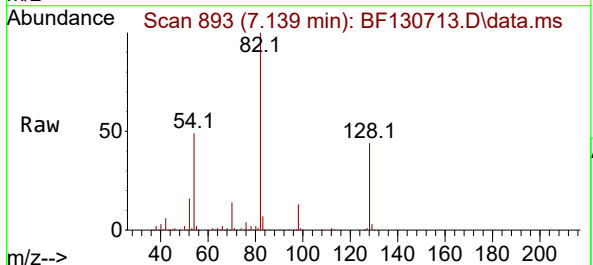






#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.851 min Scan# 1014
Delta R.T. -0.006 min
Lab File: BF130713.D
Acq: 19 Oct 2022 16:23


Instrument :
BNA_F
ClientSampleId :
PB148429BL

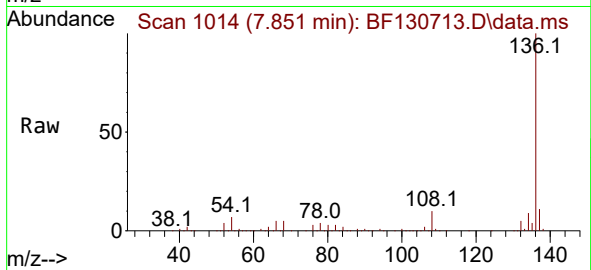



Tgt Ion:136 Resp: 327513
Ion Ratio Lower Upper
136 100
137 11.4 8.4 12.6
54 6.7 5.5 8.3
68 4.9 4.0 6.0

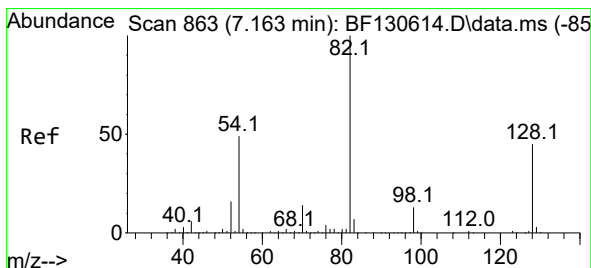


#23
Nitrobenzene-d5
Concen: 117.316 ng
RT: 7.139 min Scan# 893
Delta R.T. -0.012 min
Lab File: BF130713.D
Acq: 19 Oct 2022 16:23

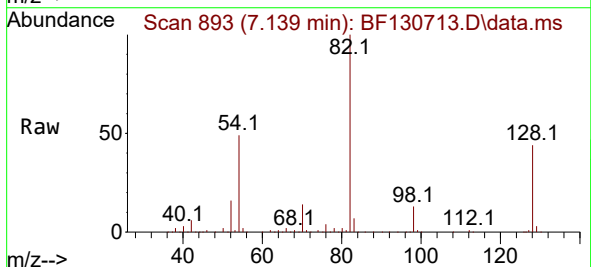

Tgt Ion: 82 Resp: 703831
Ion Ratio Lower Upper
82 100
128 44.1 35.8 53.6
54 48.9 39.3 58.9



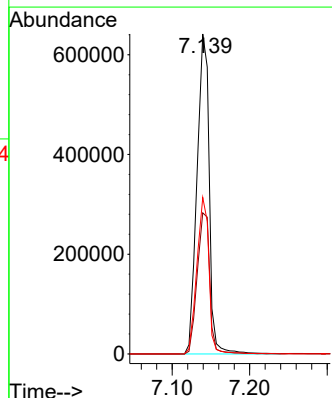
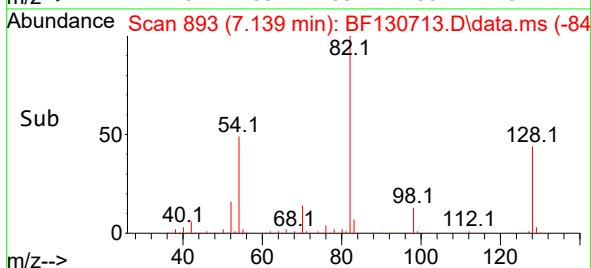




#25
Isophorone
Concen: 70.487 ng
RT: 7.139 min Scan# 893
Delta R.T. -0.271 min
Lab File: BF130713.D
Acq: 19 Oct 2022 16:23




Instrument :
BNA_F
ClientSampleId :
PB148429BL


Tgt Ion: 82 Resp: 703822
Ion Ratio Lower Upper
82 100
95 0.0 6.1 9.1#
138 0.0 14.9 22.3#

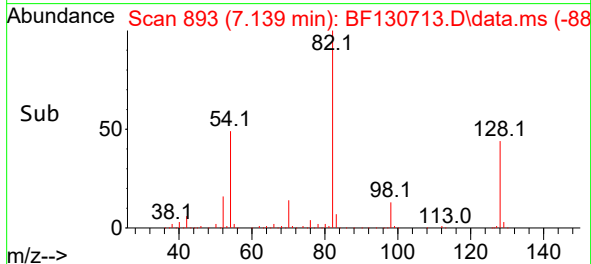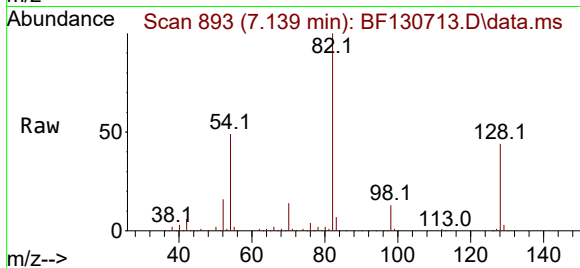

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.598 min Scan# 1311
Delta R.T. -0.012 min
Lab File: BF130713.D
Acq: 19 Oct 2022 16:23

Tgt Ion:164 Resp: 179899
Ion Ratio Lower Upper
164 100
162 103.6 81.0 121.4
160 43.8 34.5 51.7

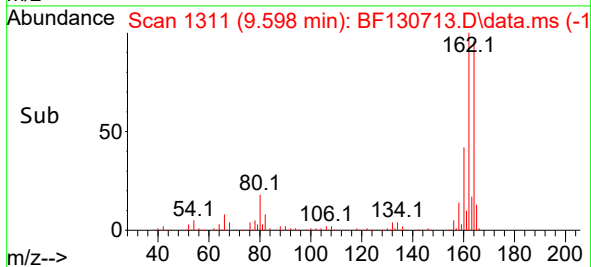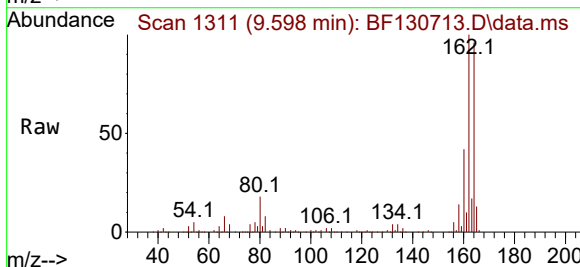



#42

2,4,6-Tribromophenol

Concen: 175.381 ng

RT: 10.392 min Scan# 1415

Delta R.T. -0.006 min

Lab File: BF130713.D

Acq: 19 Oct 2022 16:23

Instrument :

BNA_F

ClientSampleId :

PB148429BL





Tgt Ion:330 Resp: 308724

Ion Ratio Lower Upper

330 100

332 105.0 84.2 126.4

141 31.1 26.8 40.2

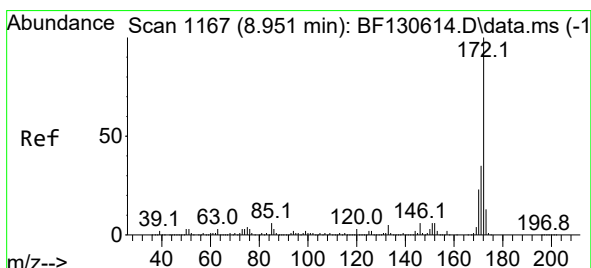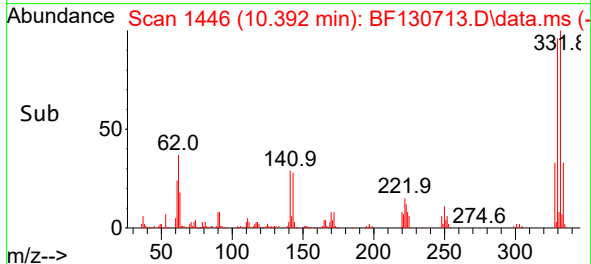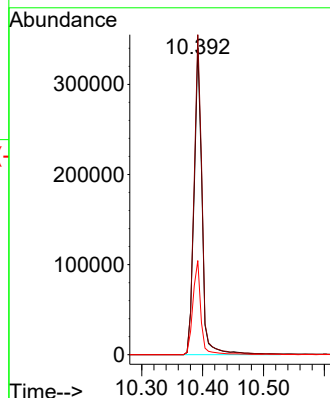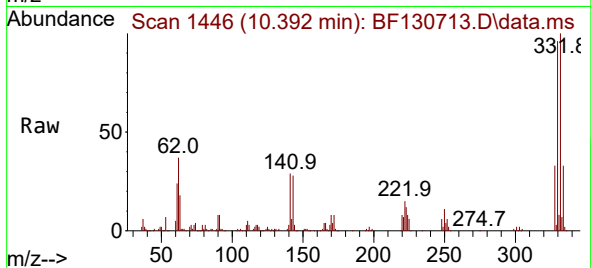

#45

2-Fluorobiphenyl

Concen: 113.481 ng

RT: 8.927 min Scan# 1197

Delta R.T. -0.012 min

Lab File: BF130713.D

Acq: 19 Oct 2022 16:23




Tgt Ion:172 Resp: 1347752


Ion Ratio Lower Upper

172 100

171 35.1 27.8 41.8

170 23.5 18.6 27.8


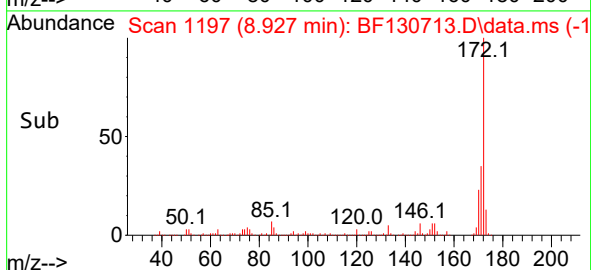
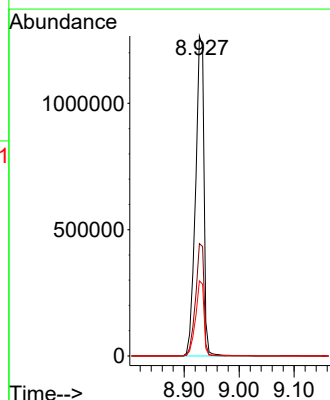





#50
Dimethylphthalate
Concen: 2.647 ng
RT: 9.598 min Scan# 1311
Delta R.T. 0.253 min
Lab File: BF130713.D
Acq: 19 Oct 2022 16:23




Instrument :
BNA_F
ClientSampleId :
PB148429BL


Tgt Ion:163 Resp: 32958
Ion Ratio Lower Upper
163 100
194 0.0 3.0 4.6#
164 573.4 8.5 12.7#

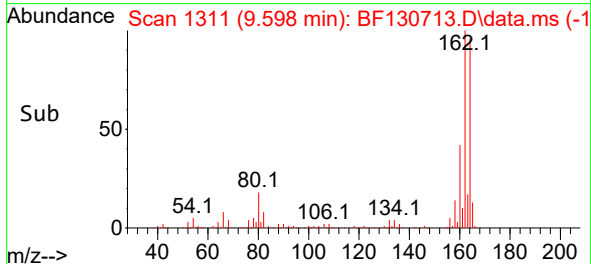

#51
2,6-Dinitrotoluene
Concen: 8.583 ng
RT: 9.598 min Scan# 1311
Delta R.T. 0.188 min
Lab File: BF130713.D
Acq: 19 Oct 2022 16:23

Tgt Ion:165 Resp: 23447
Ion Ratio Lower Upper
165 100
63 0.9 45.3 67.9#
89 1.2 45.6 68.4#


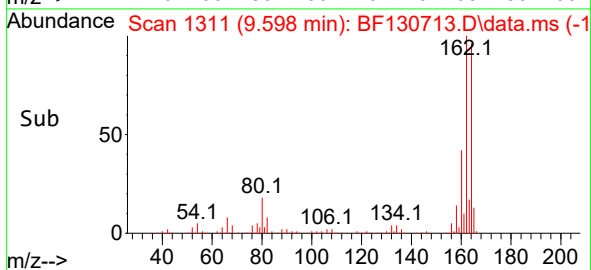

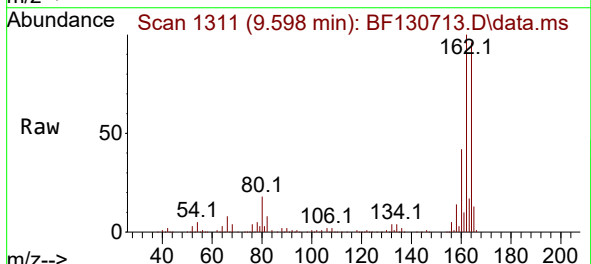




#57
2,4-Dinitrotoluene
Concen: 6.679 ng
RT: 9.598 min Scan# 11
Delta R.T. -0.218 min
Lab File: BF130713.D
Acq: 19 Oct 2022 16:23




Instrument :
BNA_F
ClientSampleId :
PB148429BL


Tgt Ion:165 Resp: 23447
Ion Ratio Lower Upper
165 100
63 0.9 50.6 76.0#
89 1.2 68.6 102.8#
182 0.0 2.0 3.0#

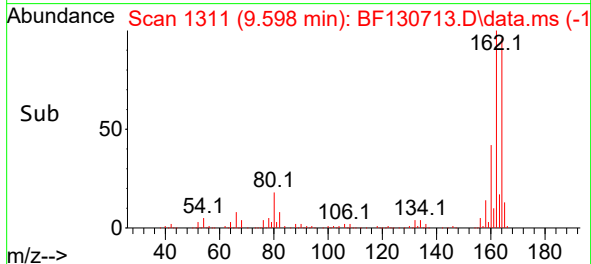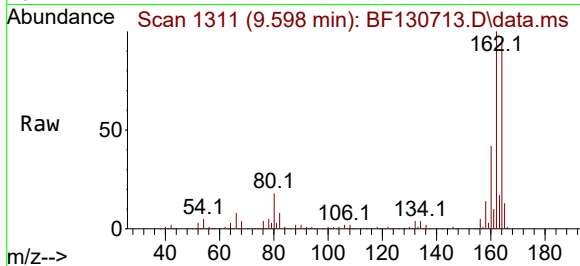

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.080 min Scan# 1563
Delta R.T. -0.006 min
Lab File: BF130713.D
Acq: 19 Oct 2022 16:23

Tgt Ion:188 Resp: 327017
Ion Ratio Lower Upper
188 100
94 8.5 7.4 11.2
80 8.6 8.0 12.0


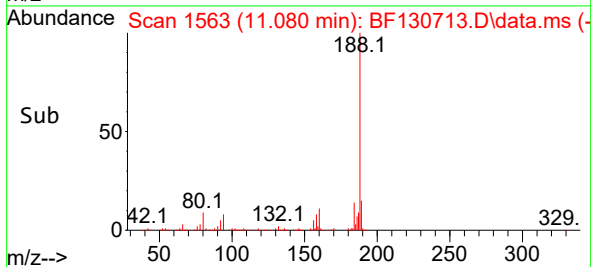

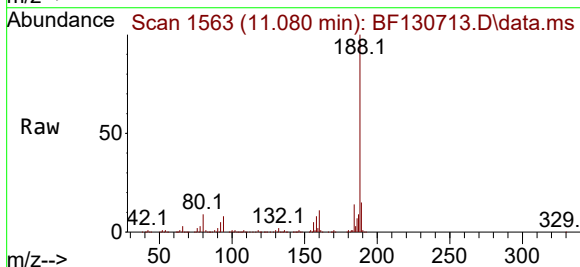


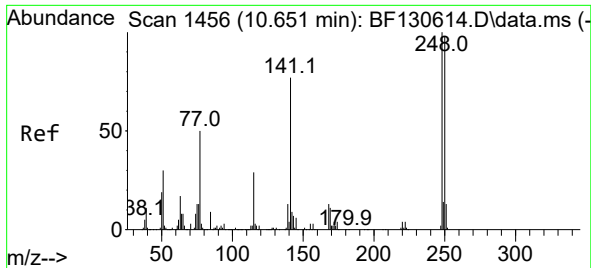

#67
4-Bromophenyl-phenylether
Concen: 4.828 ng
RT: 10.392 min Scan# 1456
Delta R.T. -0.247 min
Lab File: BF130713.D
Acq: 19 Oct 2022 16:23




Instrument :
BNA_F
ClientSampleId :
PB148429BL


Tgt Ion:248 Resp: 17864
Ion Ratio Lower Upper
248 100
250 202.3 78.7 118.1#
141 521.3 61.6 92.4#

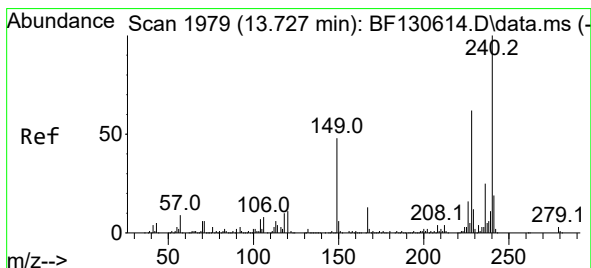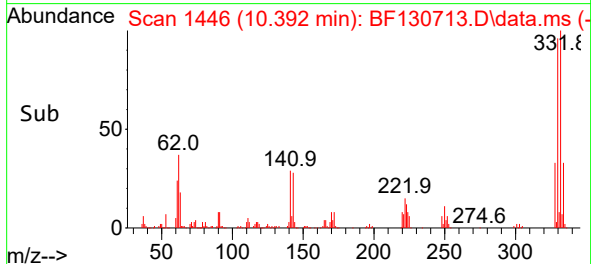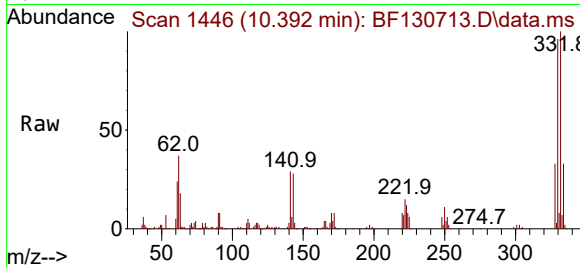

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.710 min Scan# 2010
Delta R.T. -0.012 min
Lab File: BF130713.D
Acq: 19 Oct 2022 16:23

Tgt Ion:240 Resp: 221736
Ion Ratio Lower Upper
240 100
120 11.2 8.6 13.0
236 24.7 20.2 30.4


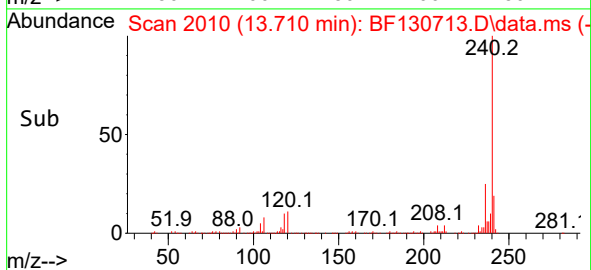

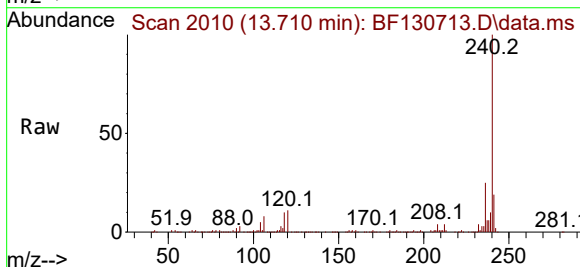




#79
 Terphenyl-d14
 Concen: 105.641 ng
 RT: 12.668 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF130713.D
 Acq: 19 Oct 2022 16:23

Instrument :
 BNA_F
 ClientSampleId :
 PB148429BL

Tgt Ion:244 Resp: 1411336
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.4 8.0
 122 11.9 7.5 11.3#

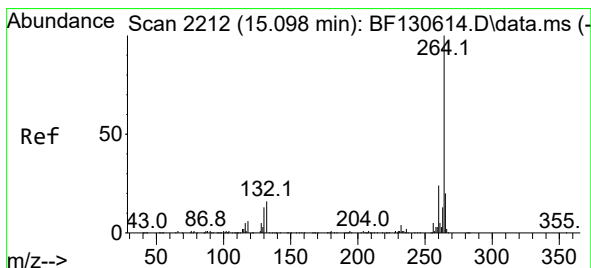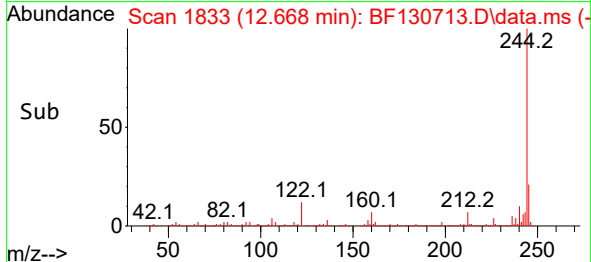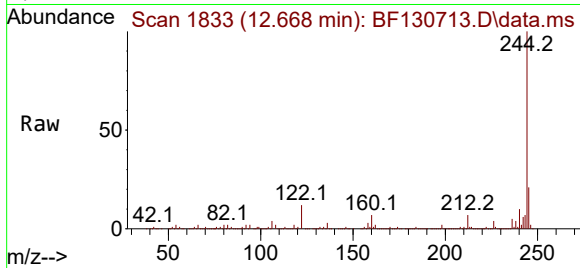

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.086 min Scan# 2244
 Delta R.T. -0.000 min
 Lab File: BF130713.D
 Acq: 19 Oct 2022 16:23

Tgt Ion:264 Resp: 183001
 Ion Ratio Lower Upper
 264 100
 260 23.2 19.1 28.7
 265 21.1 16.4 24.6

