

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101922\
 Data File : BF130713.D
 Acq On : 19 Oct 2022 16:23
 Operator : CG\JU
 Sample : PB148429BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB148429BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.751	483	487	501	rBV	307544	520981	13.63%	2.437%
2	5.187	557	561	580	rBV	2448226	2740551	71.68%	12.820%
3	6.228	734	738	741	rBV	2394123	2487535	65.06%	11.637%
4	6.569	792	796	807	rVB	611094	545200	14.26%	2.550%
5	7.139	889	893	907	rBV	1832793	2004951	52.44%	9.379%
6	7.851	1010	1014	1025	rBV	688620	643031	16.82%	3.008%
7	8.927	1192	1197	1200	rBV	3702676	3823495	100.00%	17.886%
8	9.598	1307	1311	1320	rBV	931729	756838	19.79%	3.540%
9	10.392	1442	1446	1462	rBV	2402007	2195866	57.43%	10.272%
10	11.080	1559	1563	1576	rBV	911776	786020	20.56%	3.677%
11	12.668	1828	1833	1836	rBV	4065274	3708699	97.00%	17.349%
12	13.710	2007	2010	2019	rBV	660228	593689	15.53%	2.777%
13	13.810	2023	2027	2033	rBV	46643	57598	1.51%	0.269%
14	15.086	2240	2244	2256	rBV	415255	512178	13.40%	2.396%




Sum of corrected areas: 21376632

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101922\
Data File : BF130713.D
Acq On : 19 Oct 2022 16:23
Operator : CG\JU
Sample : PB148429BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148429BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

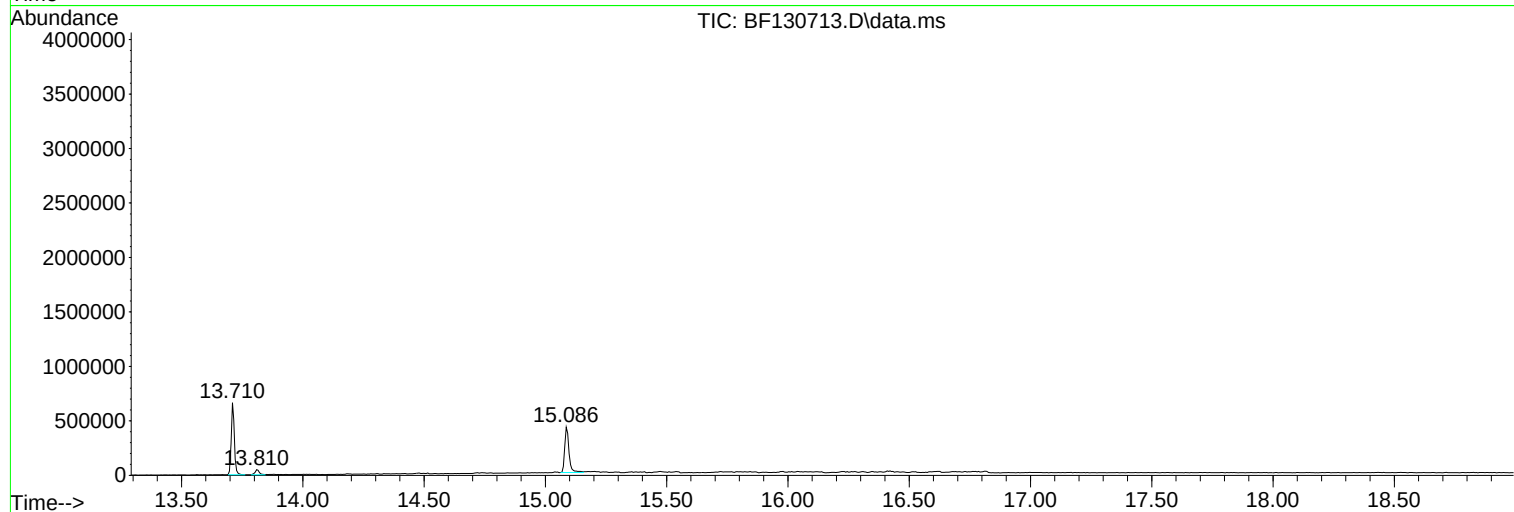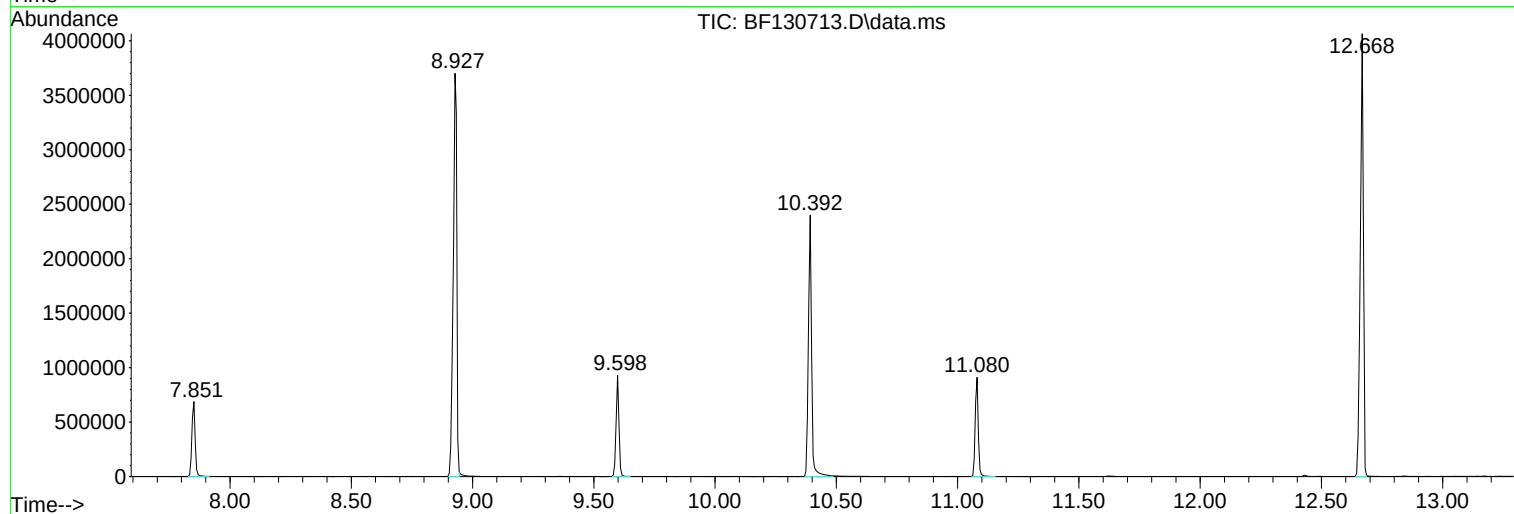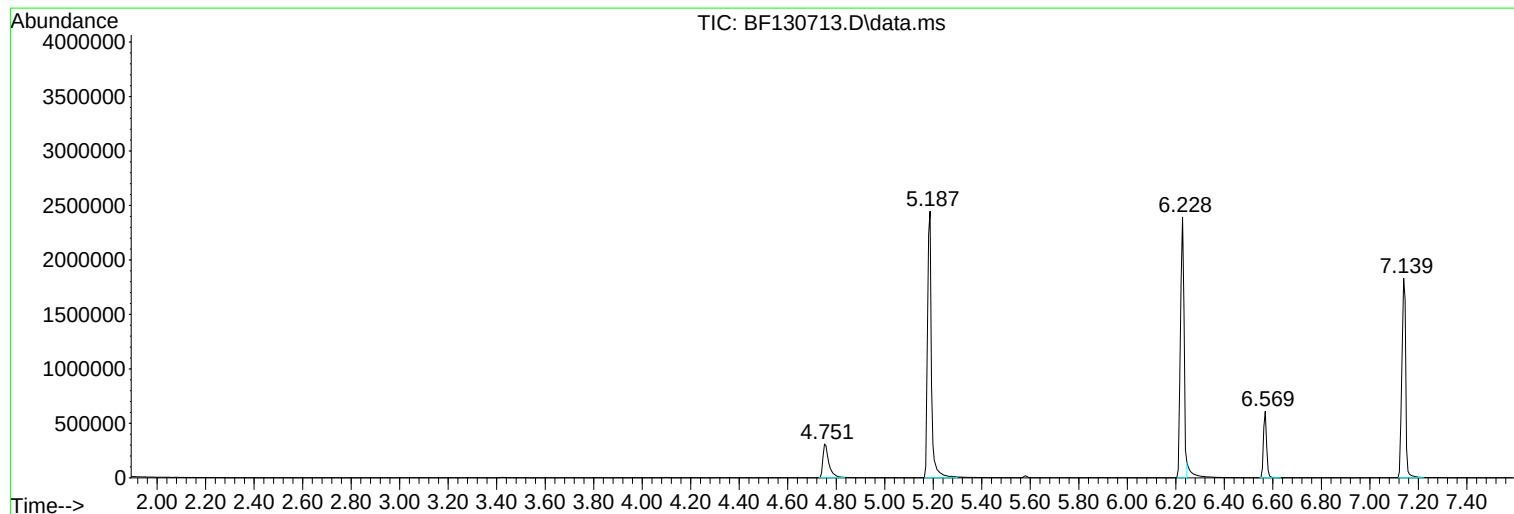

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101922\
Data File : BF130713.D
Acq On : 19 Oct 2022 16:23
Operator : CG\JU
Sample : PB148429BL
Misc :
ALS Vial : 6 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB148429BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
4.751	19.11 ng	520981	1,4-Dichlorobenzene-d4		6.569	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	64
2	1-Propen-2-ol, acetate		100	C5H8O2	000108-22-5	10
3	2,3-Butanedione, monooxime		101	C4H7NO2	000057-71-6	9
4	Morpholine, 4-methyl-		101	C5H11NO	000109-02-4	9
5	5-Hexen-2-one		98	C6H10O	000109-49-9	9

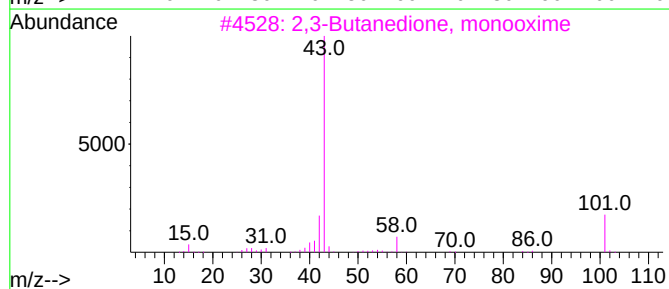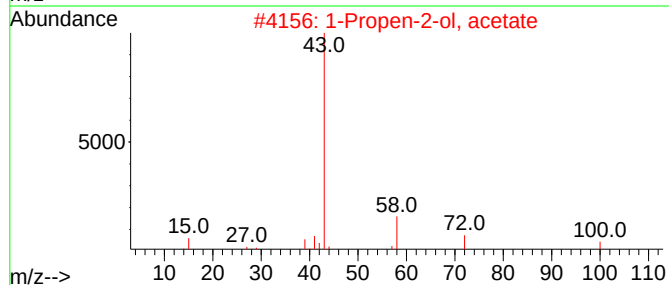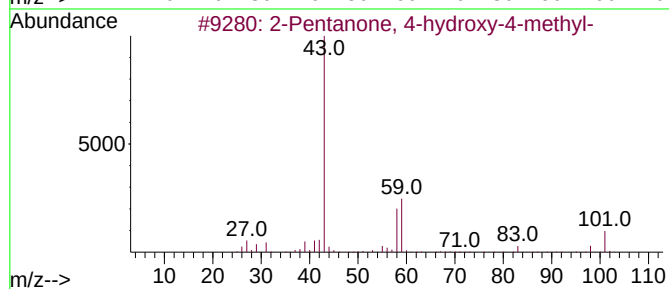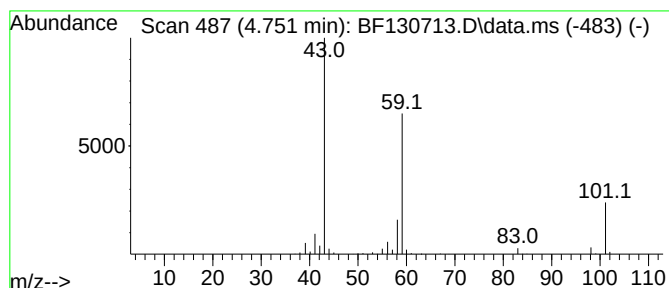

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101922\
Data File : BF130713.D
Acq On : 19 Oct 2022 16:23
Operator : CG\JU
Sample : PB148429BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148429BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.751	19.1	ng	520981	1	6.569	545200	20.0