

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101922\
 Data File : BF130719.D
 Acq On : 19 Oct 2022 19:30
 Operator : CG\JU
 Sample : N5176-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 5236-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130719.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.740	482	485	500	rBV	99092	133039	3.56%	0.852%
2	5.175	556	559	584	rBV	846704	999187	26.71%	6.398%
3	6.222	735	737	759	rBV	580168	713995	19.08%	4.572%
4	6.569	792	796	805	rBV	507727	464965	12.43%	2.977%
5	7.145	889	894	907	rBV	1457247	1628747	43.53%	10.429%
6	7.851	1010	1014	1030	rVB	789450	695221	18.58%	4.451%
7	8.928	1192	1197	1200	rBV	4082009	3741501	100.00%	23.957%
8	9.598	1307	1311	1321	rVB	1094475	910072	24.32%	5.827%
9	10.392	1442	1446	1463	rBV	1983916	2017499	53.92%	12.918%
10	11.074	1559	1562	1572	rBV	942248	868551	23.21%	5.561%
11	12.663	1828	1832	1835	rBV	2795873	2412250	64.47%	15.445%
12	13.710	2006	2010	2020	rVB	547682	514201	13.74%	3.292%
13	15.086	2240	2244	2253	rBV	415780	518609	13.86%	3.321%




Sum of corrected areas: 15617837

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101922\
Data File : BF130719.D
Acq On : 19 Oct 2022 19:30
Operator : CG\JU
Sample : N5176-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
5236-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

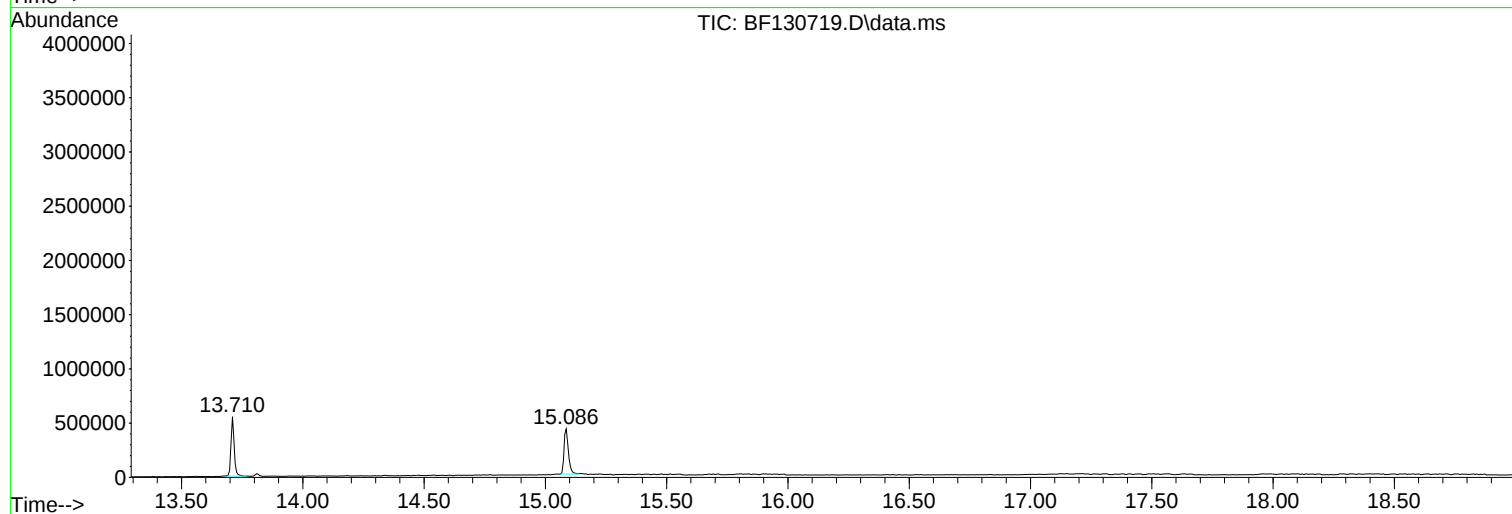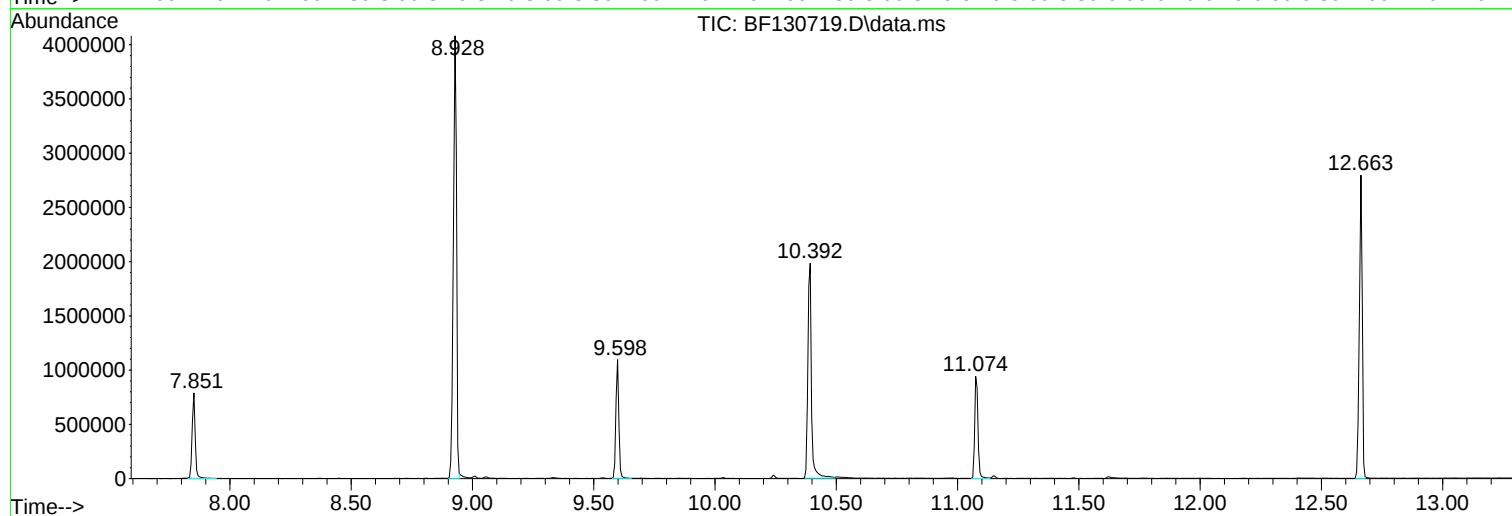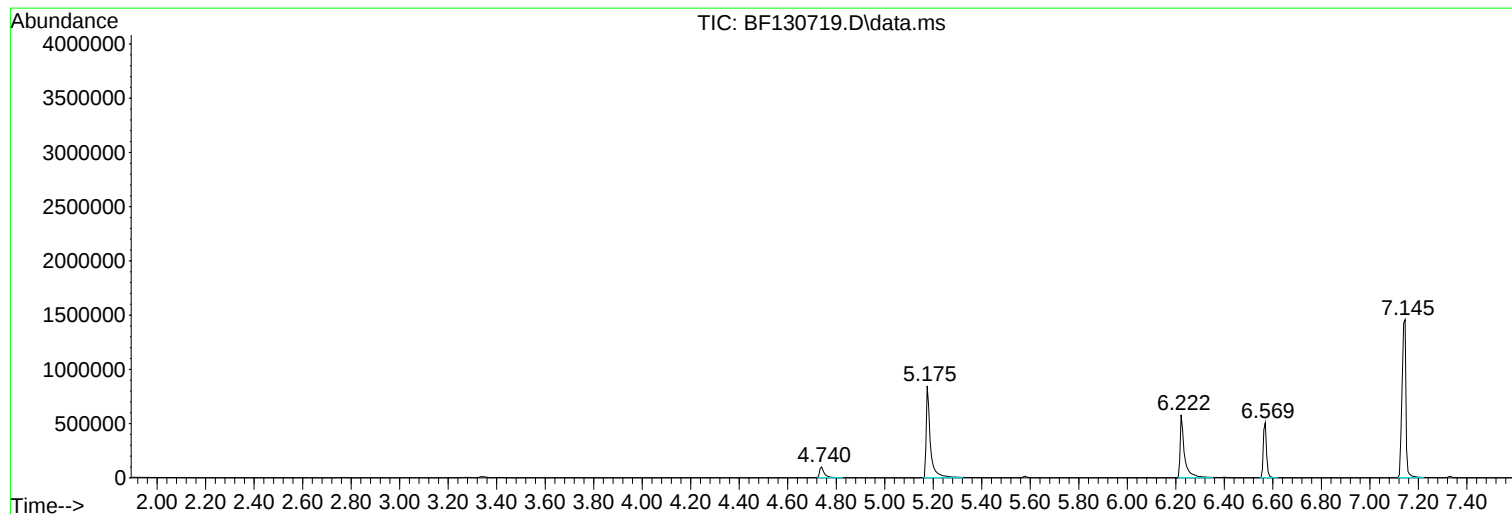

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101922\
Data File : BF130719.D
Acq On : 19 Oct 2022 19:30
Operator : CG\JU
Sample : N5176-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
5236-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.740	5.72 ng	133039	1,4-Dichlorobenzene-d4	6.569

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9		

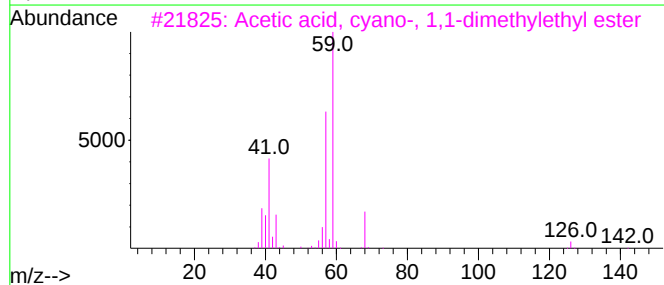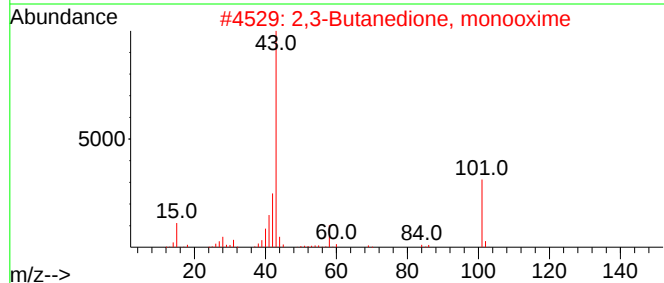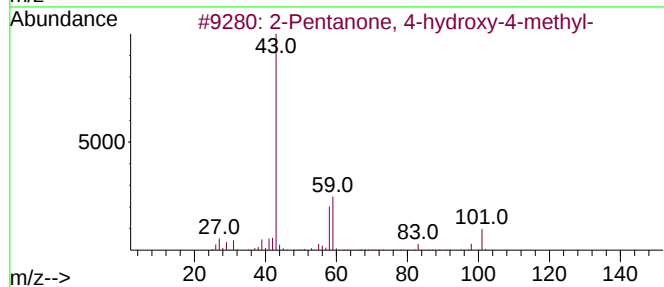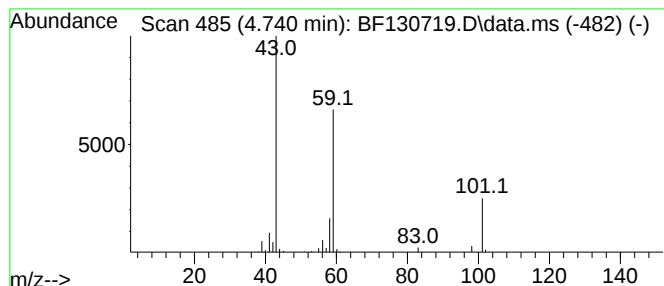

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101922\
Data File : BF130719.D
Acq On : 19 Oct 2022 19:30
Operator : CG\JU
Sample : N5176-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
5236-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.740	5.7	ng	133039	1	6.569	464965	20.0