

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101922\
 Data File : BF130720.D
 Acq On : 19 Oct 2022 20:01
 Operator : CG\JU
 Sample : N5176-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 5236-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130720.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.740	481	485	502	rBV	119641	158782	5.05%	1.055%
2	5.175	556	559	579	rBV	1120559	1334083	42.41%	8.866%
3	6.222	735	737	761	rBV	562662	641859	20.40%	4.266%
4	6.569	792	796	808	rVB	514369	472079	15.01%	3.137%
5	7.145	889	894	908	rBV	1417436	1595846	50.73%	10.606%
6	7.851	1010	1014	1030	rVB	713040	657843	20.91%	4.372%
7	8.928	1192	1197	1200	rBV	3315208	3145662	100.00%	20.906%
8	9.598	1307	1311	1321	rVB	916436	765610	24.34%	5.088%
9	10.392	1441	1446	1463	rBV	1962313	1961355	62.35%	13.035%
10	11.080	1559	1563	1571	rBV	806351	782316	24.87%	5.199%
11	12.663	1827	1832	1835	rBV	2954907	2526258	80.31%	16.789%
12	13.710	2006	2010	2018	rVB	618273	560699	17.82%	3.726%
13	15.086	2240	2244	2255	rBV	371398	444304	14.12%	2.953%




Sum of corrected areas: 15046696

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101922\
Data File : BF130720.D
Acq On : 19 Oct 2022 20:01
Operator : CG\JU
Sample : N5176-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
5236-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

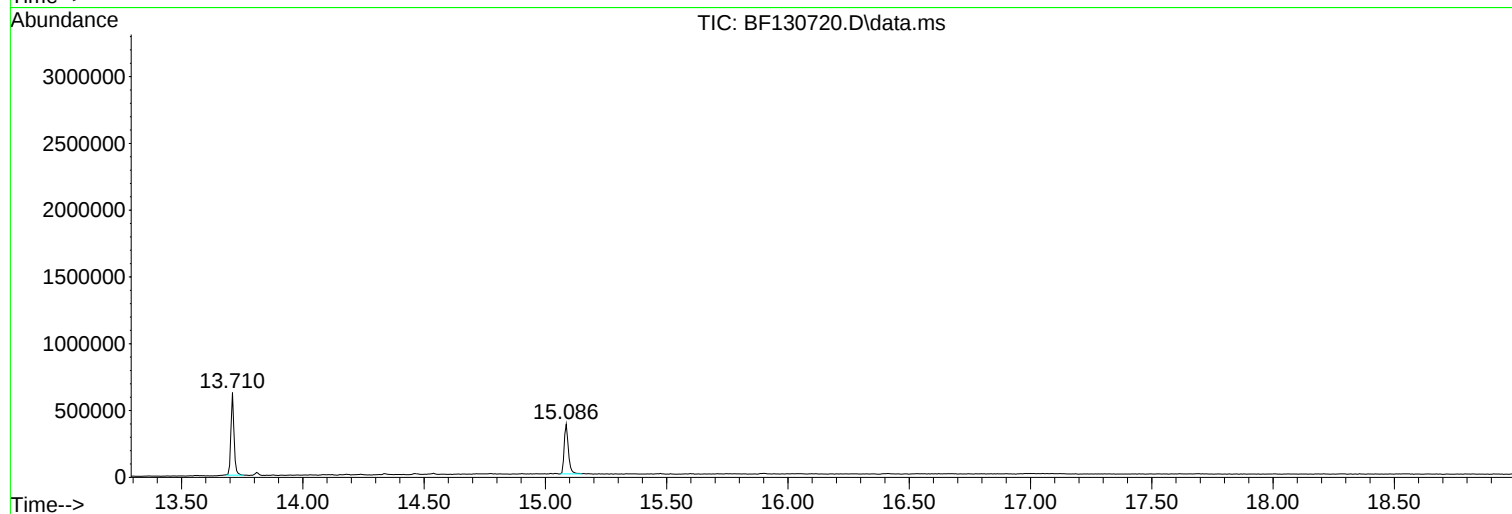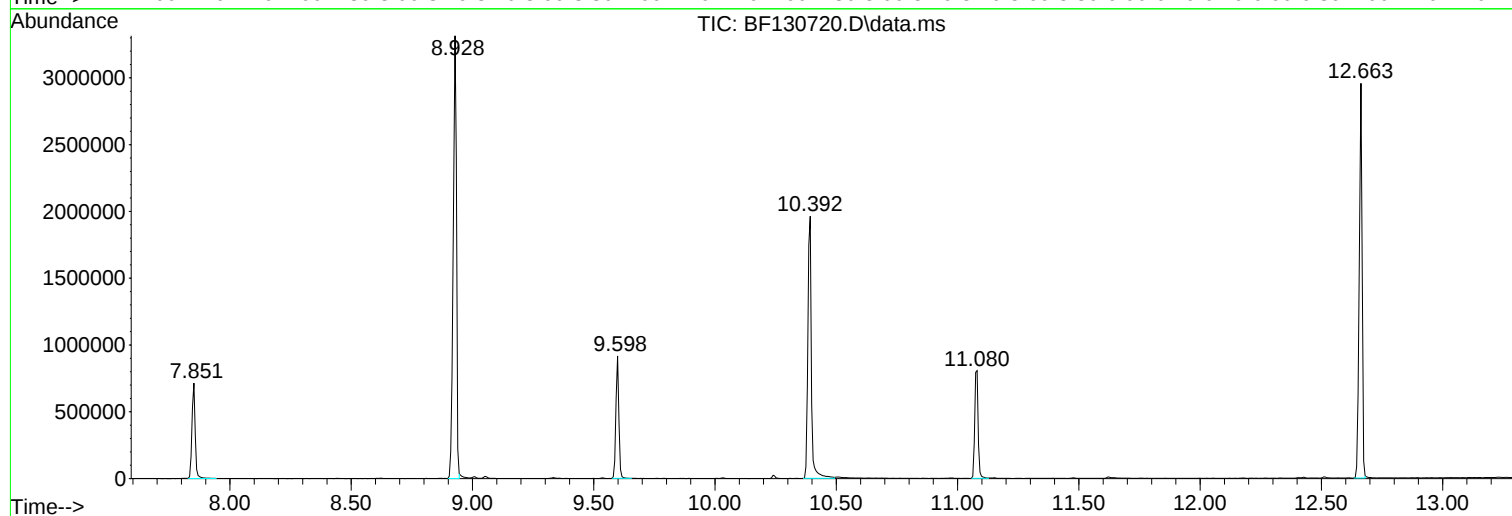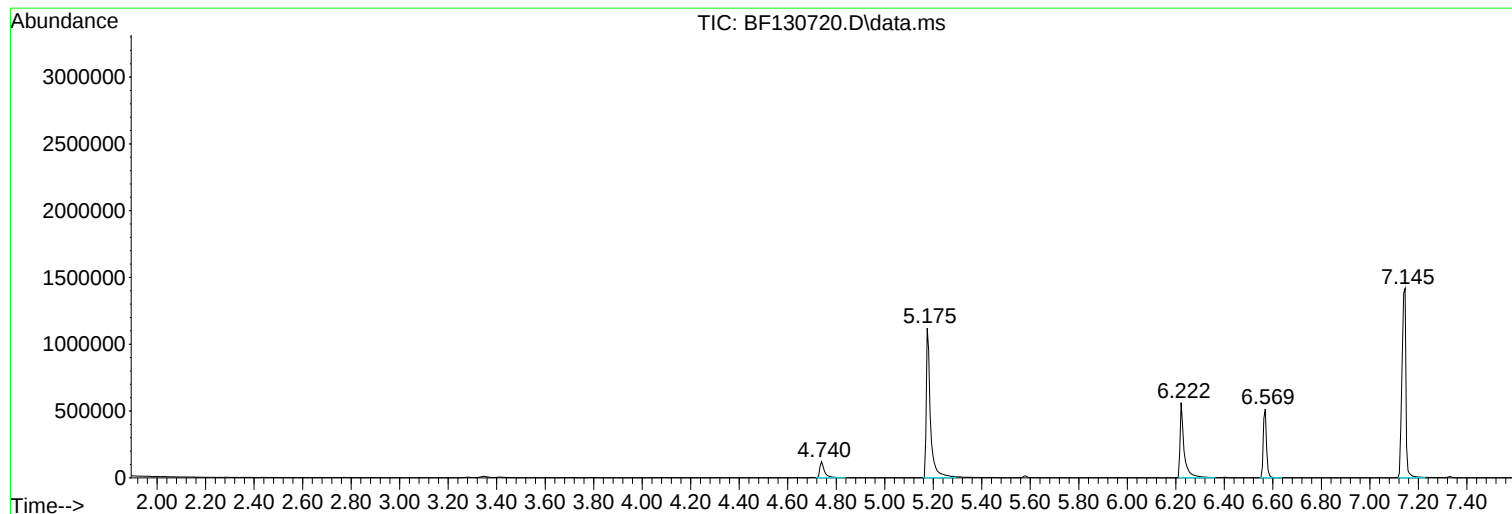

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101922\
Data File : BF130720.D
Acq On : 19 Oct 2022 20:01
Operator : CG\JU
Sample : N5176-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
5236-2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.740	6.73 ng	158782	1,4-Dichlorobenzene-d4	6.569

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25		
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17		
4	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		

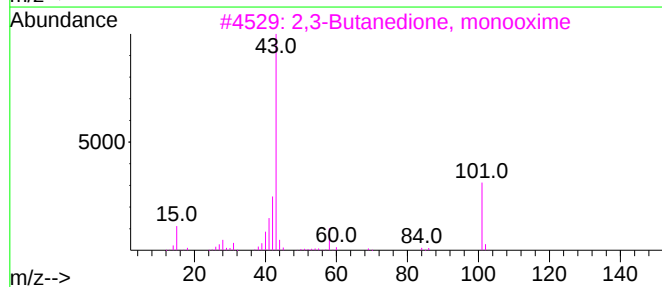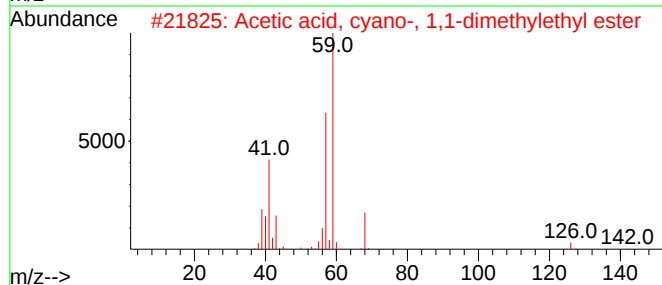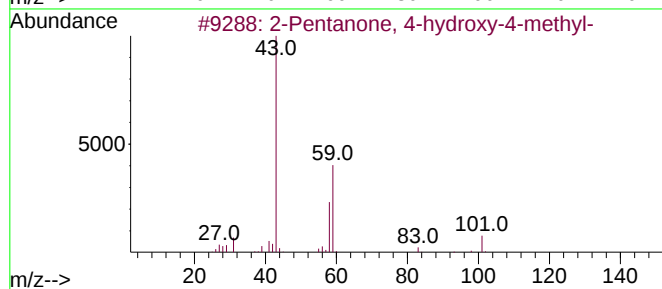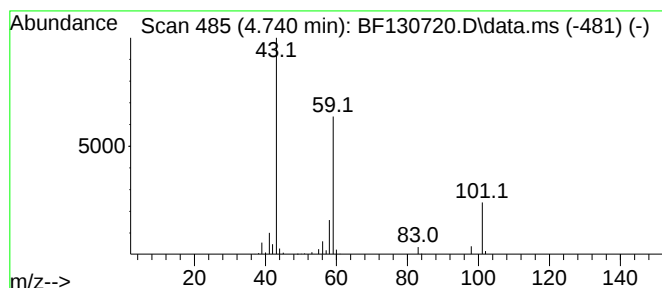

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101922\
Data File : BF130720.D
Acq On : 19 Oct 2022 20:01
Operator : CG\JU
Sample : N5176-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
5236-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.740	6.7	ng	158782	1	6.569	472079	20.0