
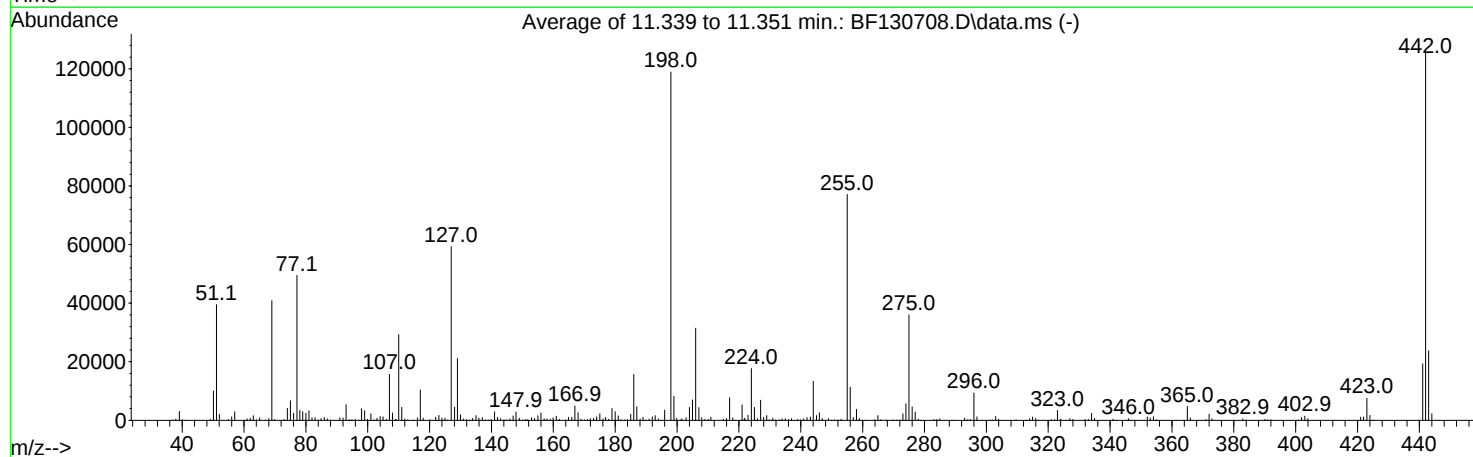


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101922\
 Data File : BF130708.D
 Acq On : 19 Oct 2022 12:05
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 18 03:15:54 2022

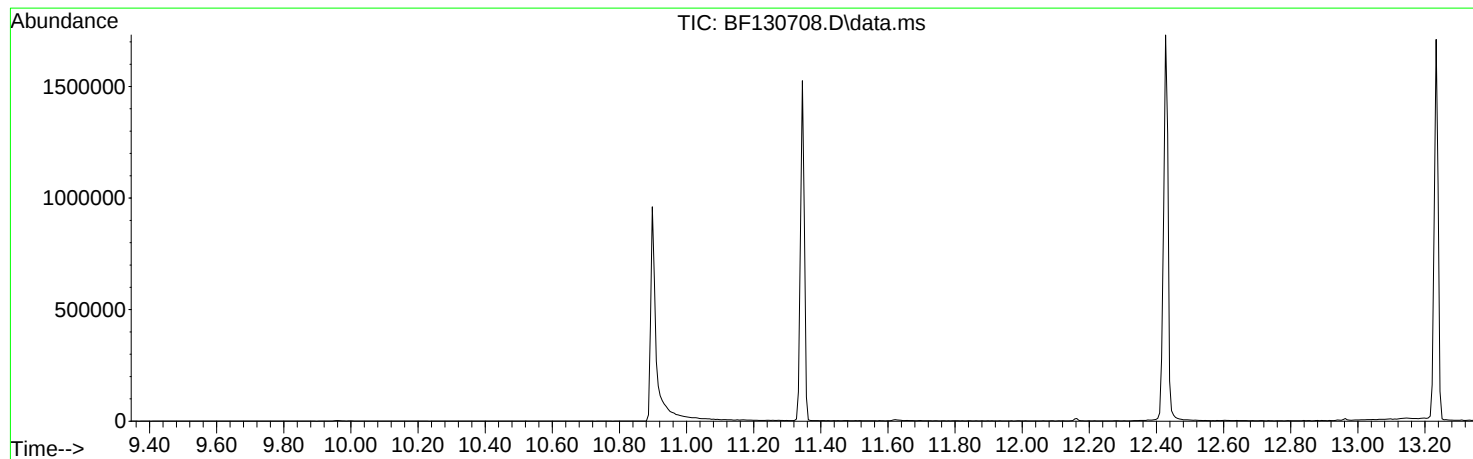




AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	39496	PASS
68	69	0.00	2	1.4	558	PASS
69	198	0.00	100	34.4	40853	PASS
70	69	0.00	2	0.8	315	PASS
127	198	10	80	49.9	59323	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	118915	PASS
199	198	5	9	6.9	8215	PASS
275	198	10	60	30.2	35955	PASS
365	198	1	100	4.0	4726	PASS
441	198	0.01	100	16.2	19267	PASS
442	442	50	100	100.0	125597	PASS
443	442	15	24	18.9	23745	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101922\
 Data File : BF130708.D
 Acq On : 19 Oct 2022 12:05
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 20 04:57:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 18 03:15:54 2022
 Response via : Initial Calibration

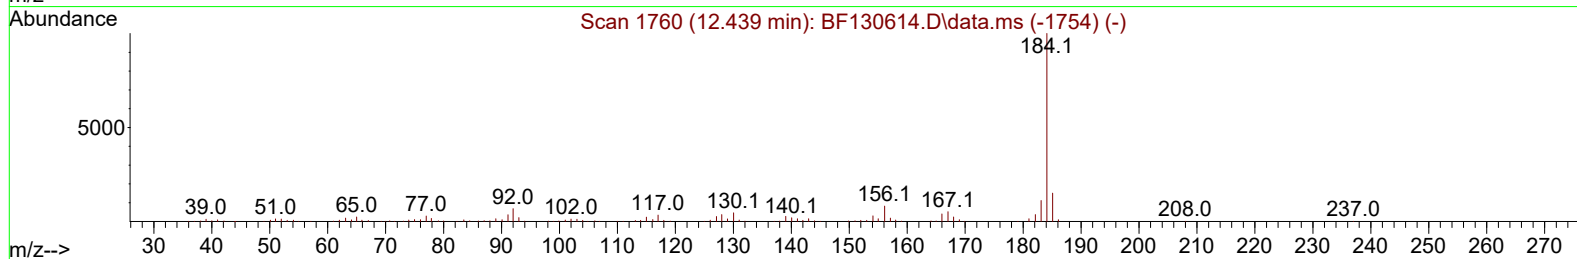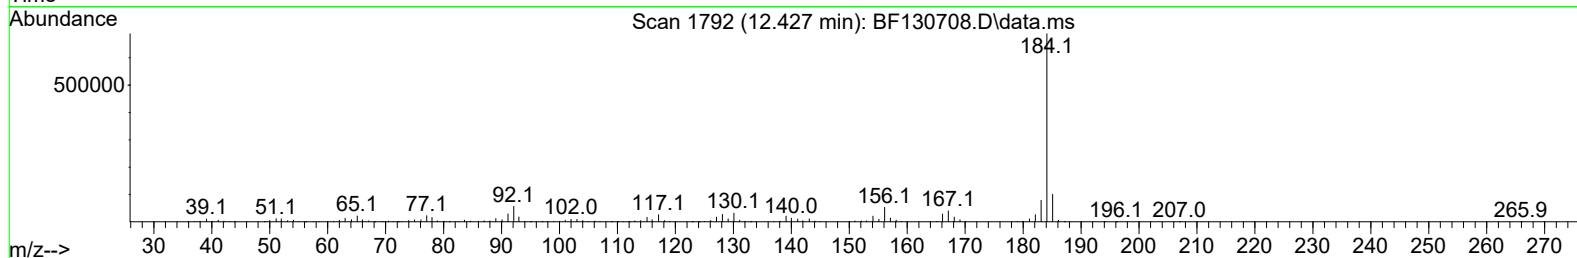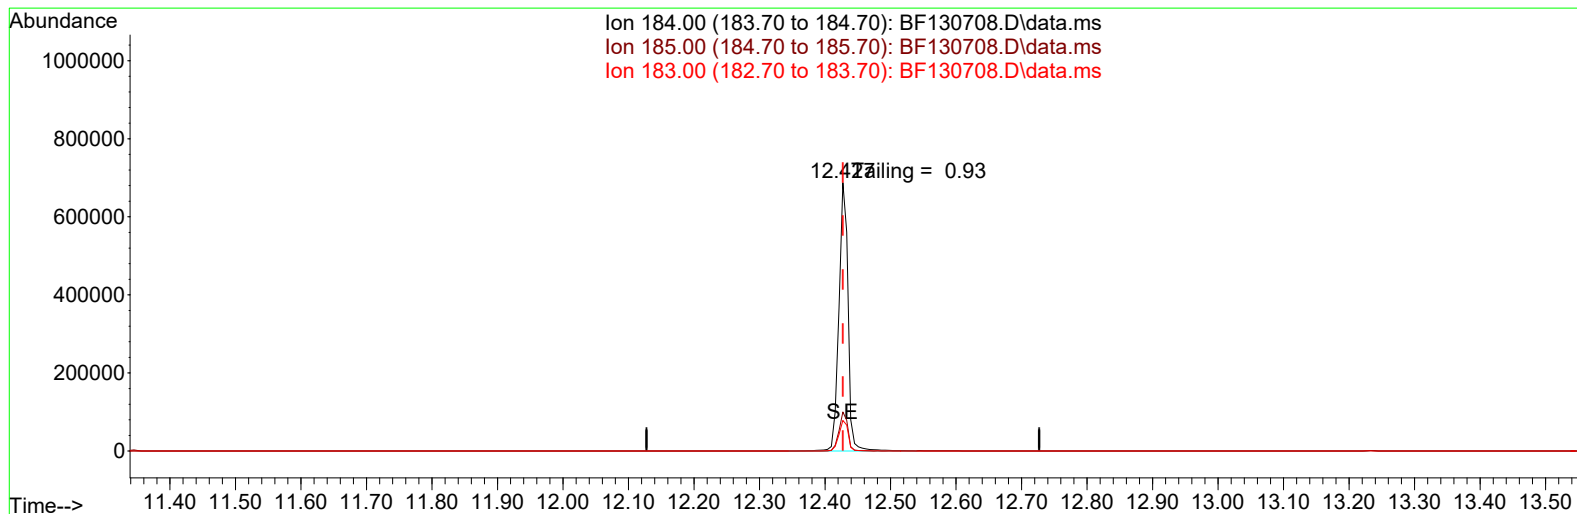

TIC: BF130708.D\data.ms

(77) Benzidine

12.427min (-0.000) 0.00 ng




response 667443

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.56
183.00	11.20	11.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101922\
 Data File : BF130708.D
 Acq On : 19 Oct 2022 12:05
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 20 04:57:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 18 03:15:54 2022
 Response via : Initial Calibration

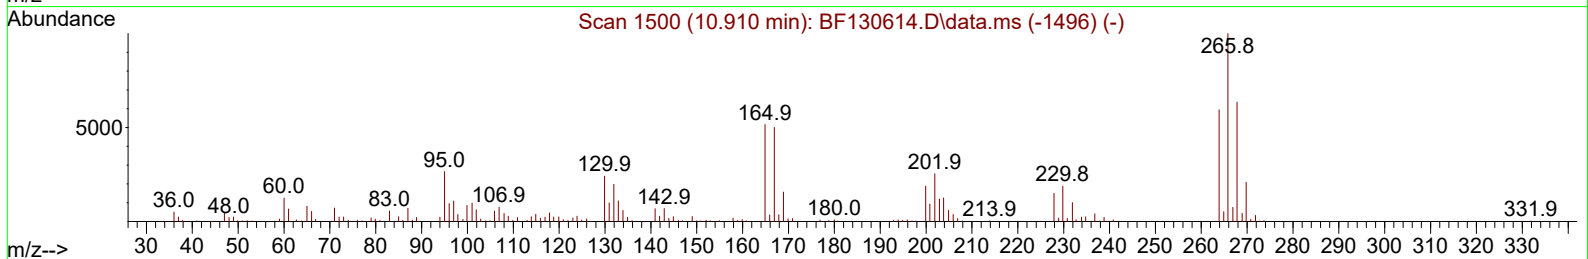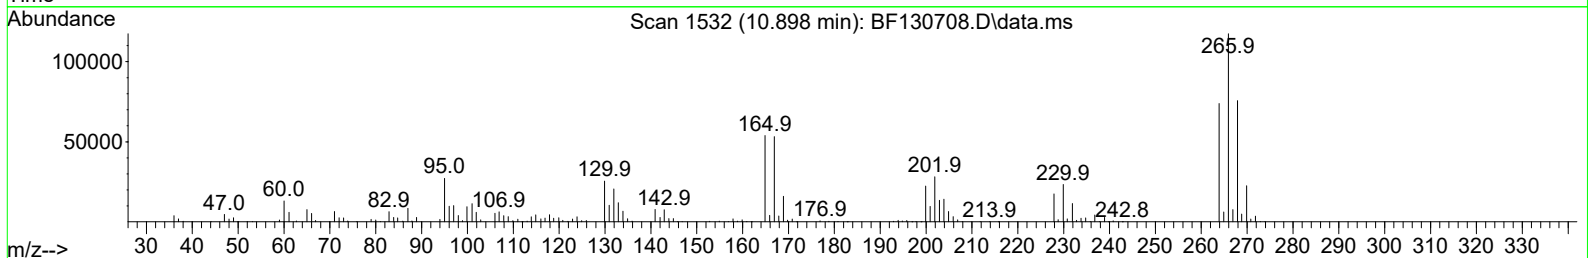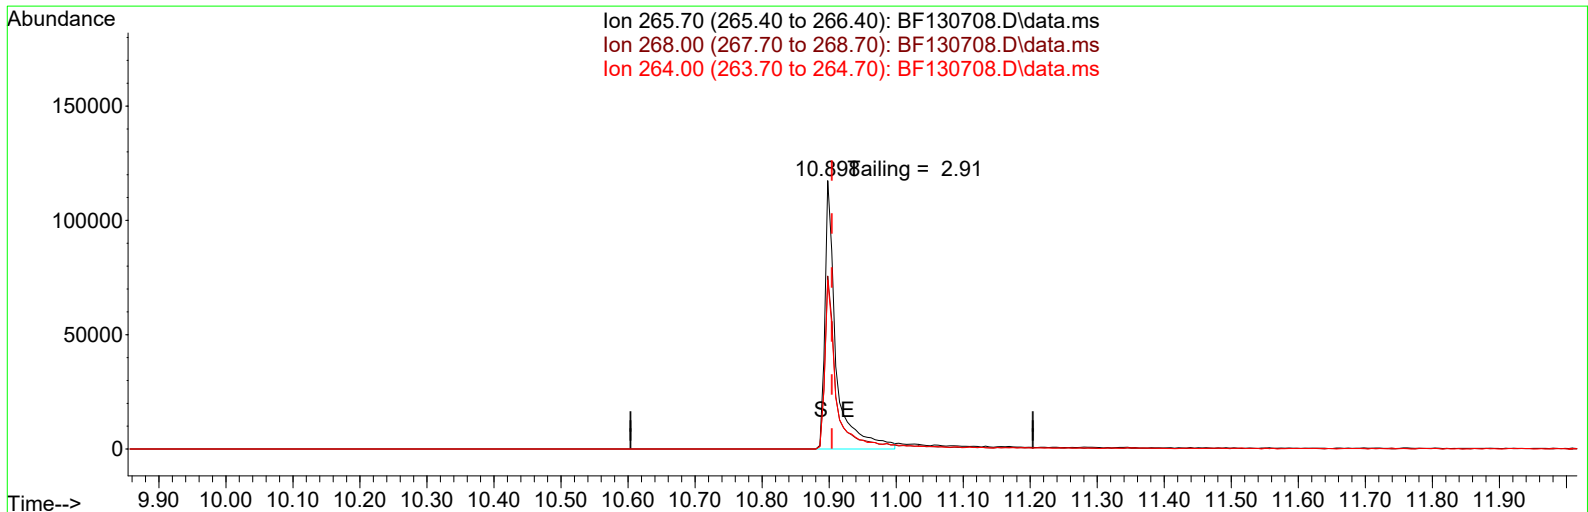

TIC: BF130708.D\data.ms

(70) Pentachlorophenol (C)

10.898min (-0.006) 58275.80 ng

response 139540

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	64.48
264.00	59.40	62.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/19/2022	BNA_F	<u>BF130708.D</u>
Compound Name	Response	Retention Time
DDT	275162	13.233
DDD	2769	12.963
DDE	783	12.604
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3552	278714	1.27

Instrument :
BNA_F
ClientSampleId :
DFTPP