
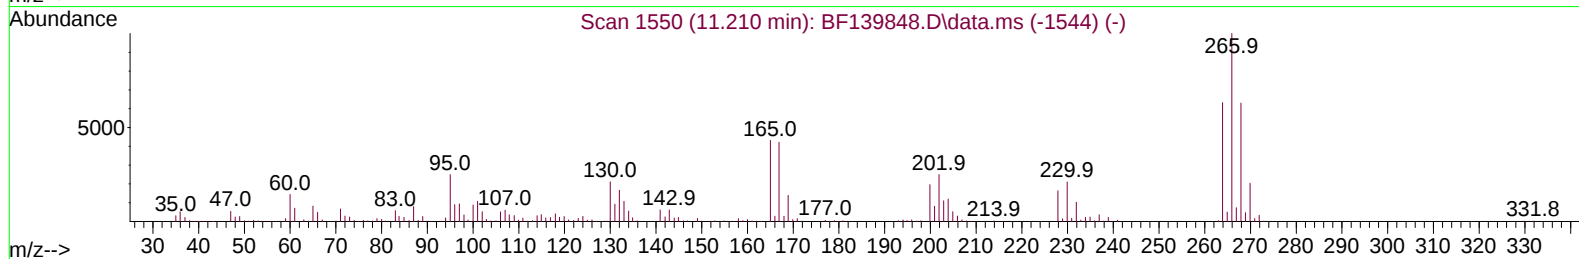
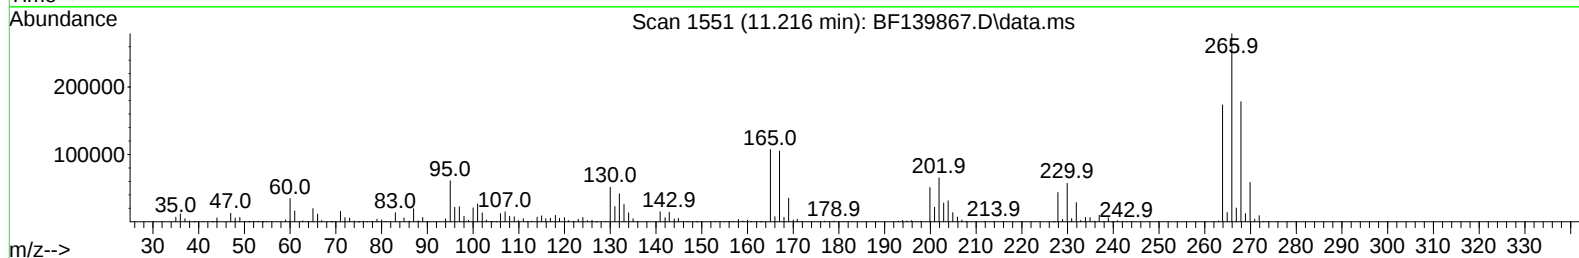


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101924\
Data File : BF139867.D
Acq On : 19 Oct 2024 12:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 21 05:30:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

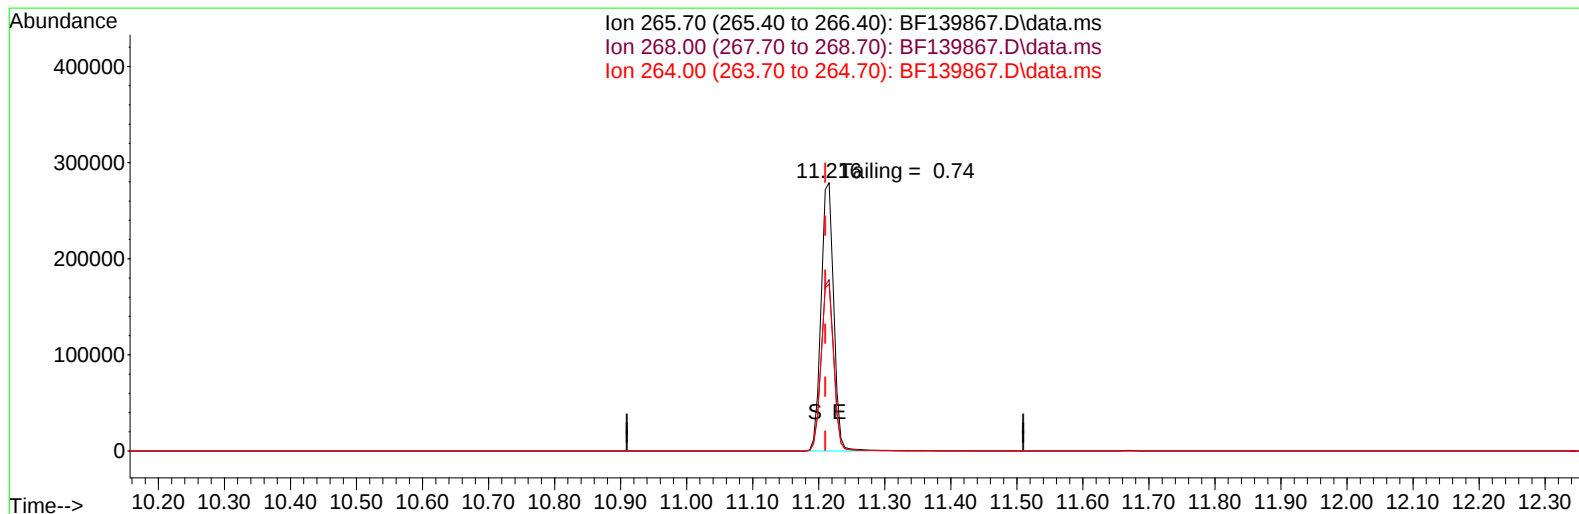

TIC: BF139867.D\data.ms

(70) Pentachlorophenol (C)




11.216min (+ 0.006) 59090.39 ng

response 372710

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.85
264.00	63.20	62.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101924\
 Data File : BF139867.D
 Acq On : 19 Oct 2024 12:51
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 21 05:30:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 18 15:07:50 2024
 Response via : Initial Calibration

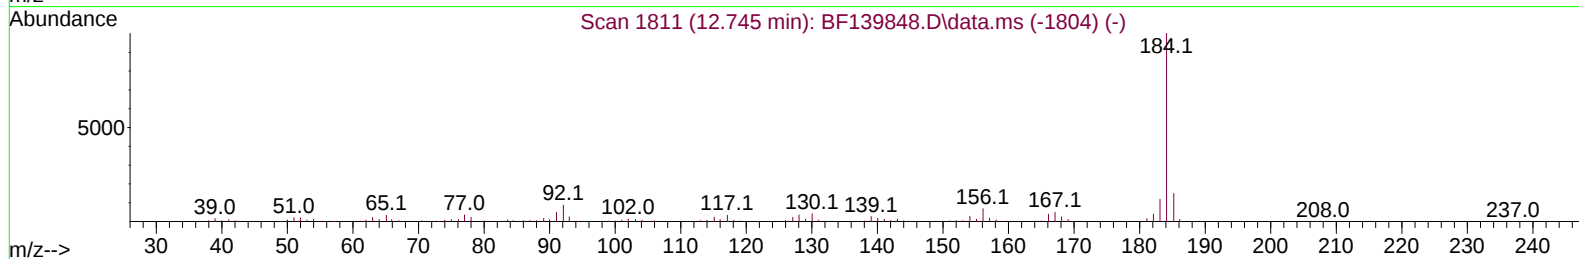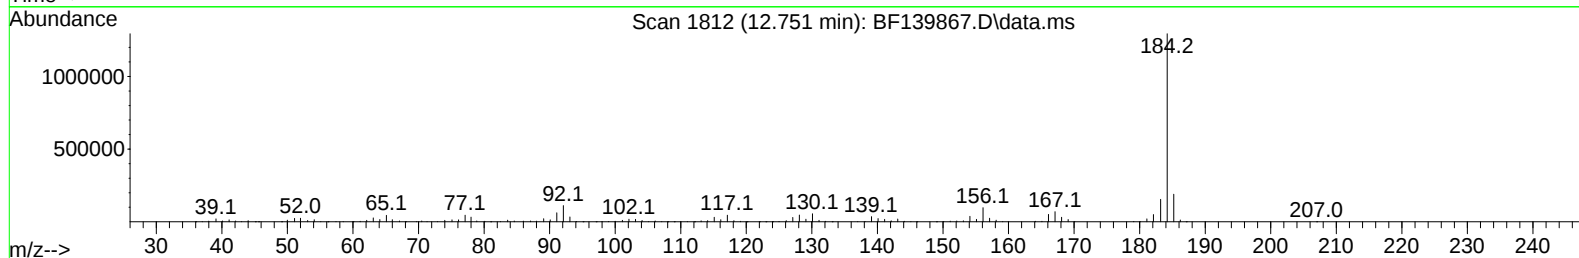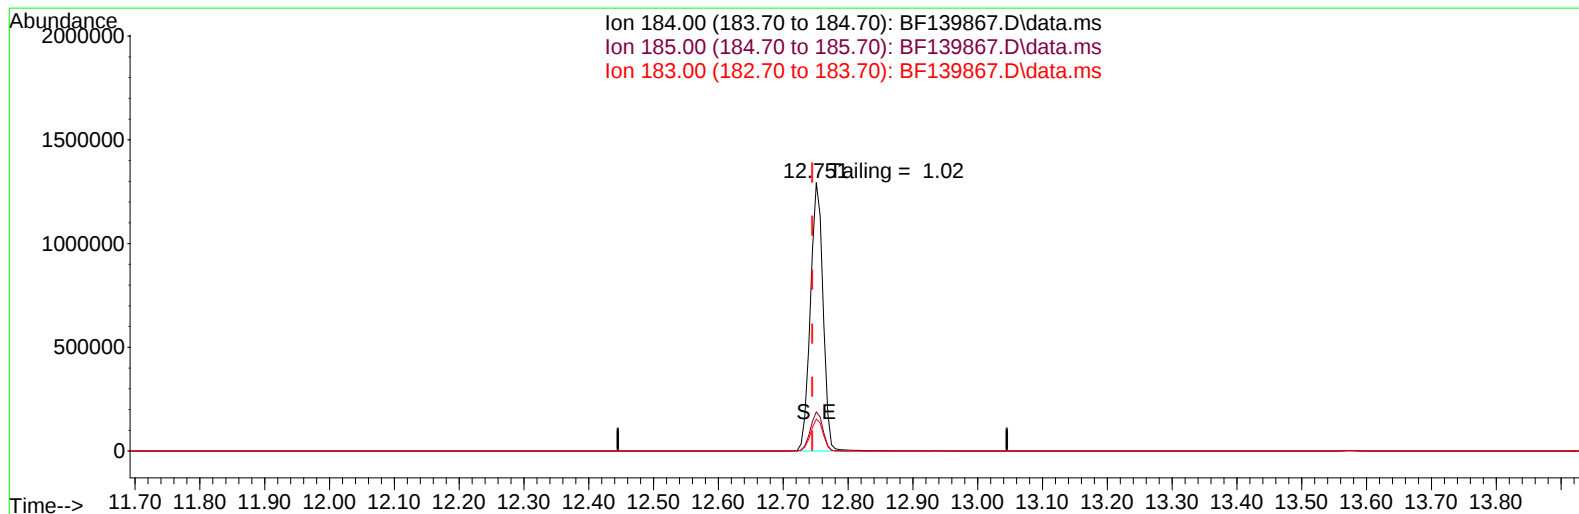

TIC: BF139867.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 68596.81 ng

response 1755113

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.63
183.00	11.80	11.94
0.00	0.00	0.00