
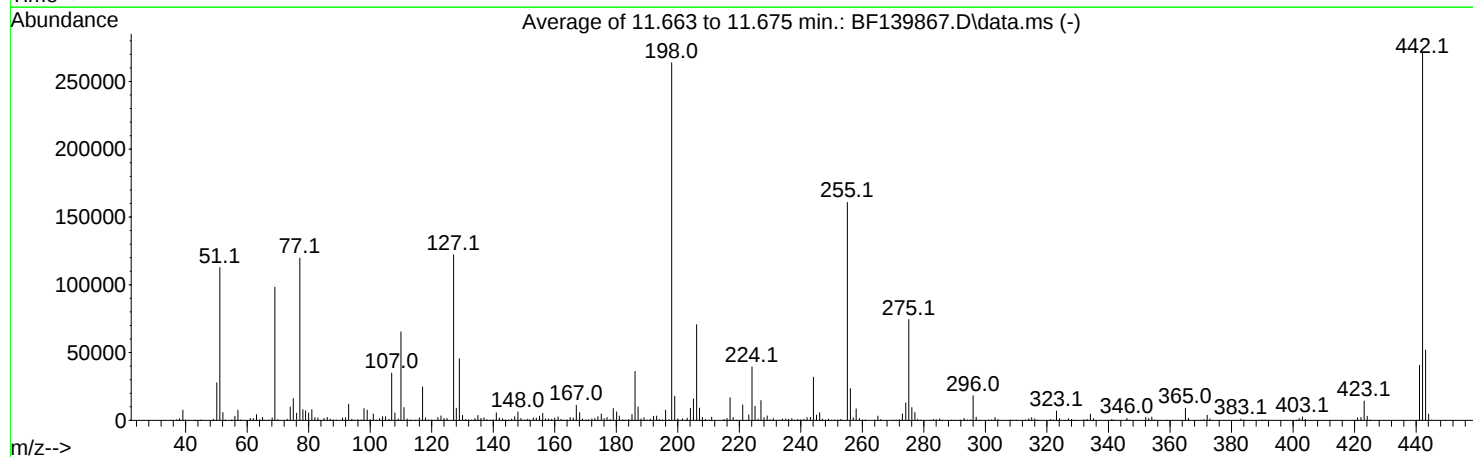


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101924\
Data File : BF139867.D
Acq On : 19 Oct 2024 12:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 18 15:07:50 2024

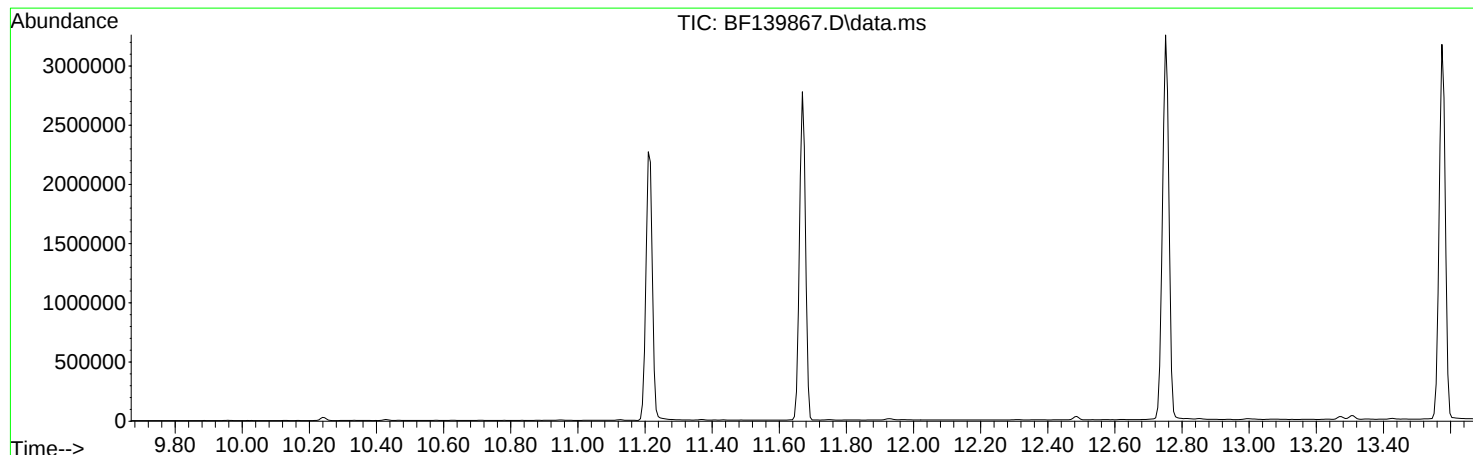




AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	112659	PASS
68	69	0.00	2	1.8	1784	PASS
69	198	0.00	100	37.3	98373	PASS
70	69	0.00	2	0.6	551	PASS
127	198	10	80	46.3	122115	PASS
197	198	0.00	2	0.2	540	PASS
198	198	100	100	100.0	263765	PASS
199	198	5	9	6.8	17875	PASS
275	198	10	60	28.2	74413	PASS
365	198	1	100	3.4	9034	PASS
441	198	0.01	100	15.4	40661	PASS
442	442	50	100	100.0	271339	PASS
443	442	15	24	19.1	51861	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101924\
Data File : BF139867.D
Acq On : 19 Oct 2024 12:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 21 05:30:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

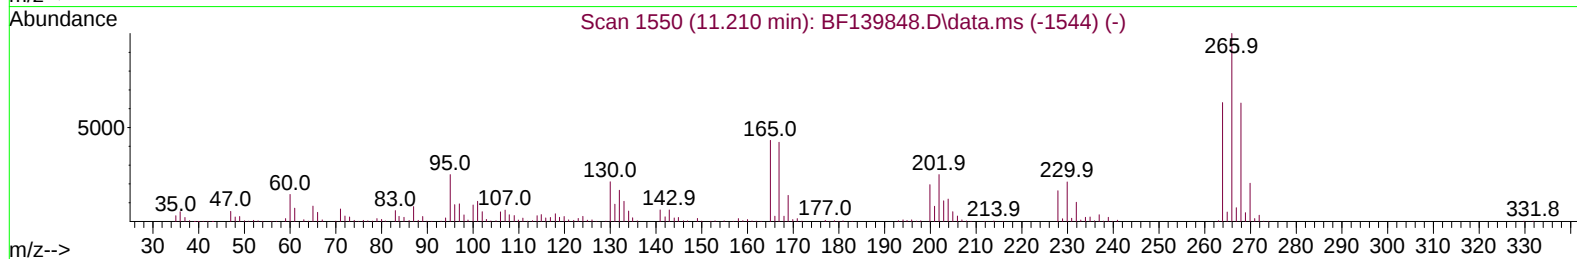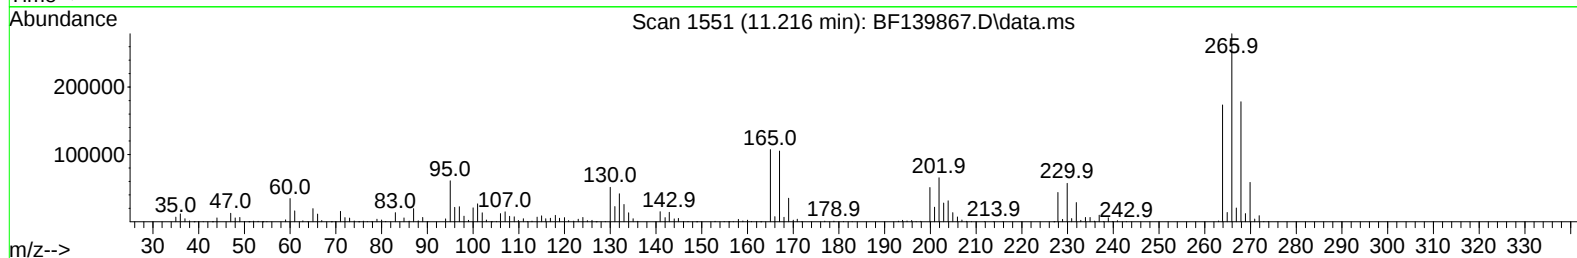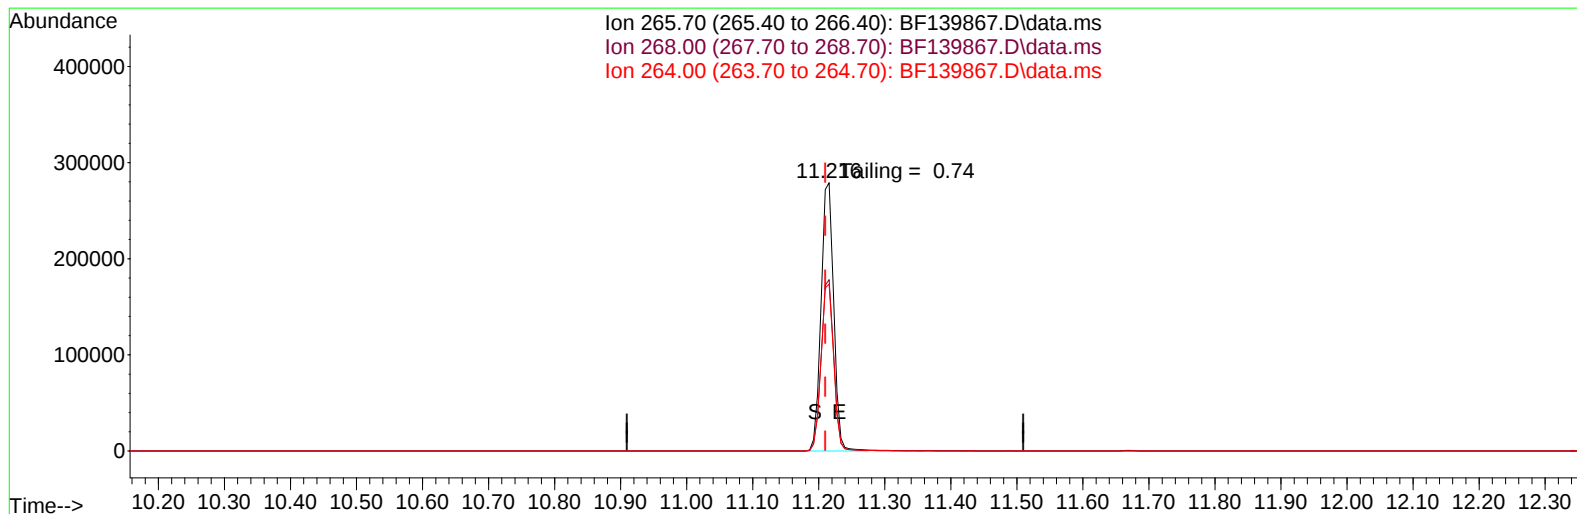

TIC: BF139867.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 59090.39 ng




response 372710

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.85
264.00	63.20	62.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101924\
 Data File : BF139867.D
 Acq On : 19 Oct 2024 12:51
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 21 05:30:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 18 15:07:50 2024
 Response via : Initial Calibration

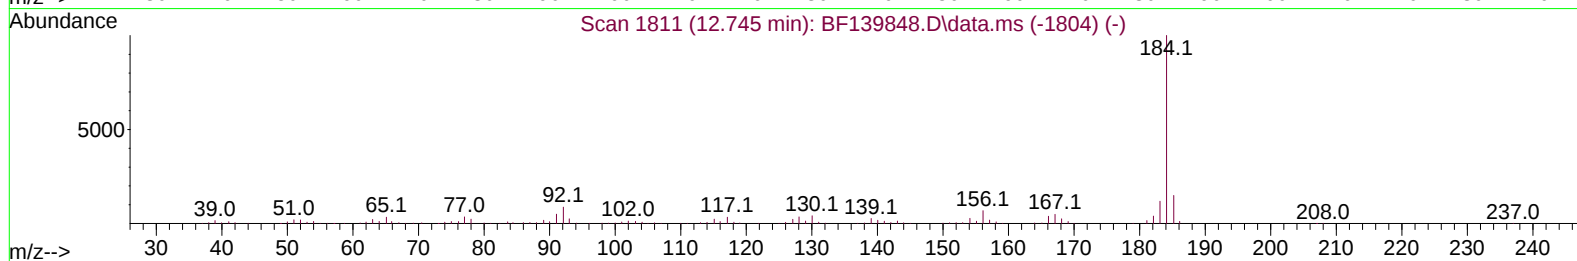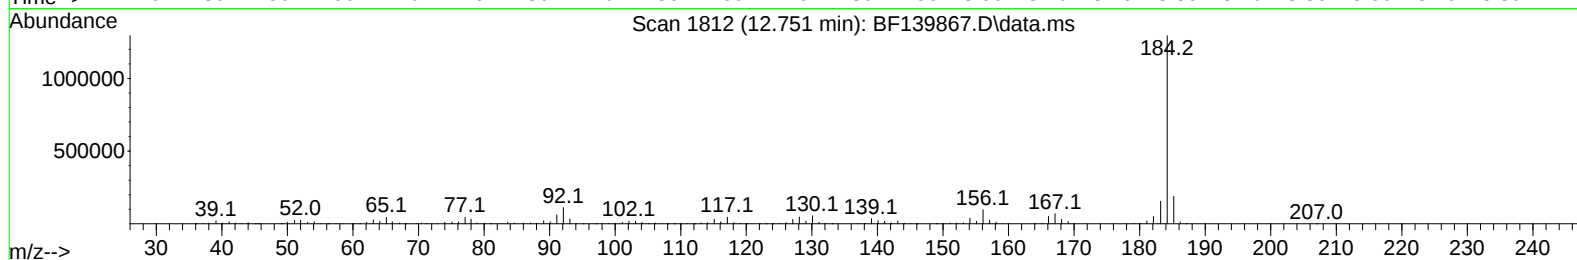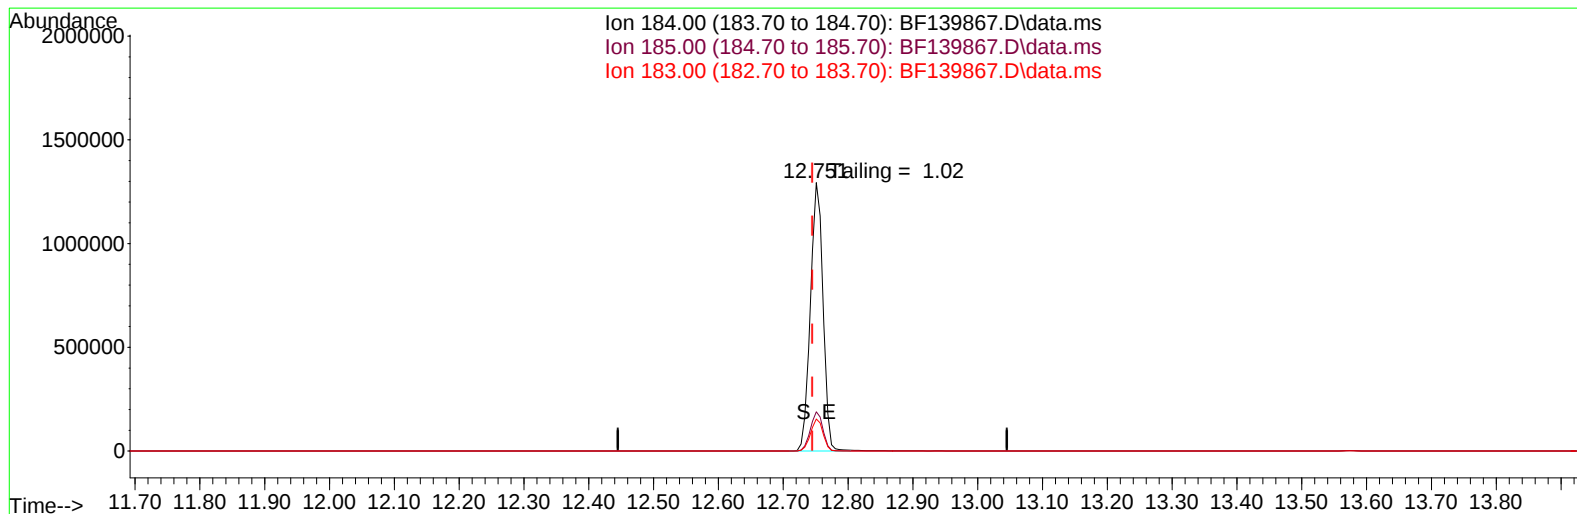

TIC: BF139867.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 68596.81 ng

response 1755113

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.63
183.00	11.80	11.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/19/2024	BNA_F	<u>BF139867.D</u>
Compound Name	Response	Retention Time
DDT	795748	13.574
DDD	13557	13.31
DDE	235	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13792	809540	1.70

Instrument :
BNA_F
ClientSampleId :
DFTPP