
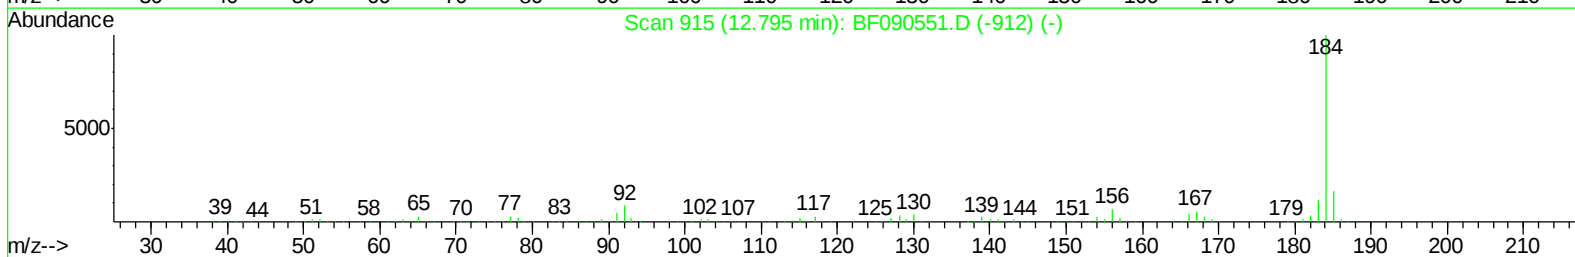
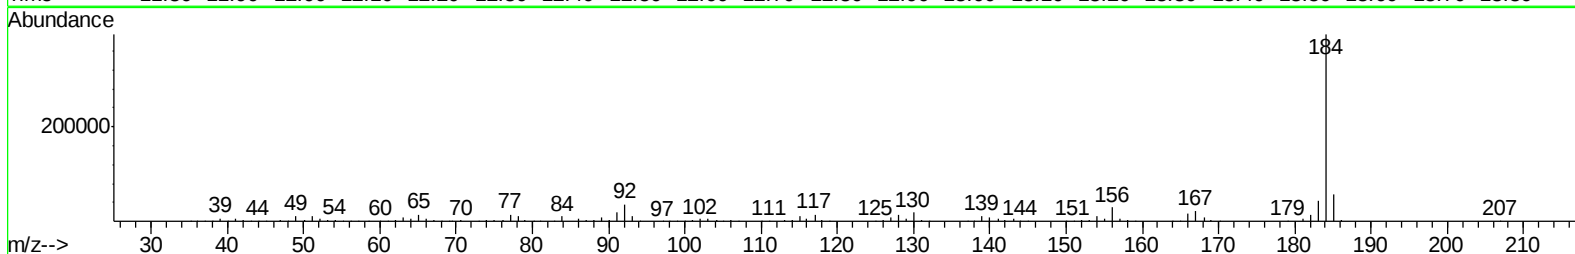


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102016\
Data File : BF090677.D
Acq On : 20 Oct 2016 12:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 20 19:15:33 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 20 18:12:00 2016
Response via : Initial Calibration

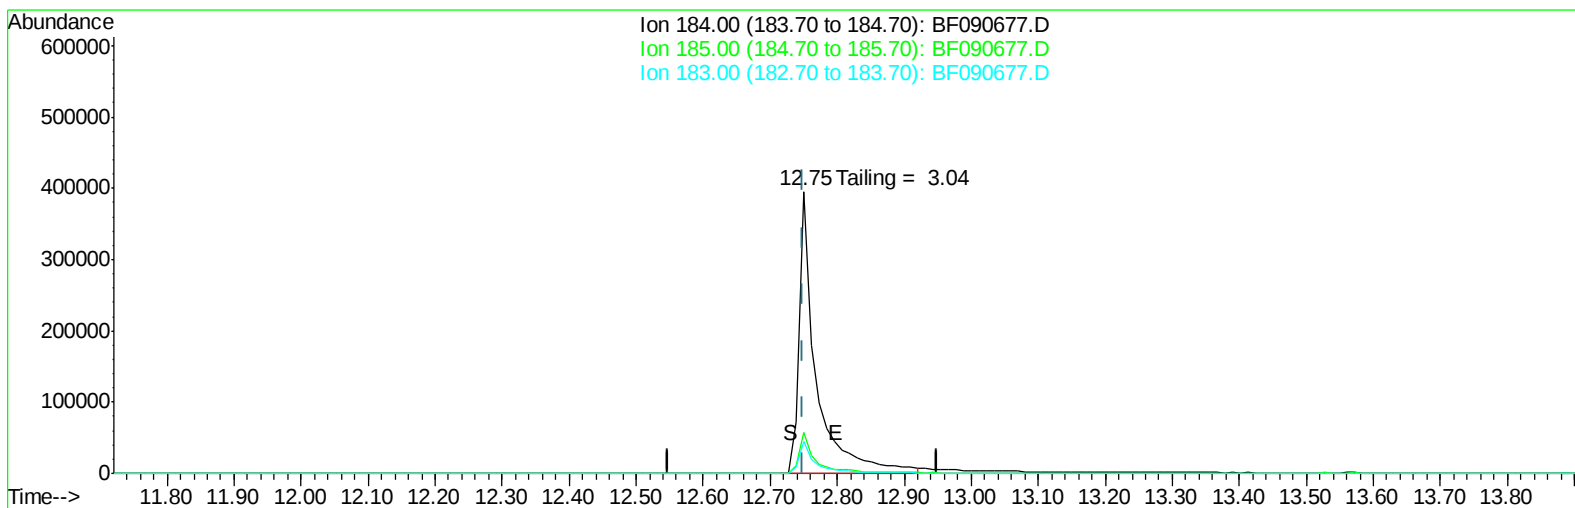

TIC: BF090677.D

(76) Benzidine

12.749min (-0.000) 0.00ng

response 700345

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.65
183.00	11.70	11.26
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102016\
 Data File : BF090677.D
 Acq On : 20 Oct 2016 12:03
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 20 19:15:33 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 20 18:12:00 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ng	-6.89
21) Naphthalene-d8	0.00	136	0	0.00	ng	-8.17
38) Acenaphthene-d10	0.00	164	0	0.00	ng	-9.93
63) Phenanthrene-d10	0.00	188	0	0.00	ng	-11.41
75) Chrysene-d12	0.00	240	0	0.00	ng	-14.05
86) Perylene-d12	0.00	264	0	0.00	ng	-15.50
System Monitoring Compounds						
5) 2-Fluorophenol	0.00	112	0	0.00	ng	
7) Phenol-d6	0.00	99	0	0.00	ng	
23) Nitrobenzene-d5	0.00	82	0	0.00	ng	
41) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng	
44) 2-Fluorobiphenyl	0.00	172	0	0.00	ng	
78) Terphenyl-d14	12.99	244	540	0.00	ng	-0.01

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102016\
Data File : BF090677.D
Acq On : 20 Oct 2016 12:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 20 19:15:33 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 20 18:12:00 2016
Response via : Initial Calibration

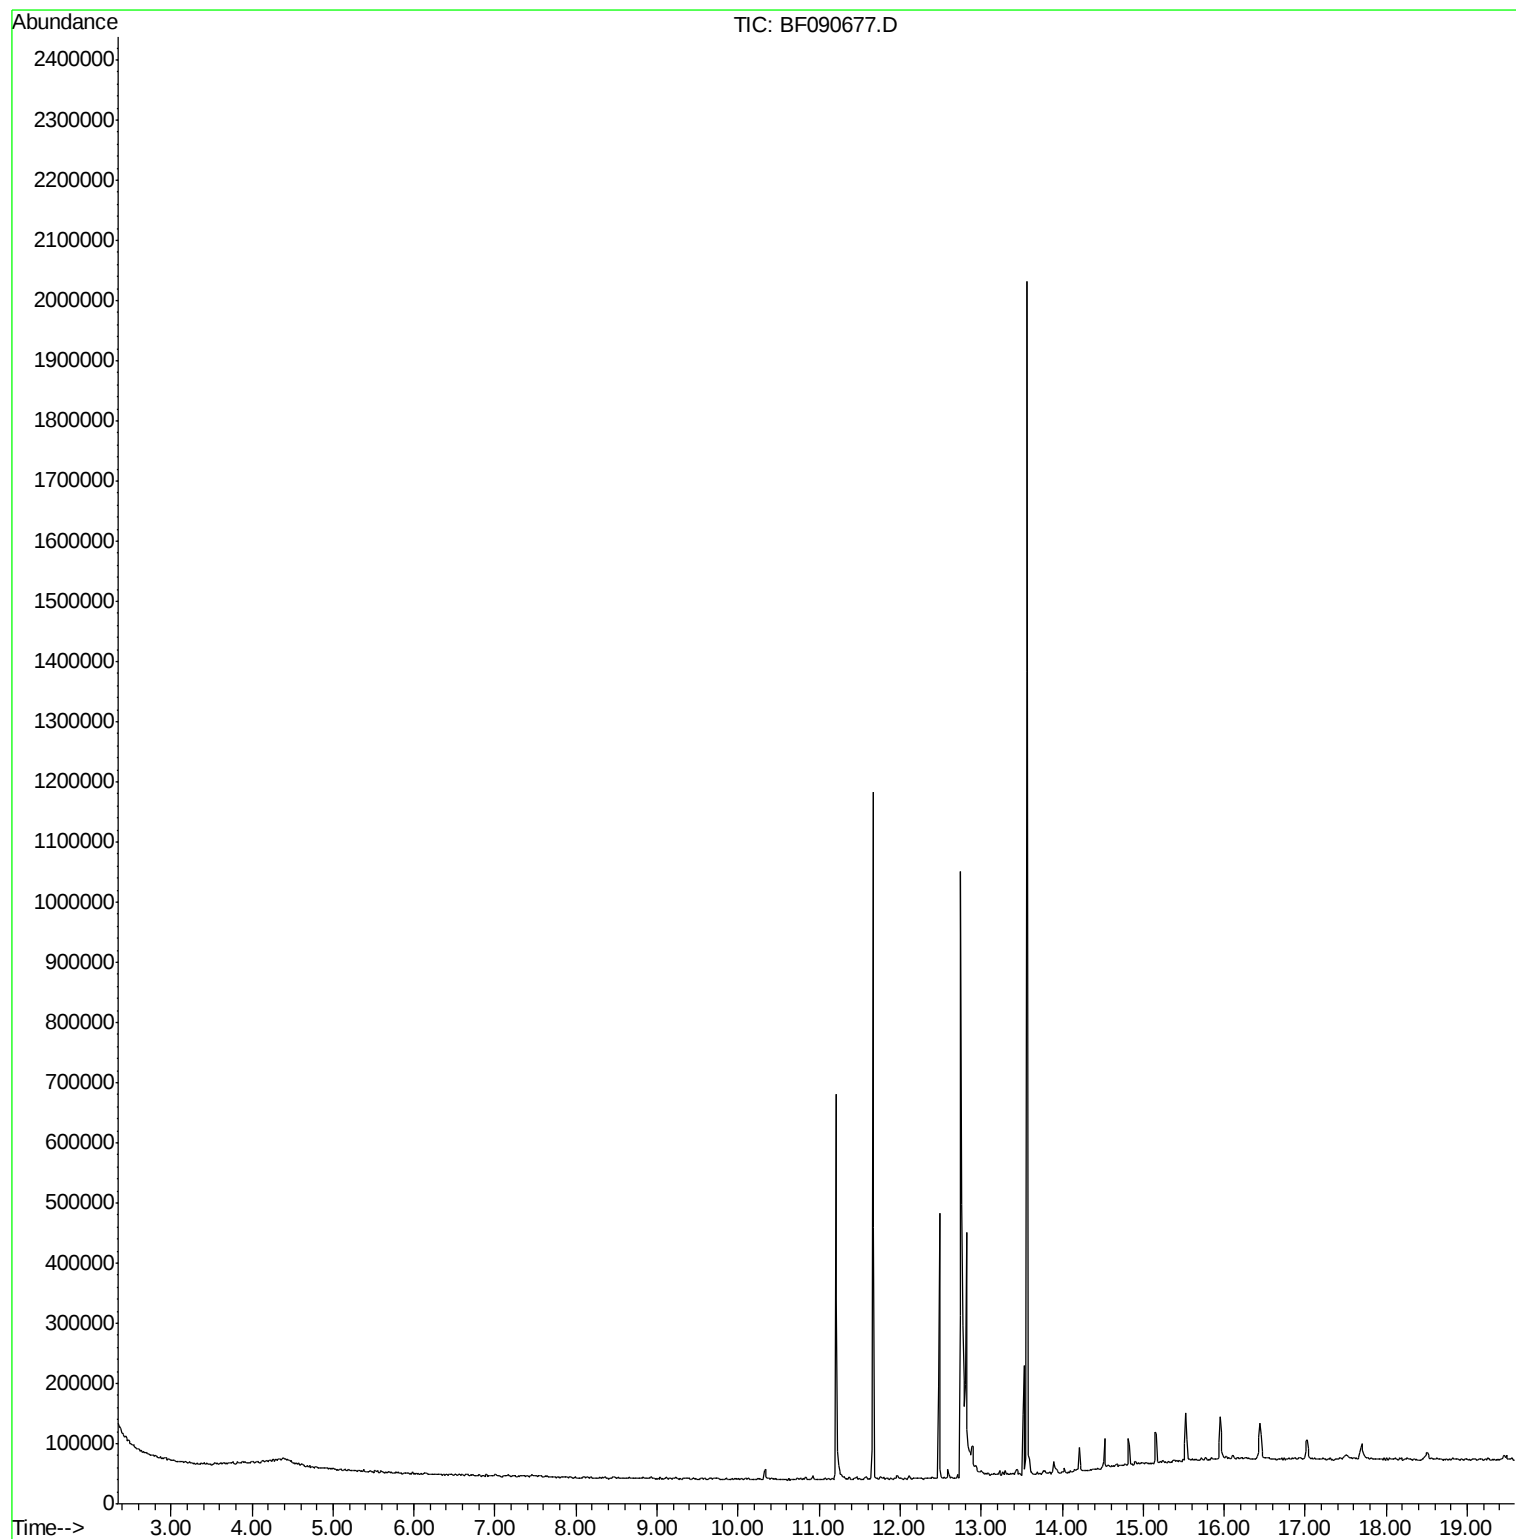

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102016\
Data File : BF090677.D
Acq On : 20 Oct 2016 12:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 20 19:15:33 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 20 18:12:00 2016
Response via : Initial Calibration

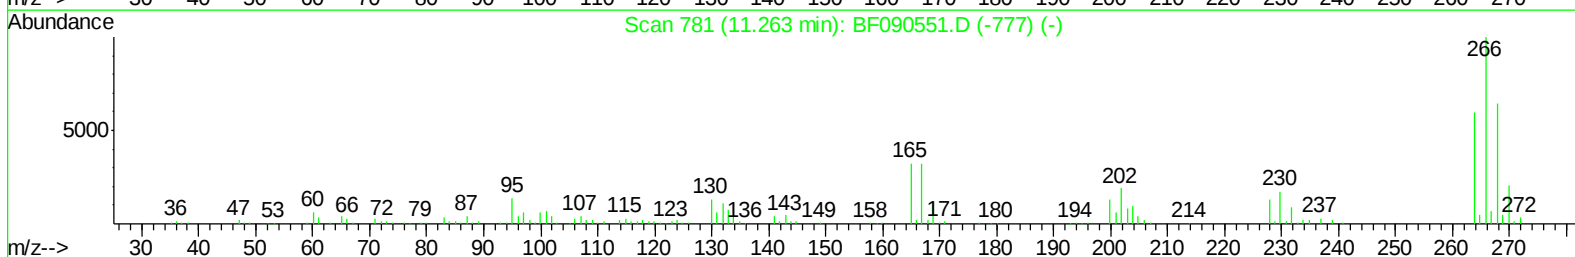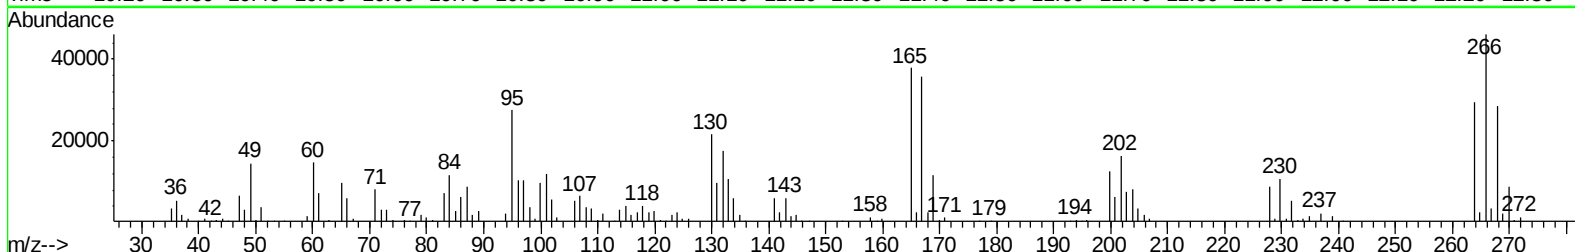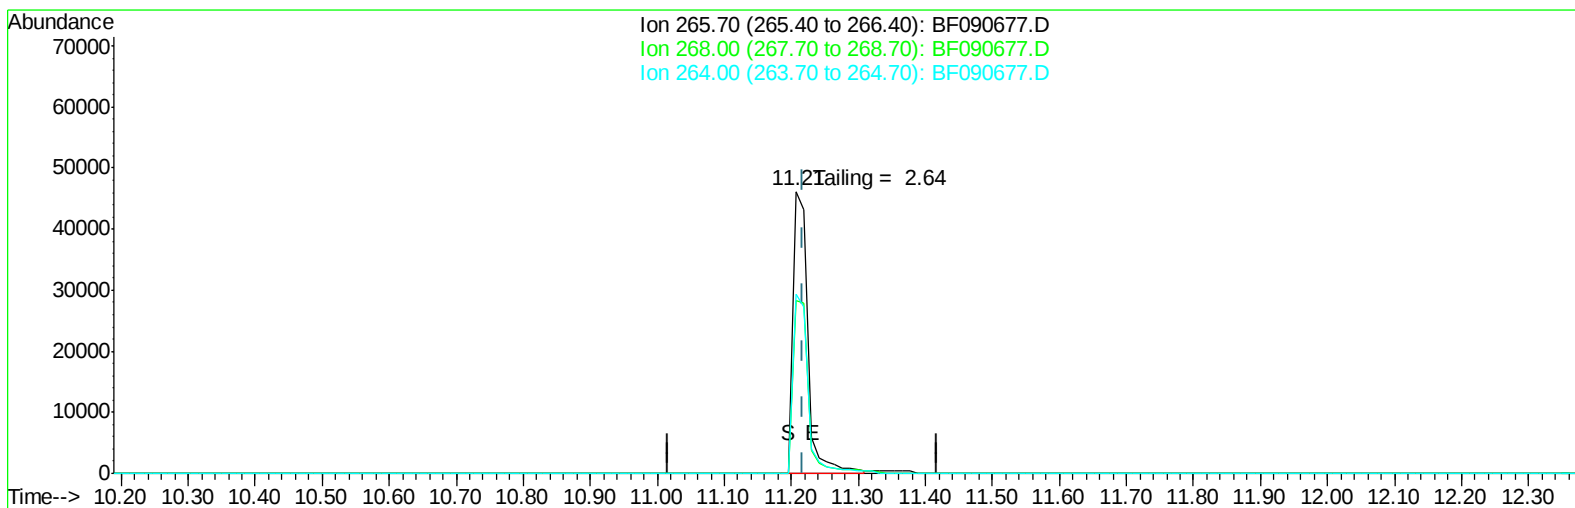

TIC: BF090677.D

(69) Pentachlorophenol (C)




11.206min (-0.011) 0.00ng

response 72922

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	61.60
264.00	59.90	63.87
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102016\
Data File : BF090677.D
Acq On : 20 Oct 2016 12:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 20 19:15:33 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 20 18:12:00 2016
Response via : Initial Calibration

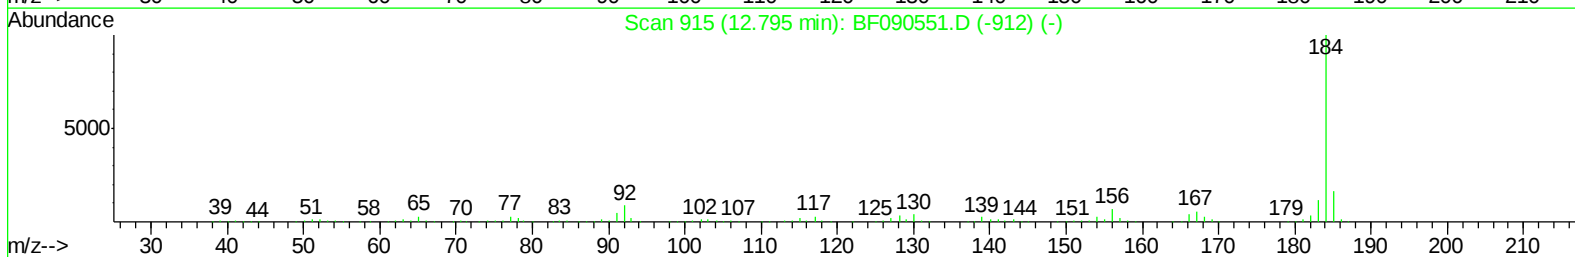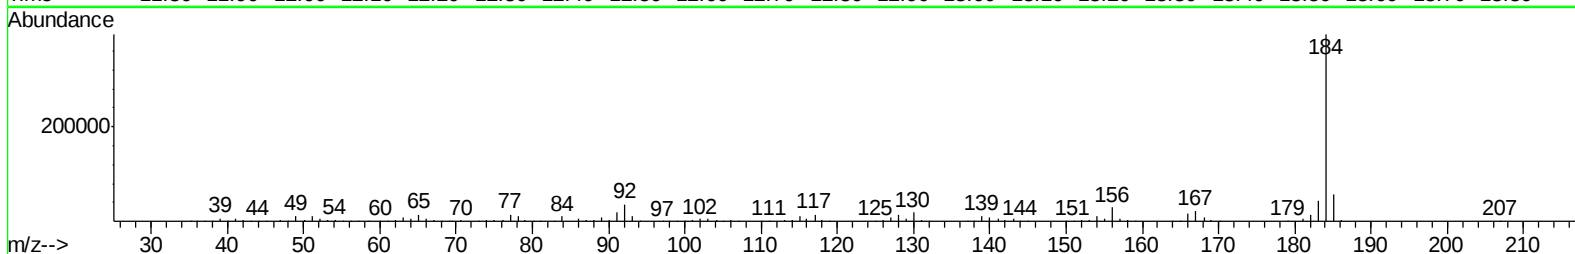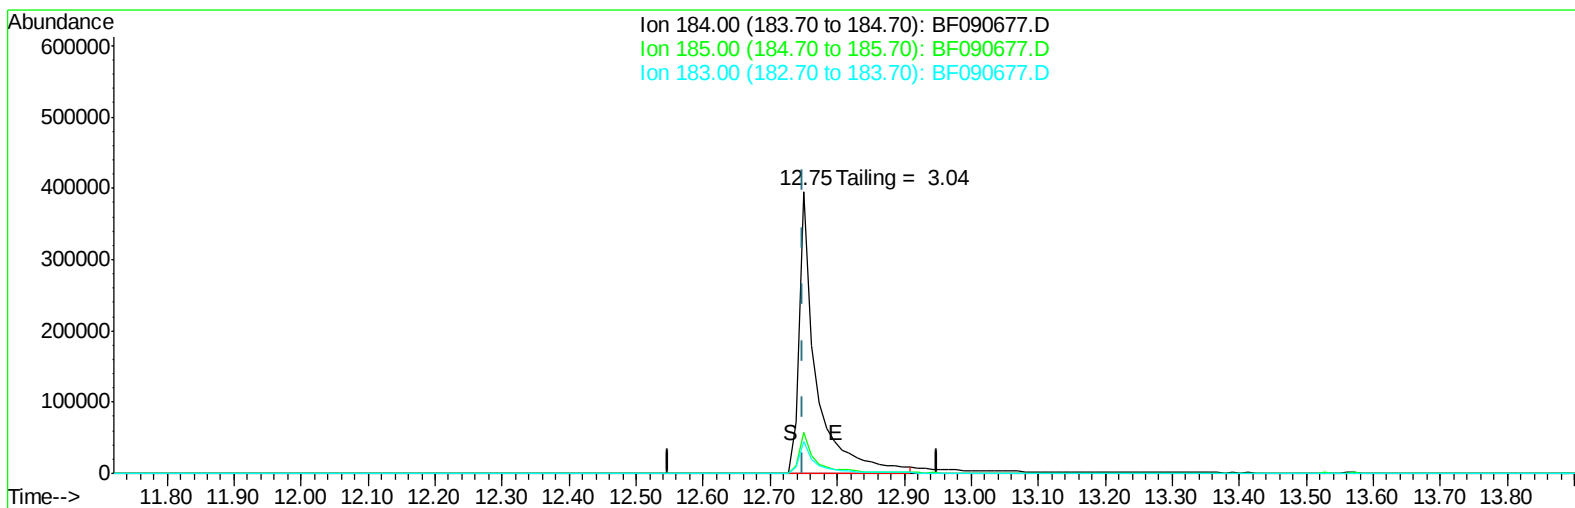

TIC: BF090677.D

(76) Benzidine

12.749min (-0.000) 0.00ng

response 700345

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.65
183.00	11.70	11.26
0.00	0.00	0.00