

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102016\
 Data File : BF090685.D
 Acq On : 20 Oct 2016 16:36
 Operator : UM/SJ
 Sample : H5315-04 2X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FO-TANK-SIDEWALL-SOUTH

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.046	233	237	246	rBV	530477	658013	20.30%	1.918%
2	5.480	271	275	292	rBV	2181793	2826701	87.19%	8.239%
3	6.509	359	365	374	rBV	2678160	2935085	90.53%	8.555%
4	6.646	374	377	394	rVV	3176155	3242187	100.00%	9.450%
5	6.874	395	397	408	rVV	1270474	1542971	47.59%	4.497%
6	7.034	408	411	431	rVB	2481482	2364600	72.93%	6.892%
7	7.446	441	447	453	rBV	953913	1607933	49.59%	4.687%
8	7.537	453	455	466	rVB	73724	164543	5.08%	0.480%
9	8.166	507	510	519	rBV	2343071	2198506	67.81%	6.408%
10	9.240	601	604	610	rBV	3128143	2739869	84.51%	7.986%
11	9.640	635	639	646	rBV	465986	610629	18.83%	1.780%
12	9.926	660	664	671	rBV	1441749	2172221	67.00%	6.331%
13	10.326	697	699	706	rBV3	48309	107885	3.33%	0.314%
14	10.703	729	732	739	rBV2	1135294	1325752	40.89%	3.864%
15	10.829	740	743	747	rVB2	97948	153196	4.73%	0.447%
16	10.920	747	751	753	rBV2	52729	112329	3.46%	0.327%
17	11.126	766	769	777	rVB3	38791	128980	3.98%	0.376%
18	11.275	779	782	788	rVB	83819	139295	4.30%	0.406%
19	11.401	791	793	805	rBV	1110459	1743667	53.78%	5.082%
20	11.629	811	813	817	rBV	189343	336744	10.39%	0.981%
21	12.452	884	885	888	rBV	72023	126421	3.90%	0.368%
22	12.612	896	899	906	rVB	168638	255606	7.88%	0.745%
23	12.818	914	917	928	rBV3	250492	658069	20.30%	1.918%
24	12.989	928	932	937	rBV2	1704145	1858308	57.32%	5.416%
25	13.526	977	979	981	rBV	120100	125703	3.88%	0.366%
26	13.892	1009	1011	1016	rVB	144488	212893	6.57%	0.621%
27	14.052	1021	1025	1030	rBV	1101985	1937921	59.77%	5.648%
28	15.081	1113	1115	1119	rBV	150952	311708	9.61%	0.909%
29	15.492	1149	1151	1156	rVB	837910	1421246	43.84%	4.142%
30	16.612	1246	1249	1255	rVB	128674	290609	8.96%	0.847%


Sum of corrected areas: 34309590

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102016\
Data File : BF090685.D
Acq On : 20 Oct 2016 16:36
Operator : UM/SJ
Sample : H5315-04 2X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FO-TANK-SIDEWALL-SOUTH

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: rteint.p

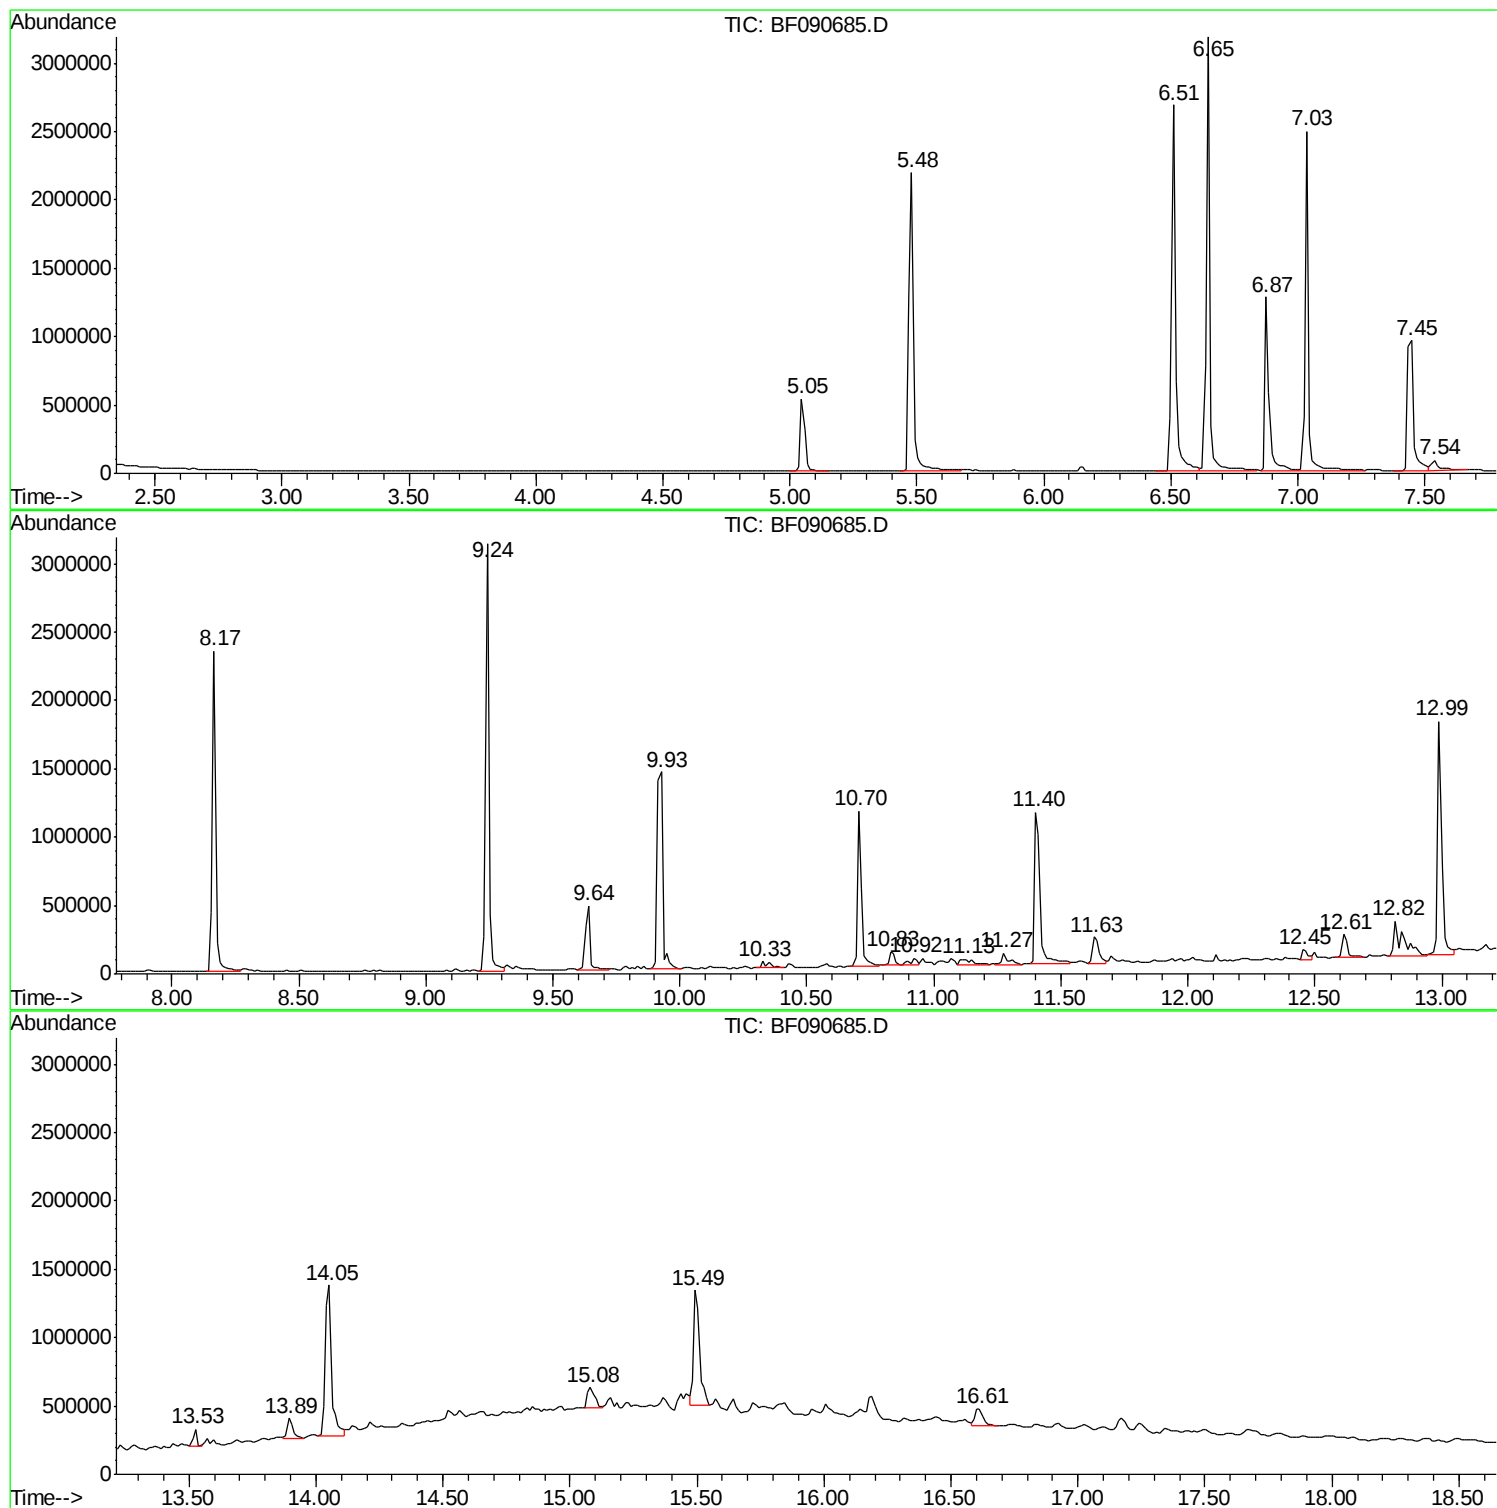

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF102016\
Data_File : BF090685.D
Acq_On : 20_Oct_2016_ 16:366
Operator : UM/SJJ
Sample : H5315-04_2XX
Misc :
ALS_Vial : 8 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
FO-TANK-SIDEWALL-SOUTH

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: rteint.pp

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
