


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102016\
 Data File : BF090677.D
 Acq On : 20 Oct 2016 12:03
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 19 15:13:23 2016

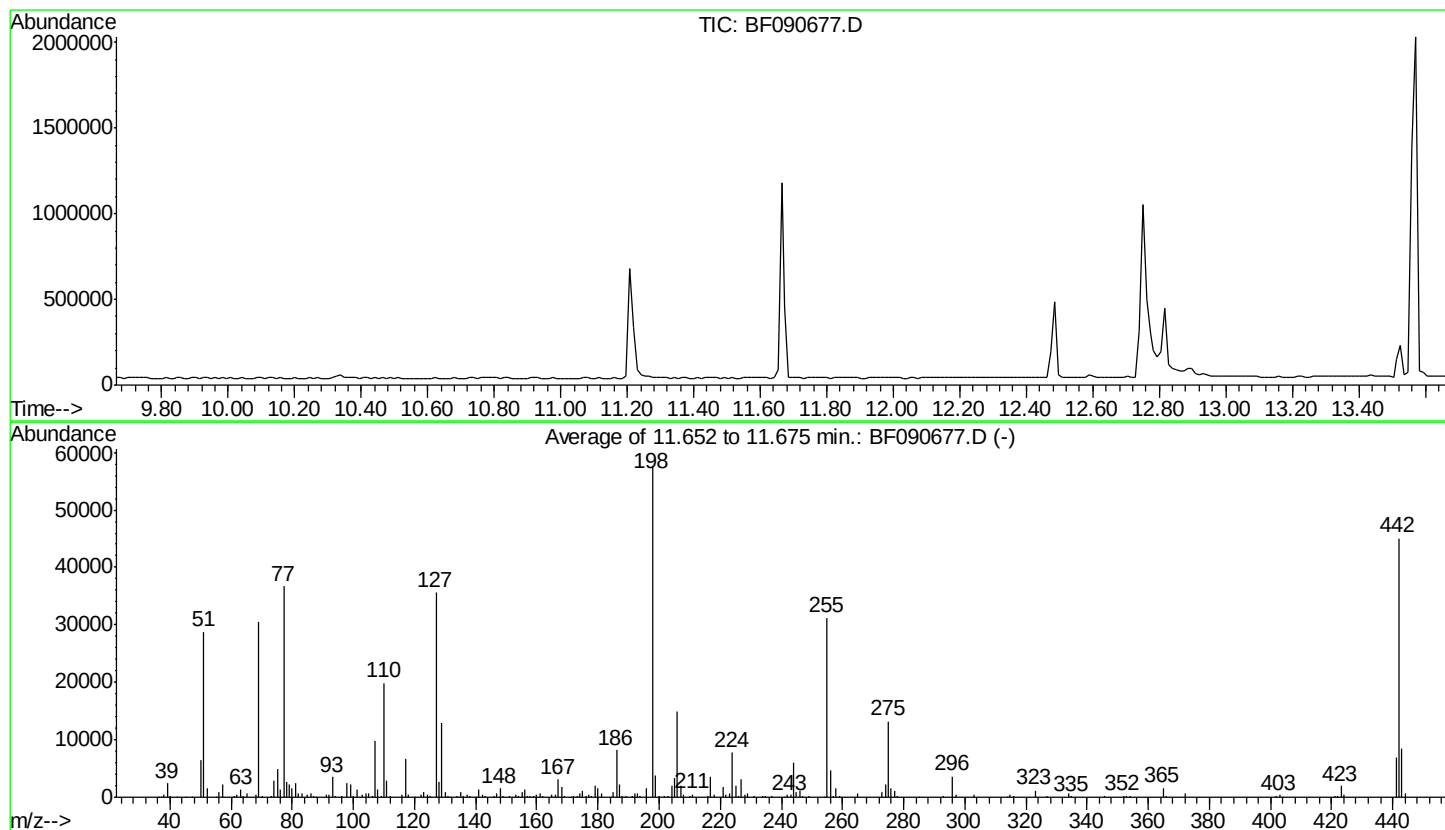

AutoFind: Scans 815, 816, 817; Background Corrected with Scan 812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.9	28775	PASS
68	69	0.00	2	1.4	417	PASS
69	198	0.00	100	53.1	30629	PASS
70	69	0.00	2	0.5	138	PASS
127	198	10	80	61.6	35560	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	57697	PASS
199	198	5	9	6.6	3791	PASS
275	198	10	60	22.9	13208	PASS
365	198	1	100	2.8	1596	PASS
441	442	0.01	24	15.3	6882	PASS
442	198	50	100	78.0	45021	PASS
443	442	15	24	18.6	8375	PASS