
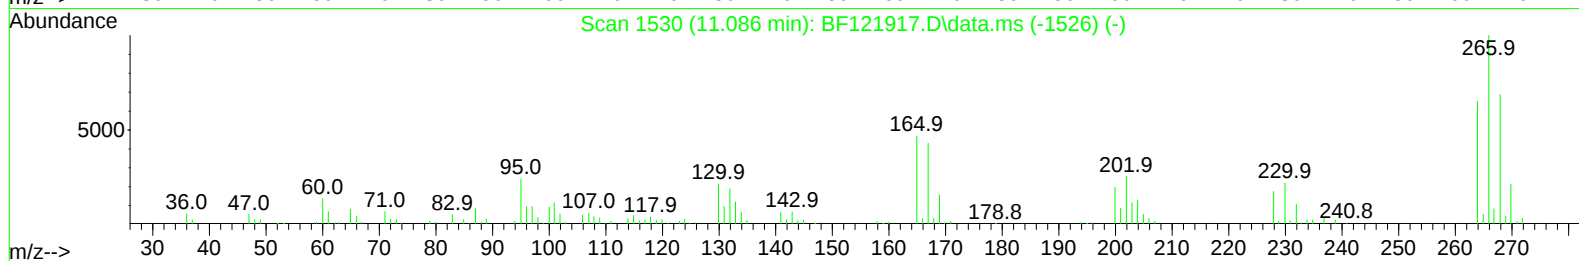
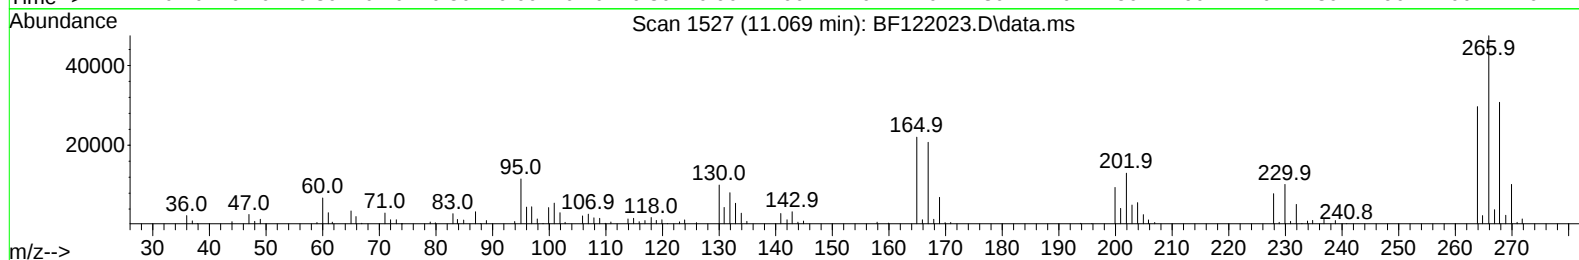


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102020\
Data File : BF122023.D
Acq On : 20 Oct 2020 10:56
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 21 01:51:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 12:55:05 2020
Response via : Initial Calibration

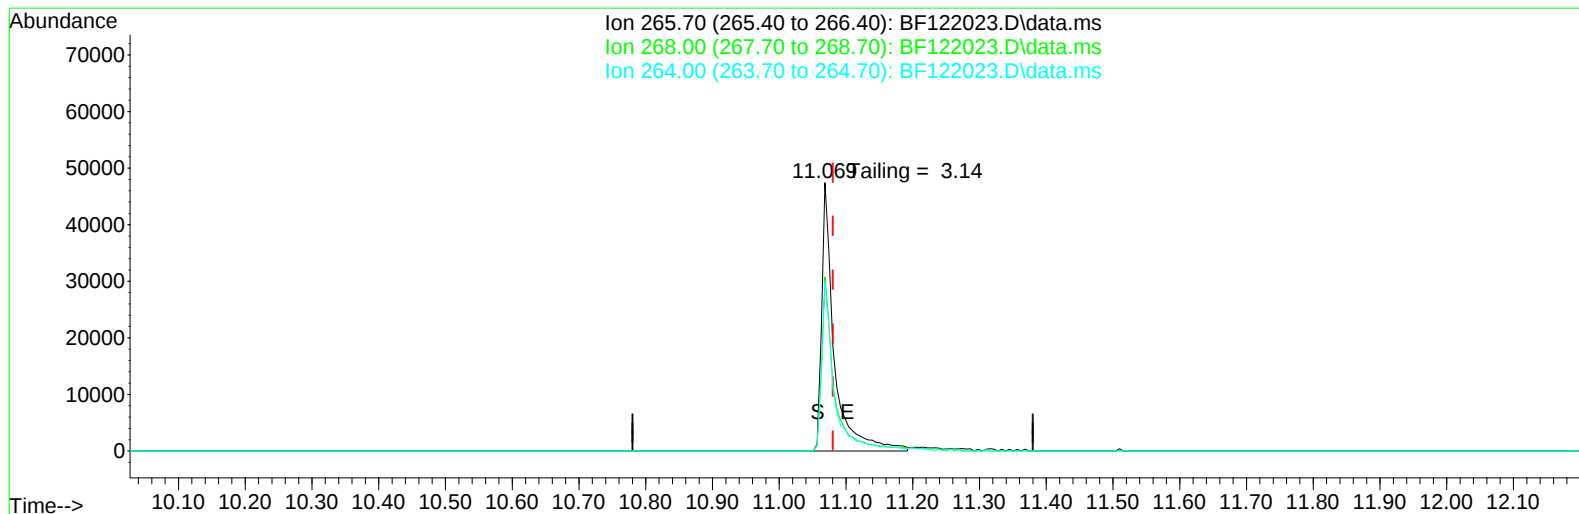

TIC: BF122023.D\data.ms

(70) Pentachlorophenol (C)




11.069min (-0.012) 22269.25 ng

response 62522

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	64.87
264.00	62.40	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102020\
Data File : BF122023.D
Acq On : 20 Oct 2020 10:56
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 21 01:51:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 12:55:05 2020
Response via : Initial Calibration

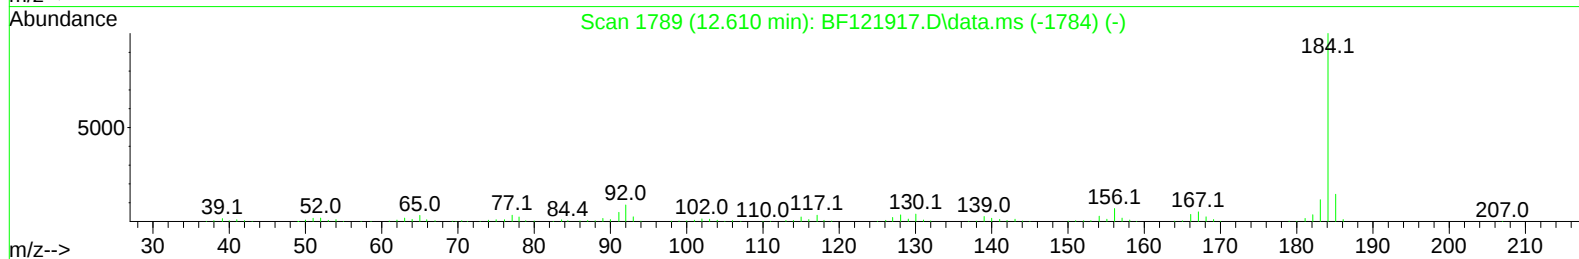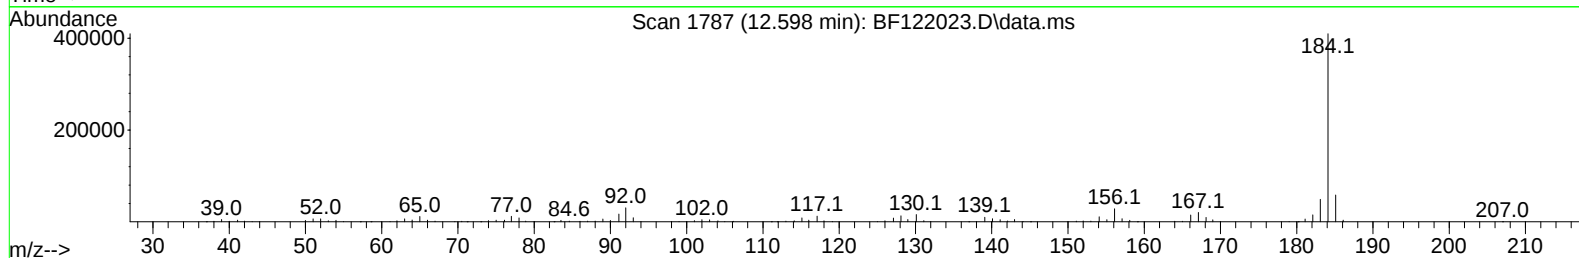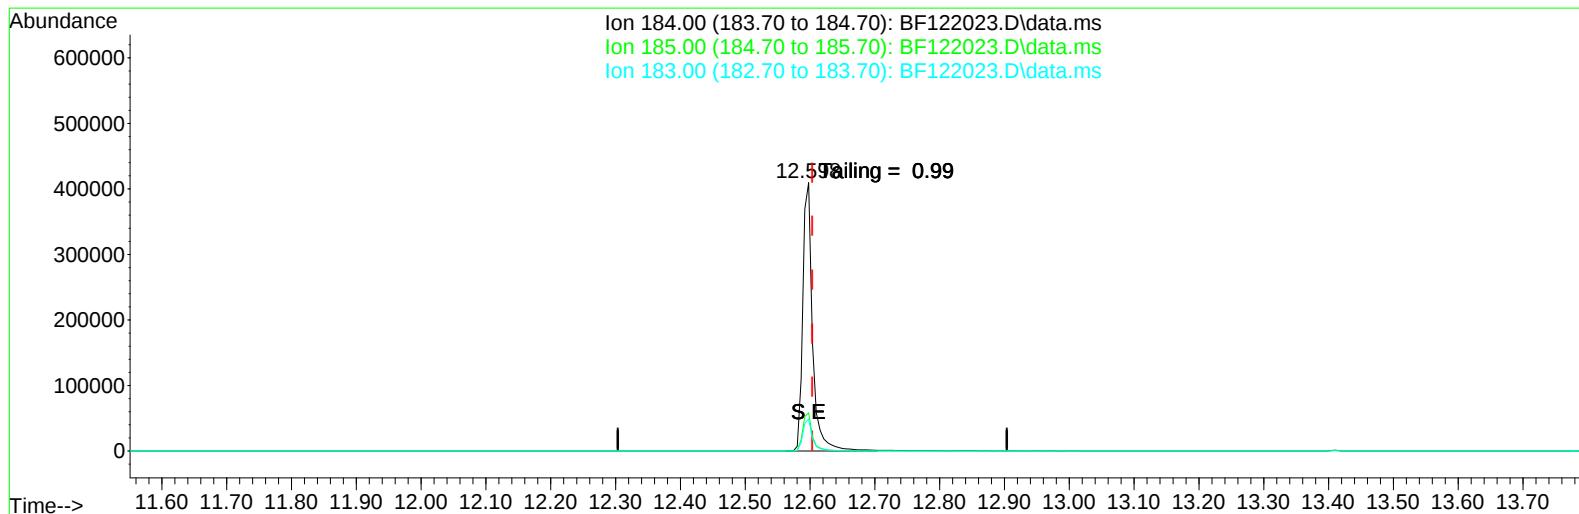

TIC: BF122023.D\data.ms

(77) Benzidine

12.598min (-0.006) 0.00 ng

response 435711

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.25
183.00	11.70	12.02
0.00	0.00	0.00