
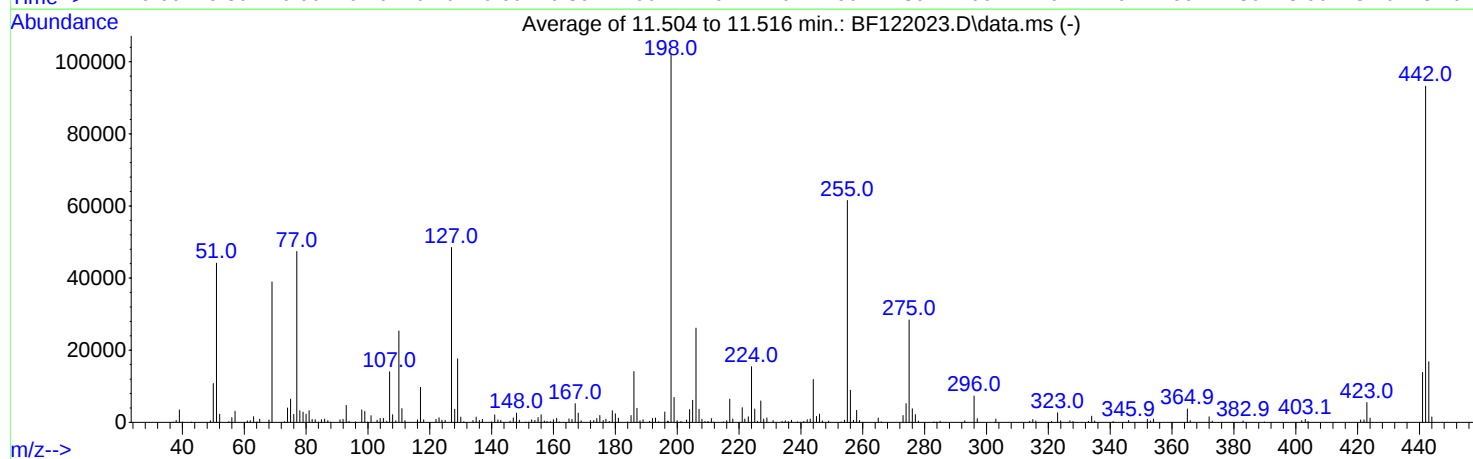


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102020\
 Data File : BF122023.D
 Acq On : 20 Oct 2020 10:56
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 21 12:04:42 2020

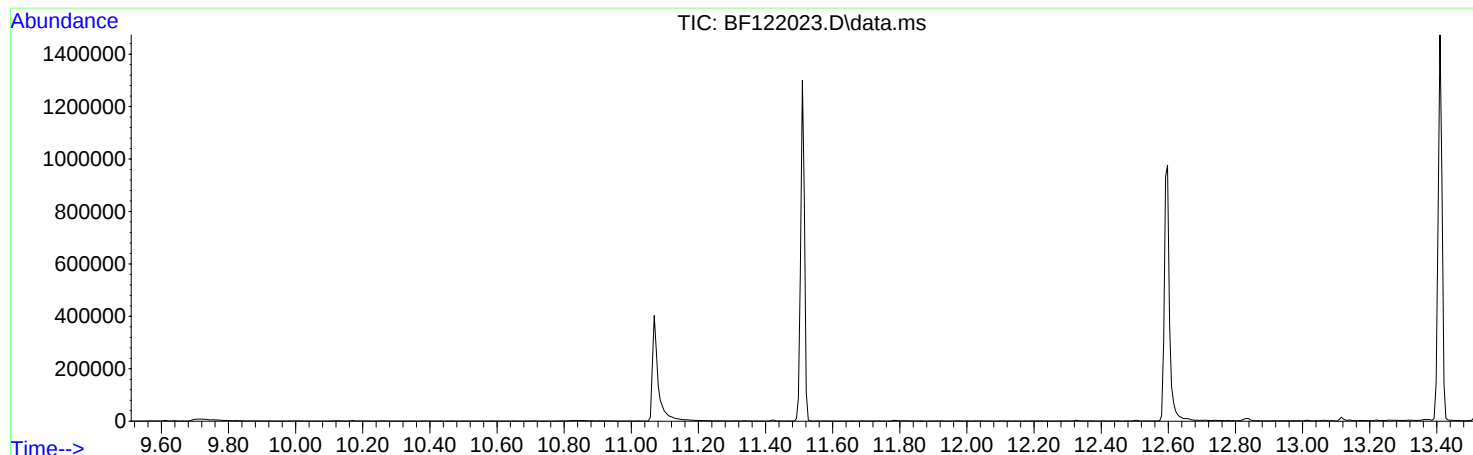

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.3	44157	PASS
68	69	0.00	2	1.7	670	PASS
69	198	0.00	100	38.2	38955	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.6	48504	PASS
197	198	0.00	2	0.4	378	PASS
198	198	100	100	100.0	101997	PASS
199	198	5	9	6.8	6940	PASS
275	198	10	60	27.8	28377	PASS
365	198	1	100	3.6	3714	PASS
441	198	0.01	100	13.6	13832	PASS
442	198	50	100	91.4	93197	PASS
443	442	15	24	18.0	16806	PASS