

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102115\
 Data File : BF082434.D
 Acq On : 22 Oct 2015 6:32
 Operator : UM/IZ
 Sample : G4116-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 AB-AC-02(0-2)

Quant Time: Oct 22 13:15:00 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 21 13:20:24 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.77	152	108682	20.00	ng	-0.01
21) Naphthalene-d8	8.06	136	416200	20.00	ng	-0.01
38) Acenaphthene-d10	9.82	164	189941	20.00	ng	0.00
63) Phenanthrene-d10	11.30	188	314249	20.00	ng	0.00
75) Chrysene-d12	13.98	240	256481	20.00	ng	-0.03
86) Perylene-d12	15.50	264	249371	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	674578	125.27	ng	0.01
7) Phenol-d6	6.42	99	948086	135.29	ng	0.00
23) Nitrobenzene-d5	7.35	82	564382	91.06	ng	0.00
41) 2,4,6-Tribromophenol	10.61	330	141807	79.61	ng	-0.01
44) 2-Fluorobiphenyl	9.14	172	1029447	89.88	ng	0.00
78) Terphenyl-d14	12.89	244	559029	57.76	ng	-0.01
Target Compounds						Qvalue
49) Dimethylphthalate	9.54	163	218289	16.32	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102115\
Data File : BF082434.D
Acq On : 22 Oct 2015 6:32
Operator : UM/IZ
Sample : G4116-19
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AB-AC-02(0-2)

Quant Time: Oct 22 13:15:00 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 21 13:20:24 2015
Response via : Initial Calibration

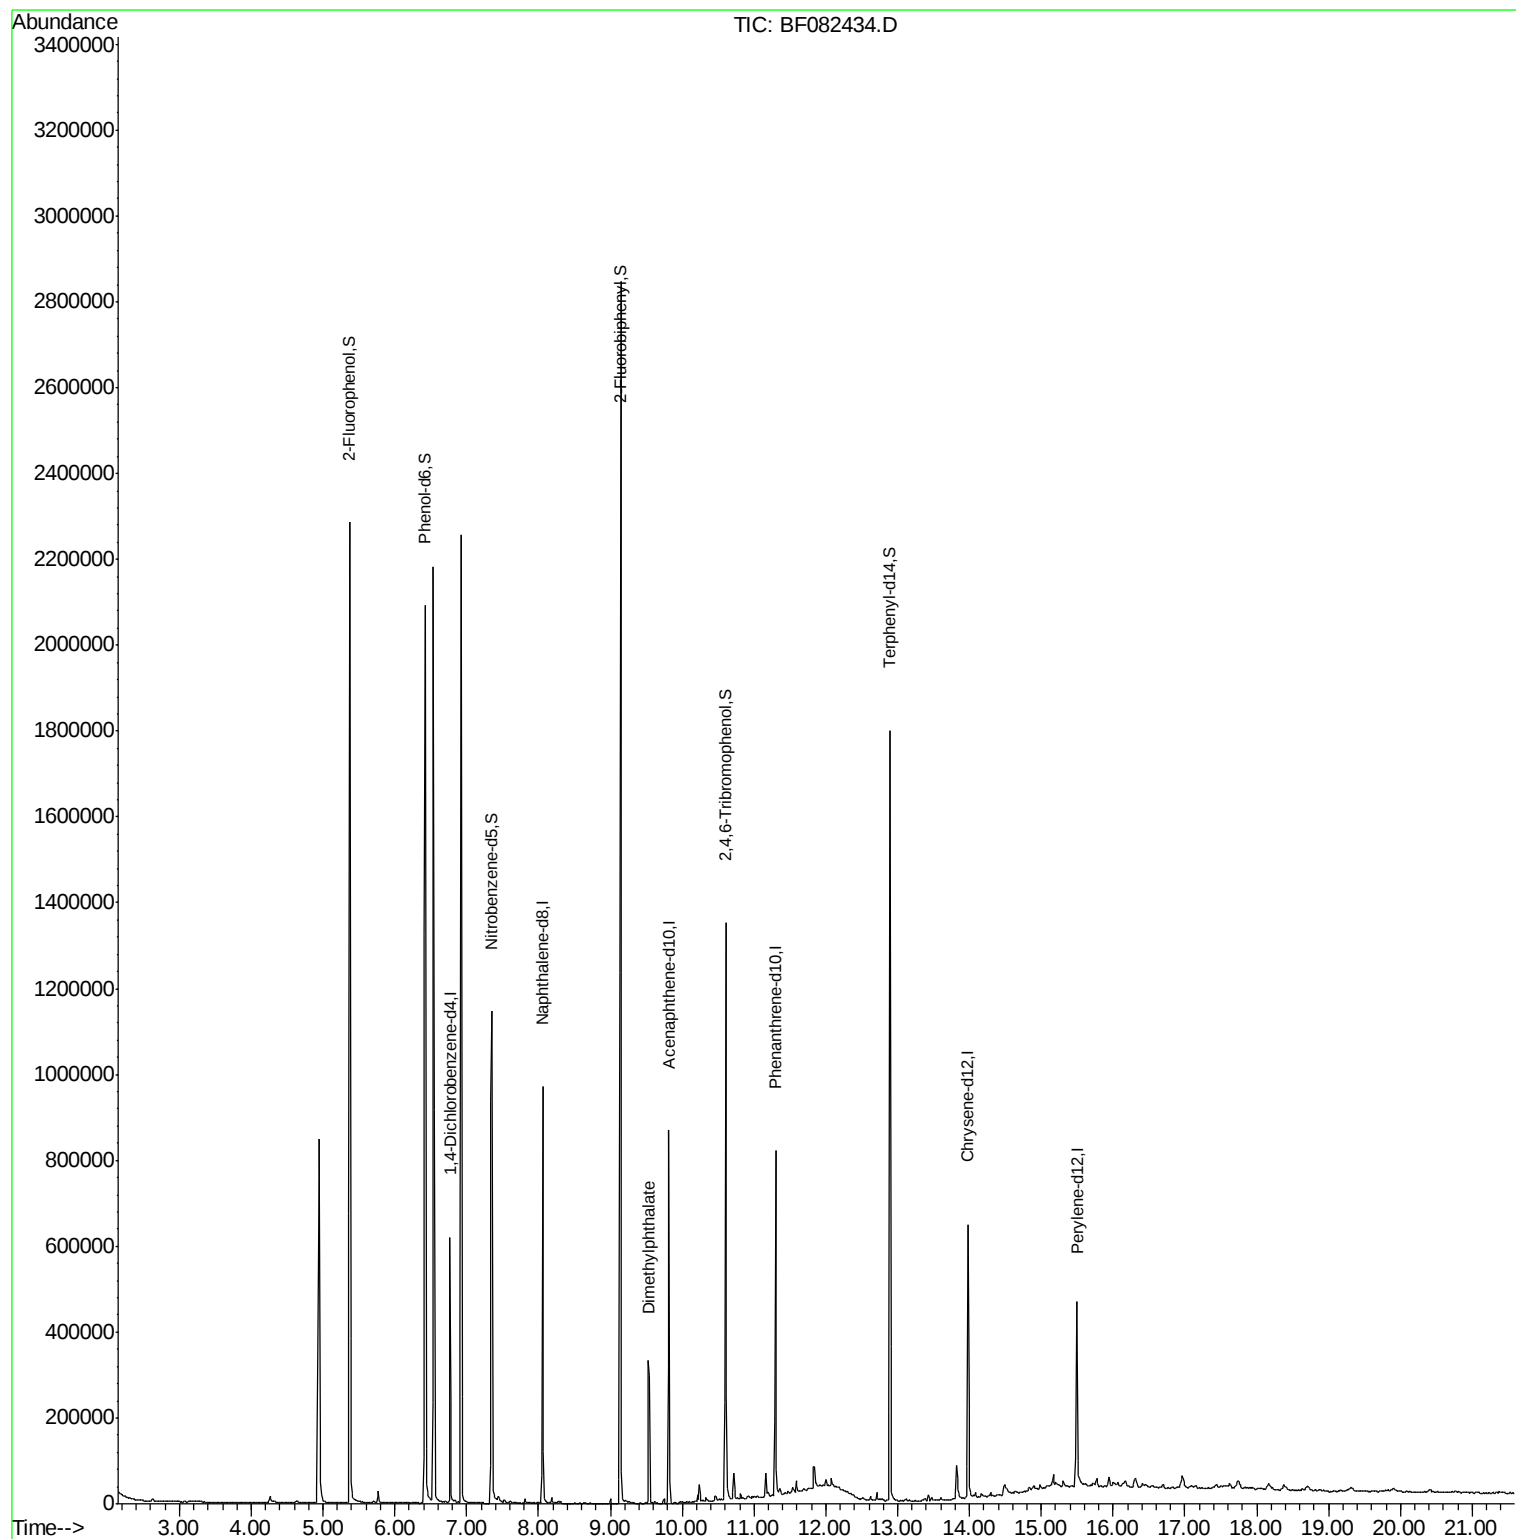

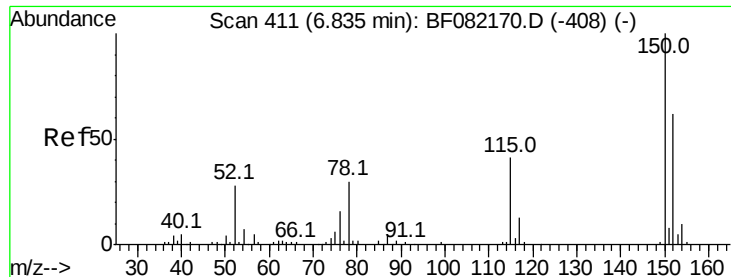

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.77 min Scan# 405

Delta R.T. -0.01 min

Lab File: BF082434.D

Acq: 22 Oct 2015 6:32

Instrument :

BNA_F

ClientSampleId :

AB-AC-02(0-2)


Tot Ion:152 Resp: 108682

Ion Ratio Lower Upper

152 100

150 160.2 129.0 193.4




115 63.4 52.1 78.1

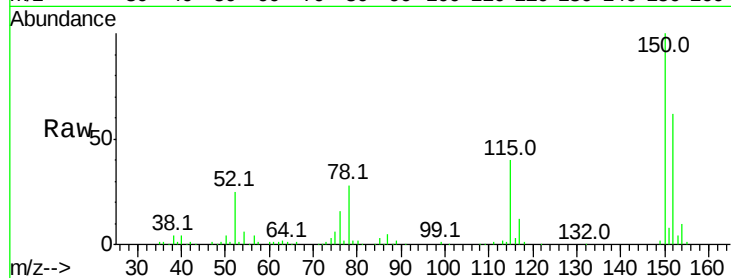

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

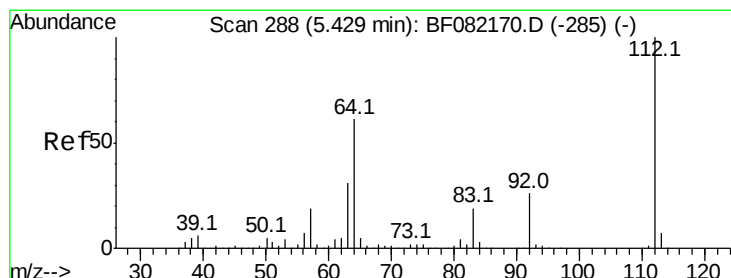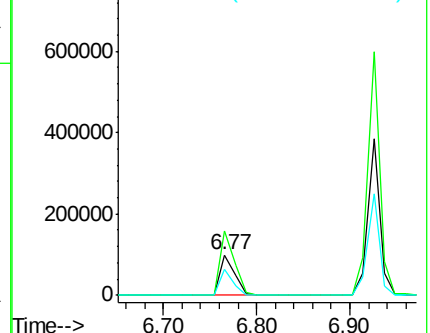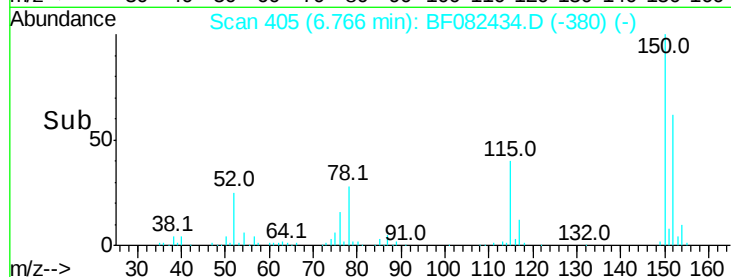

#5

2-Fluorophenol

Concen: 125.27 ng

RT: 5.37 min Scan# 283

Delta R.T. 0.01 min

Lab File: BF082434.D

Acq: 22 Oct 2015 6:32


Tgt Ion:112 Resp: 674578

Ion Ratio Lower Upper

112 100

64 63.1 48.6 73.0



63 33.4 25.1 37.7

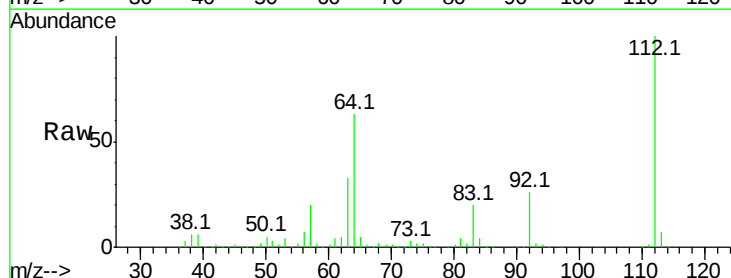

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

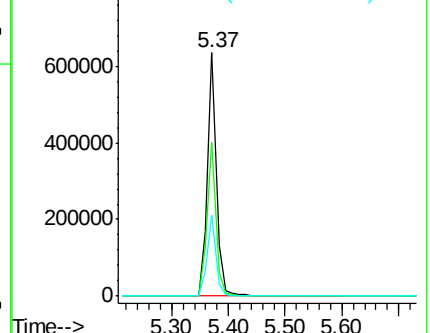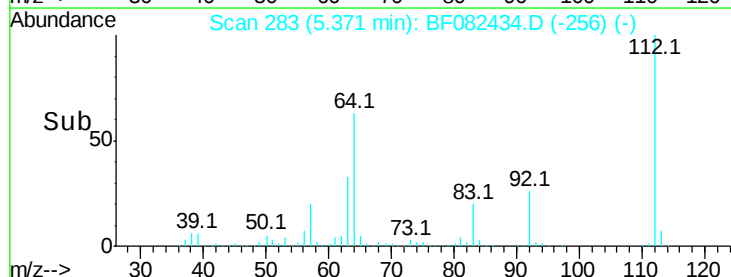



#7

Phenol-d6

Concen: 135.29 ng

RT: 6.42 min Scan# 375

Delta R.T. -0.00 min

Lab File: BF082434.D

Acq: 22 Oct 2015 6:32

Instrument :

BNA_F

ClientSampleId :

AB-AC-02(0-2)





Tot Ion: 99 Resp: 948086

Ion Ratio Lower Upper

99 100

42 16.3 13.2 19.8

71 33.8 25.6 38.4

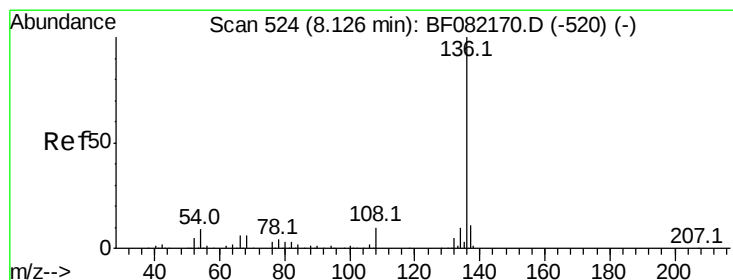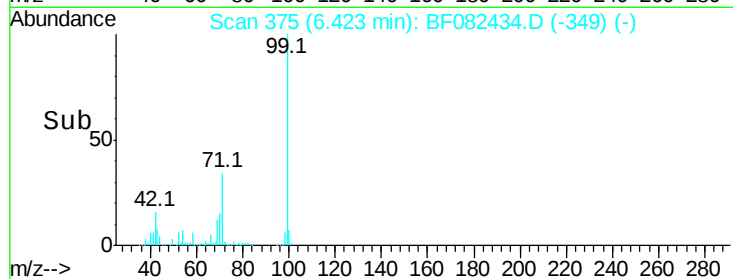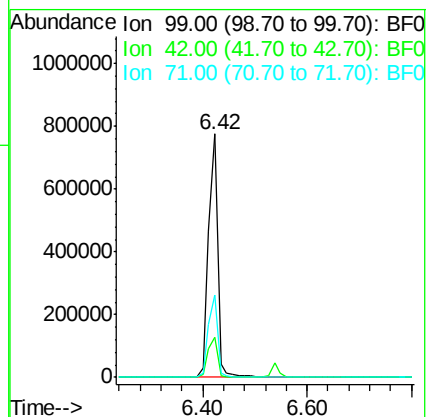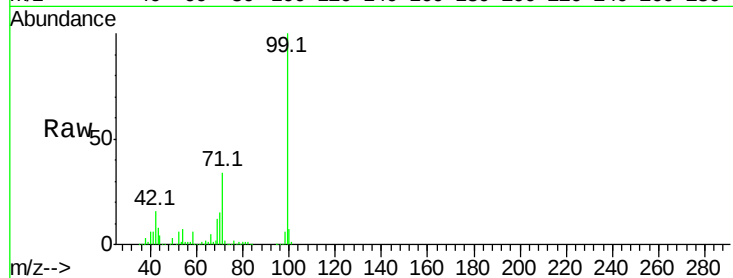

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.06 min Scan# 518

Delta R.T. -0.01 min

Lab File: BF082434.D

Acq: 22 Oct 2015 6:32

Tgt Ion: 136 Resp: 416200




Ion Ratio Lower Upper


136 100

137 11.2 9.0 13.6

54 8.4 7.5 11.3

68 5.3 4.6 7.0


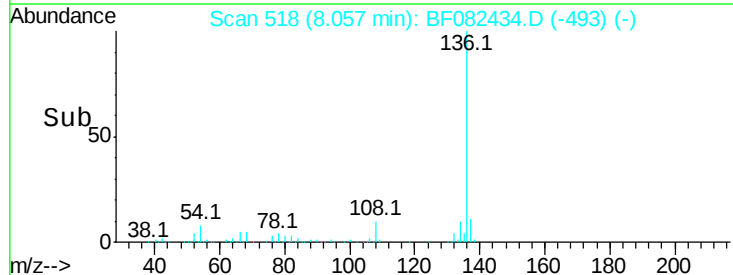
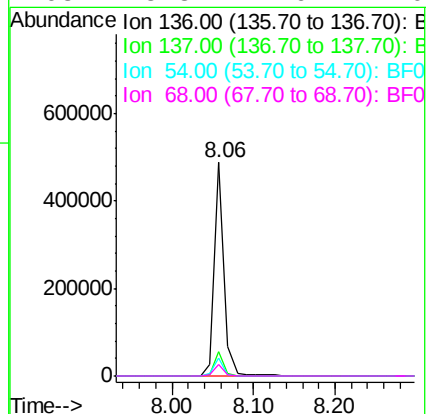
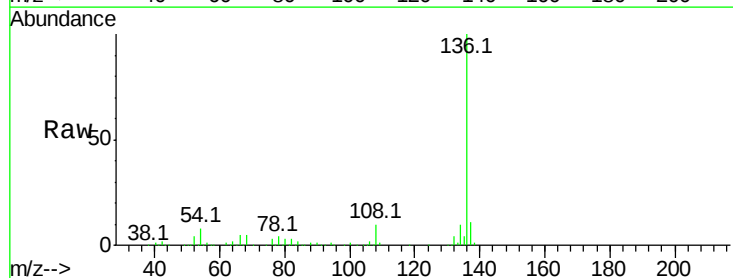


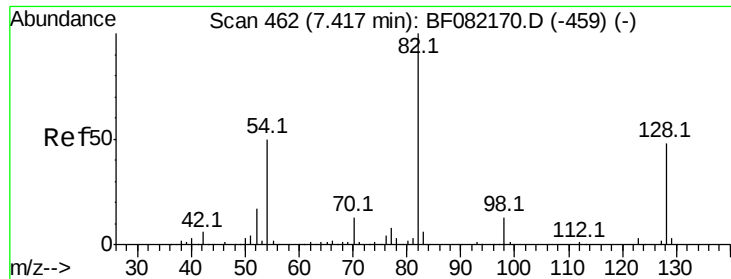

#23
 Nitrobenzene-d5
 Concen: 91.06 ng
 RT: 7.35 min Scan# 456
 Delta R.T. -0.00 min
 Lab File: BF082434.D
 Acq: 22 Oct 2015 6:32




Instrument :
 BNA_F
 ClientSampleId :
 AB-AC-02(0-2)

Tot Ion: 82 Resp: 564382
 Ion Ratio Lower Upper
 82 100
 128 53.3 38.7 58.1
 54 46.3 40.1 60.1

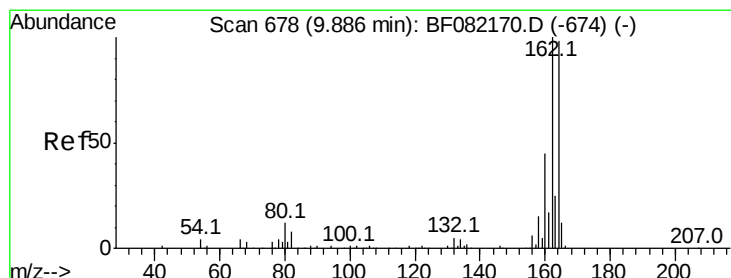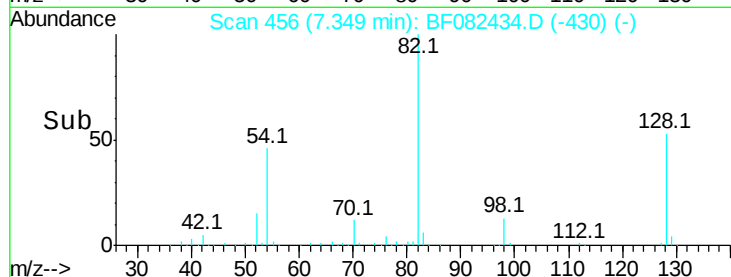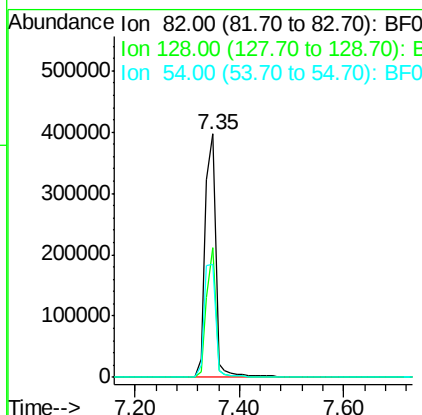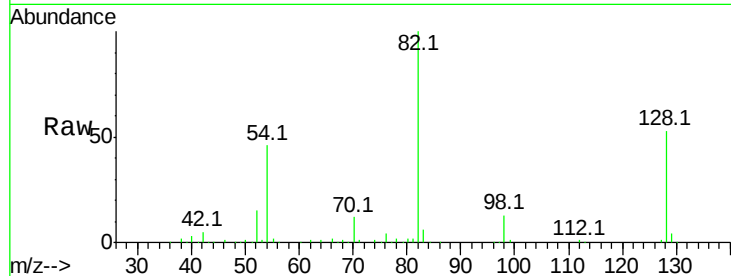

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.82 min Scan# 672
 Delta R.T. -0.00 min
 Lab File: BF082434.D
 Acq: 22 Oct 2015 6:32

Tgt Ion:164 Resp: 189941
 Ion Ratio Lower Upper
 164 100
 162 103.5 81.6 122.4
 160 45.8 36.4 54.6

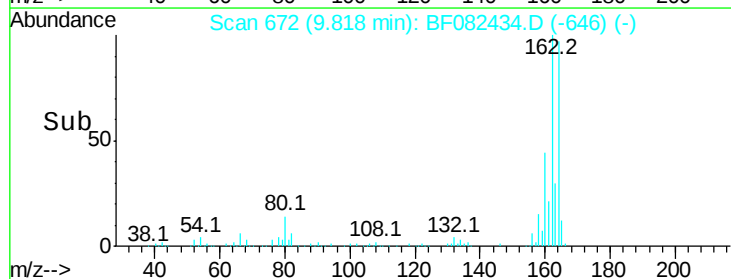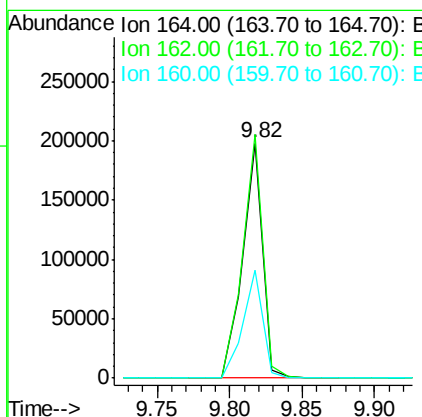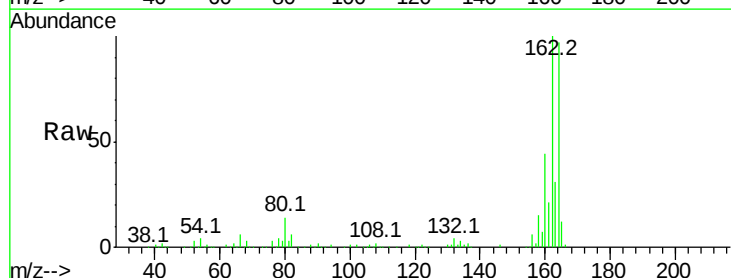







#41
 2,4,6-Tribromophenol
 Concen: 79.61 ng
 RT: 10.61 min Scan# 741
 Delta R.T. -0.01 min
 Lab File: BF082434.D
 Acq: 22 Oct 2015 6:32

Instrument :
 BNA_F
 ClientSampleId :
 AB-AC-02(0-2)

Tot Ion:330 Resp: 141807
 Ion Ratio Lower Upper
 330 100
 332 95.7 77.1 115.7
 141 45.5 29.8 44.8#

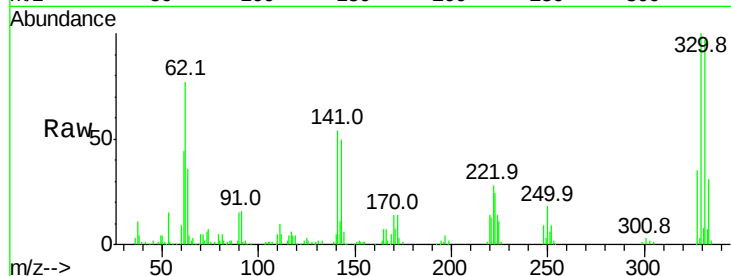


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

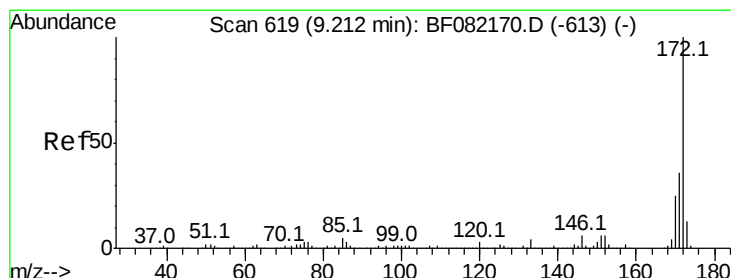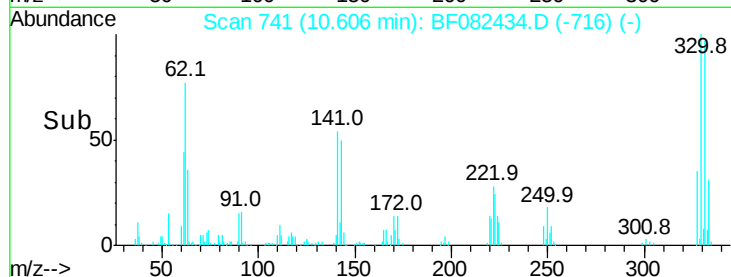
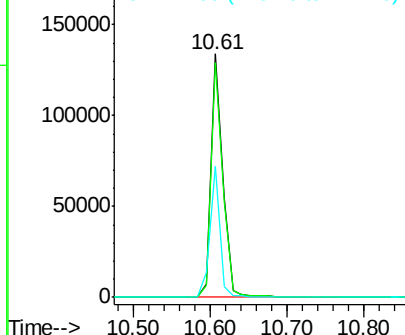



#44
 2-Fluorobiphenyl
 Concen: 89.88 ng
 RT: 9.14 min Scan# 613
 Delta R.T. -0.00 min
 Lab File: BF082434.D
 Acq: 22 Oct 2015 6:32

Tgt Ion:172 Resp: 1029447
 Ion Ratio Lower Upper
 172 100
 171 36.9 28.6 42.8
 170 24.7 19.7 29.5

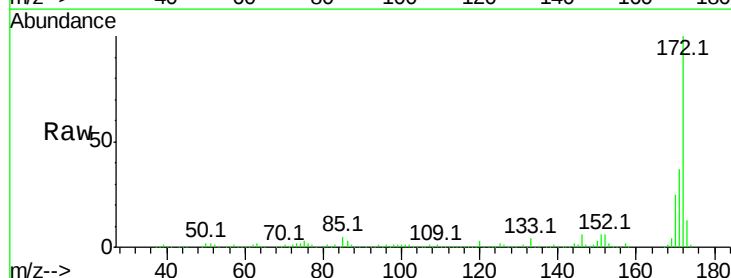

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

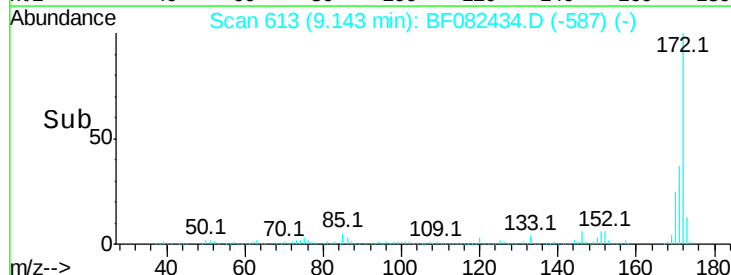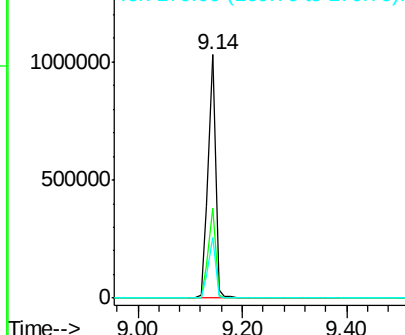

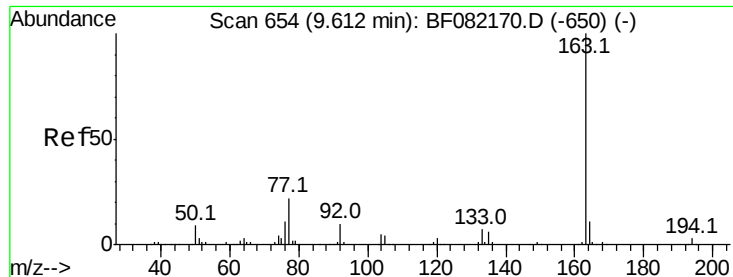

#49

Dimethylphthalate

Concen: 16.32 ng

RT: 9.54 min Scan# 648

Delta R.T. -0.01 min

Lab File: BF082434.D

Acq: 22 Oct 2015 6:32

Instrument :

BNA_F

ClientSampleId :

AB-AC-02(0-2)


Tot Ion:163 Resp: 218289

Ion Ratio Lower Upper

163 100

194 4.2 2.6 4.0#




164 10.0 8.5 12.7

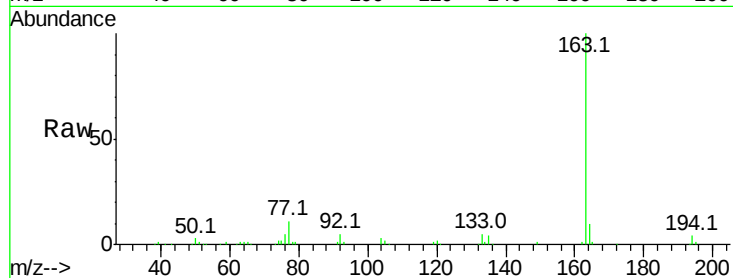

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

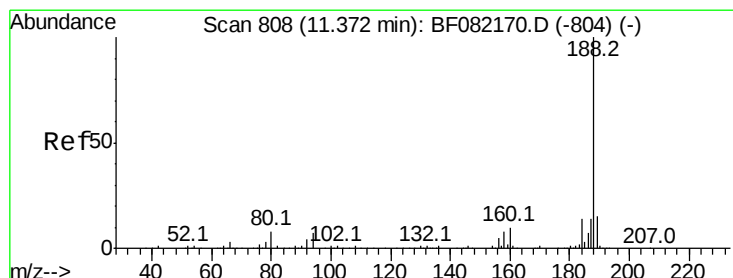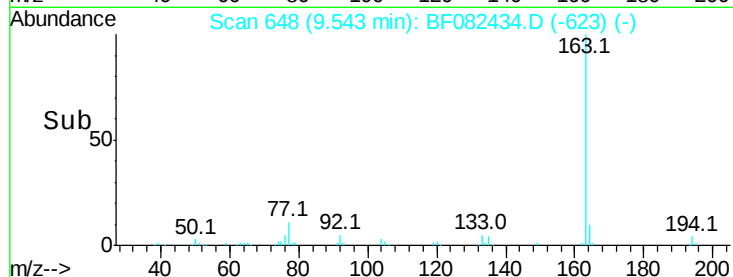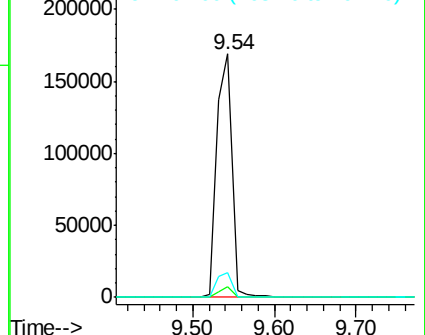

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.30 min Scan# 802

Delta R.T. -0.00 min

Lab File: BF082434.D

Acq: 22 Oct 2015 6:32


Tgt Ion:188 Resp: 314249

Ion Ratio Lower Upper

188 100

94 7.4 5.8 8.6



80 7.6 6.4 9.6

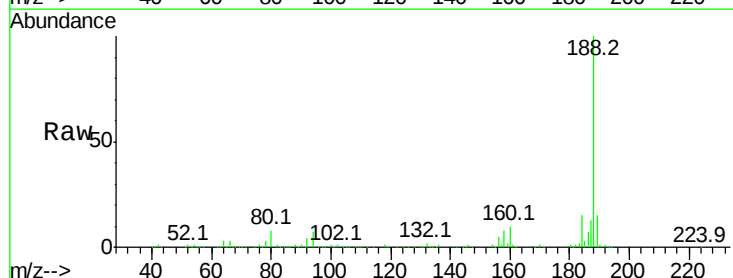


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

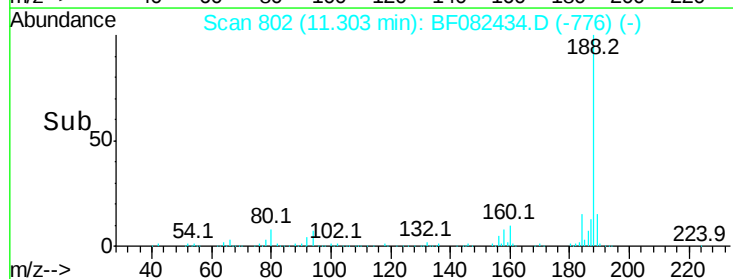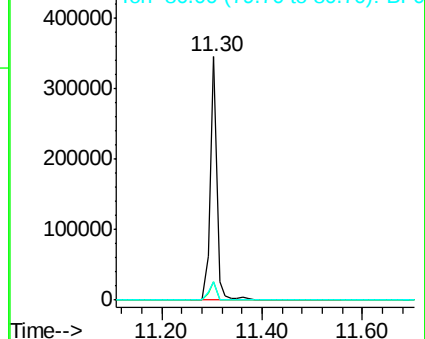

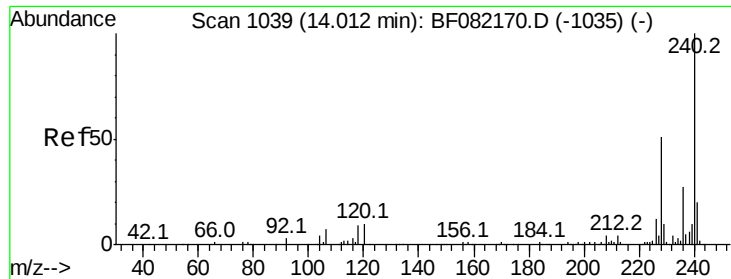

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.98 min Scan# 1036

Delta R.T. -0.03 min

Lab File: BF082434.D

Acq: 22 Oct 2015 6:32

Instrument :

BNA_F

ClientSampleId :

AB-AC-02(0-2)


Tot Ion:240 Resp: 256481

Ion Ratio Lower Upper

240 100

120 11.1 8.1 12.1




236 26.6 21.3 31.9

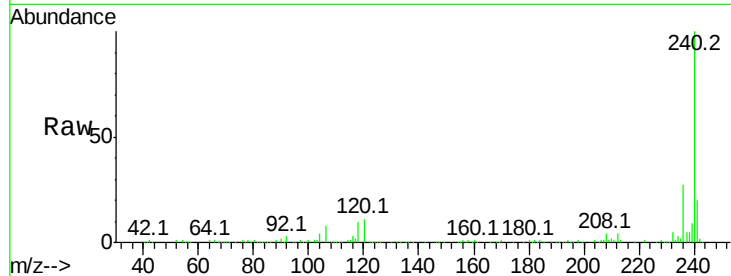

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

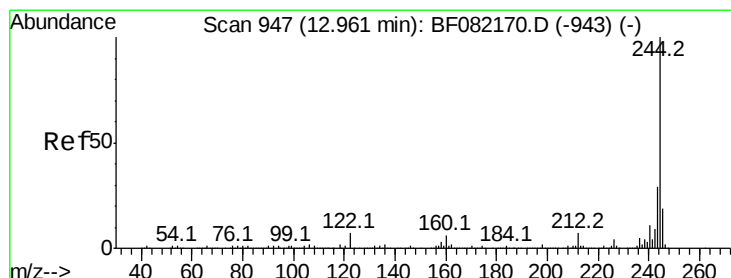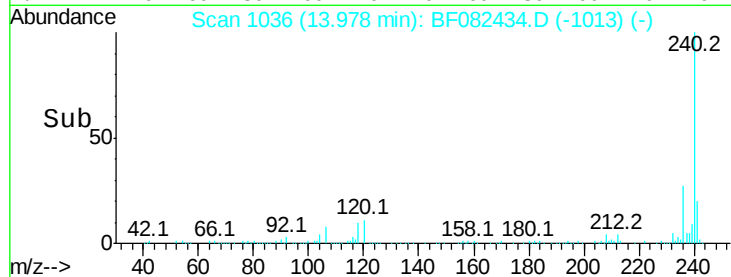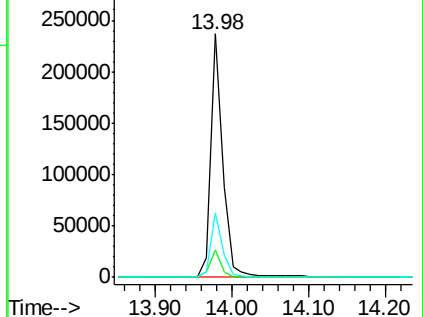

#78

Terphenyl-d14

Concen: 57.76 ng

RT: 12.89 min Scan# 941

Delta R.T. -0.01 min

Lab File: BF082434.D

Acq: 22 Oct 2015 6:32


Tgt Ion:244 Resp: 559029

Ion Ratio Lower Upper

244 100

212 8.1 5.8 8.6



122 12.6 5.9 8.9#



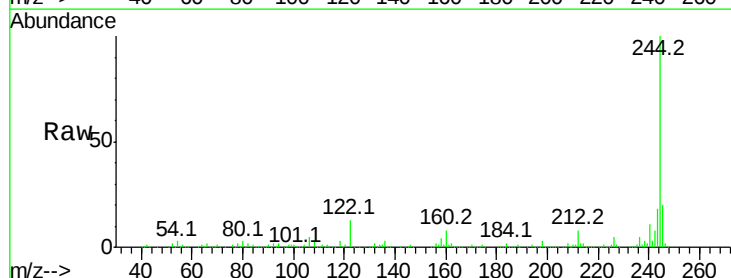


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

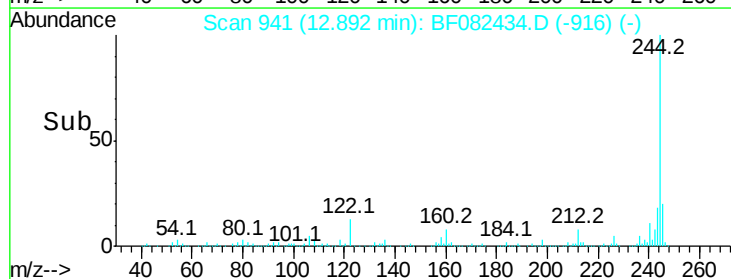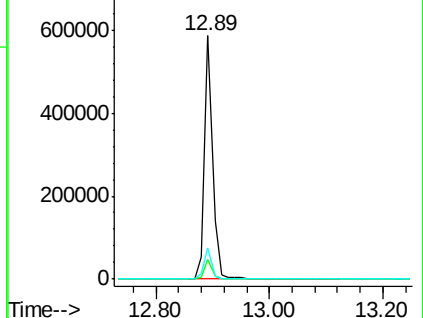

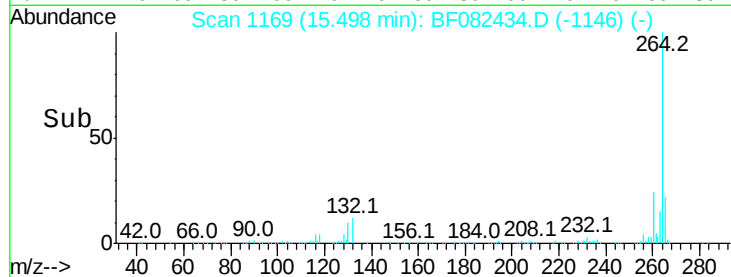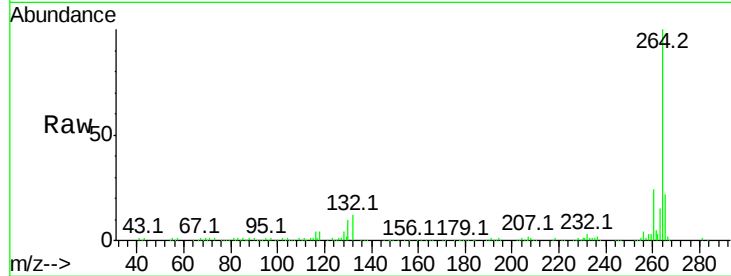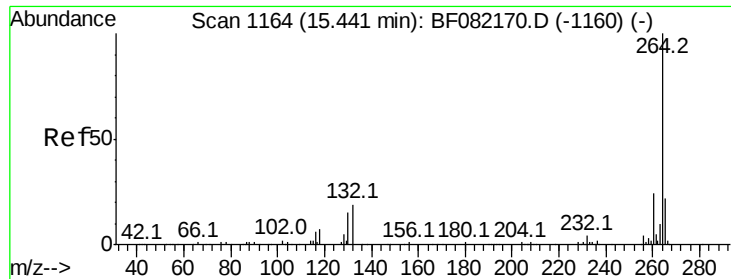

#86

Pervlene-d12

Concen: 20.00 ng

RT: 15.50 min Scan# 1169

Delta R.T. -0.03 min

Lab File: BF082434.D

Acq: 22 Oct 2015 6:32

Instrument :

BNA_F

ClientSampleId :

AB-AC-02(0-2)

Tot Ion:264 Resp: 249371

Ion Ratio Lower Upper

264 100

260 24.0 19.0 28.6

265 21.9 17.3 25.9

