

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102115\
 Data File : BF082401.D
 Acq On : 21 Oct 2015 13:36
 Operator : UM/IZ
 Sample : PB86203BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB86203BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.949	242	246	257	rBV	567475	947693	36.99%	4.610%
2	5.371	281	283	285	rBV	1904794	1839176	71.79%	8.946%
3	6.412	371	374	377	rBV	1733615	1713317	66.88%	8.334%
4	6.537	383	385	387	rBV	2199837	1938686	75.67%	9.430%
5	6.766	403	405	408	rBV	574811	577845	22.56%	2.811%
6	6.926	416	419	421	rBV	1805297	1643068	64.13%	7.992%
7	7.337	453	455	458	rBV	973532	1066927	41.65%	5.190%
8	8.057	516	518	521	rBV	866484	781924	30.52%	3.803%
9	9.143	610	613	615	rBV	2133233	2462818	96.13%	11.980%
10	9.818	669	672	674	rBV	963789	940050	36.69%	4.573%
11	10.606	738	741	744	rBV	1386095	1334235	52.08%	6.490%
12	11.303	799	802	804	rBV	1011883	951034	37.12%	4.626%
13	11.829	846	848	855	rBV2	36040	60656	2.37%	0.295%
14	12.618	915	917	921	rBV	17429	32661	1.27%	0.159%
15	12.904	939	942	945	rBV	2644034	2561930	100.00%	12.462%
16	14.012	1037	1039	1042	rBV	827553	942452	36.79%	4.584%
17	15.567	1172	1175	1178	rBV	621383	763635	29.81%	3.715%




Sum of corrected areas: 20558107

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102115\
Data File : BF082401.D
Acq On : 21 Oct 2015 13:36
Operator : UM/IZ
Sample : PB86203BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB86203BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

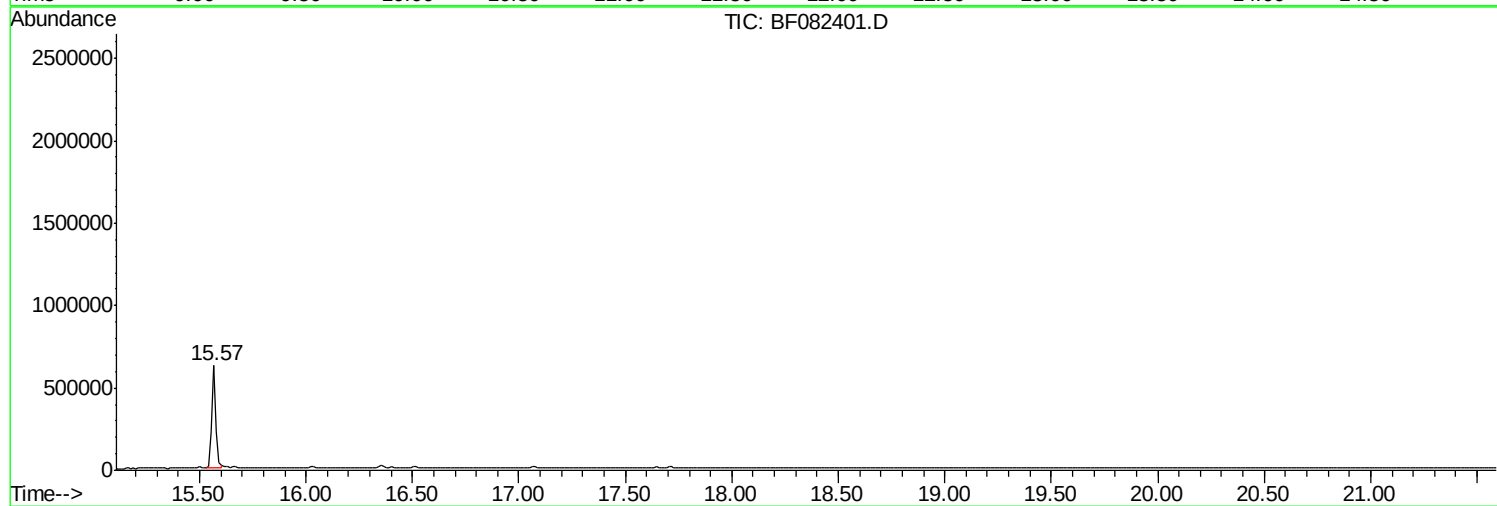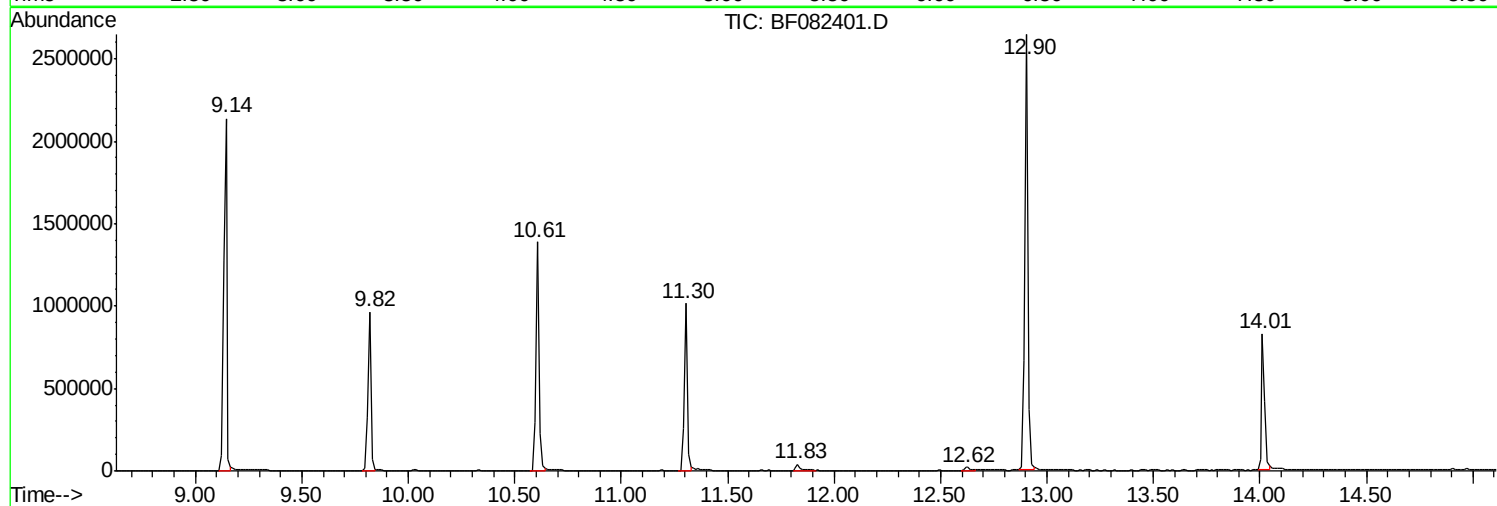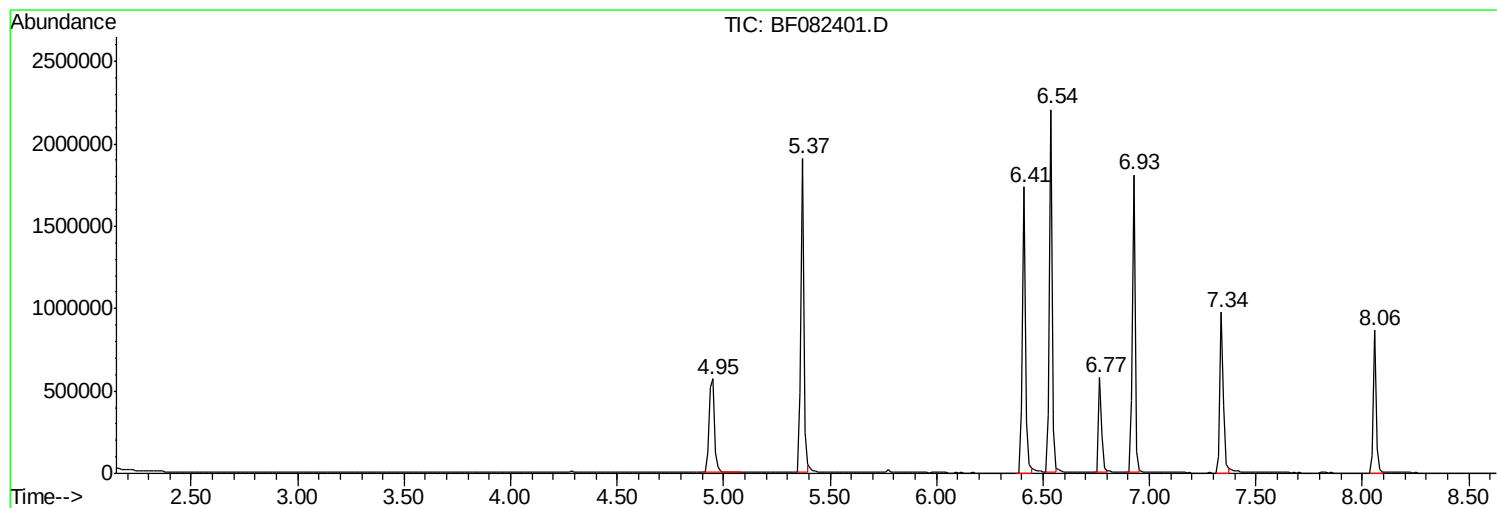

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102115\
Data File : BF082401.D
Acq On : 21 Oct 2015 13:36
Operator : UM/IZ
Sample : PB86203BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB86203BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.95	32.80 ng	947693	1,4-Dichlorobenzene-d4	6.77

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	23
3		Guanidine	59	CH5N3	000113-00-8	9
4		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
5		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9

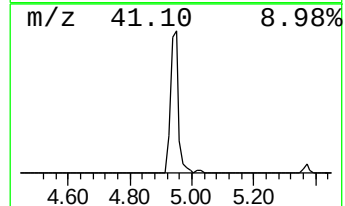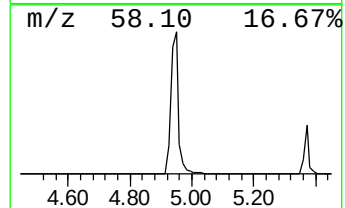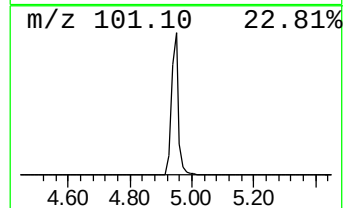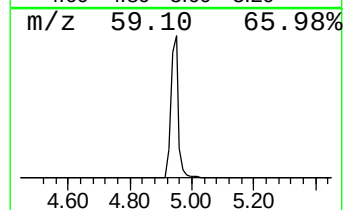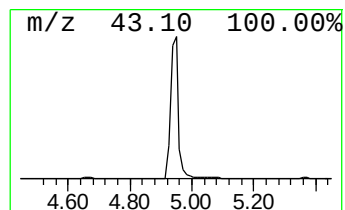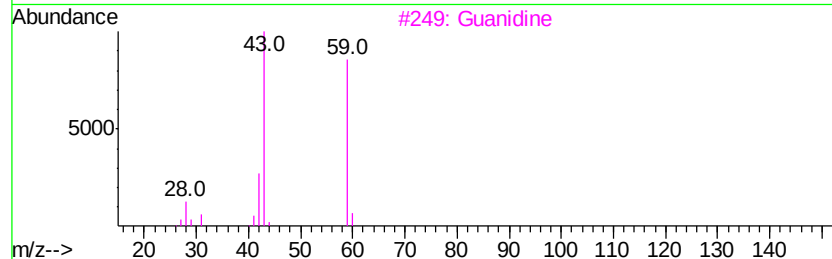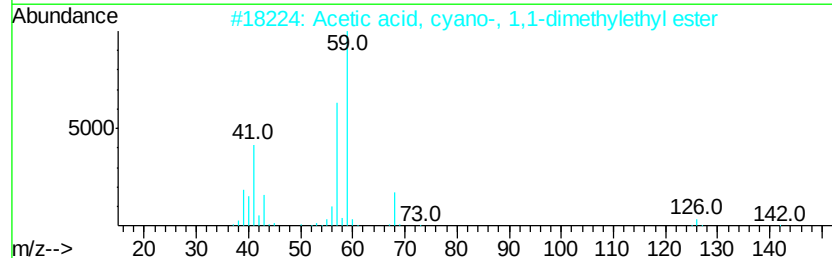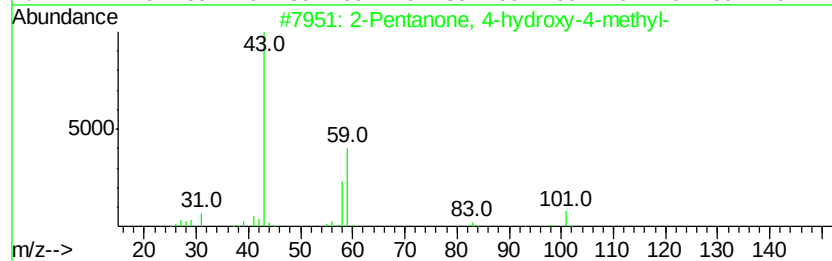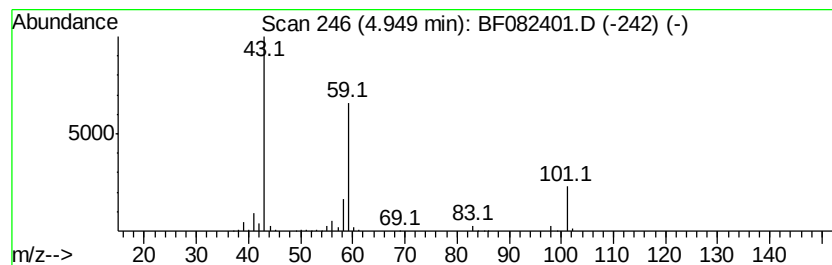

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102115\
Data File : BF082401.D
Acq On : 21 Oct 2015 13:36
Operator : UM/IZ
Sample : PB86203BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB86203BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.54 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.54	67.10 ng	1938690	1,4-Dichlorobenzene-d4	6.77

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			5-Aminoindole	132	C8H8N2	005192-03-0	12
3			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4			4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

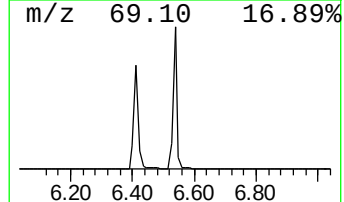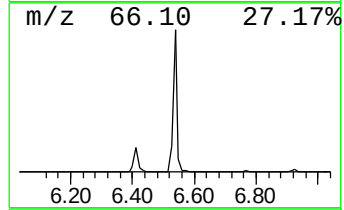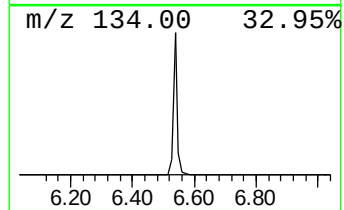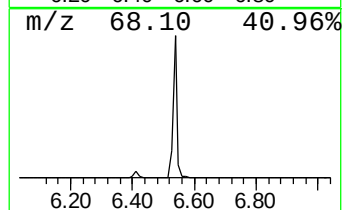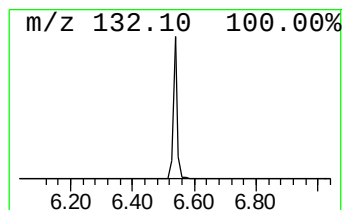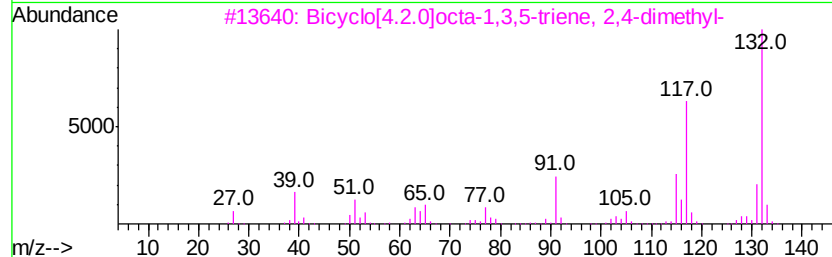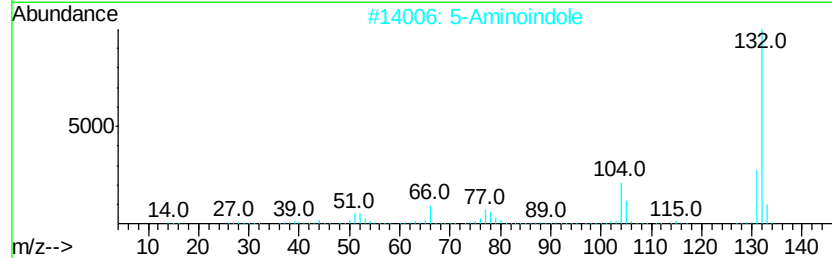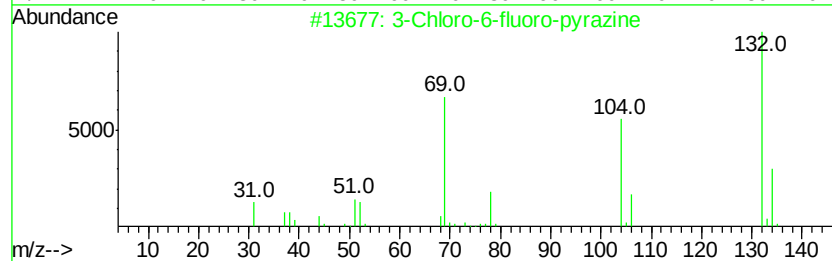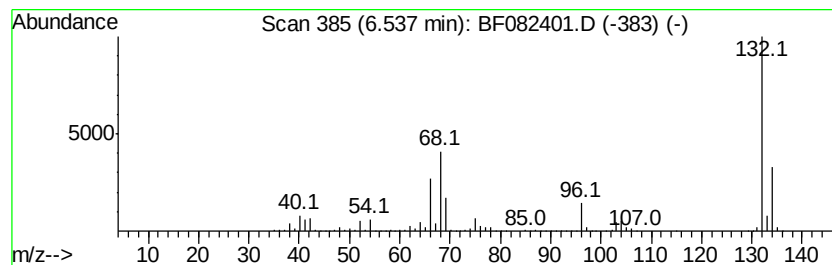

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102115\
Data File : BF082401.D
Acq On : 21 Oct 2015 13:36
Operator : UM/IZ
Sample : PB86203BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB86203BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.95	32.8	ng	947693	1	6.77	577845	20.0
unknown6.54	6.54	67.1	ng	1938690	1	6.77	577845	20.0