

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102115\
 Data File : BF082403.D
 Acq On : 21 Oct 2015 14:42
 Operator : UM/IZ
 Sample : G4099-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20151013MGP208BRV68

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.634	128	131	138	rVB	28440	51784	1.32%	0.209%
2	4.926	242	244	252	rBV	378321	467436	11.91%	1.886%
3	5.360	280	282	293	rBV	1273779	1222174	31.14%	4.932%
4	6.412	371	374	376	rBV	494621	714405	18.20%	2.883%
5	6.537	382	385	387	rBV	2468572	2362954	60.21%	9.535%
6	6.766	403	405	408	rBV	669783	639247	16.29%	2.579%
7	6.926	416	419	421	rBV	2419544	2305441	58.74%	9.303%
8	7.337	452	455	458	rBV	1163563	1722902	43.90%	6.952%
9	8.057	516	518	524	rBV	1001612	971404	24.75%	3.920%
10	9.143	610	613	615	rBV	3707615	3834656	97.70%	15.473%
11	9.818	669	672	674	rBV	1066025	1089743	27.77%	4.397%
12	10.606	738	741	744	rBV	1859521	2111196	53.79%	8.519%
13	11.303	799	802	804	rBV	1218666	1185451	30.20%	4.783%
14	11.829	847	848	850	rBV	70871	103569	2.64%	0.418%
15	12.629	916	918	927	rBV	88355	116634	2.97%	0.471%
16	12.915	939	943	945	rBV	2887906	3924835	100.00%	15.837%
17	14.035	1038	1041	1043	rBV	907623	1092759	27.84%	4.409%
18	15.612	1176	1179	1182	rBV	678113	865597	22.05%	3.493%


Sum of corrected areas: 24782187

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102115\
Data File : BF082403.D
Acq On : 21 Oct 2015 14:42
Operator : UM/IZ
Sample : G4099-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20151013MGP208BRV68

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

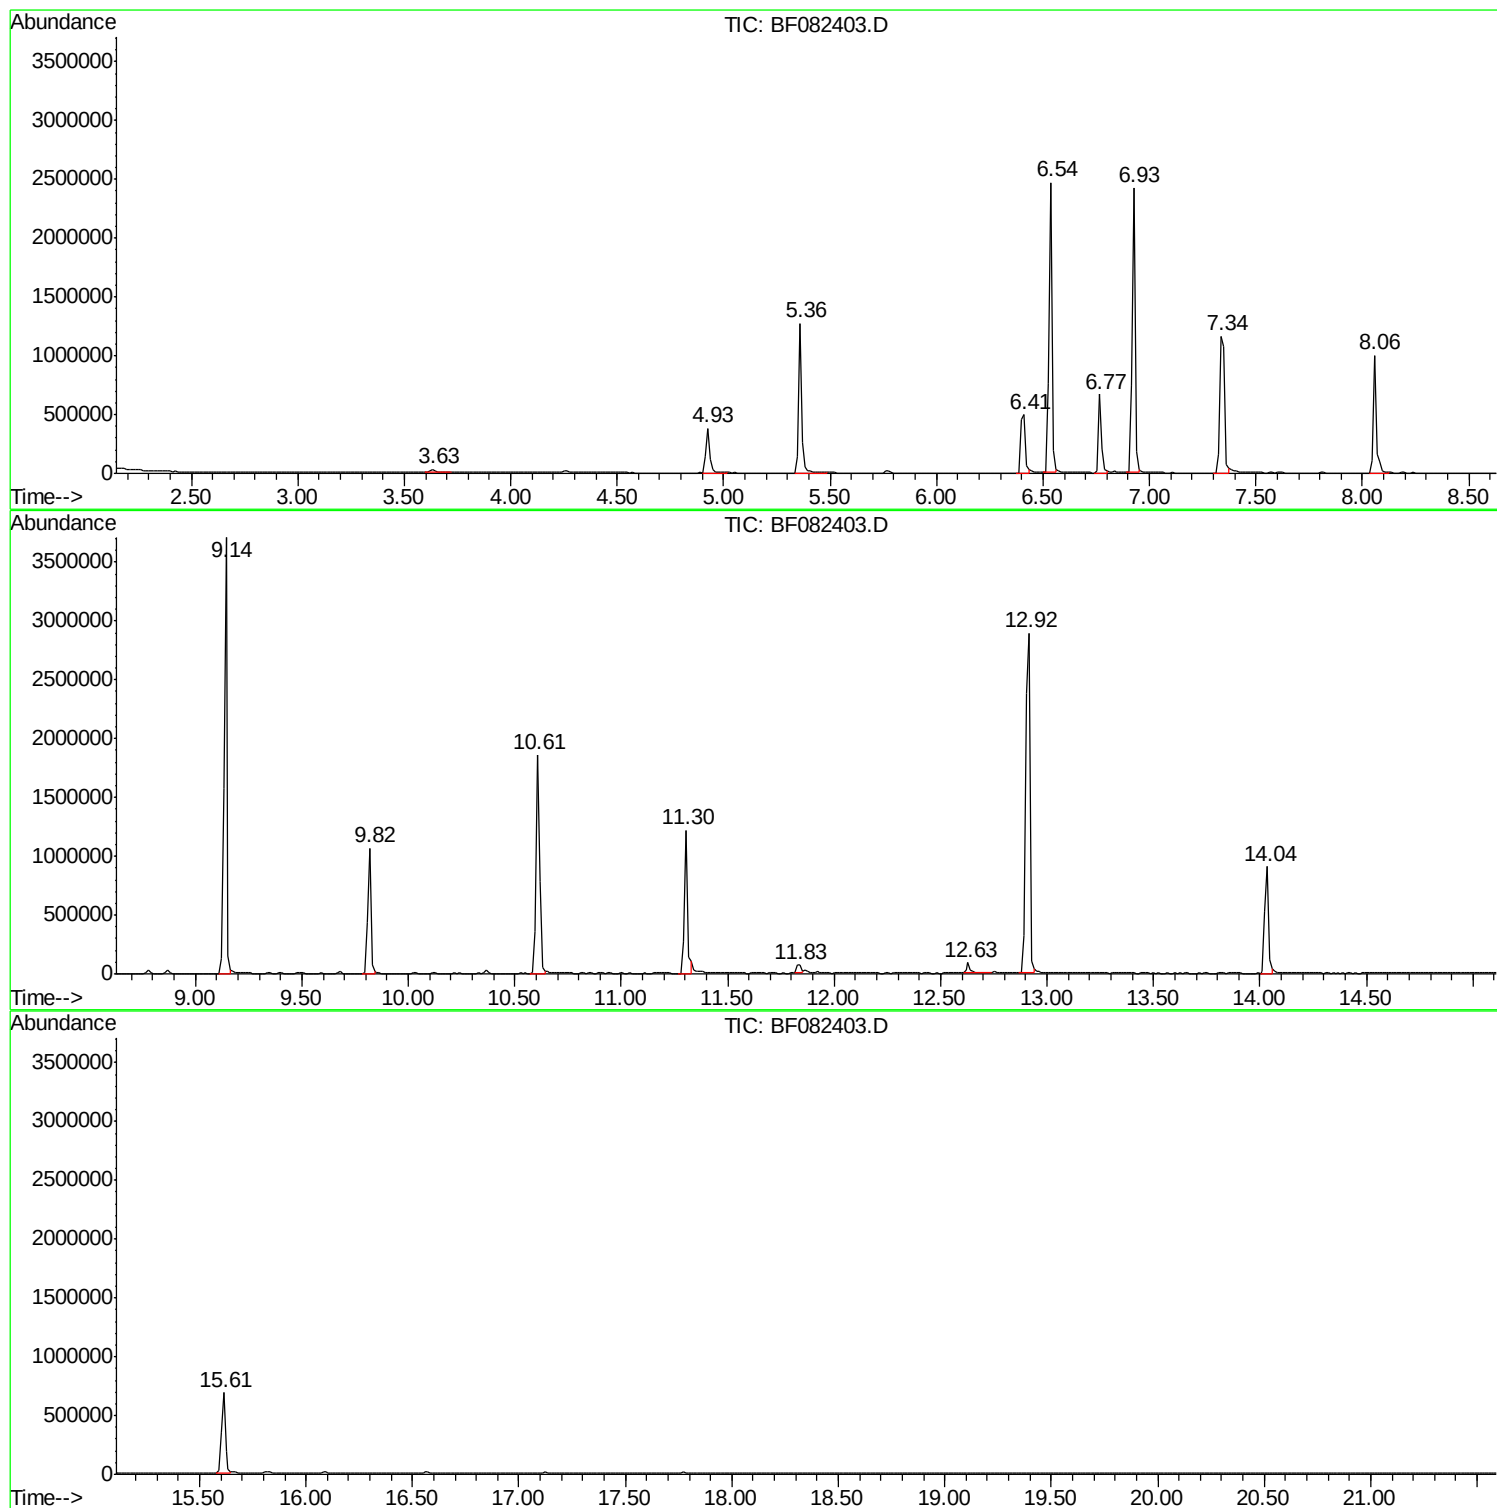

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102115\
Data File : BF082403.D
Acq On : 21 Oct 2015 14:42
Operator : UM/IZ
Sample : G4099-01
Misc :
ALS Vial : 5 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
20151013MGP208BRV68

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.		
4.93	14.62 ng	467436	1,4-Dichlorobenzene-d4	6.77		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56	
2	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	42	
3	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	28	
4	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23	
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9	

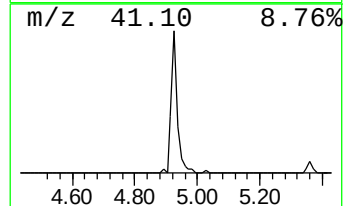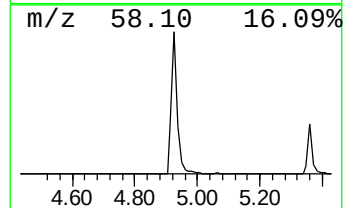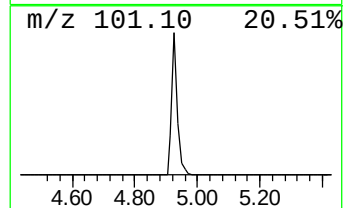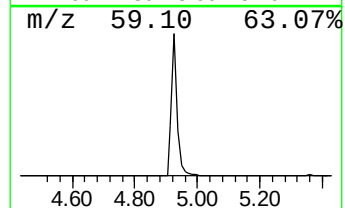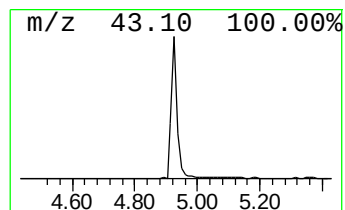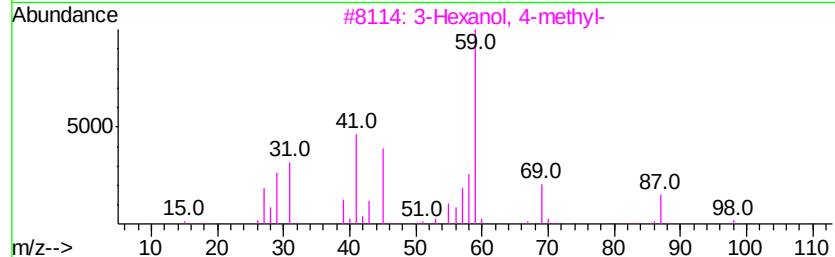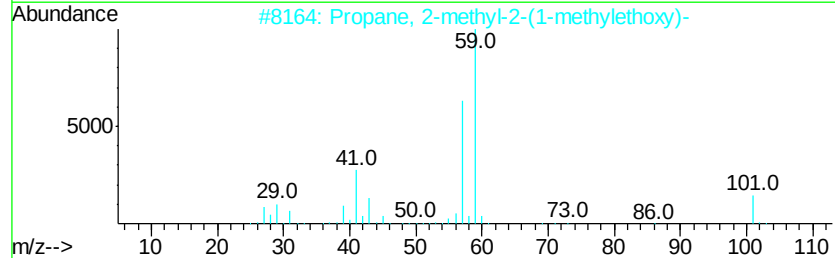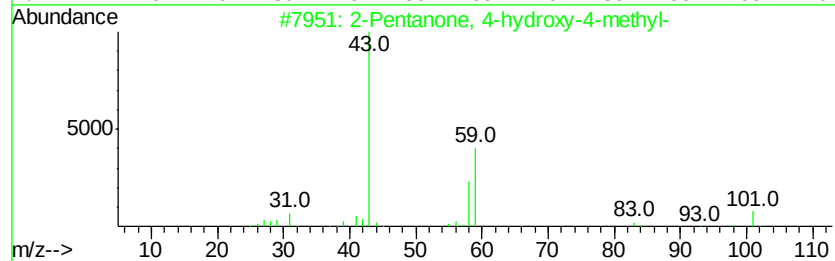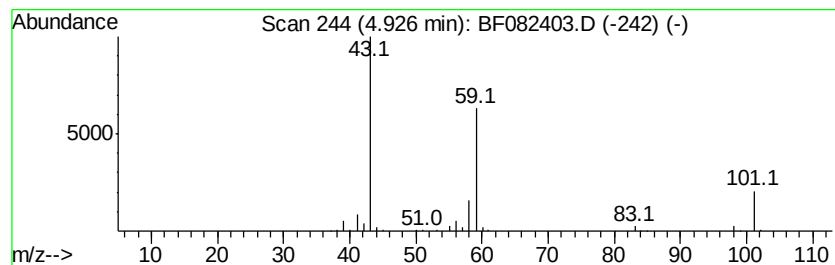

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102115\
Data File : BF082403.D
Acq On : 21 Oct 2015 14:42
Operator : UM/IZ
Sample : G4099-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20151013MGP208BRV68










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.54 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.54	73.93 ng	2362950	1,4-Dichlorobenzene-d4	6.77

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

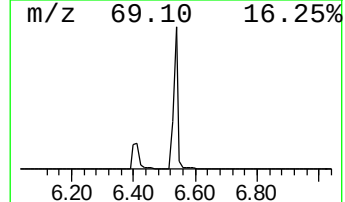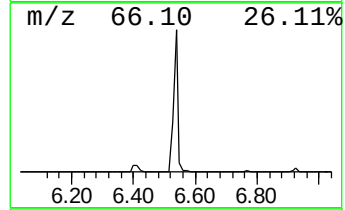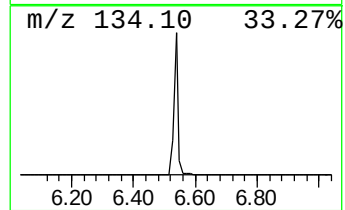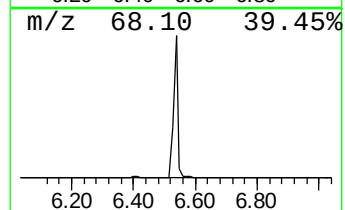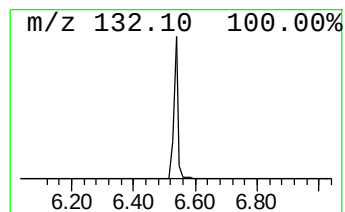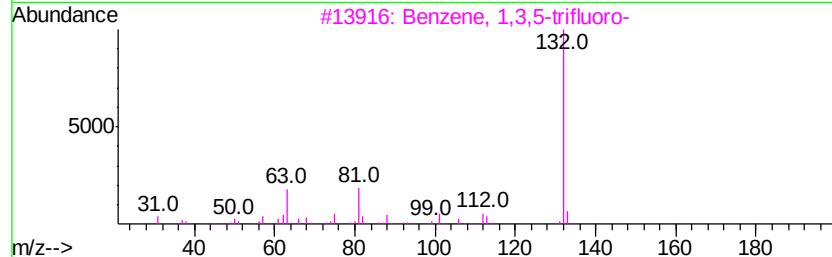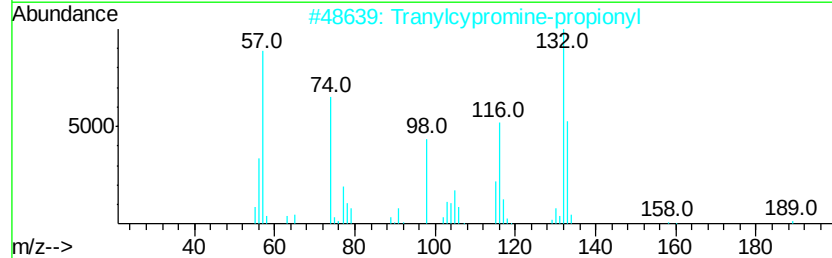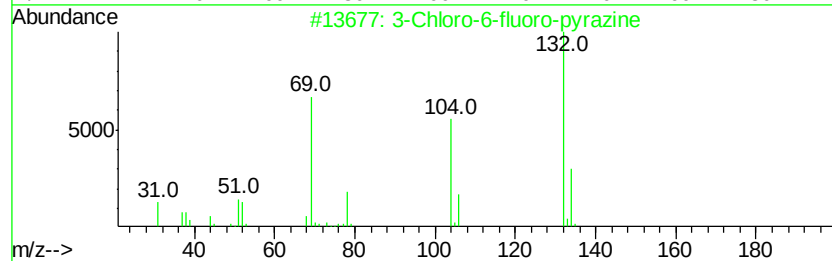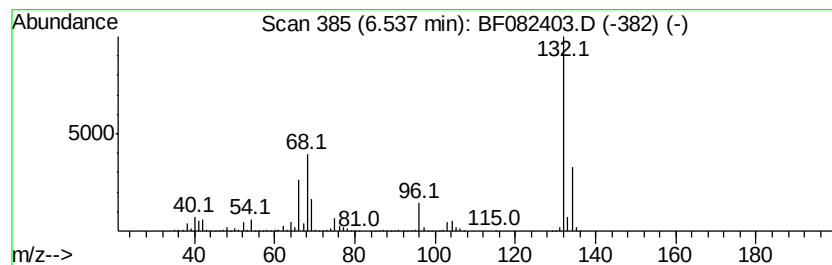

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102115\
Data File : BF082403.D
Acq On : 21 Oct 2015 14:42
Operator : UM/IZ
Sample : G4099-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20151013MGP208BRV68

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.93	14.6	ng	467436	1	6.77	639247	20.0
unknown6.54	6.54	73.9	ng	2362950	1	6.77	639247	20.0