


Data Path : Z:\HPCHEM1\BNA F\Data\BF102115\
 Data File : BF082399.D
 Acq On : 21 Oct 2015 12:26
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 21 13:20:24 2015

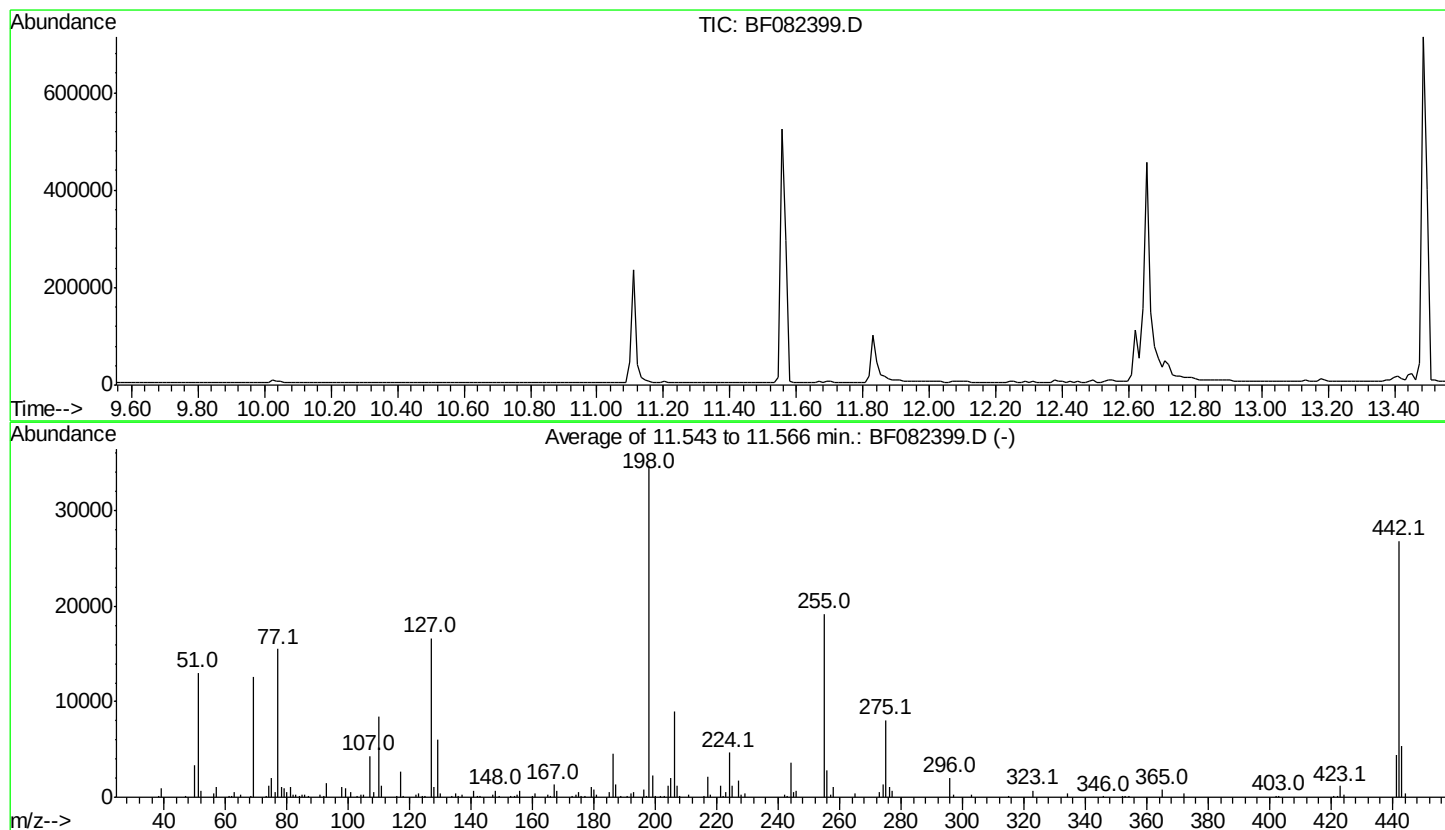

AutoFind: Scans 823, 824, 825; Background Corrected with Scan 820

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	13046	PASS
68	69	0.00	2	1.5	192	PASS
69	198	0.00	100	36.1	12550	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.9	16630	PASS
197	198	0.00	2	0.3	114	PASS
198	198	100	100	100.0	34726	PASS
199	198	5	9	6.6	2283	PASS
275	198	10	60	23.4	8112	PASS
365	198	1	100	2.2	781	PASS
441	442	0.01	24	16.3	4377	PASS
442	198	50	100	77.4	26865	PASS
443	442	15	24	19.7	5300	PASS