


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102115\
 Data File : BF082423.D
 Acq On : 22 Oct 2015 00:18
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 21 13:20:24 2015

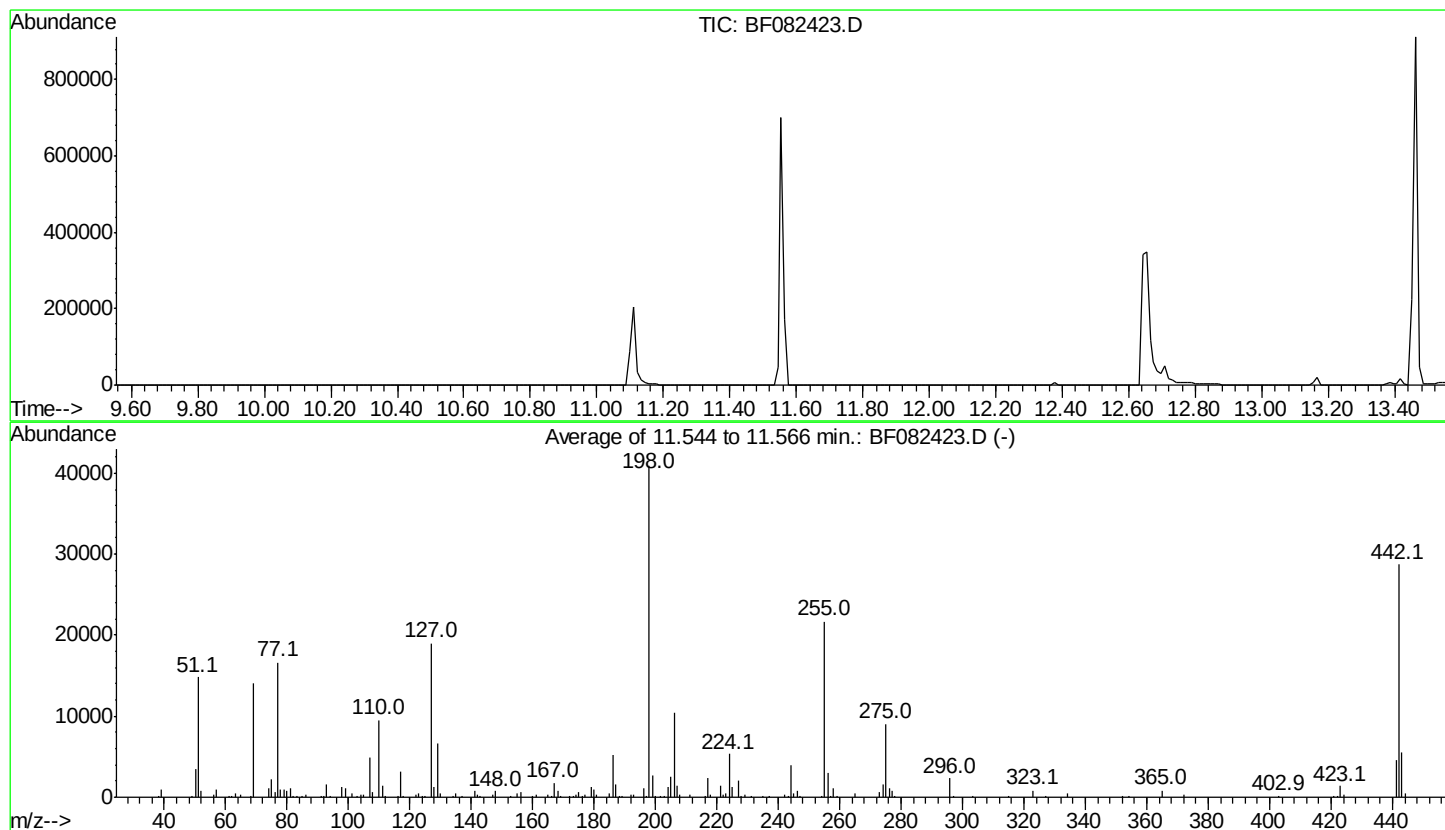

AutoFind: Scans 823, 824, 825; Background Corrected with Scan 820

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	14790	PASS
68	69	0.00	2	0.9	130	PASS
69	198	0.00	100	34.2	14014	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.4	18982	PASS
197	198	0.00	2	0.4	150	PASS
198	198	100	100	100.0	40926	PASS
199	198	5	9	6.6	2694	PASS
275	198	10	60	22.1	9065	PASS
365	198	1	100	2.1	853	PASS
441	442	0.01	24	15.9	4583	PASS
442	198	50	100	70.2	28740	PASS
443	442	15	24	19.5	5608	PASS