
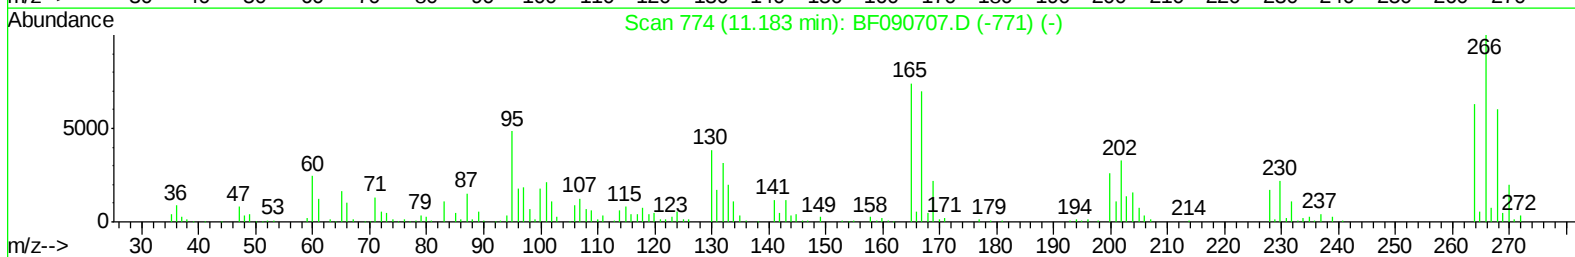
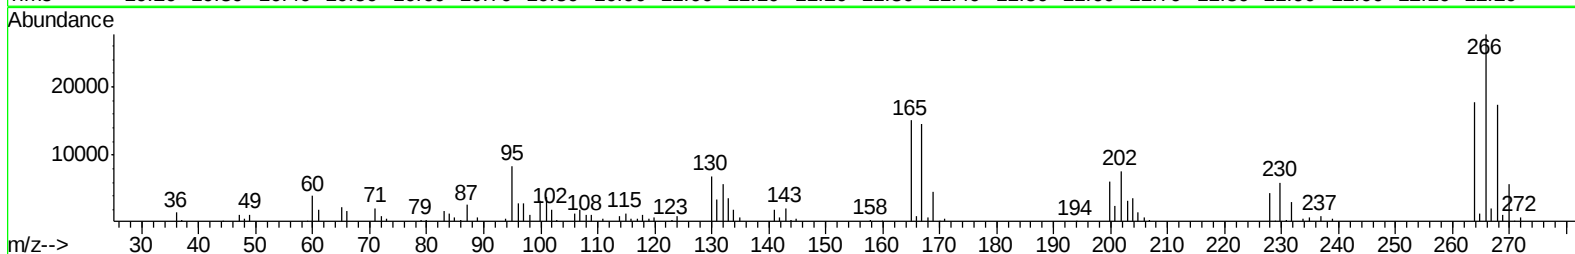


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090742.D
Acq On : 22 Oct 2016 6:01
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 04:28:16 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 21 17:36:31 2016
Response via : Initial Calibration

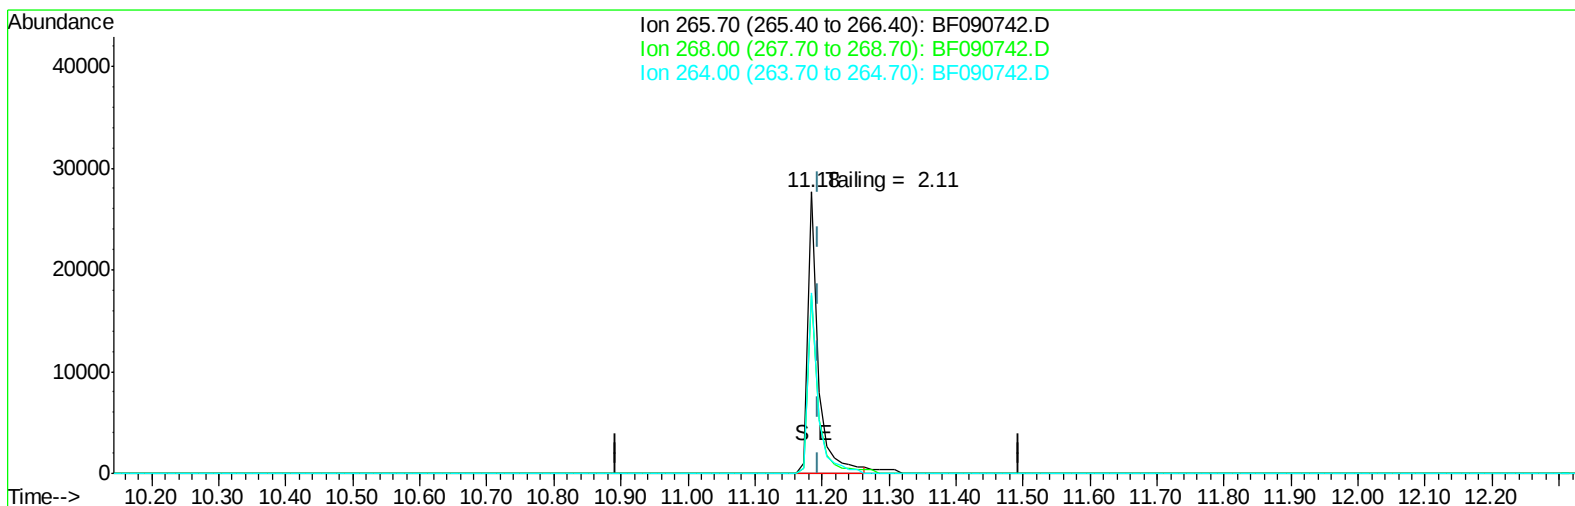

TIC: BF090742.D

(69) Pentachlorophenol (C)




11.183min (-0.011) 0.00ng

response 31033

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.08
264.00	62.70	64.30
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090742.D
Acq On : 22 Oct 2016 6:01
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 04:28:16 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 21 17:36:31 2016
Response via : Initial Calibration

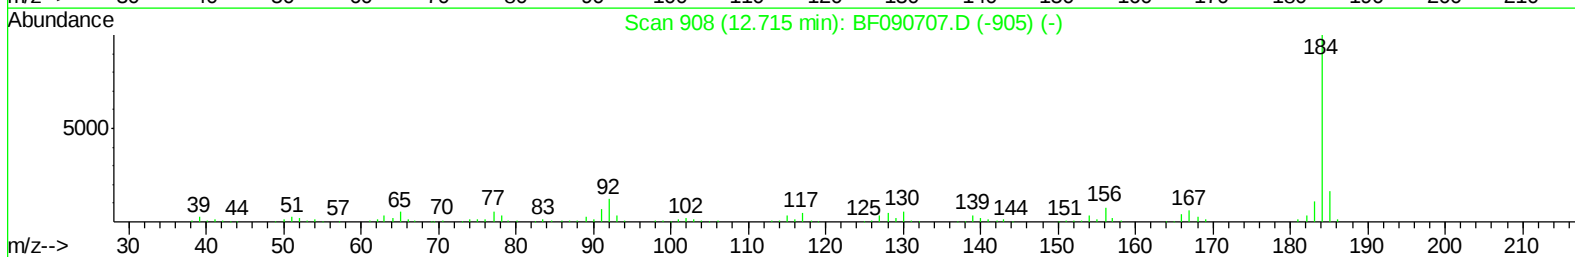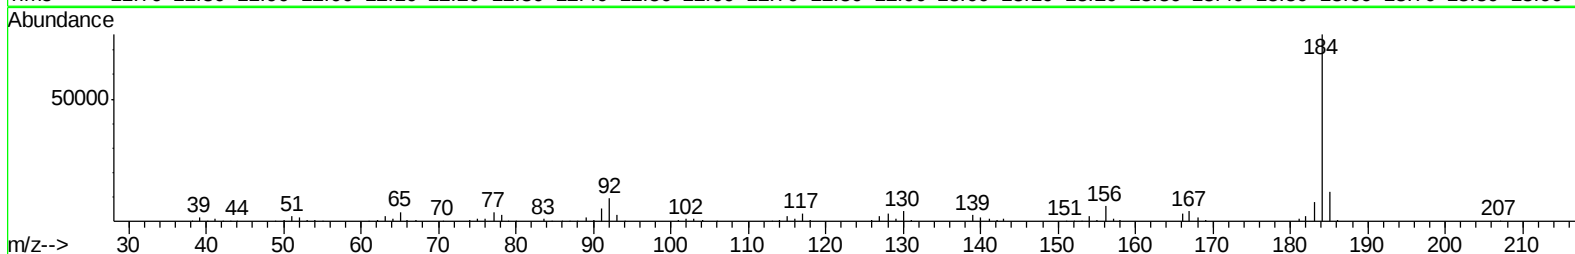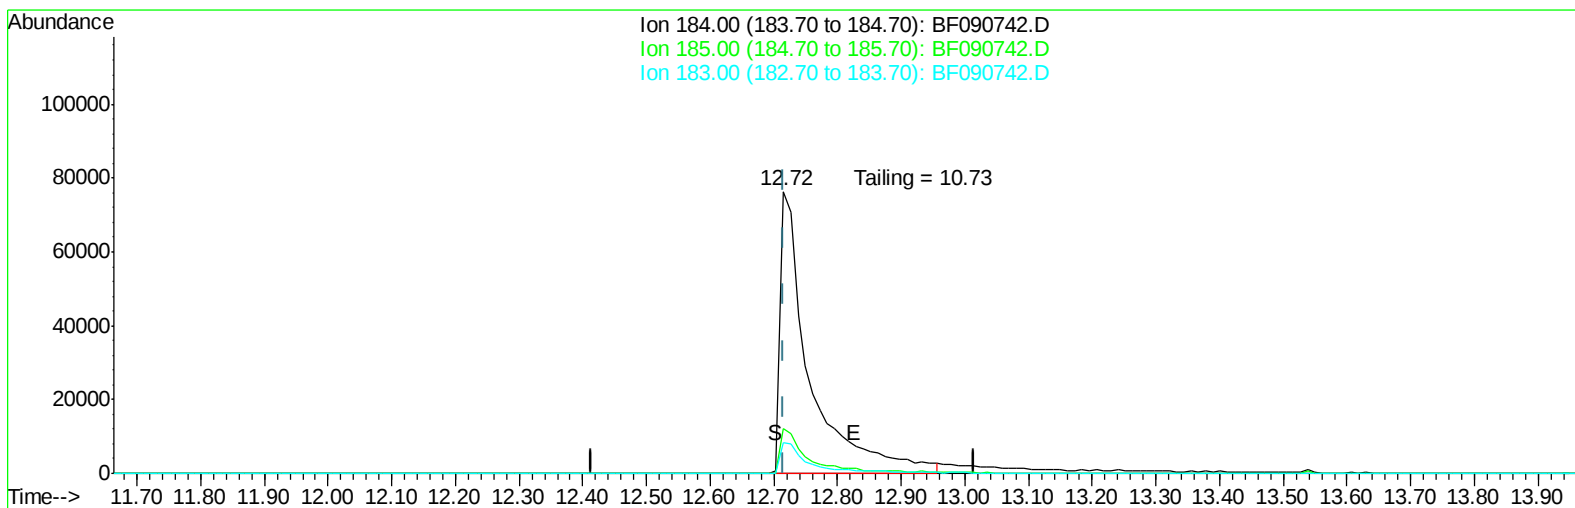

TIC: BF090742.D

(76) Benzidine

12.715min (+0.000) 0.00ng

response 246092

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	15.95
183.00	9.50	10.93
0.00	0.00	0.00