
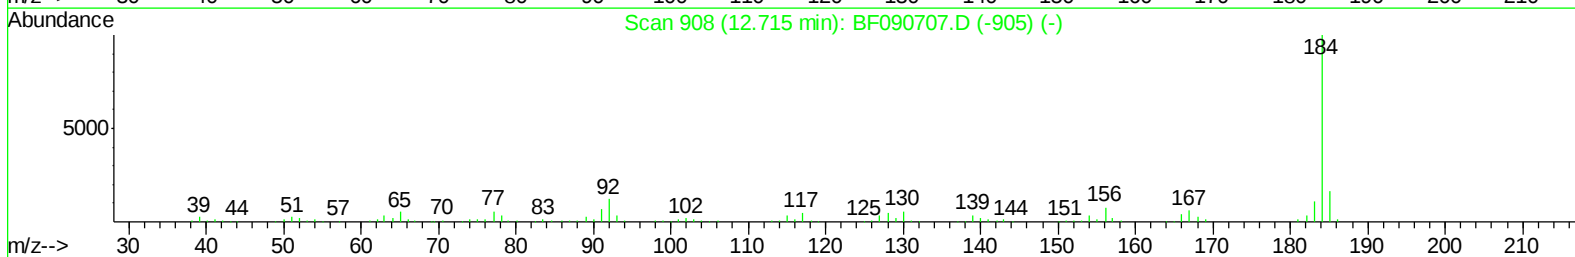
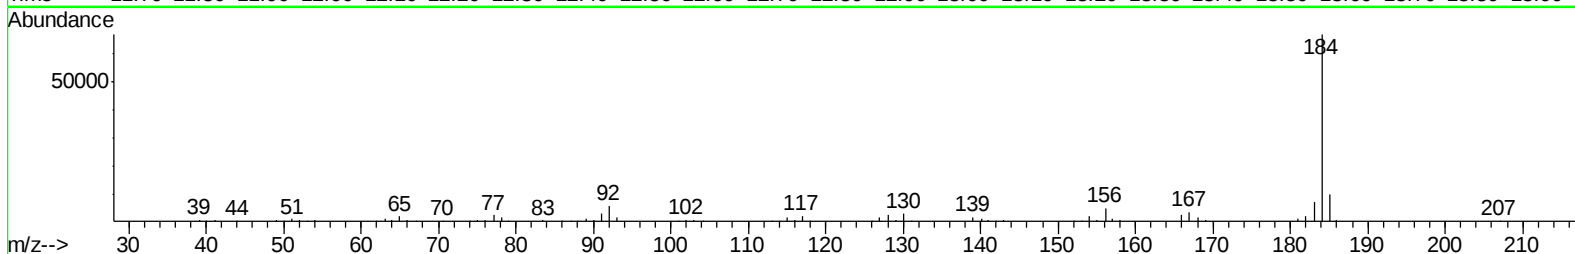


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090768.D
Acq On : 22 Oct 2016 17:54
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 04:29:12 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 21 17:36:31 2016
Response via : Initial Calibration

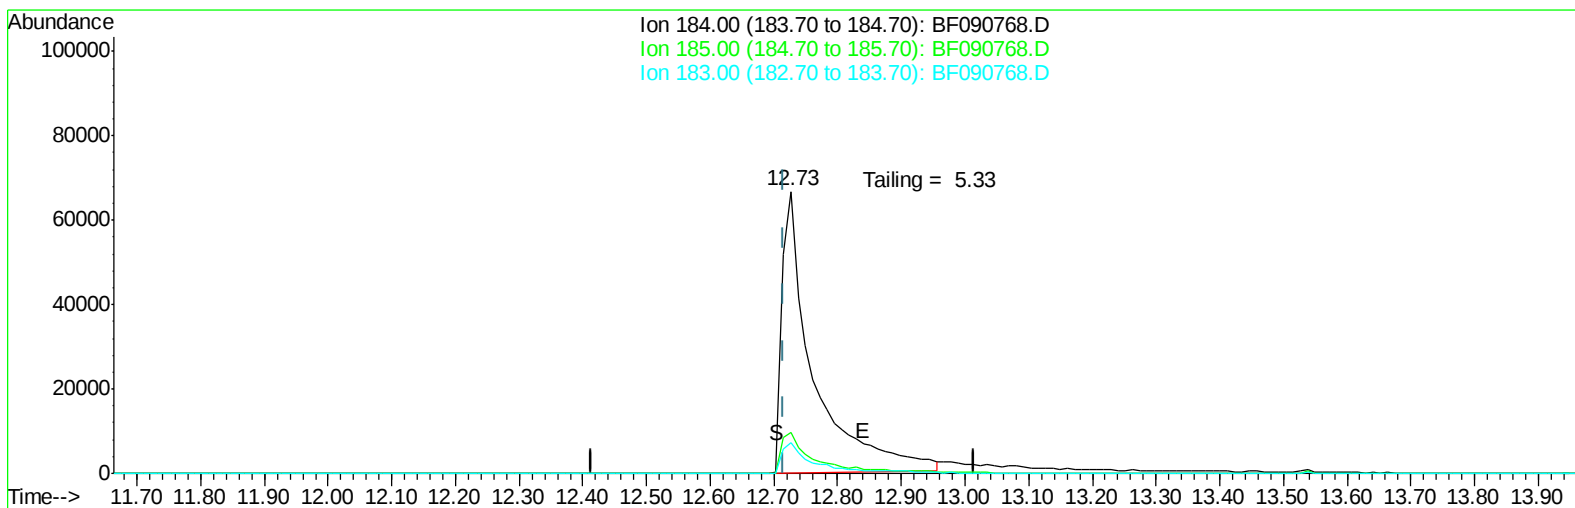

TIC: BF090768.D

(76) Benzidine




12.726min (+0.011) 0.00ng

response 233144

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.64
183.00	9.50	10.91
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090768.D
Acq On : 22 Oct 2016 17:54
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 04:29:12 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 21 17:36:31 2016
Response via : Initial Calibration

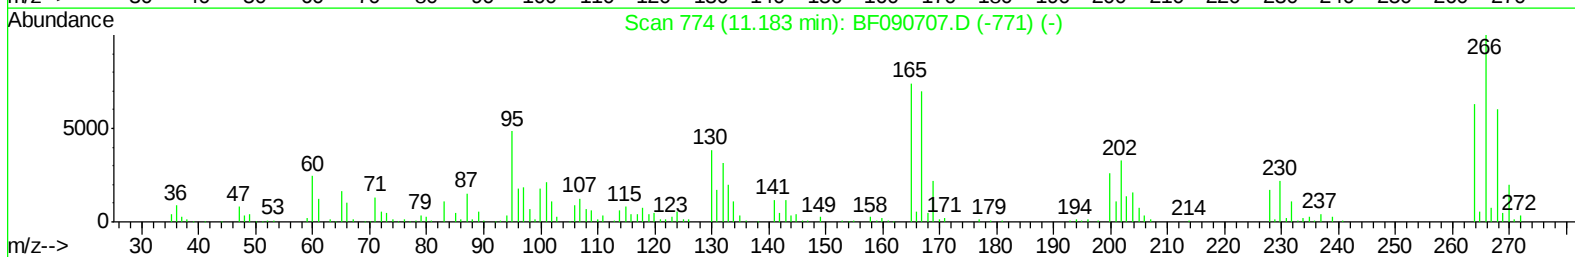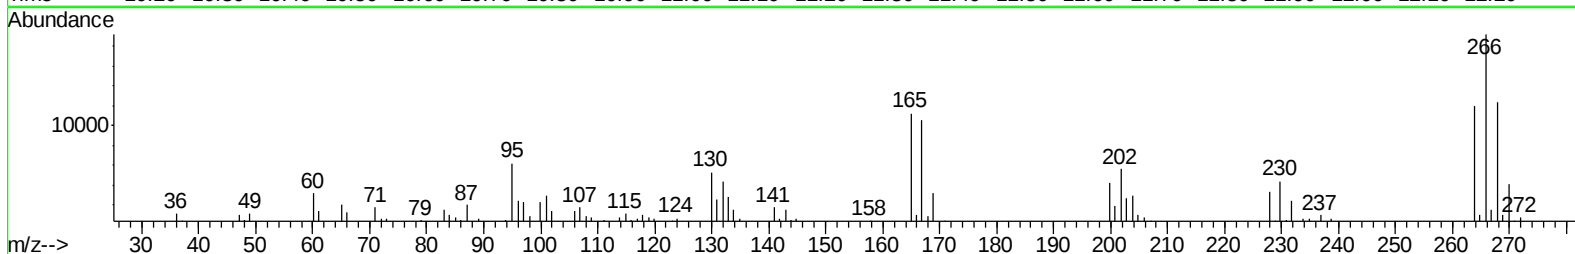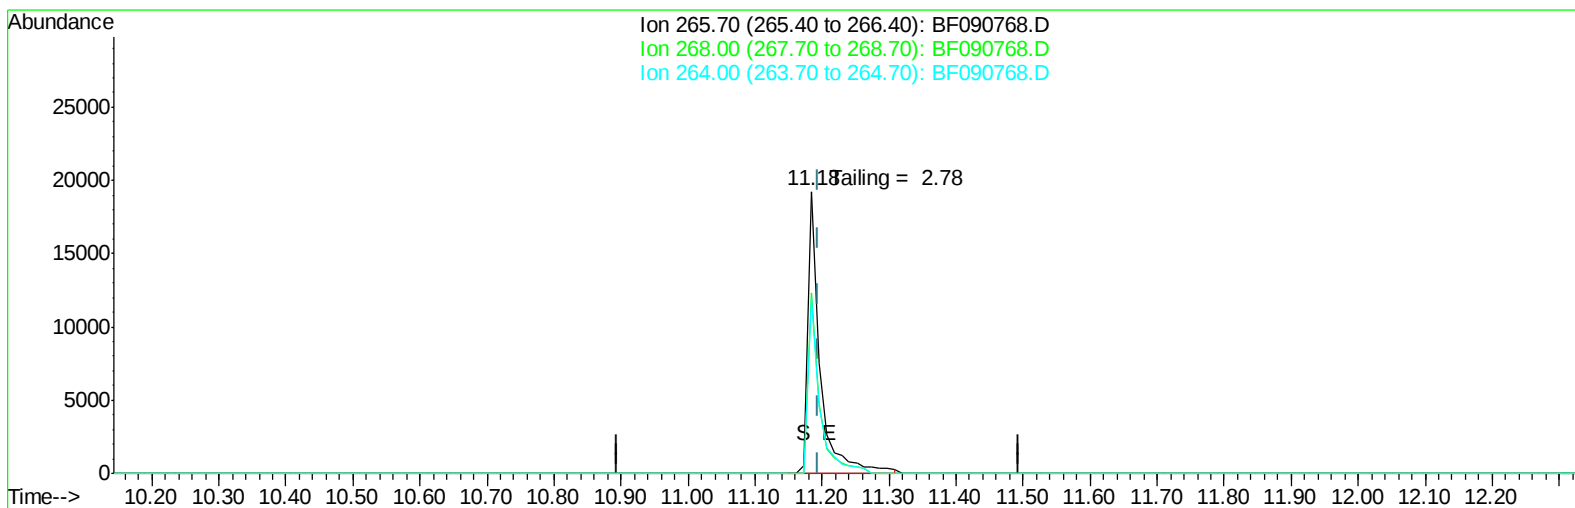

TIC: BF090768.D

(69) Pentachlorophenol (C)

11.183min (-0.011) 0.00ng

response 24589

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	64.11
264.00	62.70	62.11
0.00	0.00	0.00