

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102116\
 Data File : BF090746.D
 Acq On : 22 Oct 2016 7:51
 Operator : UM/SJ
 Sample : H5308-21
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-104D

Quant Time: Oct 24 01:11:22 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 21 17:36:31 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	256924	20.00	ng	-0.01
21) Naphthalene-d8	8.14	136	1091660	20.00	ng	0.00
38) Acenaphthene-d10	9.89	164	543633	20.00	ng	-0.01
63) Phenanthrene-d10	11.38	188	859618	20.00	ng	-0.01
75) Chrysene-d12	14.02	240	568238	20.00	ng	0.00
86) Perylene-d12	15.46	264	385644	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	1157840	72.68	ng	0.01
7) Phenol-d6	6.50	99	1254716	58.15	ng	0.00
23) Nitrobenzene-d5	7.42	82	1782002	89.53	ng	0.00
41) 2,4,6-Tribromophenol	10.69	330	732927	170.34	ng	0.00
44) 2-Fluorobiphenyl	9.22	172	2775261	79.25	ng	-0.01
78) Terphenyl-d14	12.97	244	2780155	112.13	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.62	163	130182	3.81	ng	Qvalue # 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102116\
Data File : BF090746.D
Acq On : 22 Oct 2016 7:51
Operator : UM/SJ
Sample : H5308-21
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-104D

Quant Time: Oct 24 01:11:22 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 21 17:36:31 2016
Response via : Initial Calibration

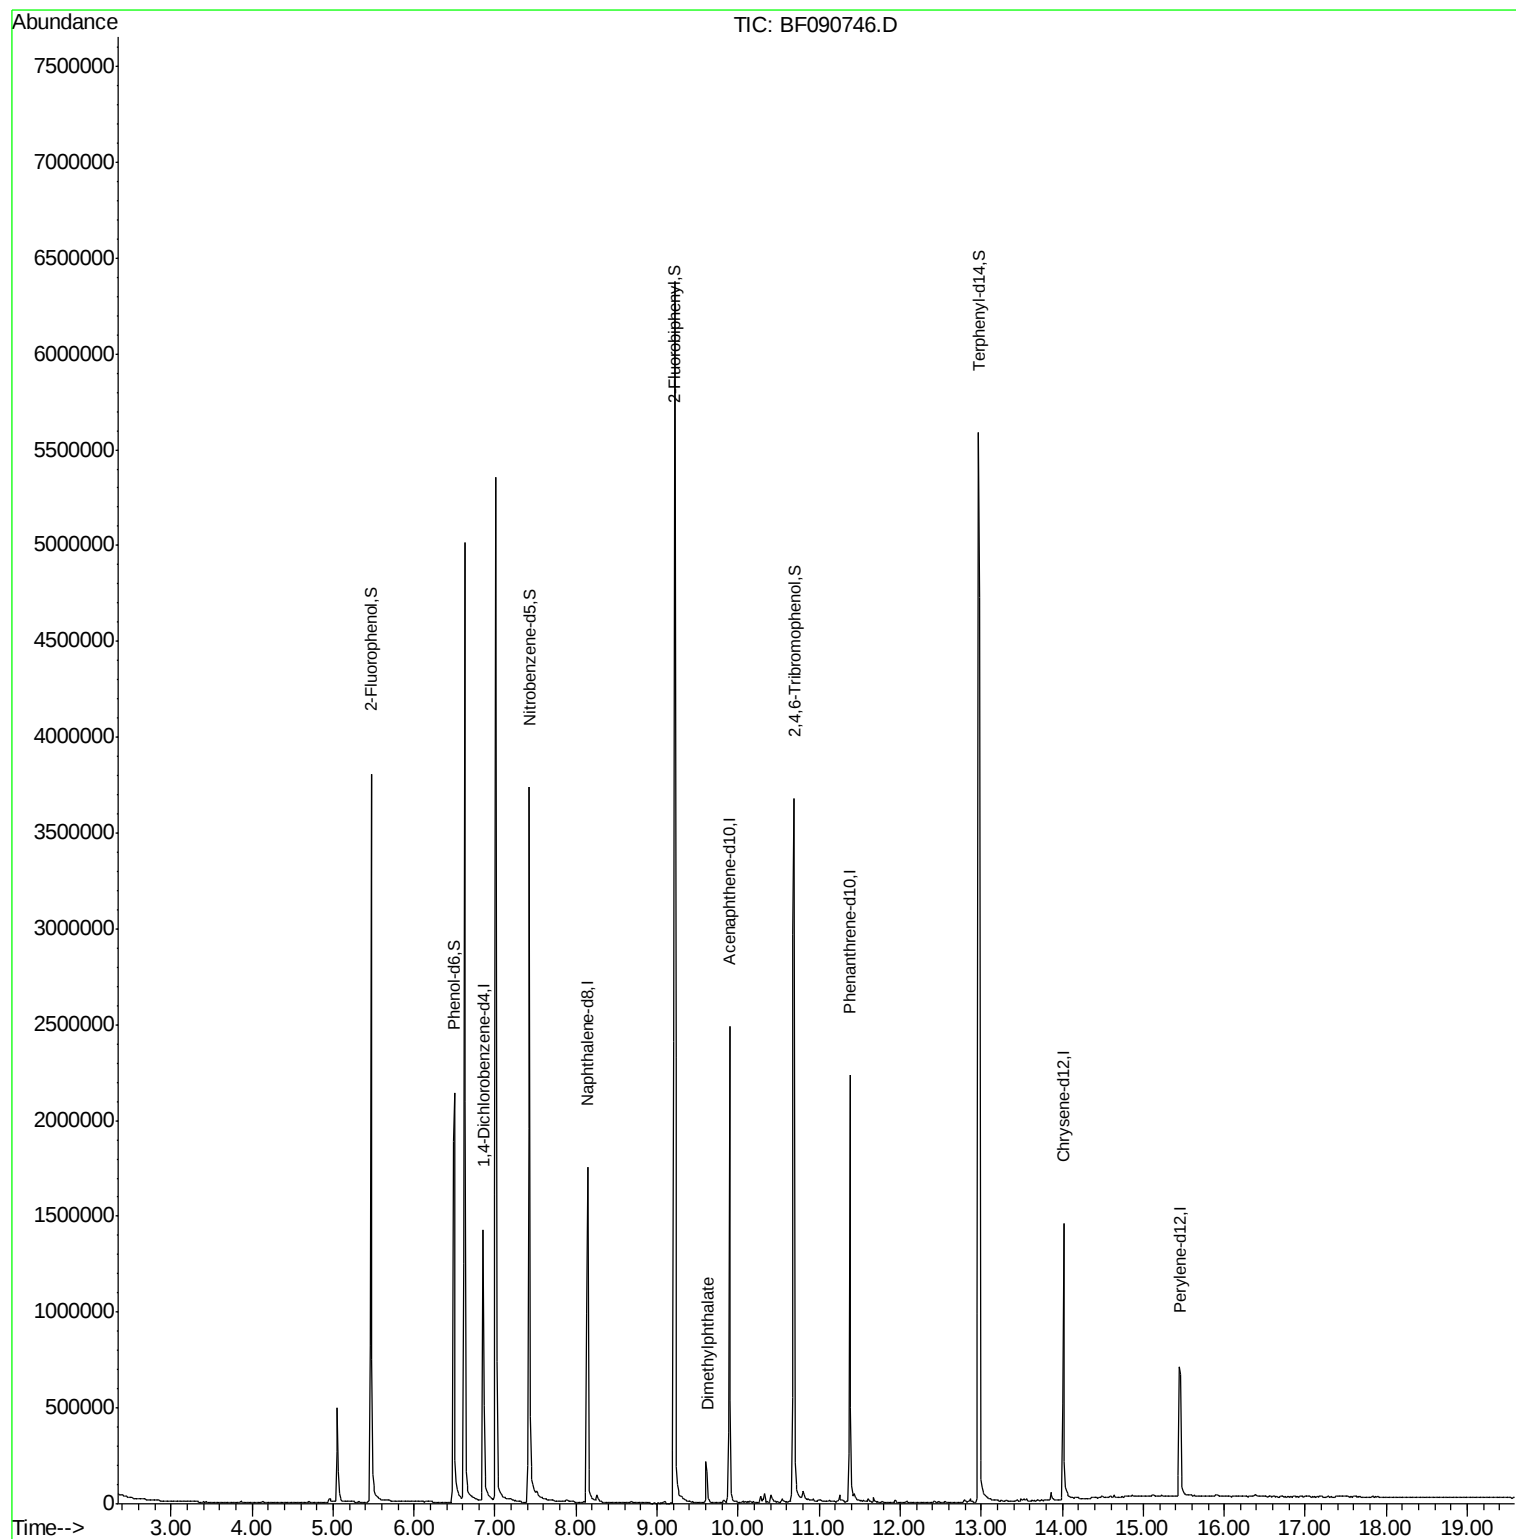

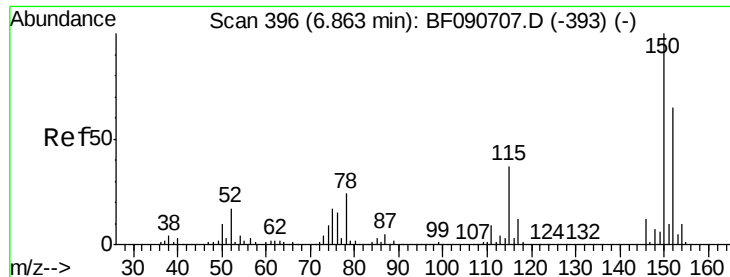

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.85 min Scan# 395

Delta R.T. -0.01 min

Lab File: BF090746.D

Acq: 22 Oct 2016 7:51

Instrument :

BNA_F

ClientSampleId :

MW-104D


Tot Ion:152 Resp: 256924

Ion Ratio Lower Upper

152 100

150 156.8 124.7 187.1




115 70.0 39.0 58.4#

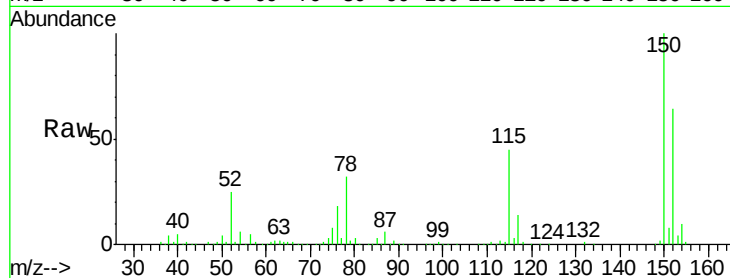

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

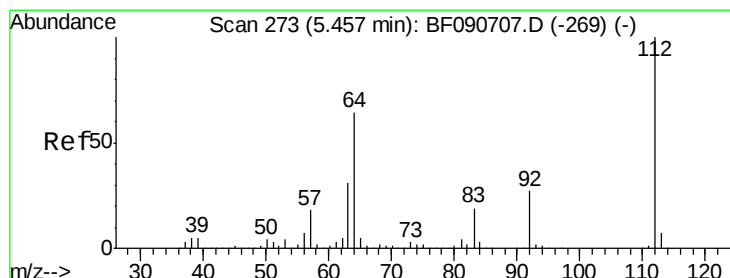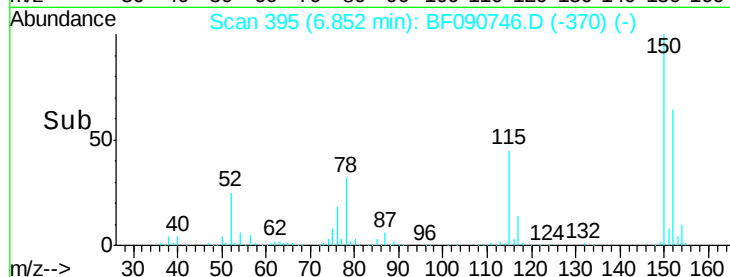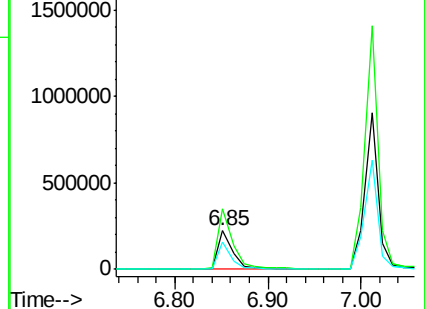

#5

2-Fluorophenol

Concen: 72.68 ng

RT: 5.47 min Scan# 274

Delta R.T. 0.01 min

Lab File: BF090746.D

Acq: 22 Oct 2016 7:51


Tgt Ion:112 Resp: 1157840

Ion Ratio Lower Upper

112 100

64 65.0 39.7 59.5#



63 32.0 17.4 26.0#

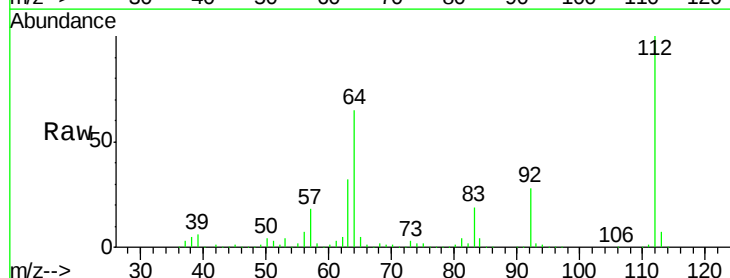


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

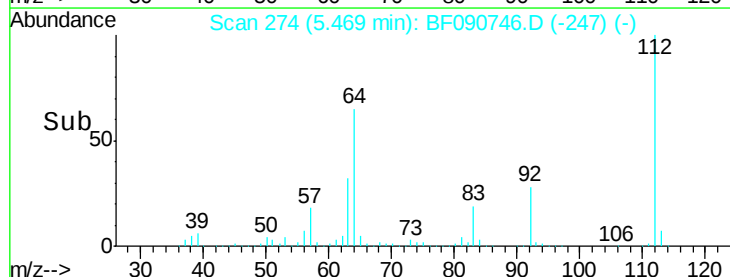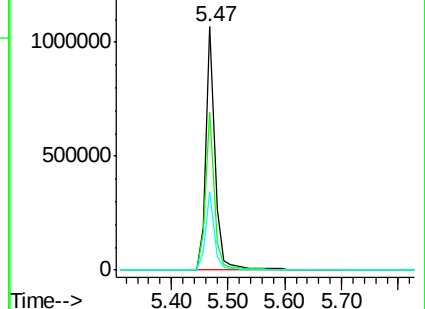

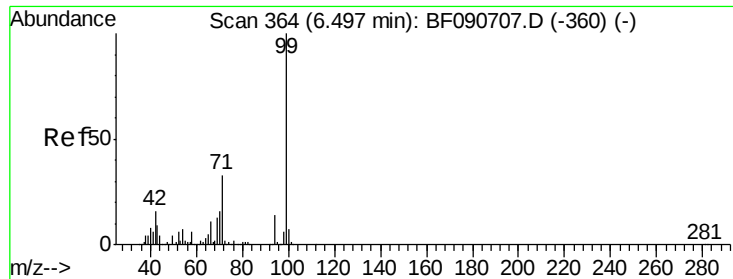

#7

Phenol-d6

Concen: 58.15 ng

RT: 6.50 min Scan# 364

Delta R.T. 0.00 min

Lab File: BF090746.D

Acq: 22 Oct 2016 7:51

Instrument :

BNA_F

ClientSampleId :

MW-104D





Tot Ion: 99 Resp: 1254716

Ion Ratio Lower Upper

99 100

42 12.2 13.7 20.5#

71 28.8 14.2 21.2#

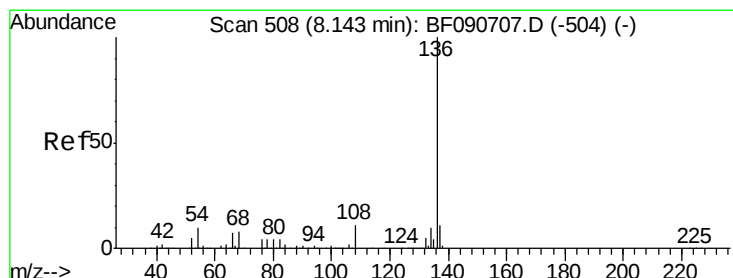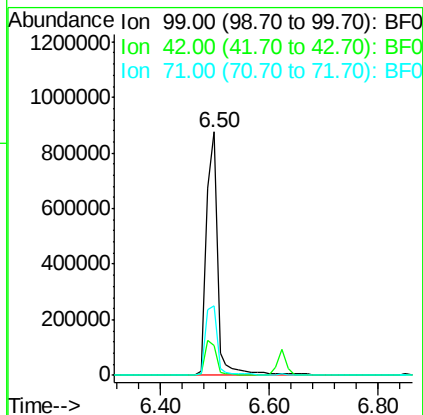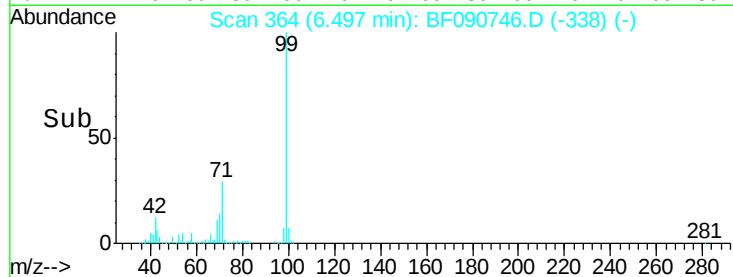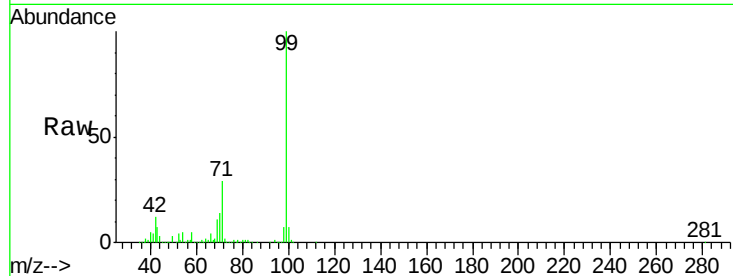

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.14 min Scan# 508

Delta R.T. 0.00 min

Lab File: BF090746.D

Acq: 22 Oct 2016 7:51

Tgt Ion: 136 Resp: 1091660




Ion Ratio Lower Upper


136 100

137 11.1 9.0 13.6

54 7.2 8.2 12.2#

68 6.5 5.8 8.6


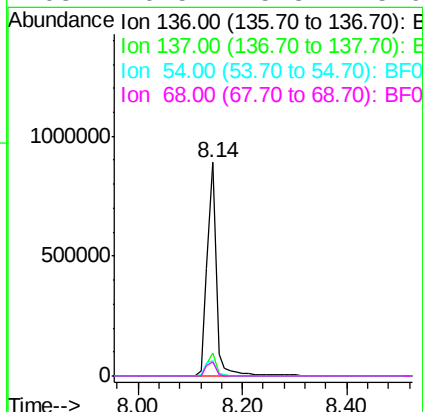
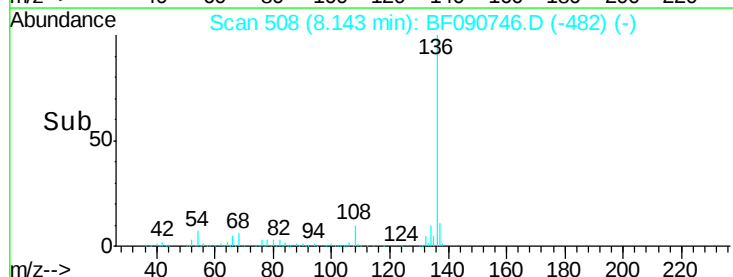
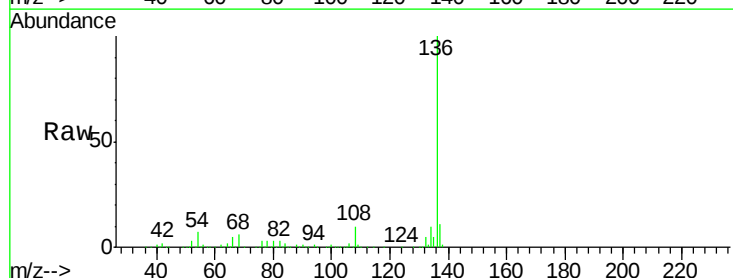


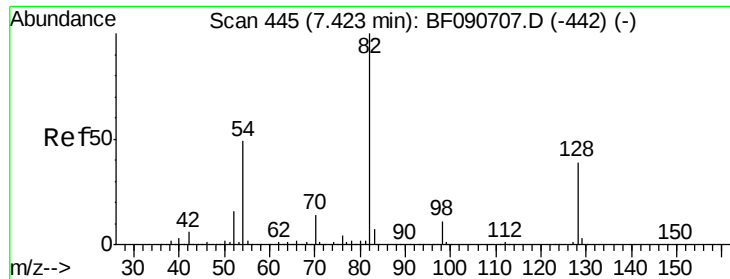

#23
 Nitrobenzene-d5
 Concen: 89.53 ng
 RT: 7.42 min Scan# 445
 Delta R.T. 0.00 min
 Lab File: BF090746.D
 Acq: 22 Oct 2016 7:51




Instrument :
 BNA_F
 ClientSampleId :
 MW-104D


Tot Ion: 82 Resp: 1782002
 Ion Ratio Lower Upper
 82 100
 128 45.1 51.0 76.6#
 54 46.6 47.5 71.3#

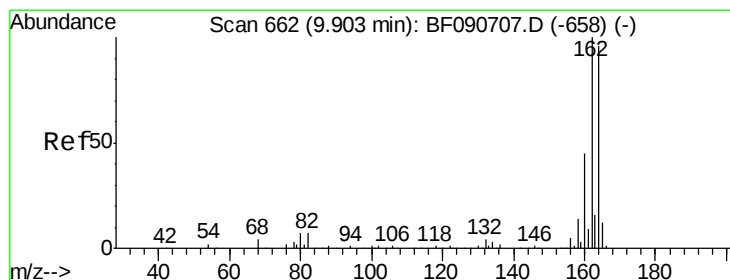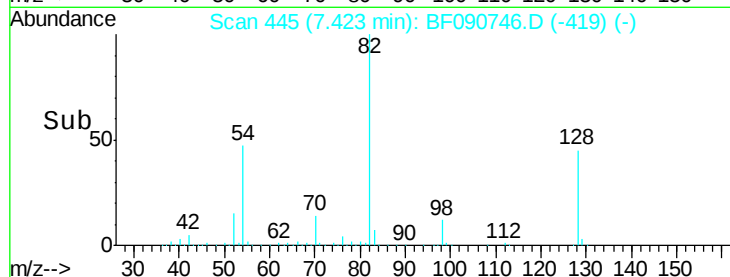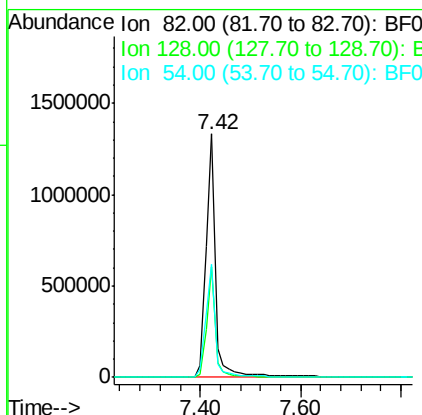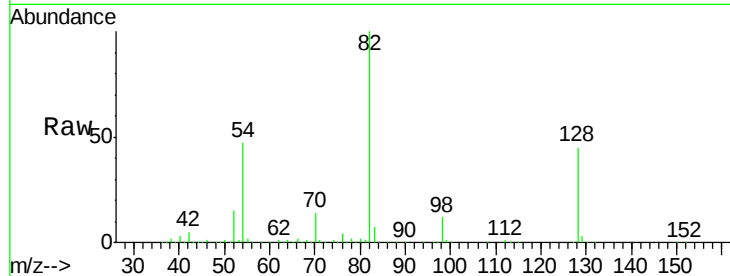

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.89 min Scan# 661
 Delta R.T. -0.01 min
 Lab File: BF090746.D
 Acq: 22 Oct 2016 7:51

Tgt Ion:164 Resp: 543633
 Ion Ratio Lower Upper
 164 100
 162 105.5 75.2 112.8
 160 47.7 31.5 47.3#


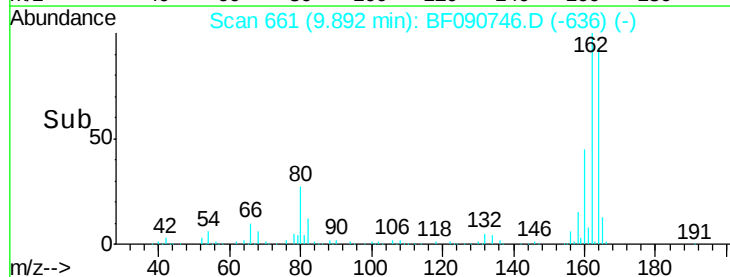
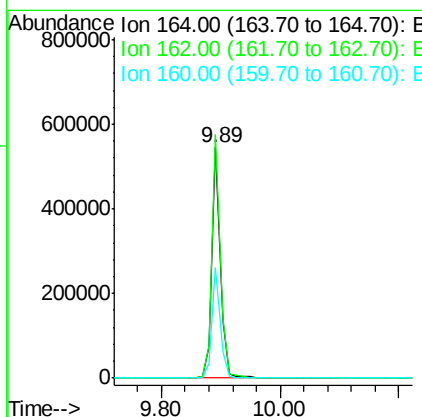
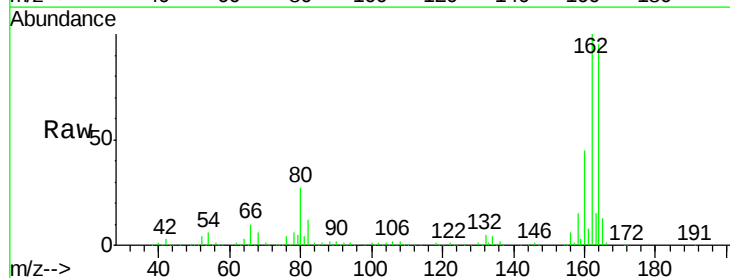


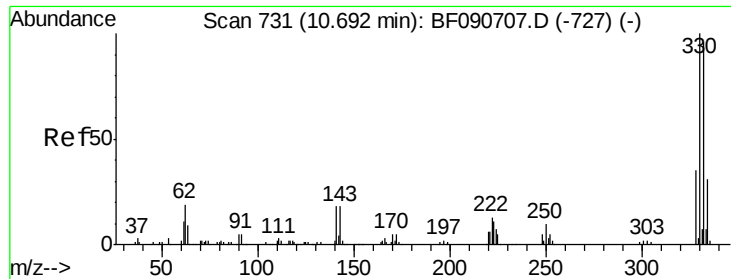

#41
 2,4,6-Tribromophenol
 Concen: 170.34 ng
 RT: 10.69 min Scan# 731
 Delta R.T. 0.00 min
 Lab File: BF090746.D
 Acq: 22 Oct 2016 7:51




Instrument :
 BNA_F
 ClientSampleId :
 MW-104D


Tot Ion	Ratio	Lower	Upper
330	100		
332	95.1	76.6	114.8
141	32.7	29.7	44.5

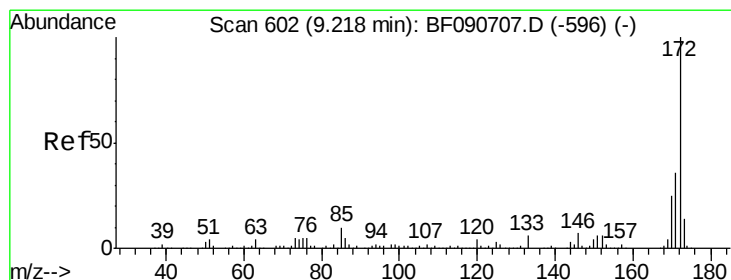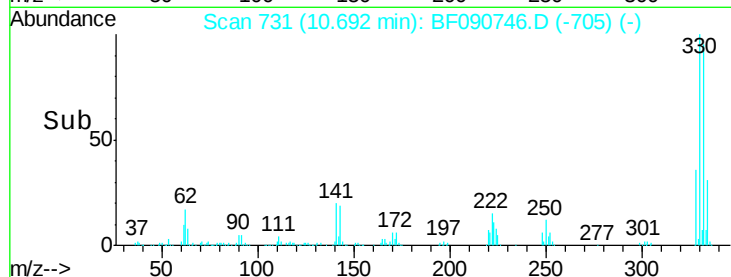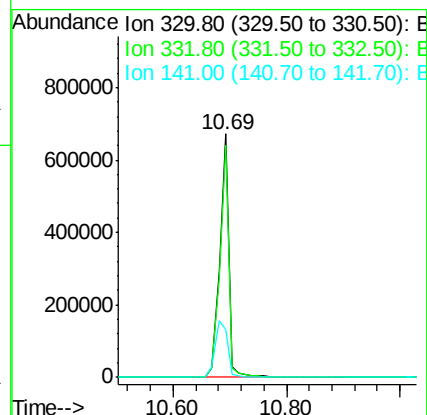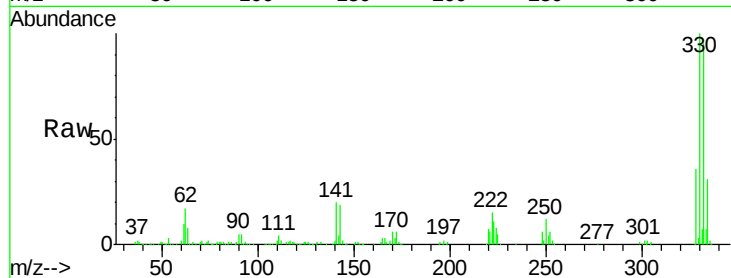

#44
 2-Fluorobiphenyl
 Concen: 79.25 ng
 RT: 9.22 min Scan# 602
 Delta R.T. -0.01 min
 Lab File: BF090746.D
 Acq: 22 Oct 2016 7:51

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.8	26.1	39.1
170	25.9	17.4	26.2

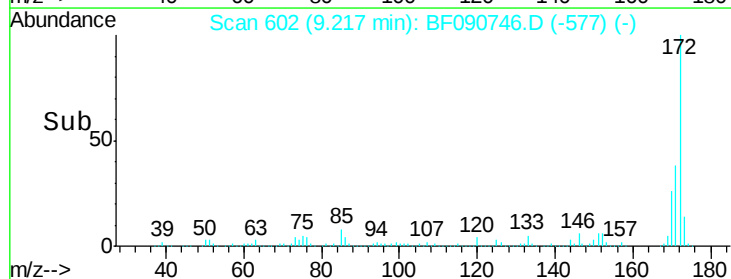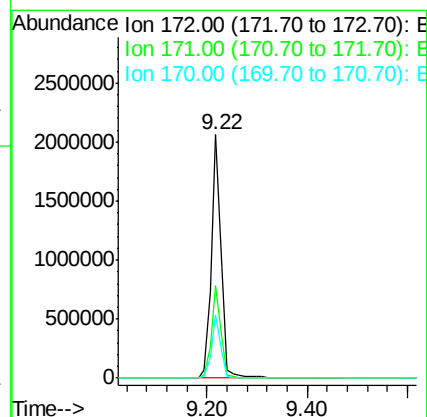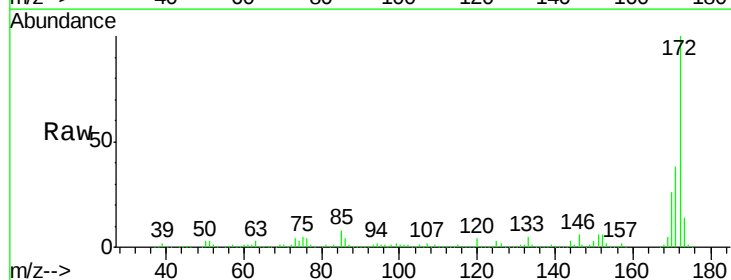


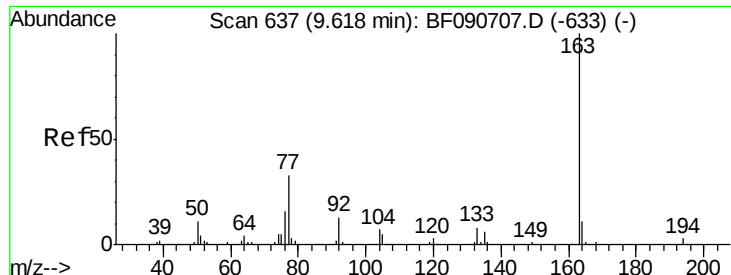




#49
Dimethylphthalate
Concen: 3.81 ng
RT: 9.62 min Scan# 637
Delta R.T. -0.01 min
Lab File: BF090746.D
Acq: 22 Oct 2016 7:51

Instrument :
BNA_F
ClientSampleId :
MW-104D

Tot Ion:163 Resp: 130182
Ion Ratio Lower Upper
163 100
194 3.5 4.4 6.6#
164 9.5 8.3 12.5

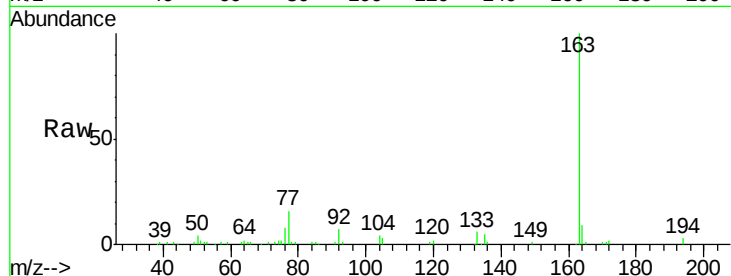


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

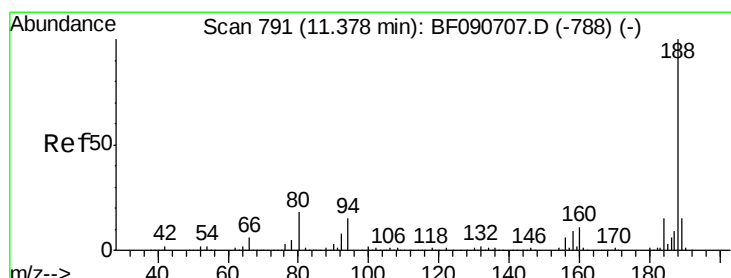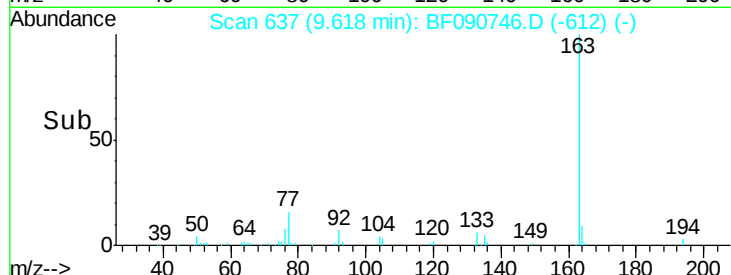
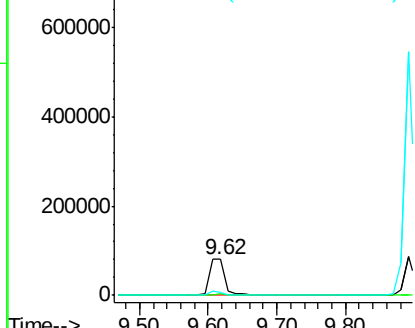



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.38 min Scan# 791
Delta R.T. -0.01 min
Lab File: BF090746.D
Acq: 22 Oct 2016 7:51

Tgt Ion:188 Resp: 859618
Ion Ratio Lower Upper
188 100
94 13.2 11.1 16.7
80 14.9 11.0 16.4

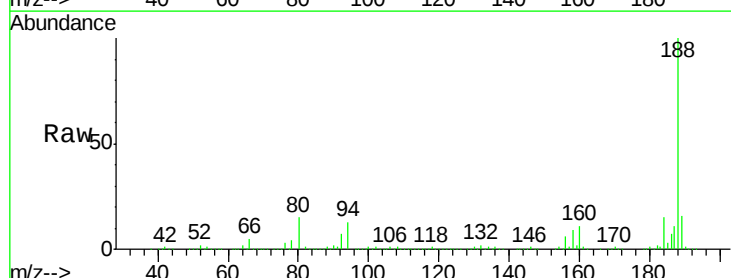

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

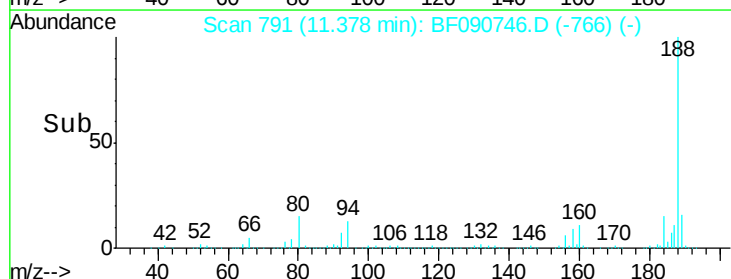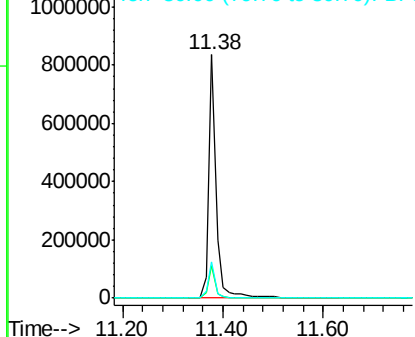

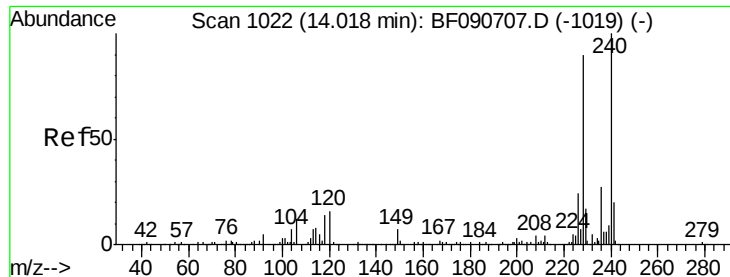

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.02 min Scan# 1022

Delta R.T. 0.00 min

Lab File: BF090746.D

Acq: 22 Oct 2016 7:51

Instrument :

BNA_F

ClientSampleId :

MW-104D


Tot Ion:240 Resp: 568238

Ion Ratio Lower Upper

240 100

120 12.0 16.2 24.2#




236 27.1 18.4 27.6

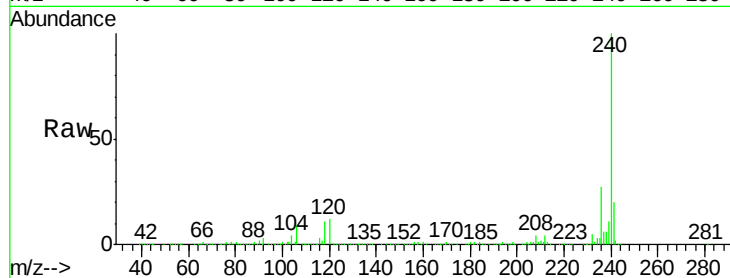

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

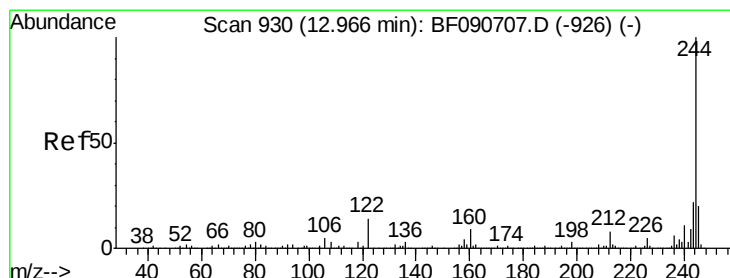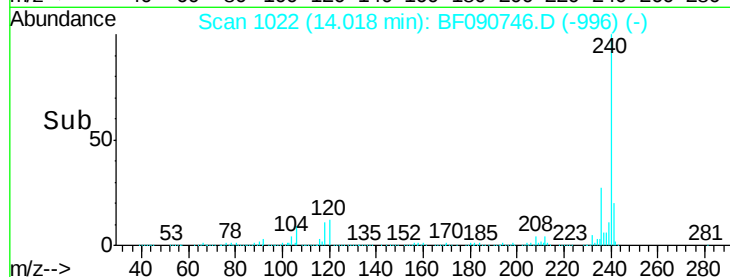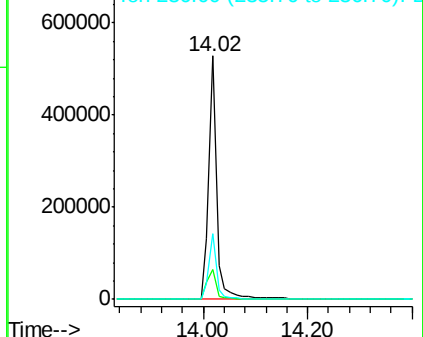

#78

Terphenyl-d14

Concen: 112.13 ng

RT: 12.97 min Scan# 930

Delta R.T. 0.00 min

Lab File: BF090746.D

Acq: 22 Oct 2016 7:51


Tgt Ion:244 Resp: 2780155

Ion Ratio Lower Upper

244 100

212 7.8 4.3 6.5#



122 14.6 17.4 26.2#

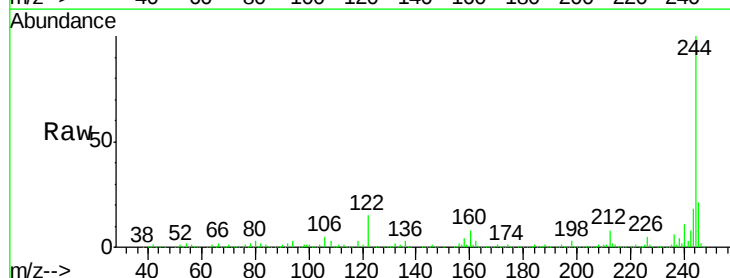


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

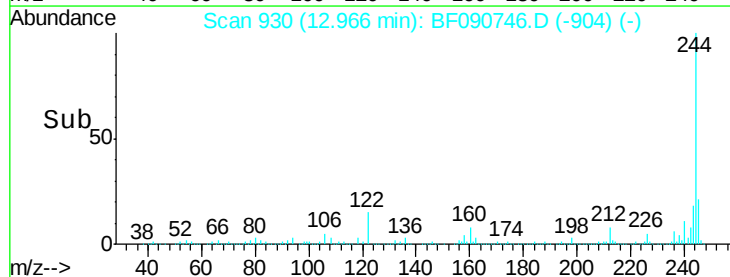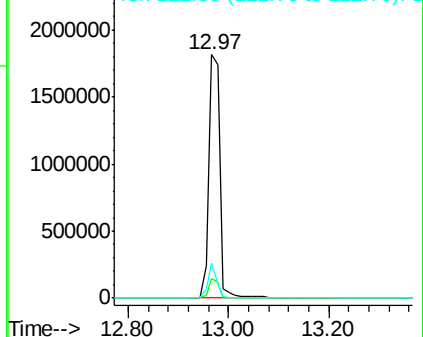


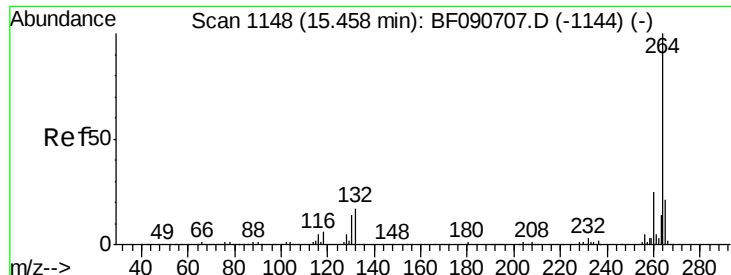

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.46 min Scan# 1148
Delta R.T. 0.00 min
Lab File: BF090746.D
Acq: 22 Oct 2016 7:51

Instrument :
BNA_F
ClientSampleId :
MW-104D

Tot Ion:264 Resp: 385644
Ion Ratio Lower Upper
264 100
260 25.0 16.7 25.1
265 21.0 17.2 25.8

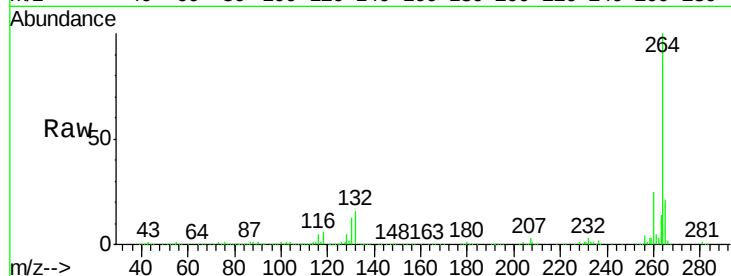

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

