

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102116\
 Data File : BF090748.D
 Acq On : 22 Oct 2016 8:46
 Operator : UM/SJ
 Sample : H5308-23
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-103D

Quant Time: Oct 24 01:16:02 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 21 17:36:31 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	252824	20.00	ng	-0.01
21) Naphthalene-d8	8.14	136	1075996	20.00	ng	0.00
38) Acenaphthene-d10	9.89	164	543955	20.00	ng	-0.01
63) Phenanthrene-d10	11.38	188	849026	20.00	ng	-0.01
75) Chrysene-d12	14.02	240	578052	20.00	ng	0.00
86) Perylene-d12	15.45	264	388396	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	1013968	64.68	ng	0.01
7) Phenol-d6	6.49	99	781688	36.81	ng	-0.01
23) Nitrobenzene-d5	7.42	82	1694925	86.40	ng	0.00
41) 2,4,6-Tribromophenol	10.69	330	702467	163.16	ng	0.00
44) 2-Fluorobiphenyl	9.22	172	2579259	73.61	ng	-0.01
78) Terphenyl-d14	12.98	244	2742919	108.75	ng	0.01
Target Compounds						
49) Dimethylphthalate	9.61	163	120028	3.51	ng	Qvalue # 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102116\
Data File : BF090748.D
Acq On : 22 Oct 2016 8:46
Operator : UM/SJ
Sample : H5308-23
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-103D

Quant Time: Oct 24 01:16:02 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 21 17:36:31 2016
Response via : Initial Calibration

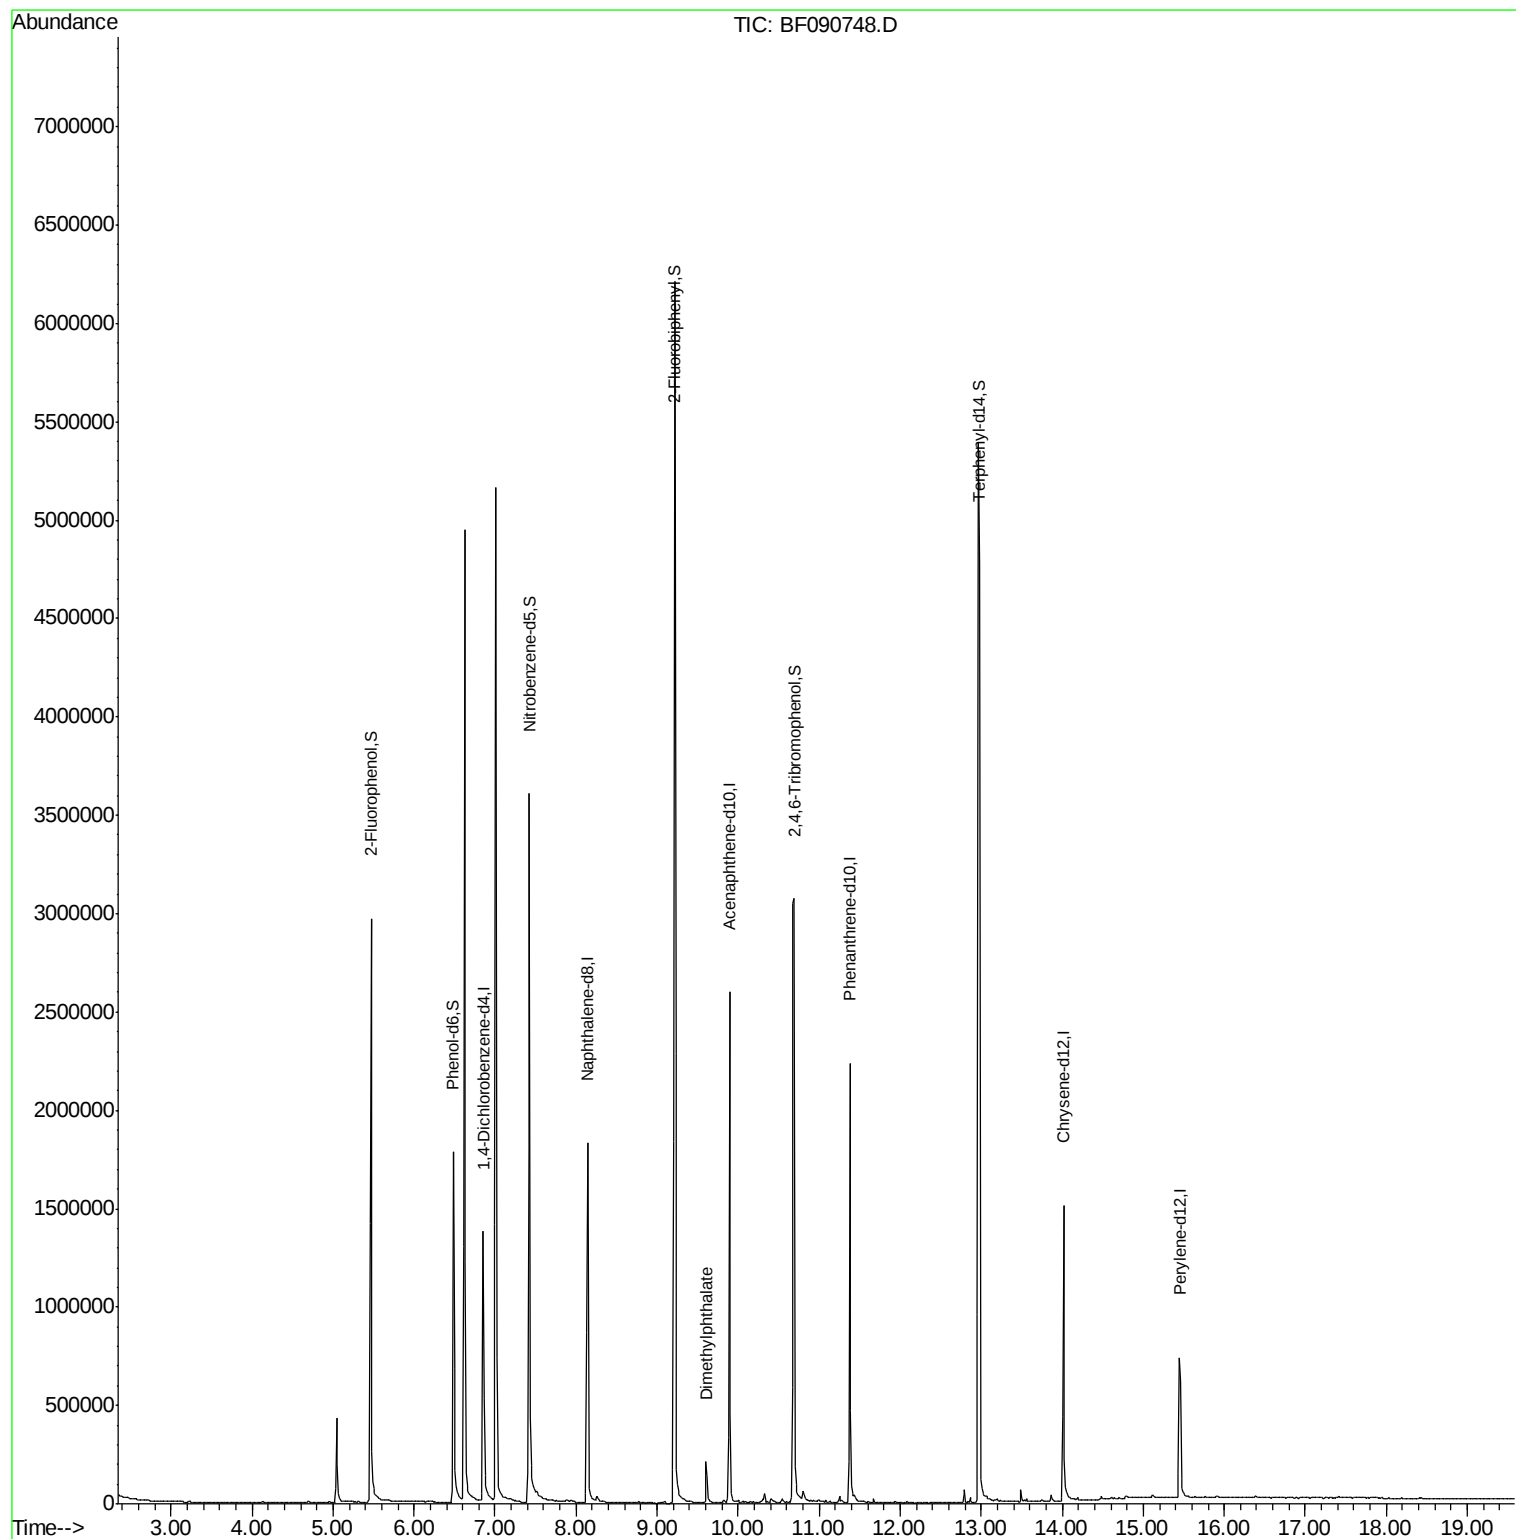

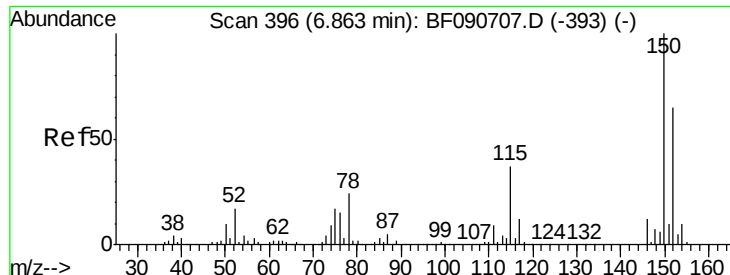

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.85 min Scan# 395

Delta R.T. -0.01 min

Lab File: BF090748.D

Acq: 22 Oct 2016 8:46

Instrument :

BNA_F

ClientSampleId :

MW-103D


Tot Ion:152 Resp: 252824

Ion Ratio Lower Upper

152 100

150 157.1 124.7 187.1




115 70.1 39.0 58.4#

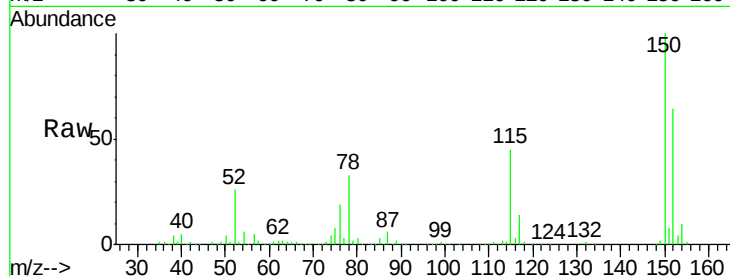

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

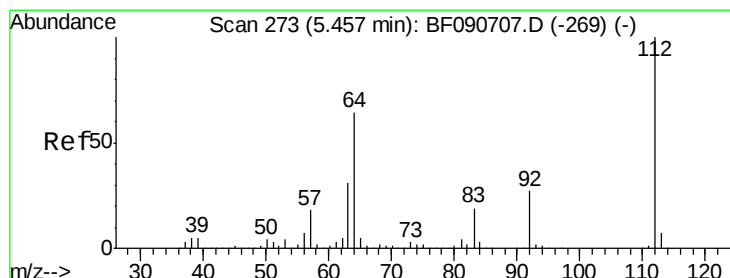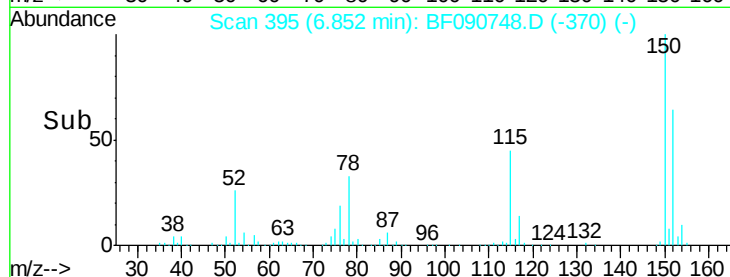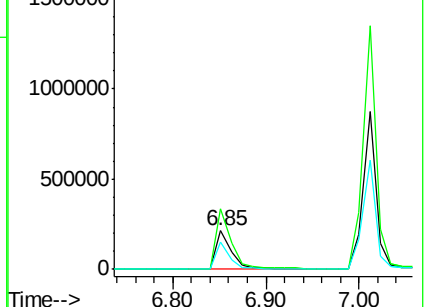

#5

2-Fluorophenol

Concen: 64.68 ng

RT: 5.47 min Scan# 274

Delta R.T. 0.01 min

Lab File: BF090748.D

Acq: 22 Oct 2016 8:46


Tgt Ion:112 Resp: 1013968

Ion Ratio Lower Upper

112 100

64 58.4 39.7 59.5



63 28.2 17.4 26.0#

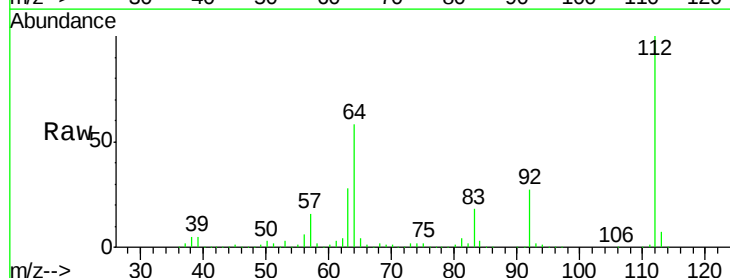

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

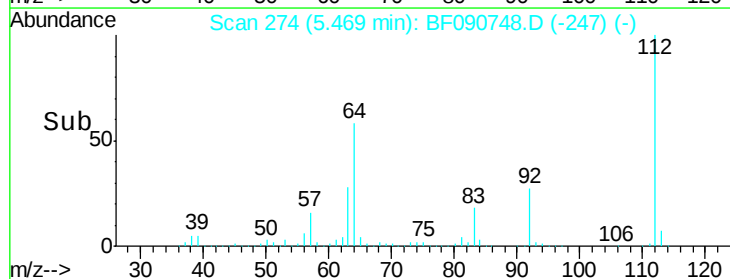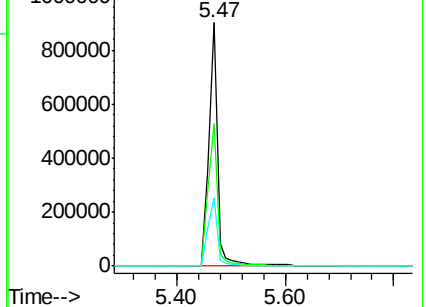



#7

Phenol-d6

Concen: 36.81 ng

RT: 6.49 min Scan# 363

Delta R.T. -0.01 min

Lab File: BF090748.D

Acq: 22 Oct 2016 8:46

Instrument :

BNA_F

ClientSampleId :

MW-103D





Tot Ion: 99 Resp: 781688

Ion Ratio Lower Upper

99 100

42 18.1 13.7 20.5

71 34.3 14.2 21.2#

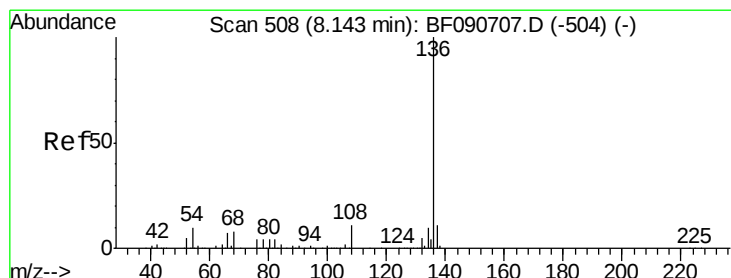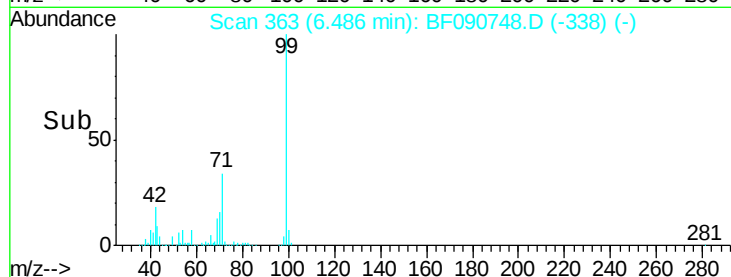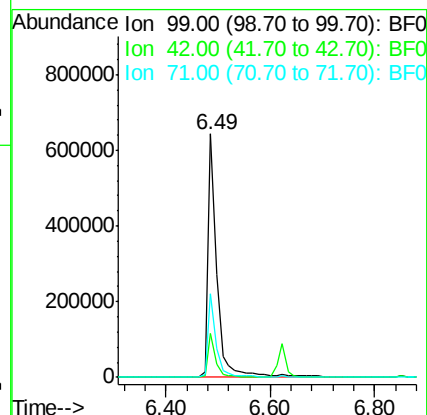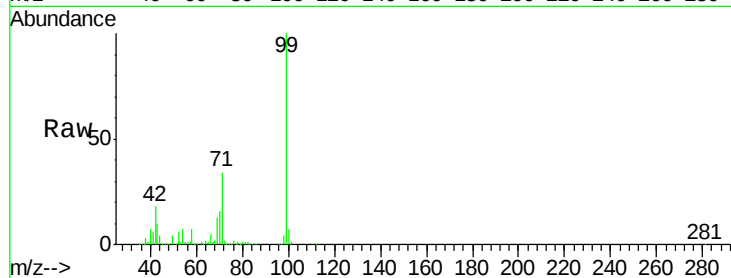

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.14 min Scan# 508

Delta R.T. 0.00 min

Lab File: BF090748.D

Acq: 22 Oct 2016 8:46

Tgt Ion: 136 Resp: 1075996




Ion Ratio Lower Upper


136 100

137 11.2 9.0 13.6

54 7.2 8.2 12.2#

68 6.3 5.8 8.6


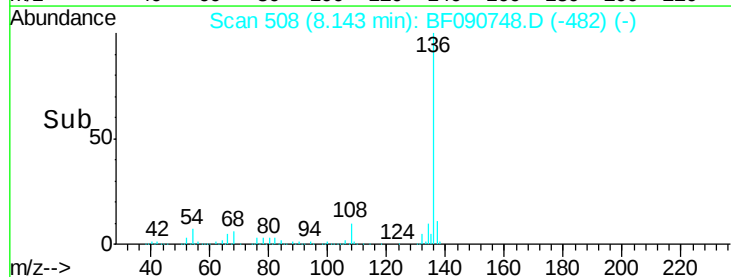
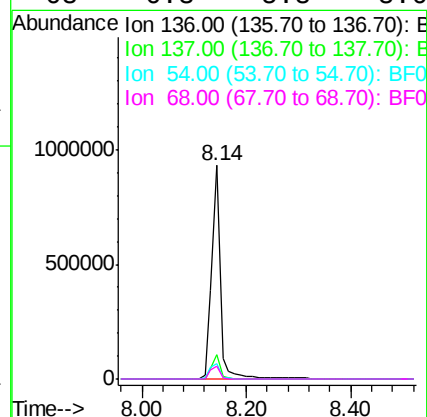
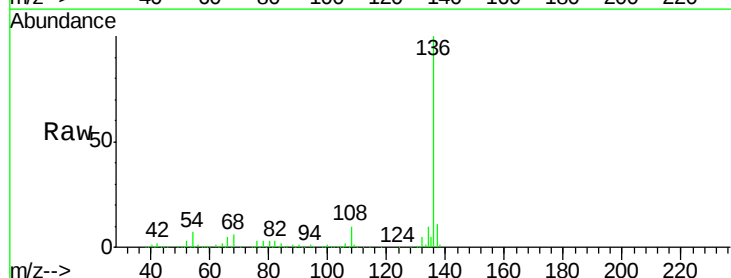


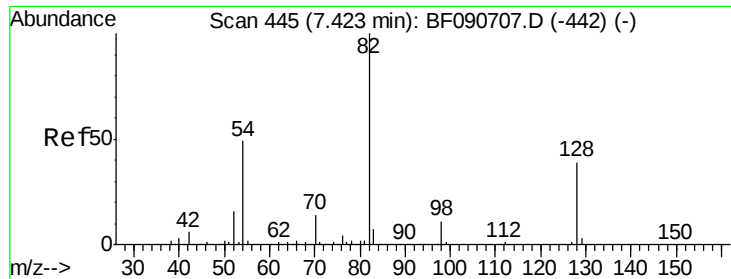

#23
 Nitrobenzene-d5
 Concen: 86.40 ng
 RT: 7.42 min Scan# 445
 Delta R.T. 0.00 min
 Lab File: BF090748.D
 Acq: 22 Oct 2016 8:46




Instrument :
 BNA_F
 ClientSampleId :
 MW-103D


Tot Ion: 82 Resp: 1694925
 Ion Ratio Lower Upper
 82 100
 128 44.9 51.0 76.6#
 54 46.7 47.5 71.3#

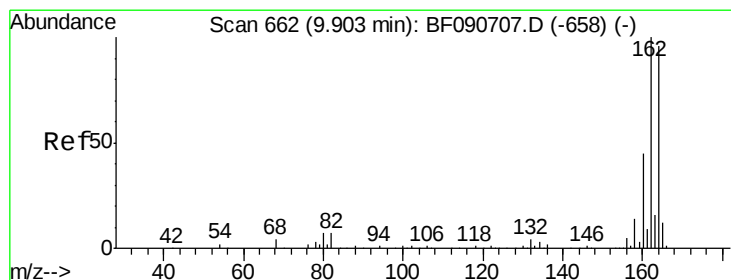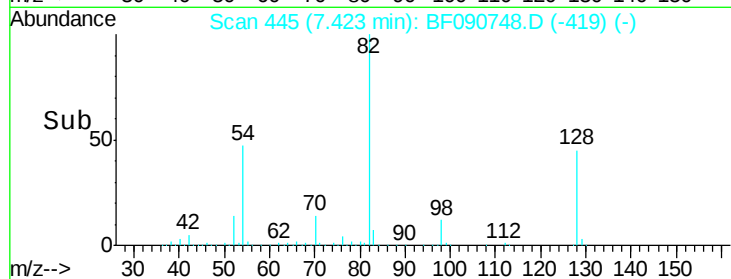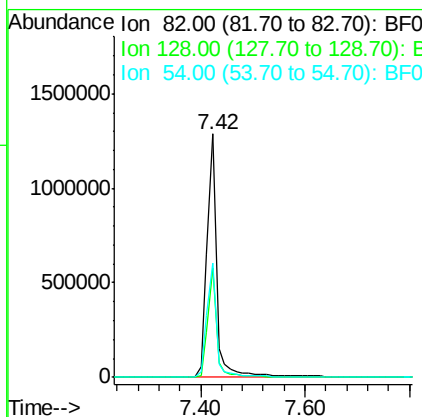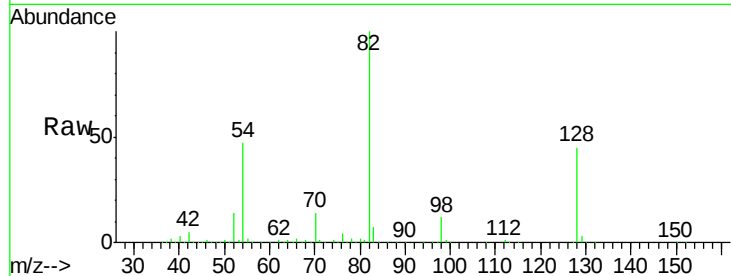

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.89 min Scan# 661
 Delta R.T. -0.01 min
 Lab File: BF090748.D
 Acq: 22 Oct 2016 8:46

Tgt Ion:164 Resp: 543955
 Ion Ratio Lower Upper
 164 100
 162 103.7 75.2 112.8
 160 47.8 31.5 47.3#

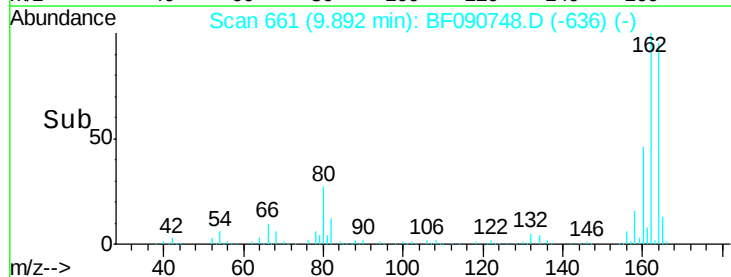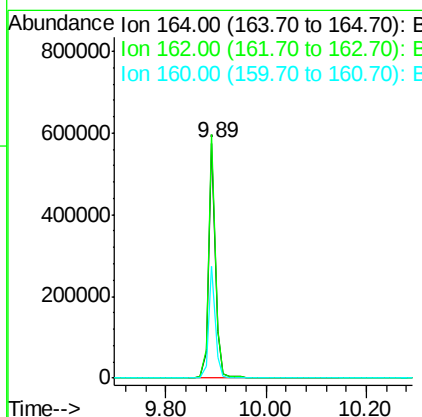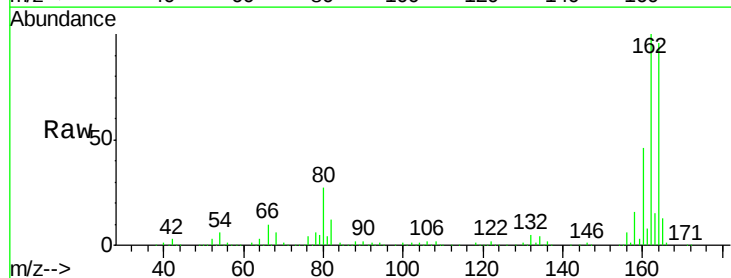


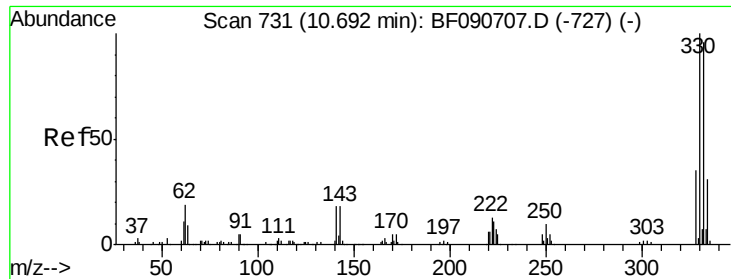




#41
 2,4,6-Tribromophenol
 Concen: 163.16 ng
 RT: 10.69 min Scan# 731
 Delta R.T. 0.00 min
 Lab File: BF090748.D
 Acq: 22 Oct 2016 8:46

Instrument :
 BNA_F
 ClientSampleId :
 MW-103D

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.1	76.6	114.8
141	30.7	29.7	44.5

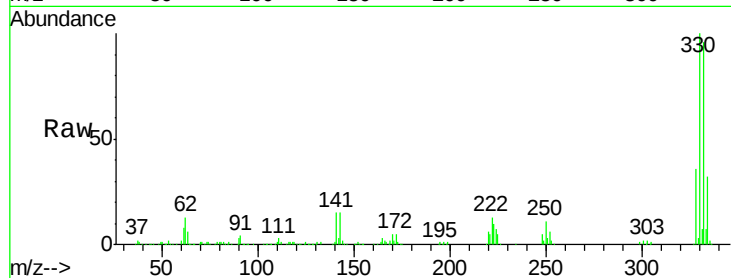


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

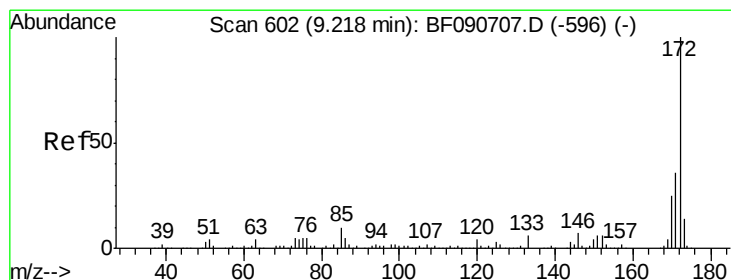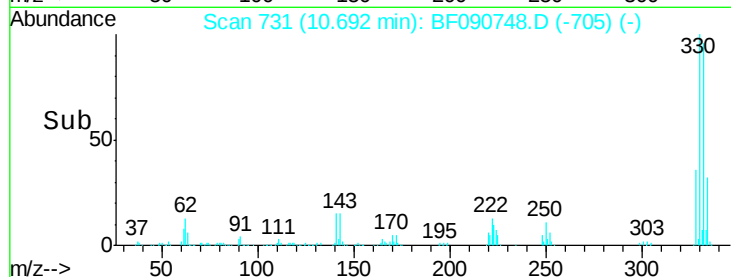
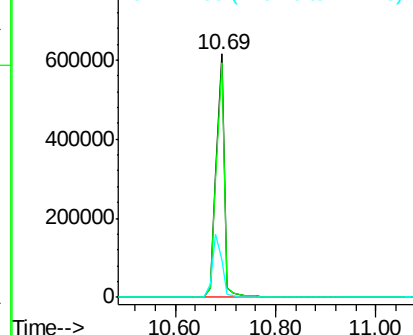


#44
 2-Fluorobiphenyl
 Concen: 73.61 ng
 RT: 9.22 min Scan# 602
 Delta R.T. -0.01 min
 Lab File: BF090748.D
 Acq: 22 Oct 2016 8:46

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.4	26.1	39.1
170	25.4	17.4	26.2

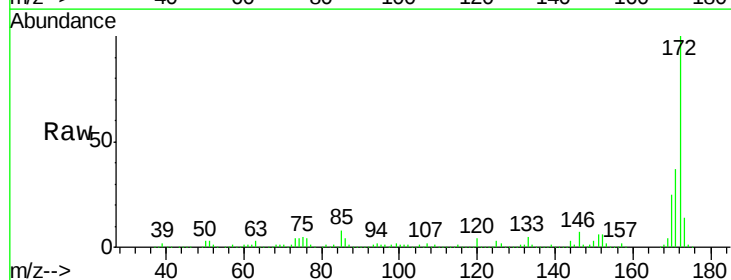

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

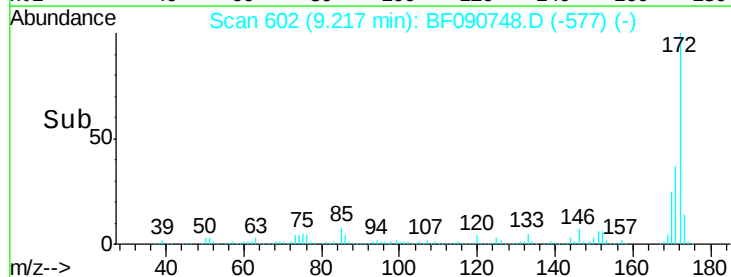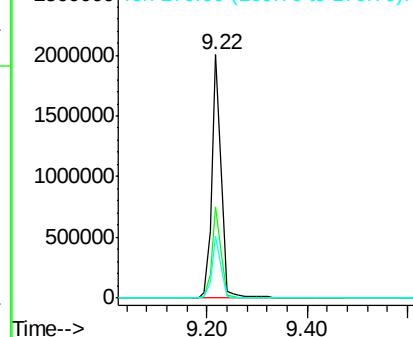







#49
Dimethylphthalate
Concen: 3.51 ng
RT: 9.61 min Scan# 636
Delta R.T. -0.02 min
Lab File: BF090748.D
Acq: 22 Oct 2016 8:46

Instrument :
BNA_F
ClientSampleId :
MW-103D

Tot Ion:163 Resp: 120028
Ion Ratio Lower Upper
163 100
194 2.6 4.4 6.6#
164 10.1 8.3 12.5

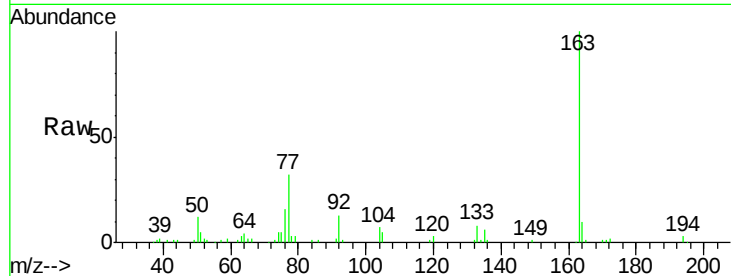


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

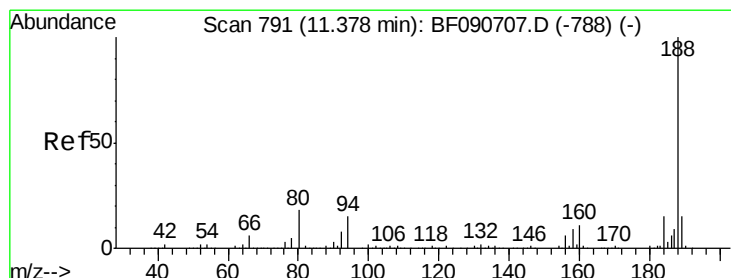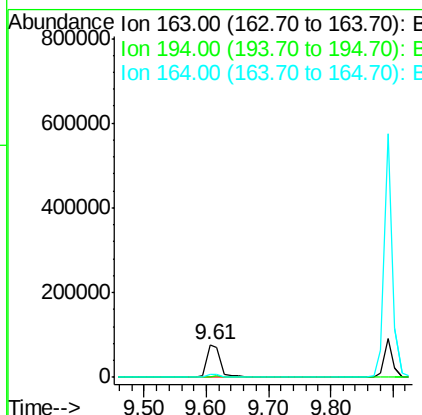
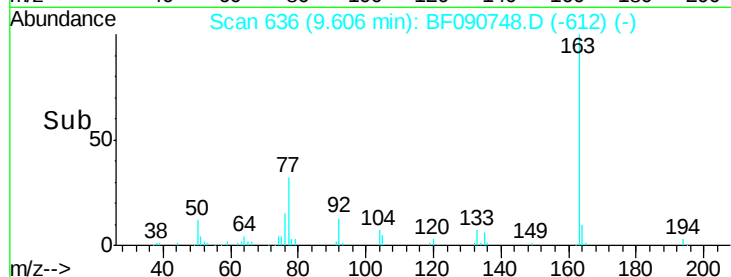


#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.38 min Scan# 791
Delta R.T. -0.01 min
Lab File: BF090748.D
Acq: 22 Oct 2016 8:46

Tgt Ion:188 Resp: 849026
Ion Ratio Lower Upper
188 100
94 13.1 11.1 16.7
80 14.7 11.0 16.4

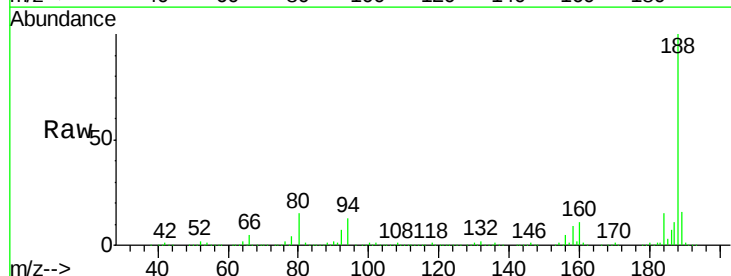

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

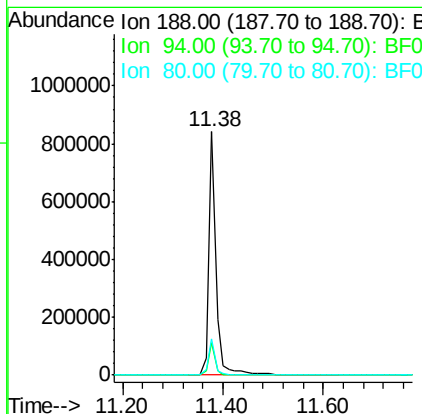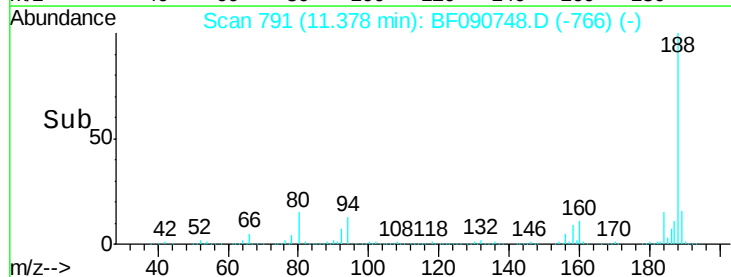



#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.02 min Scan# 1022

Delta R.T. 0.00 min

Lab File: BF090748.D

Acq: 22 Oct 2016 8:46

Instrument :

BNA_F

ClientSampleId :

MW-103D


Tot Ion:240 Resp: 578052

Ion Ratio Lower Upper

240 100

120 12.2 16.2 24.2#




236 27.4 18.4 27.6

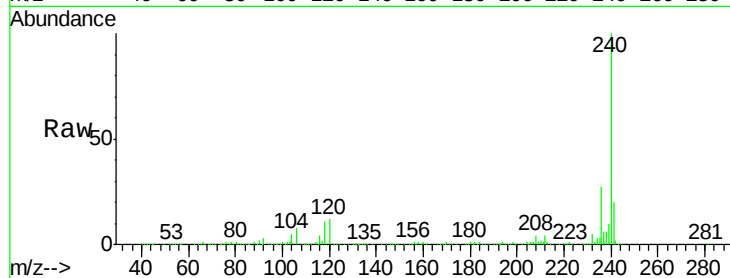

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

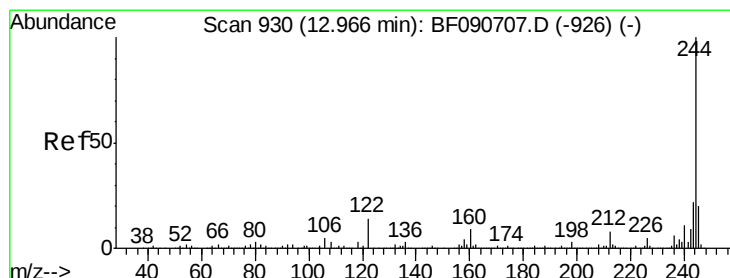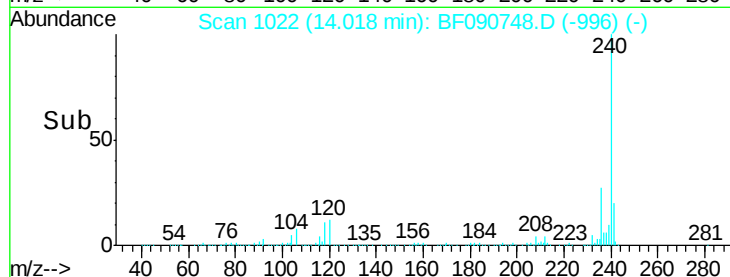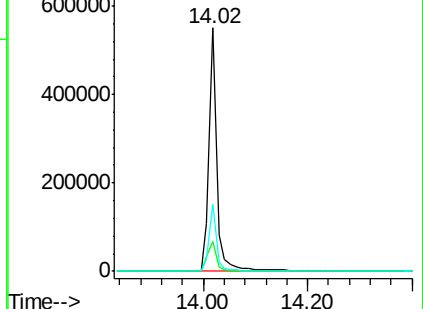

#78

Terphenyl-d14

Concen: 108.75 ng

RT: 12.98 min Scan# 931

Delta R.T. 0.01 min

Lab File: BF090748.D

Acq: 22 Oct 2016 8:46


Tgt Ion:244 Resp: 2742919

Ion Ratio Lower Upper

244 100

212 6.6 4.3 6.5#



122 6.5 17.4 26.2#

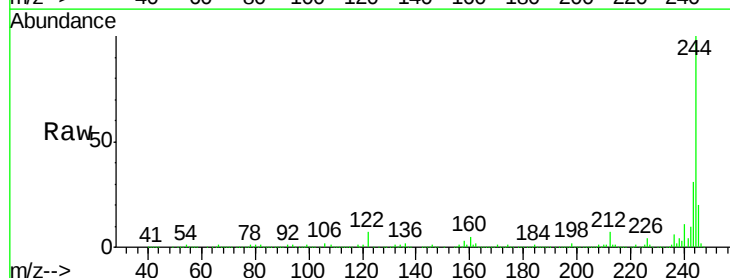


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

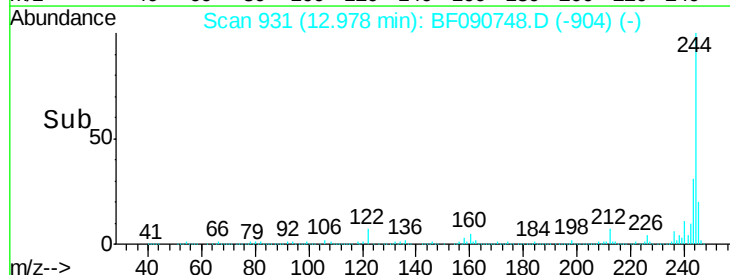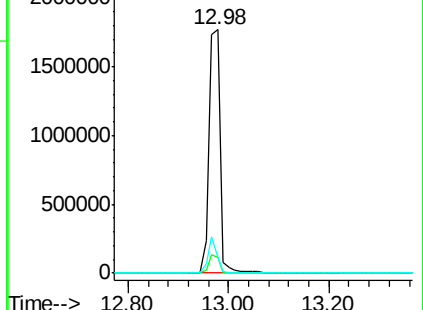

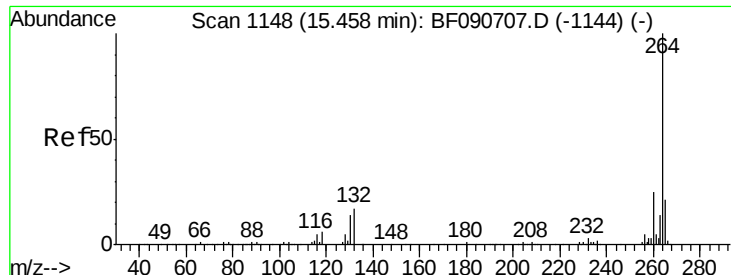

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.45 min Scan# 1147
Delta R.T. -0.01 min
Lab File: BF090748.D
Acq: 22 Oct 2016 8:46

Instrument :
BNA_F
ClientSampleId :
MW-103D

Tot Ion:264 Resp: 388396
Ion Ratio Lower Upper
264 100
260 25.4 16.7 25.1#
265 21.9 17.2 25.8

