

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
 Data File : BF090727.D
 Acq On : 21 Oct 2016 23:09
 Operator : UM/SJ
 Sample : H5308-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-102S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.046	234	237	246	rBV	387472	519718	6.36%	0.977%
2	5.457	271	273	276	rBV	1851836	2750609	33.65%	5.168%
3	6.486	361	363	372	rBV	1874237	1921887	23.51%	3.611%
4	6.623	372	375	378	rBV	5039119	5346801	65.40%	10.047%
5	6.851	393	395	406	rBV	1421437	1596944	19.53%	3.001%
6	7.011	406	409	411	rBV	5255085	5274893	64.52%	9.912%
7	7.423	441	445	447	rBV	3691728	4569548	55.90%	8.586%
8	8.143	505	508	510	rBV	1784525	2169137	26.53%	4.076%
9	8.257	516	518	530	rVB	43222	86206	1.05%	0.162%
10	9.217	598	602	605	rBV	6803786	8050793	98.48%	15.128%
11	9.892	658	661	664	rBV	2637779	2497516	30.55%	4.693%
12	10.692	727	731	733	rBV2	3234125	5094260	62.31%	9.572%
13	11.378	789	791	795	rBV	2419981	2238528	27.38%	4.206%
14	12.966	927	930	933	rBV	5653358	8175133	100.00%	15.361%
15	14.018	1019	1022	1024	rBV	1466239	1685546	20.62%	3.167%
16	14.601	1071	1073	1075	rBV	101744	98936	1.21%	0.186%
17	15.447	1144	1147	1150	rBV	879067	1142425	13.97%	2.147%




Sum of corrected areas: 53218880

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090727.D
Acq On : 21 Oct 2016 23:09
Operator : UM/SJ
Sample : H5308-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-102S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

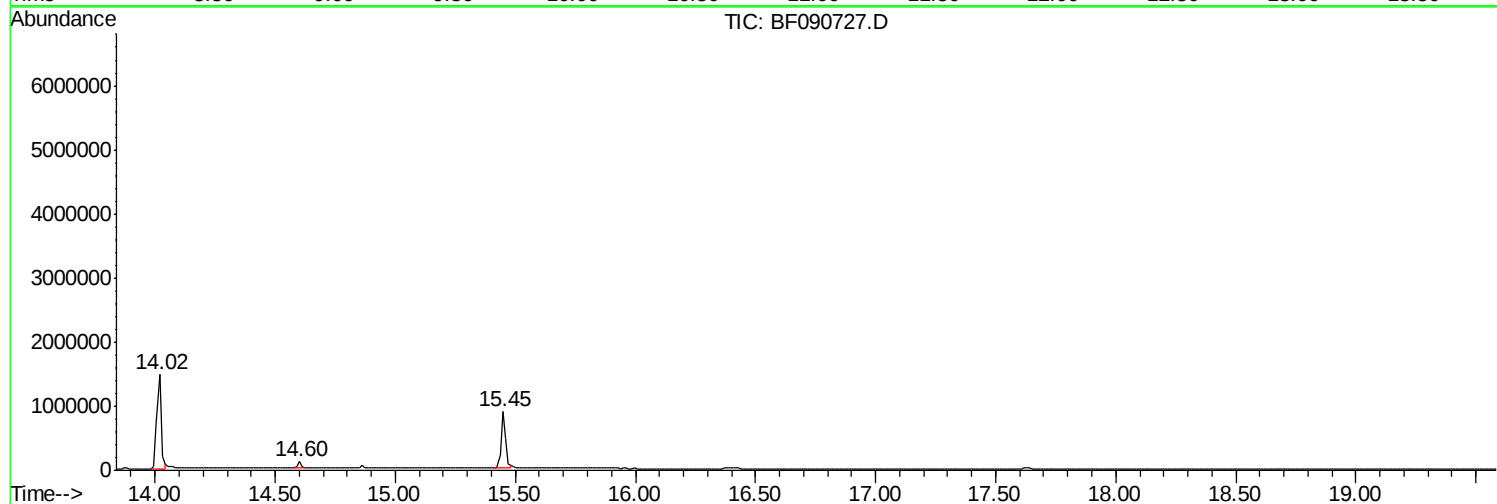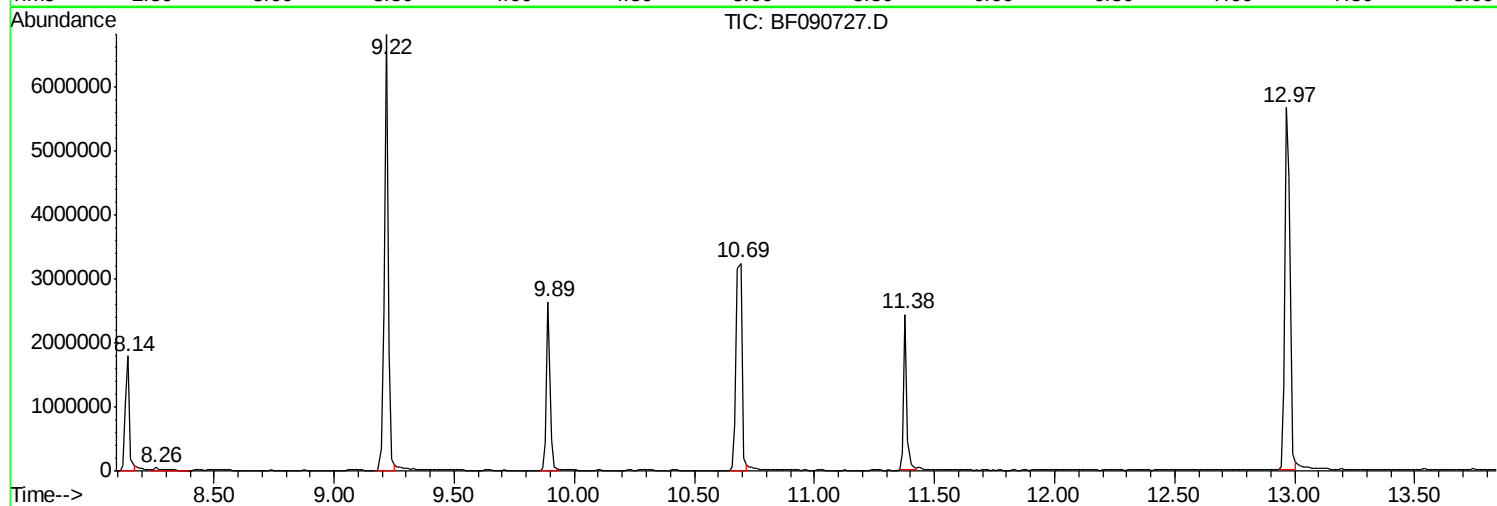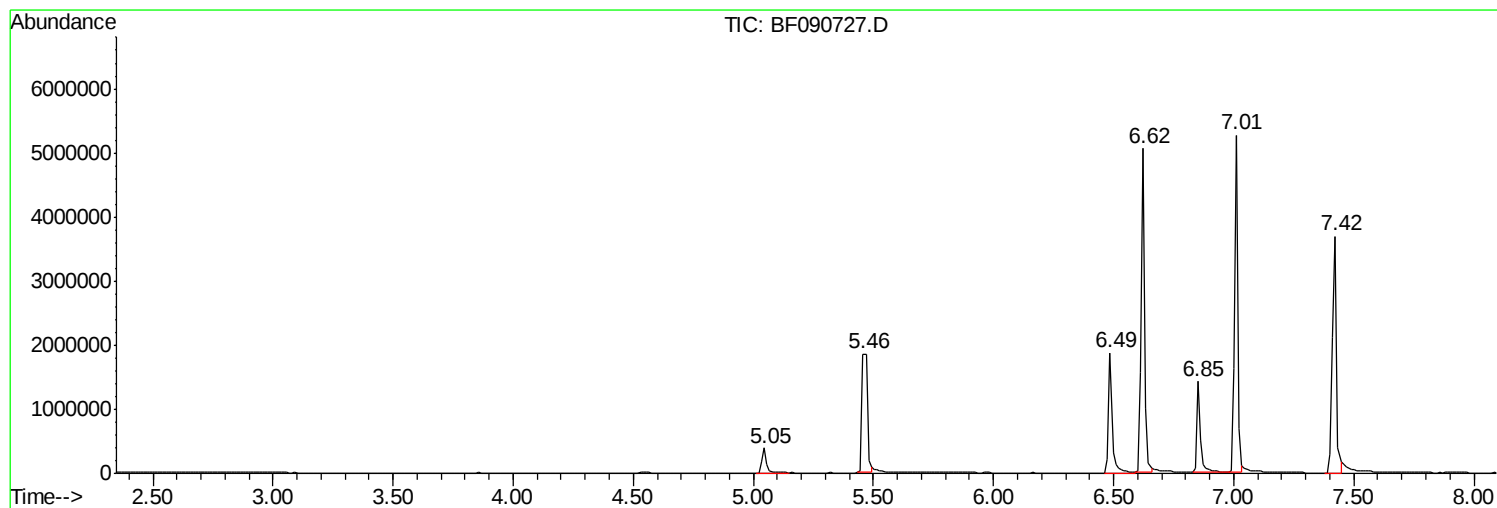

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090727.D
Acq On : 21 Oct 2016 23:09
Operator : UM/SJ
Sample : H5308-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-102S










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.05	6.51 ng	519718	1,4-Dichlorobenzene-d4	6.85

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2			Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39
3			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	33
4			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25
5			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10

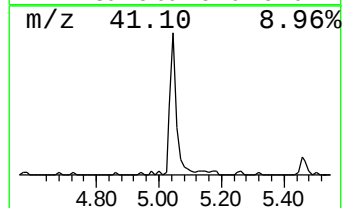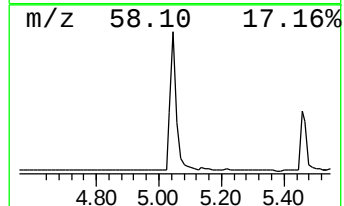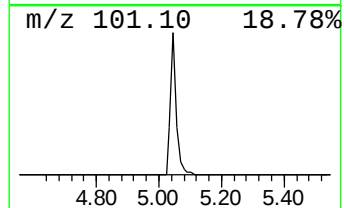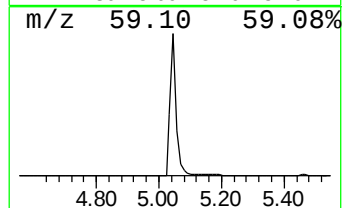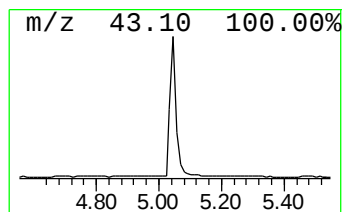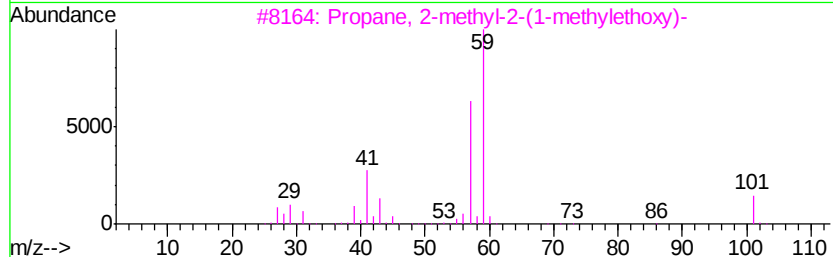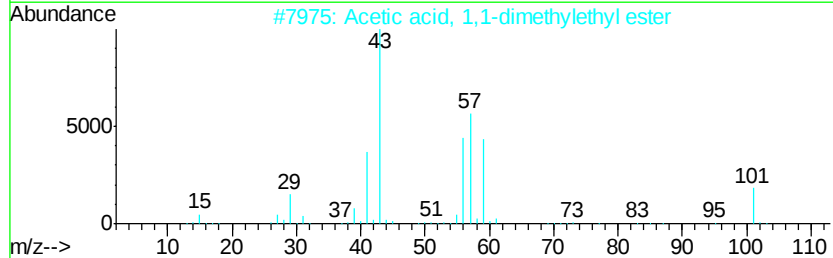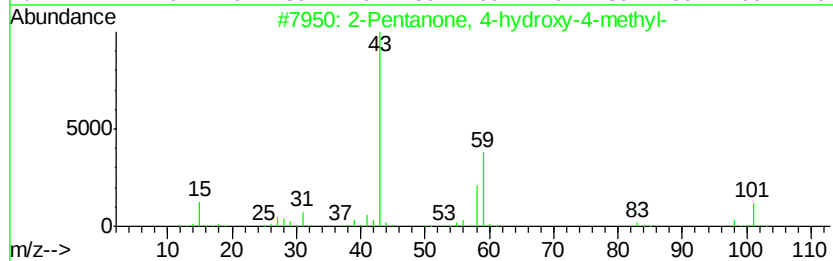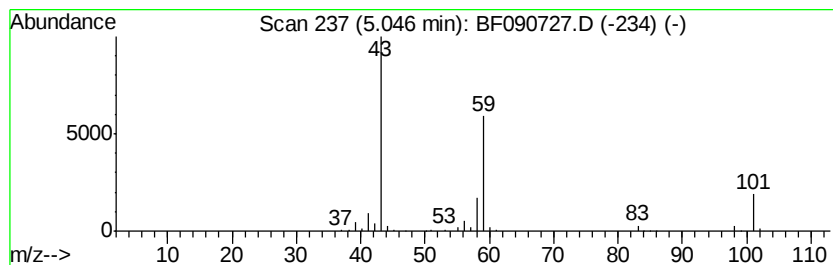

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090727.D
Acq On : 21 Oct 2016 23:09
Operator : UM/SJ
Sample : H5308-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-102S










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.62 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.62	66.96 ng	5346800	1,4-Dichlorobenzene-d4	6.85

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

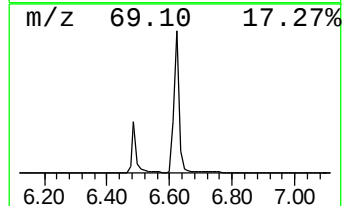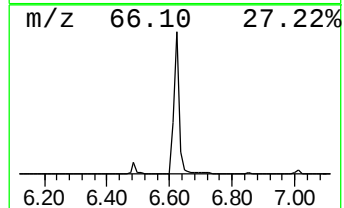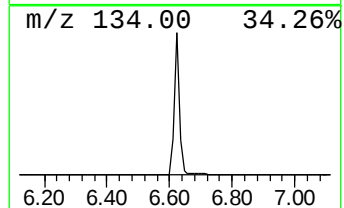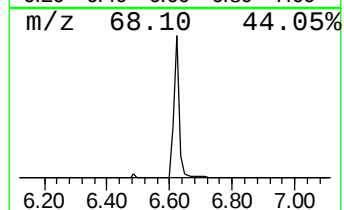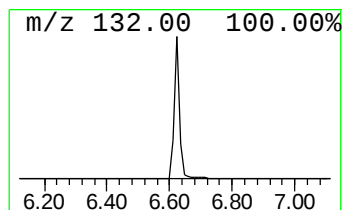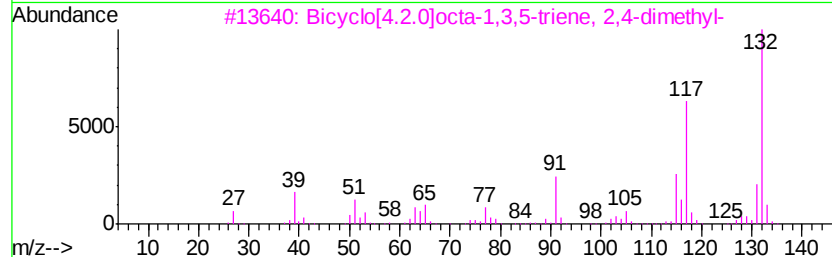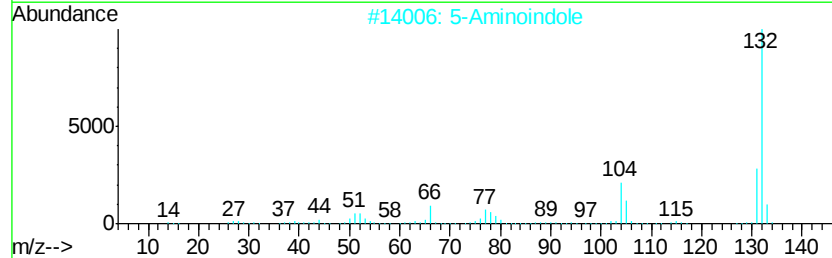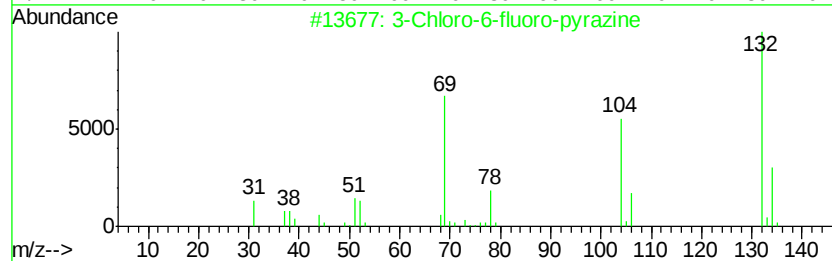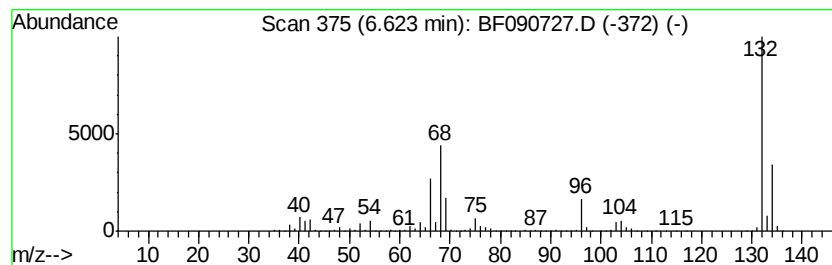

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090727.D
Acq On : 21 Oct 2016 23:09
Operator : UM/SJ
Sample : H5308-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-102S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.05	6.5	ng	519718	1	6.85	1596940	20.0
unknown6.62	6.62	67.0	ng	5346800	1	6.85	1596940	20.0