

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
 Data File : BF090730.D
 Acq On : 22 Oct 2016 00:32
 Operator : UM/SJ
 Sample : H5308-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-102I

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.428	5	8	19	rVB5	25206	99202	1.29%	0.191%
2	4.543	190	193	200	rBV	116417	160384	2.09%	0.309%
3	5.046	234	237	245	rBV	347063	482447	6.28%	0.928%
4	5.457	271	273	276	rBV	2246300	2688771	35.02%	5.174%
5	6.486	361	363	365	rBV	1709728	1680397	21.89%	3.234%
6	6.623	372	375	377	rBV	5240622	5460952	71.13%	10.509%
7	6.852	393	395	406	rBV	1418744	1574074	20.50%	3.029%
8	7.012	406	409	411	rBV	5186546	5392574	70.24%	10.377%
9	7.423	442	445	447	rBV	3519384	4556269	59.34%	8.768%
10	8.143	505	508	510	rBV	1512578	1960746	25.54%	3.773%
11	9.218	598	602	605	rBV	6236087	7559722	98.46%	14.547%
12	9.892	658	661	664	rBV	2398869	2384173	31.05%	4.588%
13	10.681	727	730	733	rBV2	3209437	5050855	65.79%	9.719%
14	11.378	788	791	795	rBV	2382948	2259719	29.43%	4.348%
15	12.967	927	930	933	rBV	5843453	7677613	100.00%	14.774%
16	14.018	1019	1022	1024	rBV	1491979	1718452	22.38%	3.307%
17	15.447	1144	1147	1165	rVB	907290	1260294	16.42%	2.425%




Sum of corrected areas: 51966644

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090730.D
Acq On : 22 Oct 2016 00:32
Operator : UM/SJ
Sample : H5308-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-102I

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

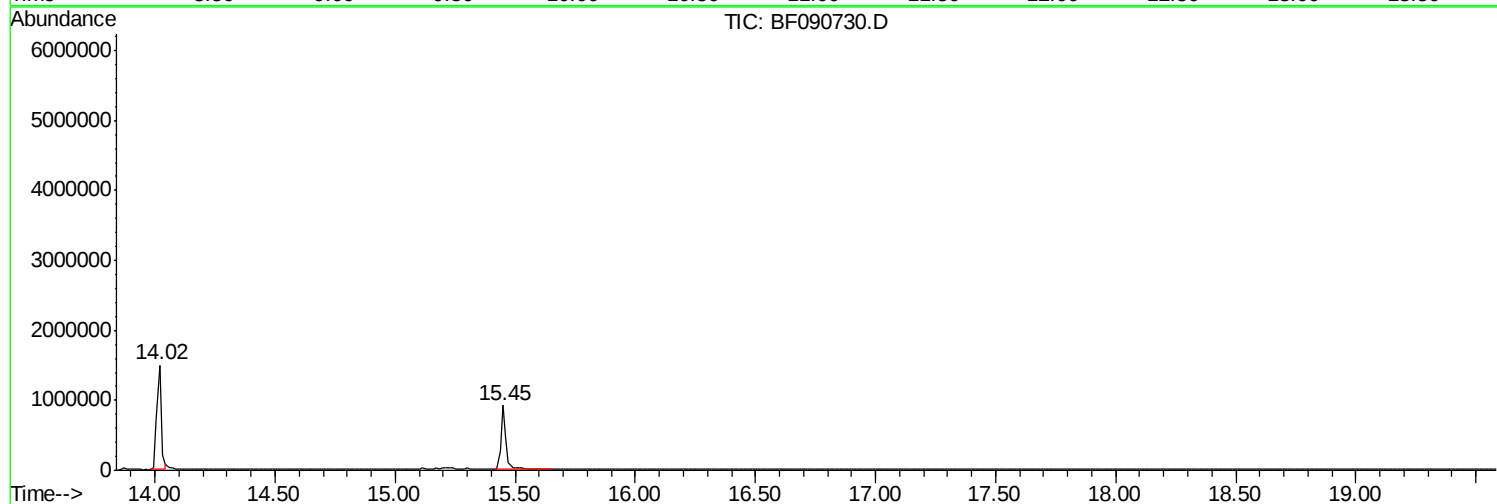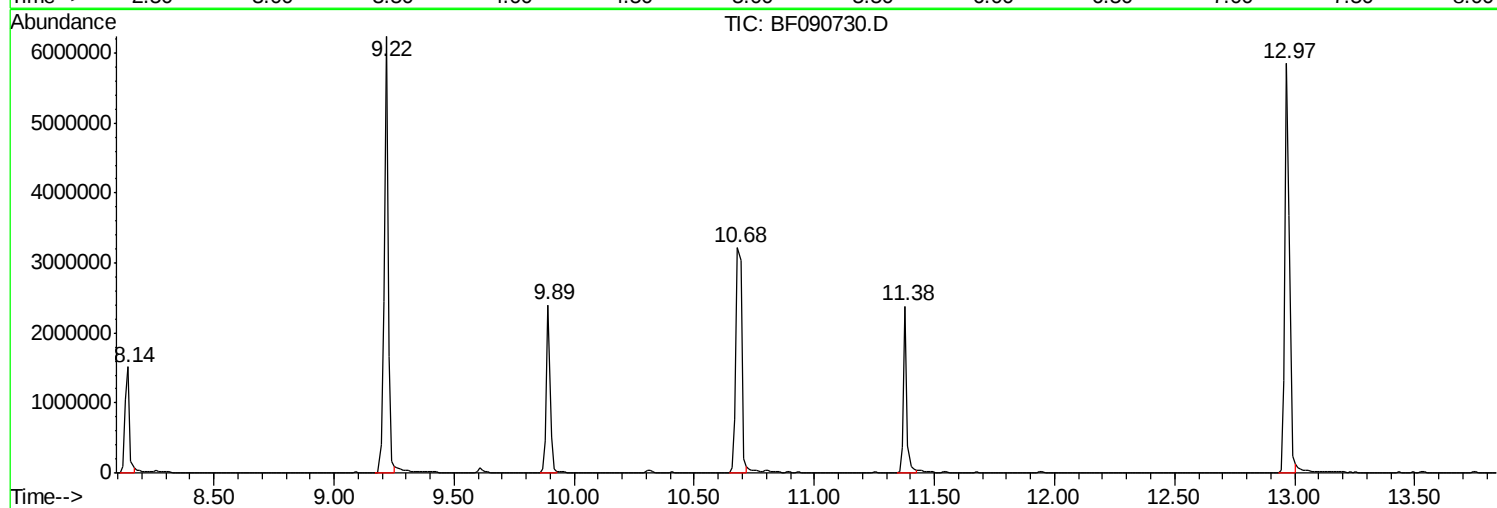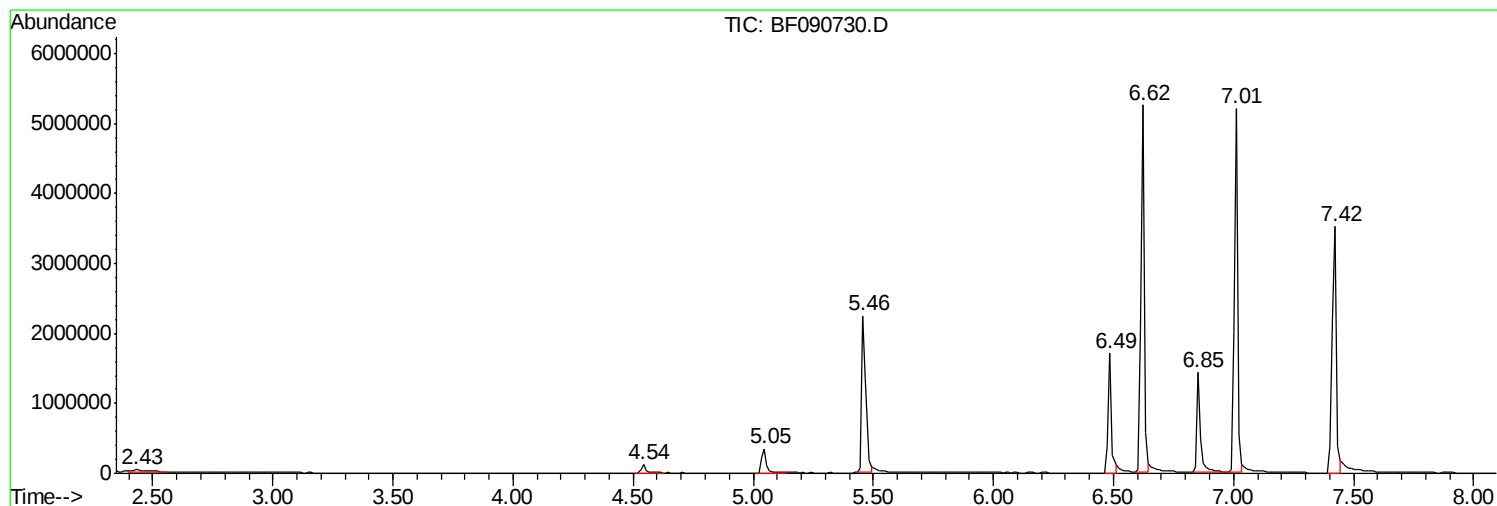

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102116\
Data File : BF090730.D
Acq On : 22 Oct 2016 00:32
Operator : UM/SJ
Sample : H5308-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-102I










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.05	6.13 ng	482447	1,4-Dichlorobenzene-d4	6.85

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2			Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39
3			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
4			Acetone	58	C3H6O	000067-64-1	9
5			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	9

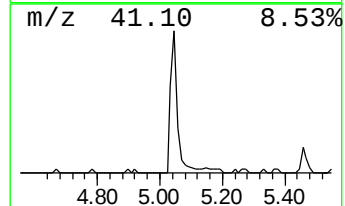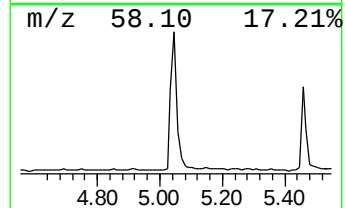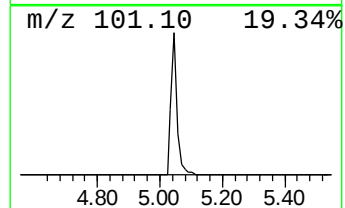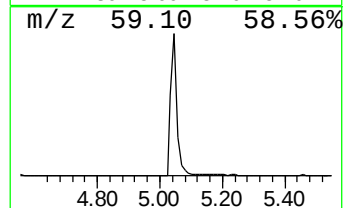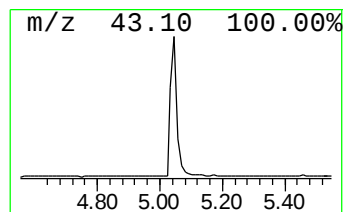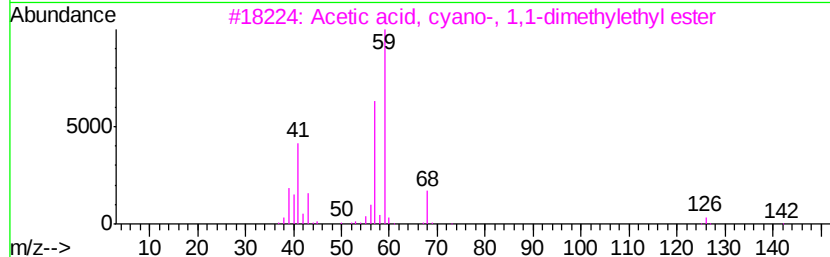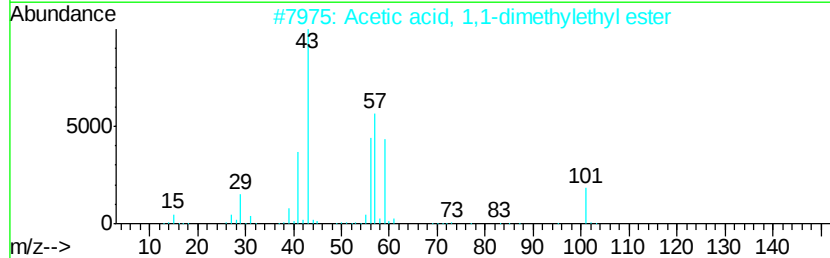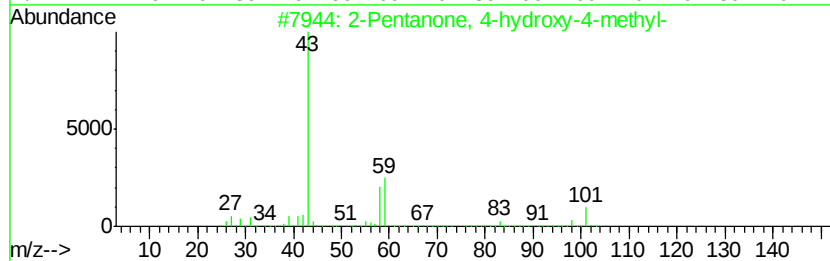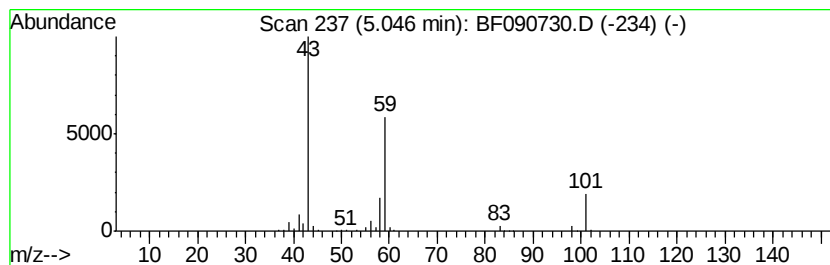

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090730.D
Acq On : 22 Oct 2016 00:32
Operator : UM/SJ
Sample : H5308-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-102I







Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown6.62 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.62	69.39 ng	5460950	1,4-Dichlorobenzene-d4	6.85

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2			5-Aminoindole	132	C8H8N2	005192-03-0	12
3			Tranvlcvpromine-propionvl	189	C12H15NO	1000123-86-3	10
4			Xenon	132	Xe	007440-63-3	9
5			4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

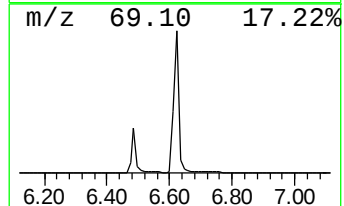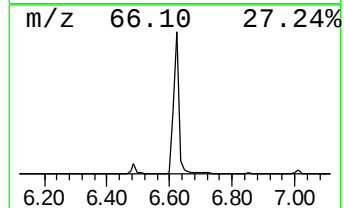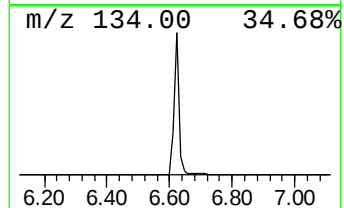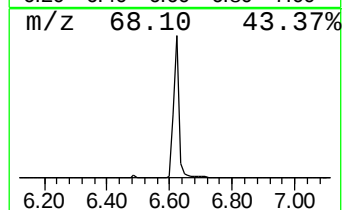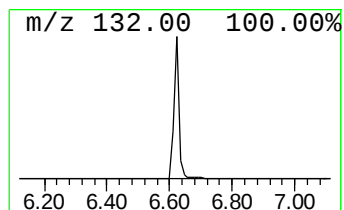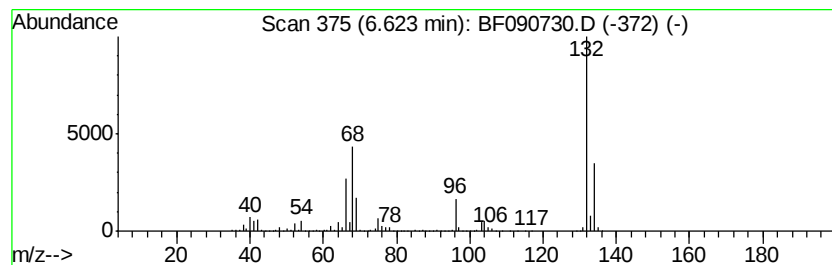

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090730.D
Acq On : 22 Oct 2016 00:32
Operator : UM/SJ
Sample : H5308-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-102I

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.05	6.1	ng	482447	1	6.85	1574070	20.0
unknown6.62	6.62	69.4	ng	5460950	1	6.85	1574070	20.0