

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
 Data File : BF090746.D
 Acq On : 22 Oct 2016 7:51
 Operator : UM/SJ
 Sample : H5308-21
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-104D

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.057	236	238	245	rBV	489309	673245	8.41%	1.211%
2	5.469	272	274	293	rBV	3798066	4024427	50.27%	7.240%
3	6.497	361	364	366	rBV	2139836	3027793	37.82%	5.447%
4	6.623	372	375	378	rBV	4983569	5811491	72.59%	10.455%
5	6.852	393	395	406	rBV	1412730	1577021	19.70%	2.837%
6	7.012	406	409	411	rBV	5332409	5333666	66.62%	9.596%
7	7.423	442	445	447	rBV	3730213	4458915	55.70%	8.022%
8	8.143	505	508	510	rBV	1747679	2072642	25.89%	3.729%
9	9.217	599	602	605	rBV	6375343	8005527	100.00%	14.402%
10	9.606	634	636	639	rBV	216787	288353	3.60%	0.519%
11	9.892	658	661	664	rBV	2484780	2380937	29.74%	4.283%
12	10.692	727	731	733	rBV	3668145	5142282	64.23%	9.251%
13	10.806	739	741	748	rVB	51228	103019	1.29%	0.185%
14	11.378	789	791	794	rBV	2223297	2114627	26.41%	3.804%
15	12.966	927	930	933	rBV	5581204	7976882	99.64%	14.351%
16	14.018	1019	1022	1024	rBV	1438917	1518059	18.96%	2.731%
17	15.447	1144	1147	1150	rBV	675640	1075703	13.44%	1.935%




Sum of corrected areas: 55584589

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090746.D
Acq On : 22 Oct 2016 7:51
Operator : UM/SJ
Sample : H5308-21
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-104D

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

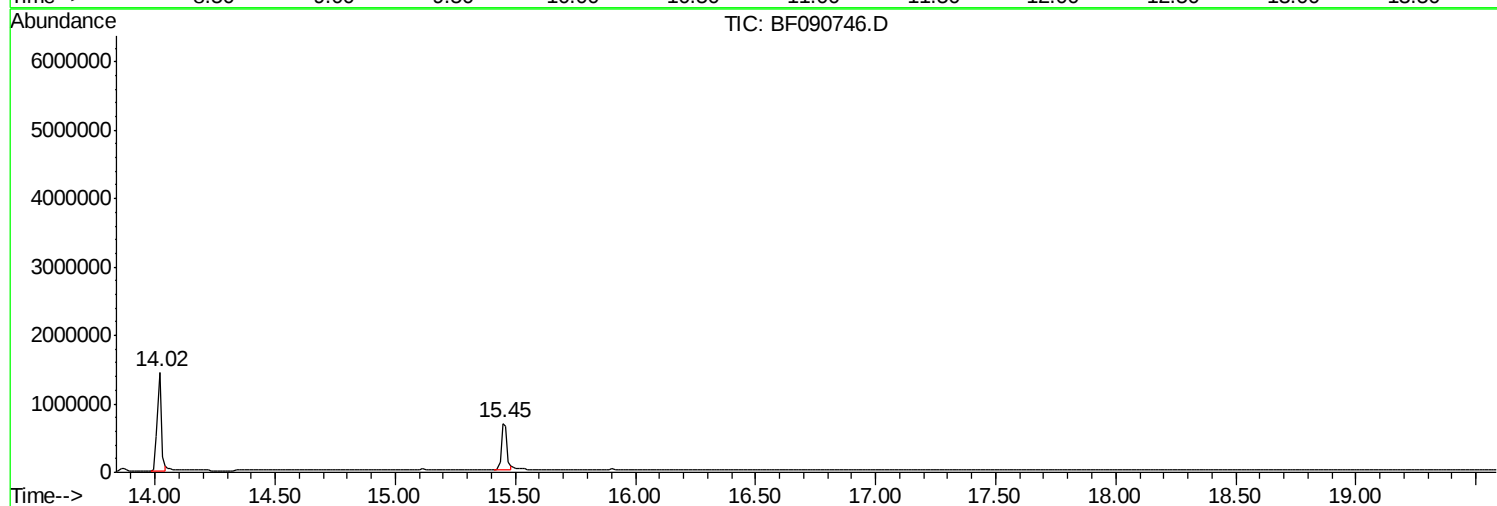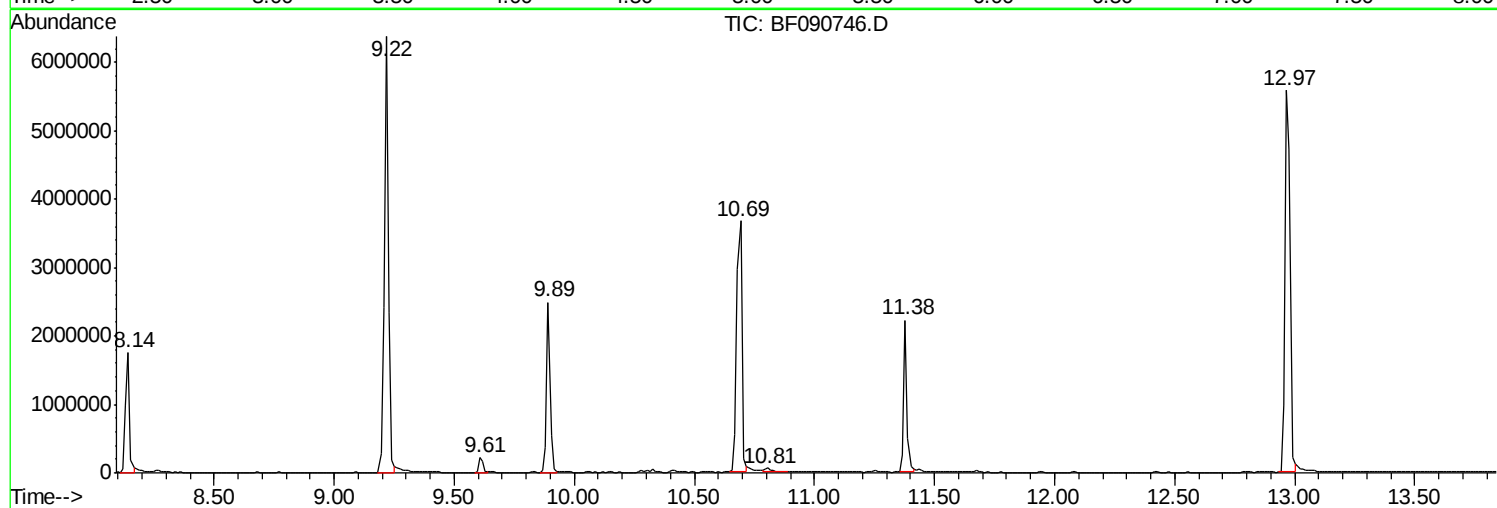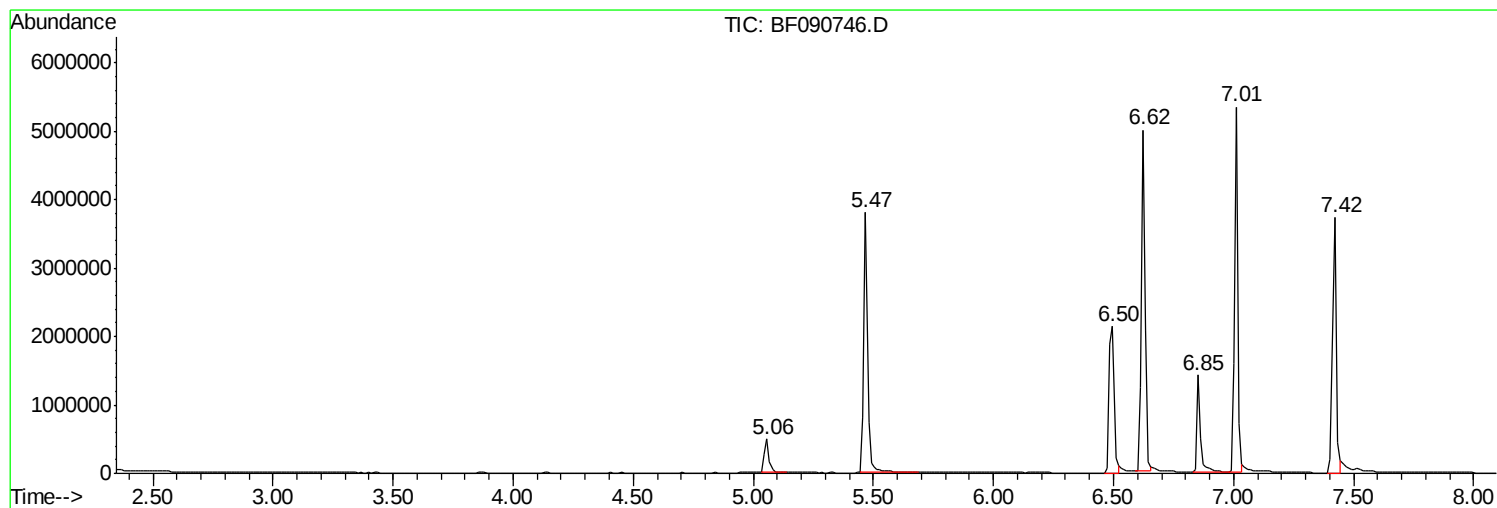

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102116\
Data File : BF090746.D
Acq On : 22 Oct 2016 7:51
Operator : UM/SJ
Sample : H5308-21
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-104D










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.06	8.54 ng	673245	1,4-Dichlorobenzene-d4	6.85

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			Propane, 2-methyl-2-(1-methylethoxy)-	116	C7H16O	017348-59-3	36
3			Acetic acid, cyano-, 1,1-dimethyl-	141	C7H11NO2	001116-98-9	23
4			Acetone	58	C3H6O	000067-64-1	9
5			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

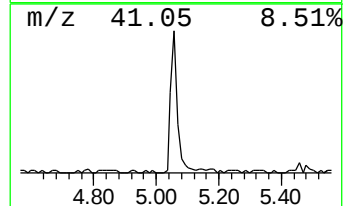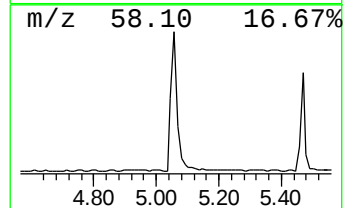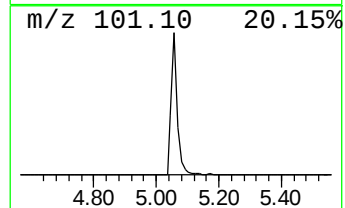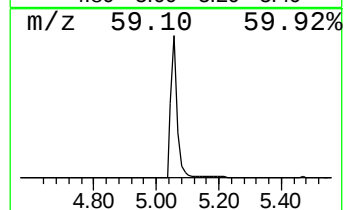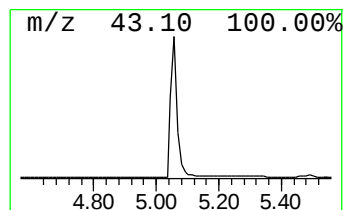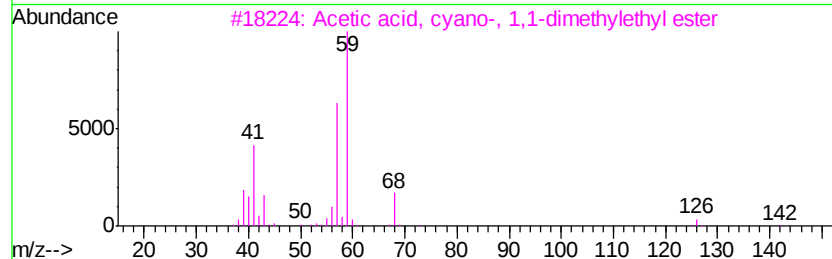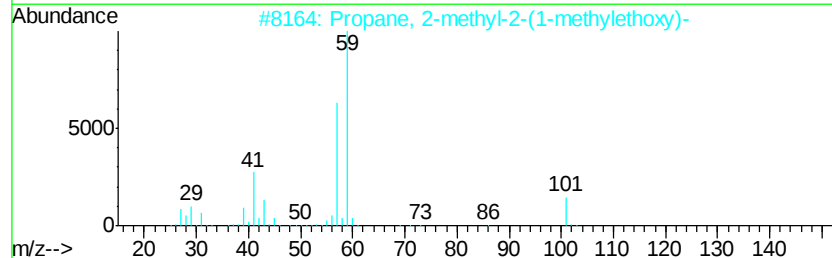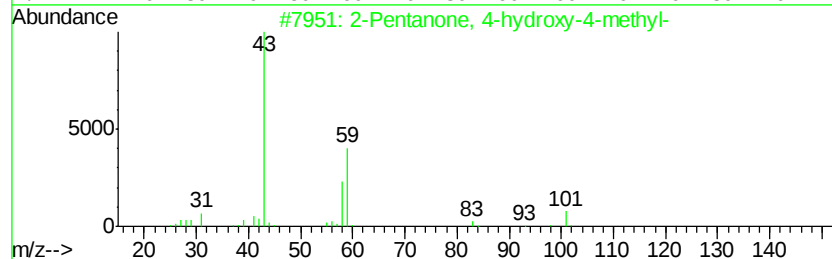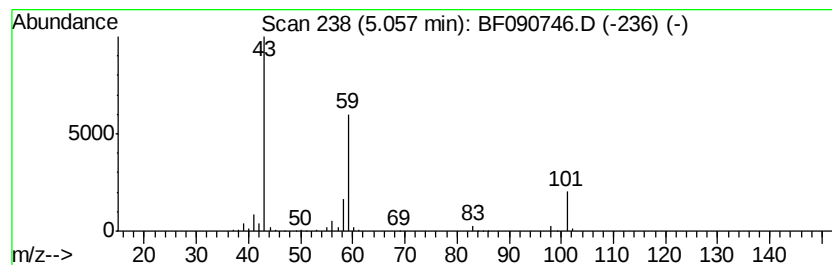

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102116\
Data File : BF090746.D
Acq On : 22 Oct 2016 7:51
Operator : UM/SJ
Sample : H5308-21
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-104D







Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.62 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.62	73.70 ng	5811490	1,4-Dichlorobenzene-d4	6.85

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2			5-Aminoindole	132	C8H8N2	005192-03-0	12
3			Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	10
4			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

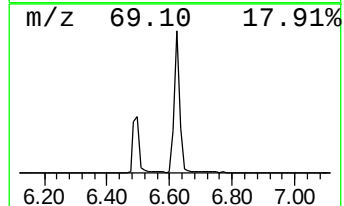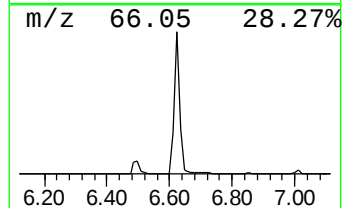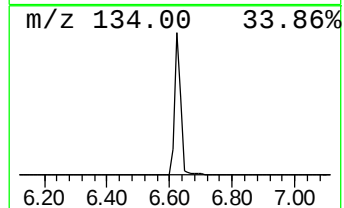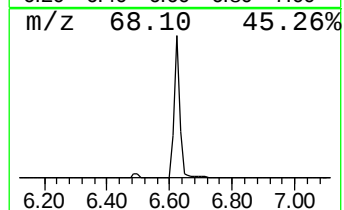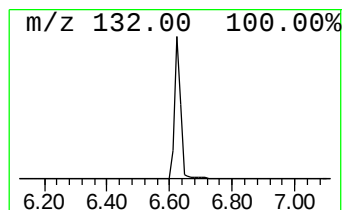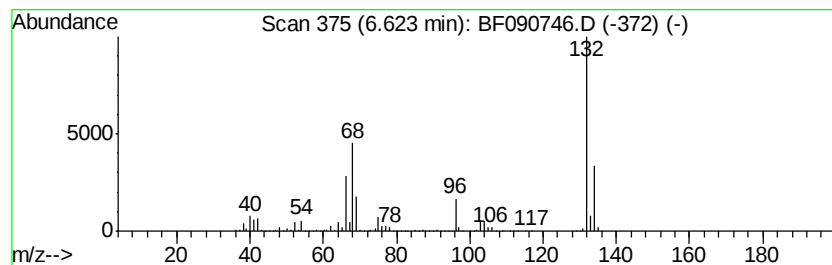

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090746.D
Acq On : 22 Oct 2016 7:51
Operator : UM/SJ
Sample : H5308-21
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-104D

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.06	8.5	ng	673245	1	6.85	1577020	20.0
unknown6.62	6.62	73.7	ng	5811490	1	6.85	1577020	20.0