

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102116\
 Data File : BF090751.D
 Acq On : 22 Oct 2016 10:09
 Operator : UM/SJ
 Sample : H5367-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-03S-101916

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.440	7	9	18	rVB	25531	77717	1.03%	0.154%
2	5.046	234	237	249	rBV	379116	480733	6.37%	0.952%
3	5.468	271	274	276	rBV	2241997	2724263	36.11%	5.395%
4	6.486	361	363	372	rBV	1671982	1759089	23.31%	3.484%
5	6.623	372	375	378	rBV	4754775	4939835	65.47%	9.782%
6	6.851	393	395	406	rBV	1409586	1578363	20.92%	3.126%
7	7.011	406	409	411	rBV	5139865	5201734	68.94%	10.301%
8	7.423	442	445	447	rBV	3514819	4250053	56.33%	8.417%
9	7.514	451	453	461	rVB	56880	155344	2.06%	0.308%
10	8.143	505	508	510	rBV	1761101	2053704	27.22%	4.067%
11	9.217	599	602	605	rBV	6194219	7545223	100.00%	14.942%
12	9.606	634	636	639	rBV	339191	433795	5.75%	0.859%
13	9.892	658	661	664	rBV	2453744	2365130	31.35%	4.684%
14	10.326	693	699	701	rBV3	63342	105655	1.40%	0.209%
15	10.680	727	730	733	rBV2	2880754	4371227	57.93%	8.656%
16	10.795	739	740	748	rVB	58293	122482	1.62%	0.243%
17	11.378	788	791	804	rBV	2310110	2239608	29.68%	4.435%
18	12.966	927	930	933	rBV	5624696	7541990	99.96%	14.936%
19	14.018	1019	1022	1024	rBV	1407613	1465807	19.43%	2.903%
20	15.447	1144	1147	1157	rBV	679581	1084918	14.38%	2.148%




Sum of corrected areas: 50496670

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090751.D
Acq On : 22 Oct 2016 10:09
Operator : UM/SJ
Sample : H5367-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-03S-101916

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

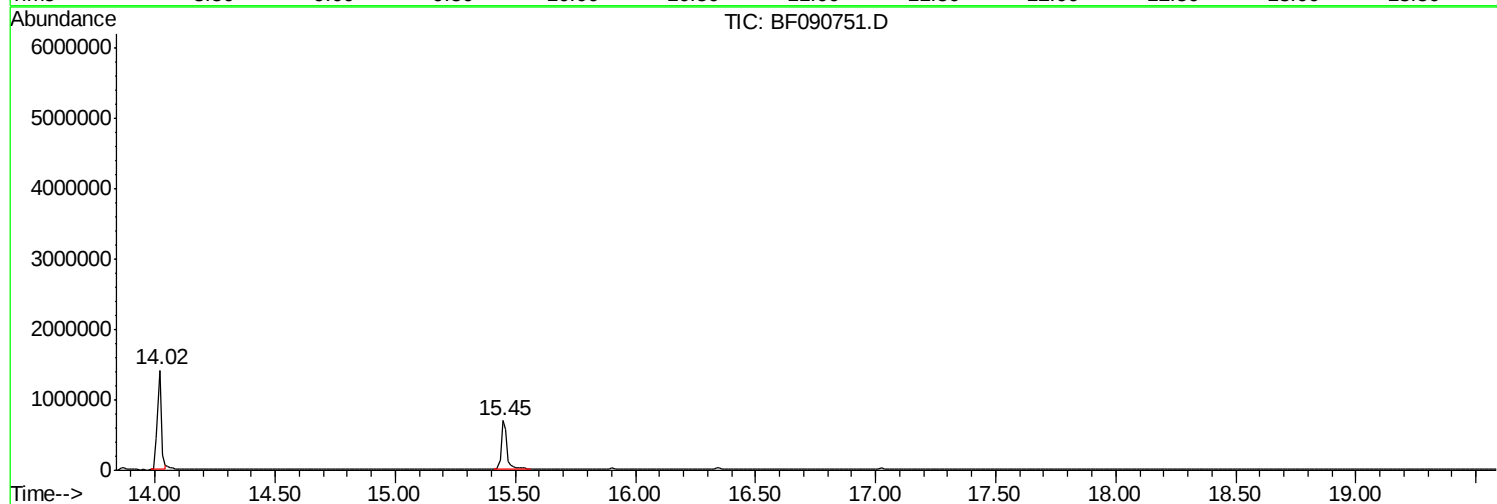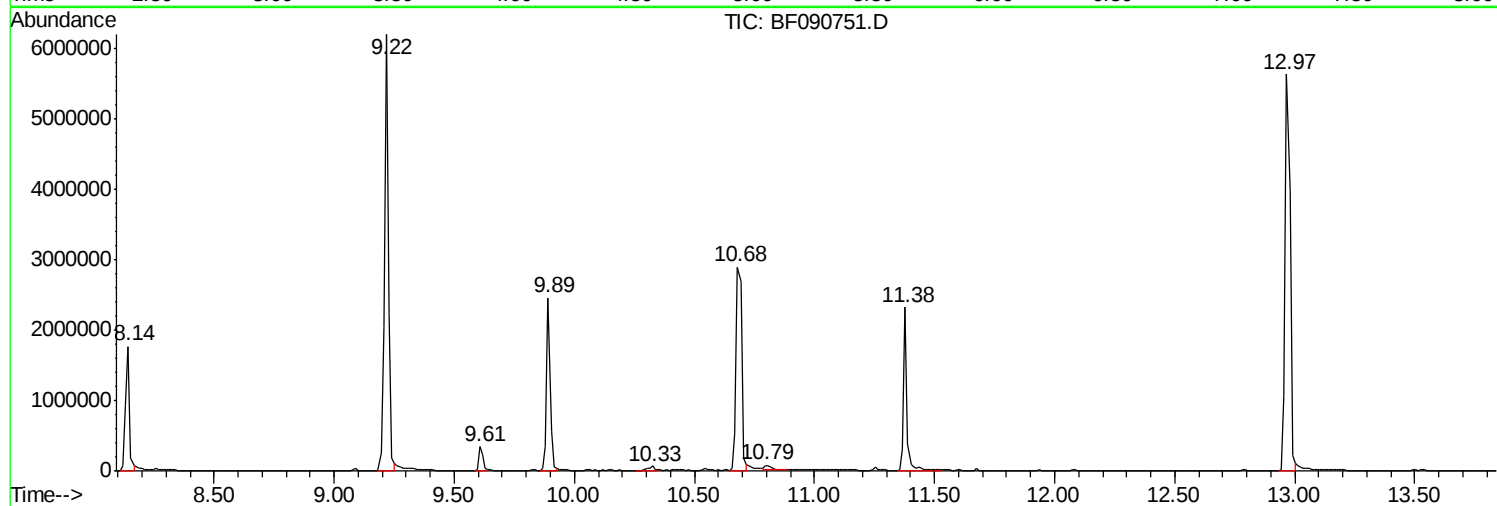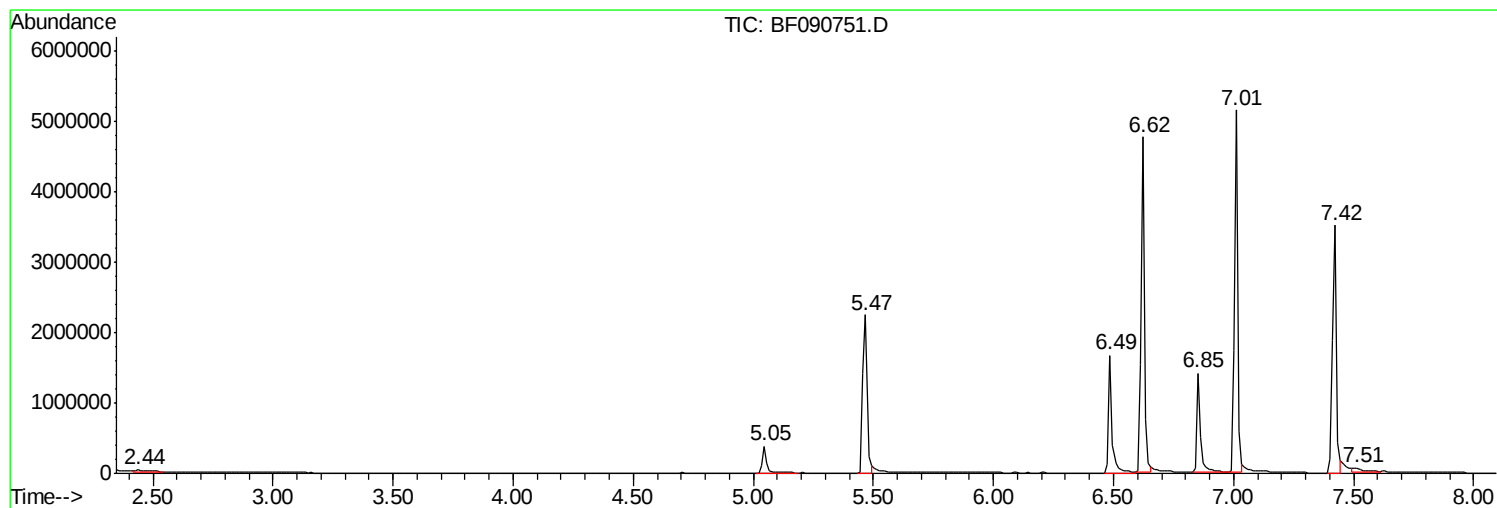

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102116\
Data File : BF090751.D
Acq On : 22 Oct 2016 10:09
Operator : UM/SJ
Sample : H5367-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-03S-101916










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.05	6.09 ng	480733	1,4-Dichlorobenzene-d4	6.85

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	33
3			Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	23
4			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
5			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

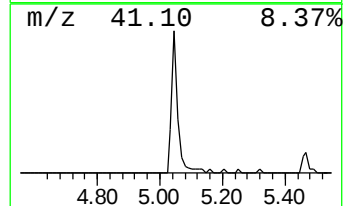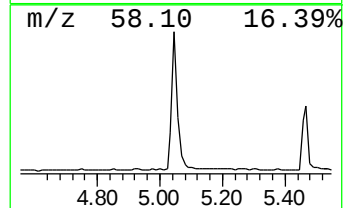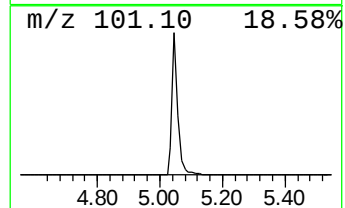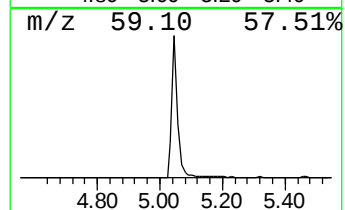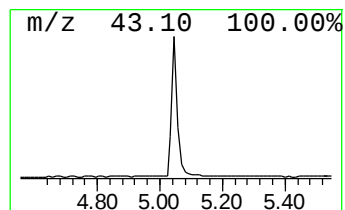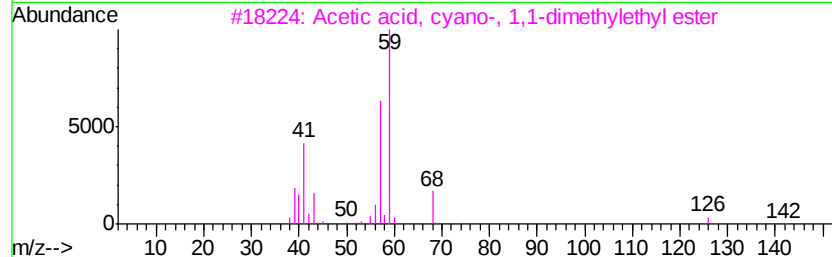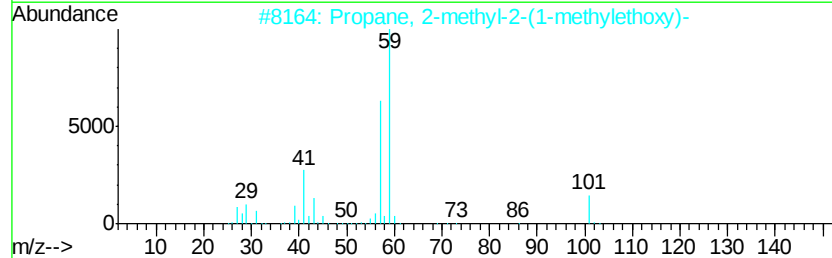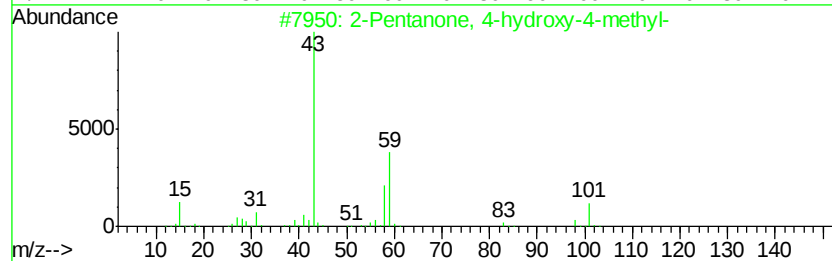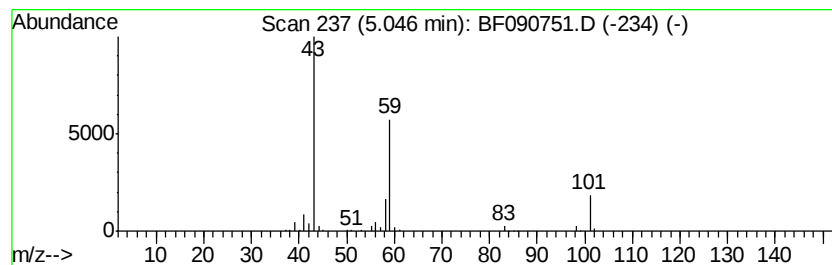

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090751.D
Acq On : 22 Oct 2016 10:09
Operator : UM/SJ
Sample : H5367-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-03S-101916









Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.62 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.62	62.59 ng	4939840	1,4-Dichlorobenzene-d4	6.85

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
5		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9

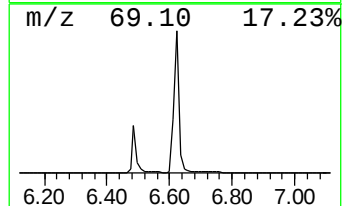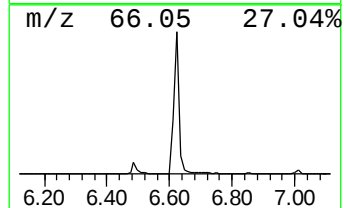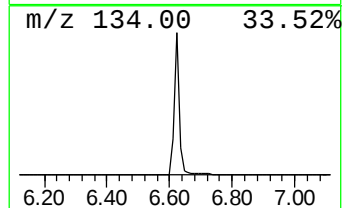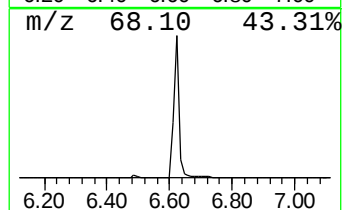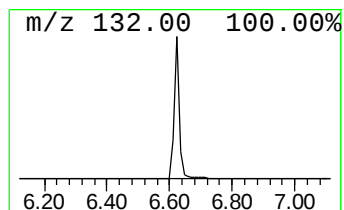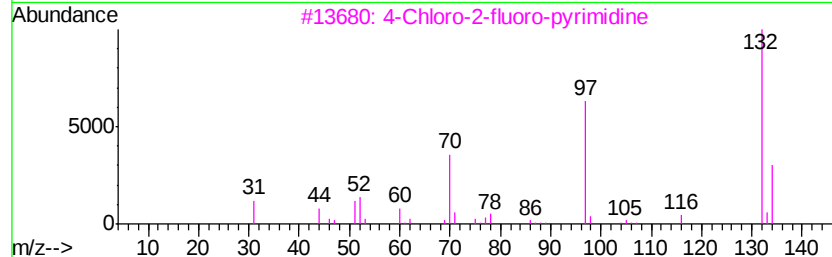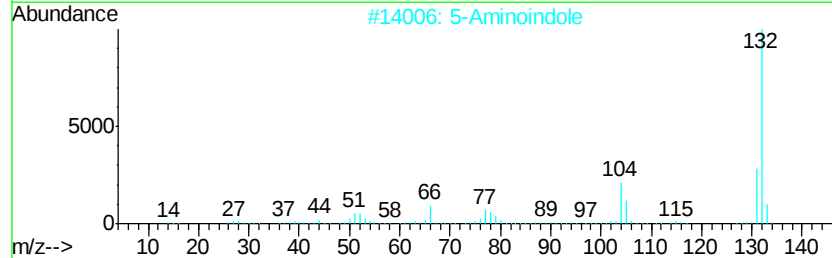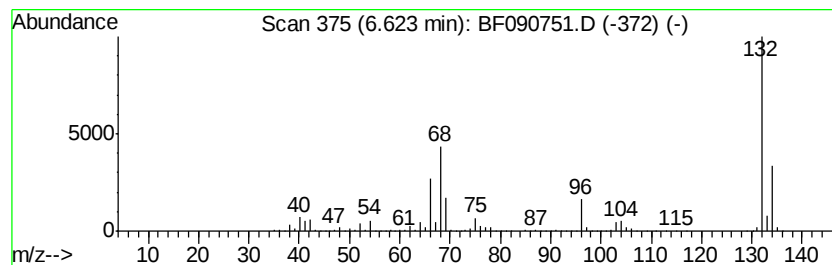

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090751.D
Acq On : 22 Oct 2016 10:09
Operator : UM/SJ
Sample : H5367-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-03S-101916

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.05	6.1	ng	480733	1	6.85	1578360	20.0
unknown6.62	6.62	62.6	ng	4939840	1	6.85	1578360	20.0