

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
 Data File : BF090756.D
 Acq On : 22 Oct 2016 12:26
 Operator : UM/SJ
 Sample : H5367-06
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-04S-101916

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.428	5	8	26	rVB	137047	350312	4.39%	0.668%
2	4.543	190	193	205	rBV	990963	1332521	16.71%	2.542%
3	5.046	234	237	247	rBV	412162	509225	6.38%	0.971%
4	5.469	271	274	276	rBV	2021644	2577697	32.32%	4.918%
5	6.486	361	363	372	rBV	1538190	1642714	20.60%	3.134%
6	6.623	372	375	378	rBV	4843911	4926579	61.77%	9.399%
7	6.852	393	395	406	rBV	1299409	1480160	18.56%	2.824%
8	7.012	406	409	411	rBV	4970823	5071346	63.59%	9.675%
9	7.423	442	445	447	rBV	3233477	4070730	51.04%	7.766%
10	8.143	505	508	510	rBV	1602943	1954376	24.51%	3.728%
11	9.217	599	602	605	rBV	6123795	7369174	92.40%	14.059%
12	9.606	634	636	639	rBV	306508	369311	4.63%	0.705%
13	9.892	658	661	664	rBV	2397583	2346749	29.42%	4.477%
14	10.680	727	730	733	rBV2	3007286	4778887	59.92%	9.117%
15	10.806	739	741	748	rVB	51053	102736	1.29%	0.196%
16	11.378	788	791	803	rBV	2309796	2301816	28.86%	4.391%
17	12.795	912	915	917	rBV	71304	88008	1.10%	0.168%
18	12.966	927	930	933	rBV	5396842	7975385	100.00%	15.215%
19	14.018	1019	1022	1024	rBV	1819606	1827286	22.91%	3.486%
20	15.447	1144	1147	1150	rBV	836528	1342703	16.84%	2.562%


Sum of corrected areas: 52417715

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090756.D
Acq On : 22 Oct 2016 12:26
Operator : UM/SJ
Sample : H5367-06
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
MW-04S-101916

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

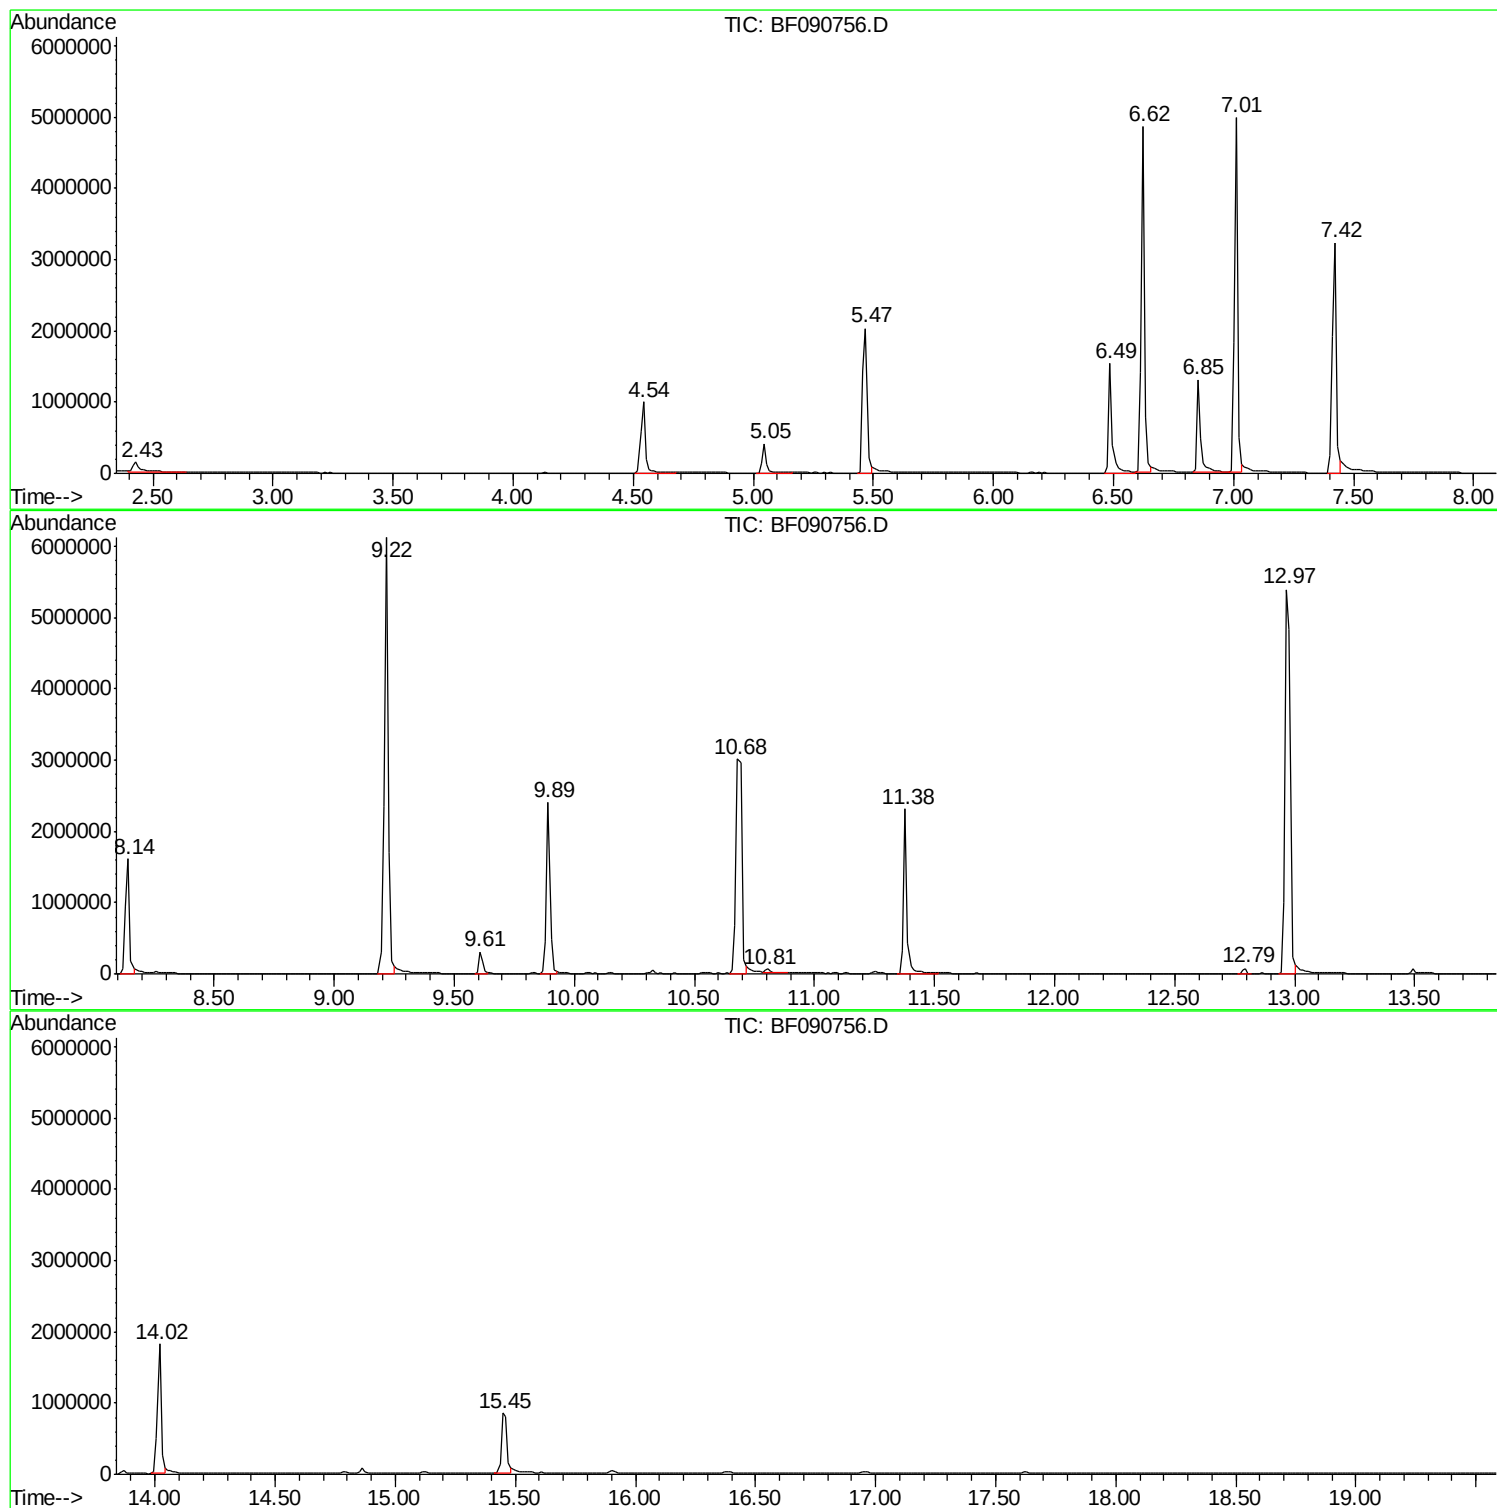

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102116\
Data File : BF090756.D
Acq On : 22 Oct 2016 12:26
Operator : UM/SJ
Sample : H5367-06
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-04S-101916










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.05	6.88 ng	509225	1,4-Dichlorobenzene-d4	6.85

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	28
3			Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	23
4			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9
5			Acetone	58	C3H6O	000067-64-1	9

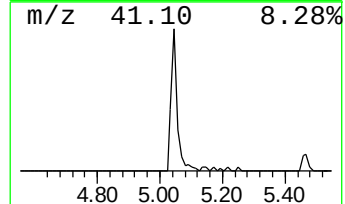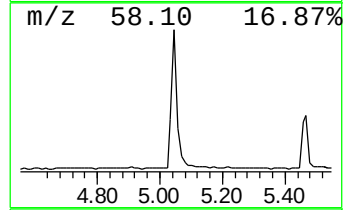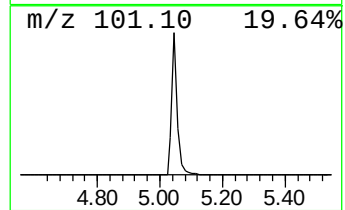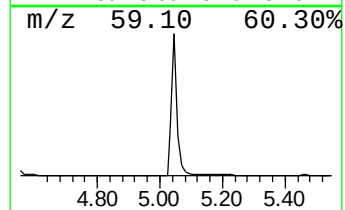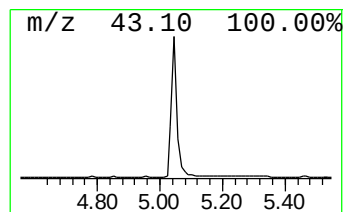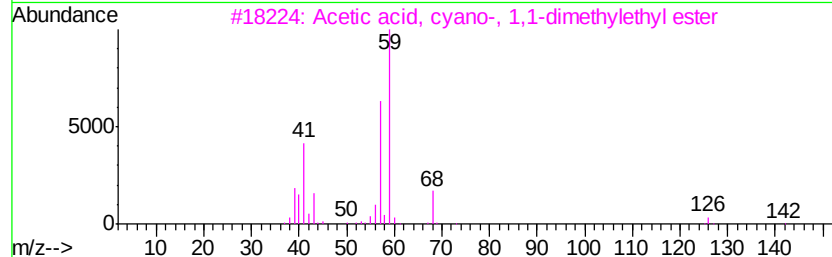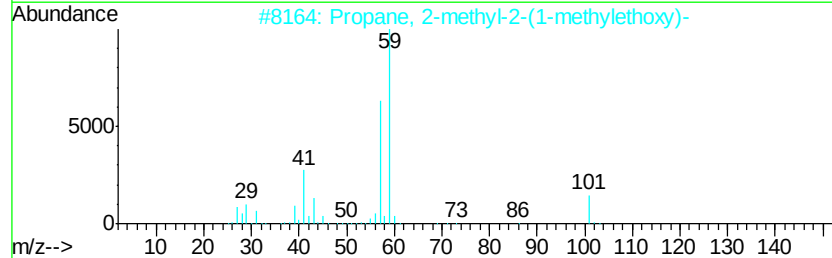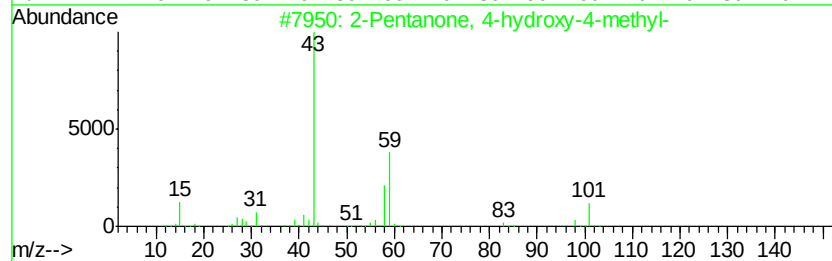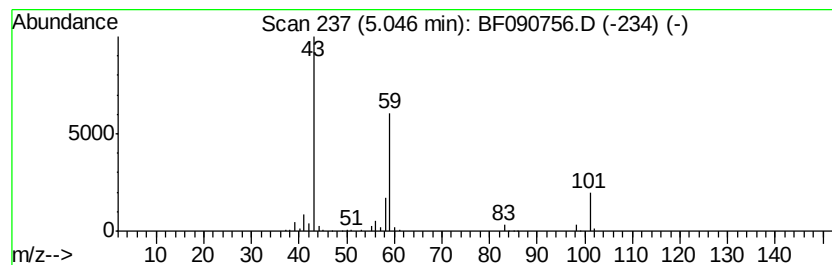

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090756.D
Acq On : 22 Oct 2016 12:26
Operator : UM/SJ
Sample : H5367-06
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-04S-101916










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown6.62 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.62	66.57 ng	4926580	1,4-Dichlorobenzene-d4	6.85

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	10
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

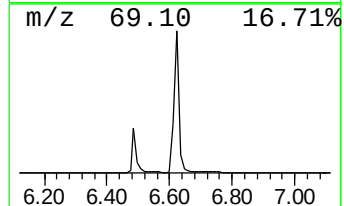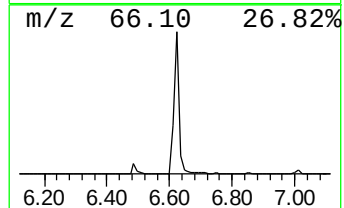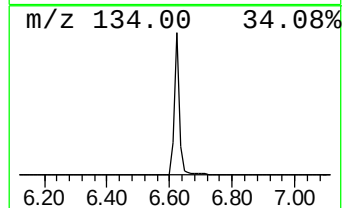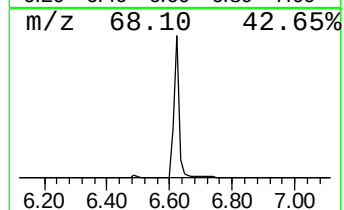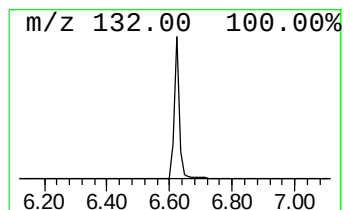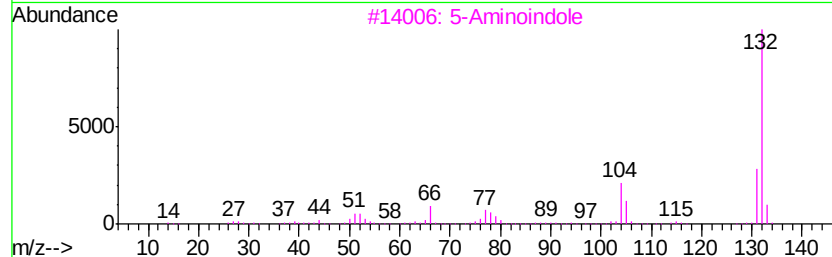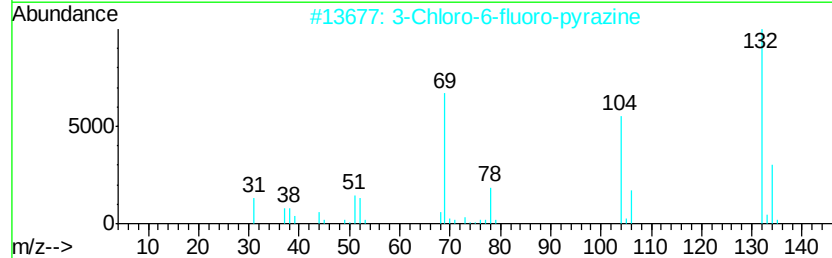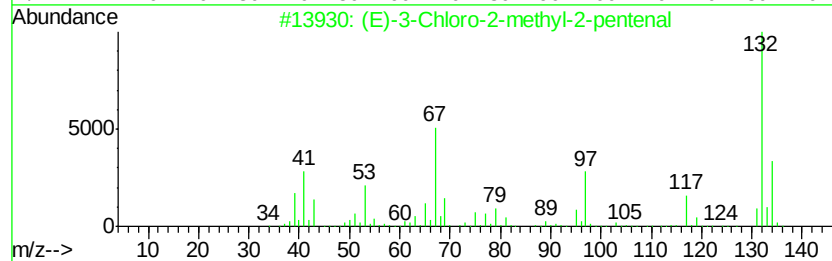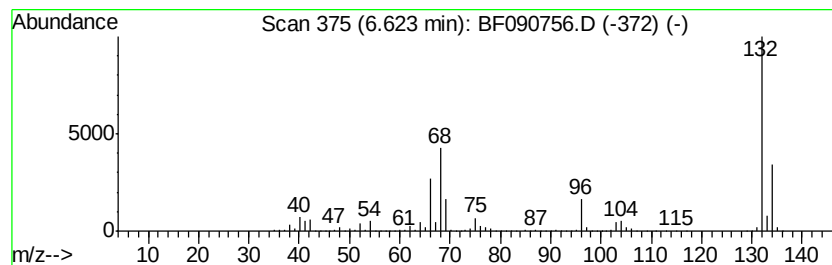

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090756.D
Acq On : 22 Oct 2016 12:26
Operator : UM/SJ
Sample : H5367-06
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-04S-101916

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.05	6.9	ng	509225	1	6.85	1480160	20.0
unknown6.62	6.62	66.6	ng	4926580	1	6.85	1480160	20.0