

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
 Data File : BF090760.D
 Acq On : 22 Oct 2016 14:15
 Operator : UM/SJ
 Sample : BLK-TEST
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BLK-TEST

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.405	3	6	8	rBV	11268	26503	1.19%	0.209%
2	5.034	234	236	245	rBV	29224	35281	1.59%	0.278%
3	5.457	271	273	290	rBV7	37442	109289	4.92%	0.862%
4	6.497	361	364	372	rBV	30360	83430	3.75%	0.658%
5	6.623	372	375	393	rVB	288498	436221	19.63%	3.442%
6	6.852	393	395	406	rBV	1283124	1438847	64.75%	11.355%
7	7.012	406	409	426	rVB	335096	485793	21.86%	3.834%
8	7.423	442	445	464	rBV	106775	286218	12.88%	2.259%
9	8.143	505	508	510	rBV	1646071	1897299	85.38%	14.973%
10	9.218	599	602	604	rBV	579886	604244	27.19%	4.768%
11	9.892	658	661	664	rBV	2381250	2222223	100.00%	17.537%
12	10.681	727	730	740	rBV	243811	279856	12.59%	2.208%
13	11.378	789	791	804	rBV	2128889	2037748	91.70%	16.081%
14	12.966	927	930	932	rBV	354719	506960	22.81%	4.001%
15	14.018	1019	1022	1024	rBV	1085235	1184004	53.28%	9.344%
16	15.447	1144	1147	1158	rBV	704261	1014676	45.66%	8.007%
17	16.384	1226	1229	1234	rVB3	12801	23277	1.05%	0.184%


Sum of corrected areas: 12671869

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090760.D
Acq On : 22 Oct 2016 14:15
Operator : UM/SJ
Sample : BLK-TEST
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BLK-TEST

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

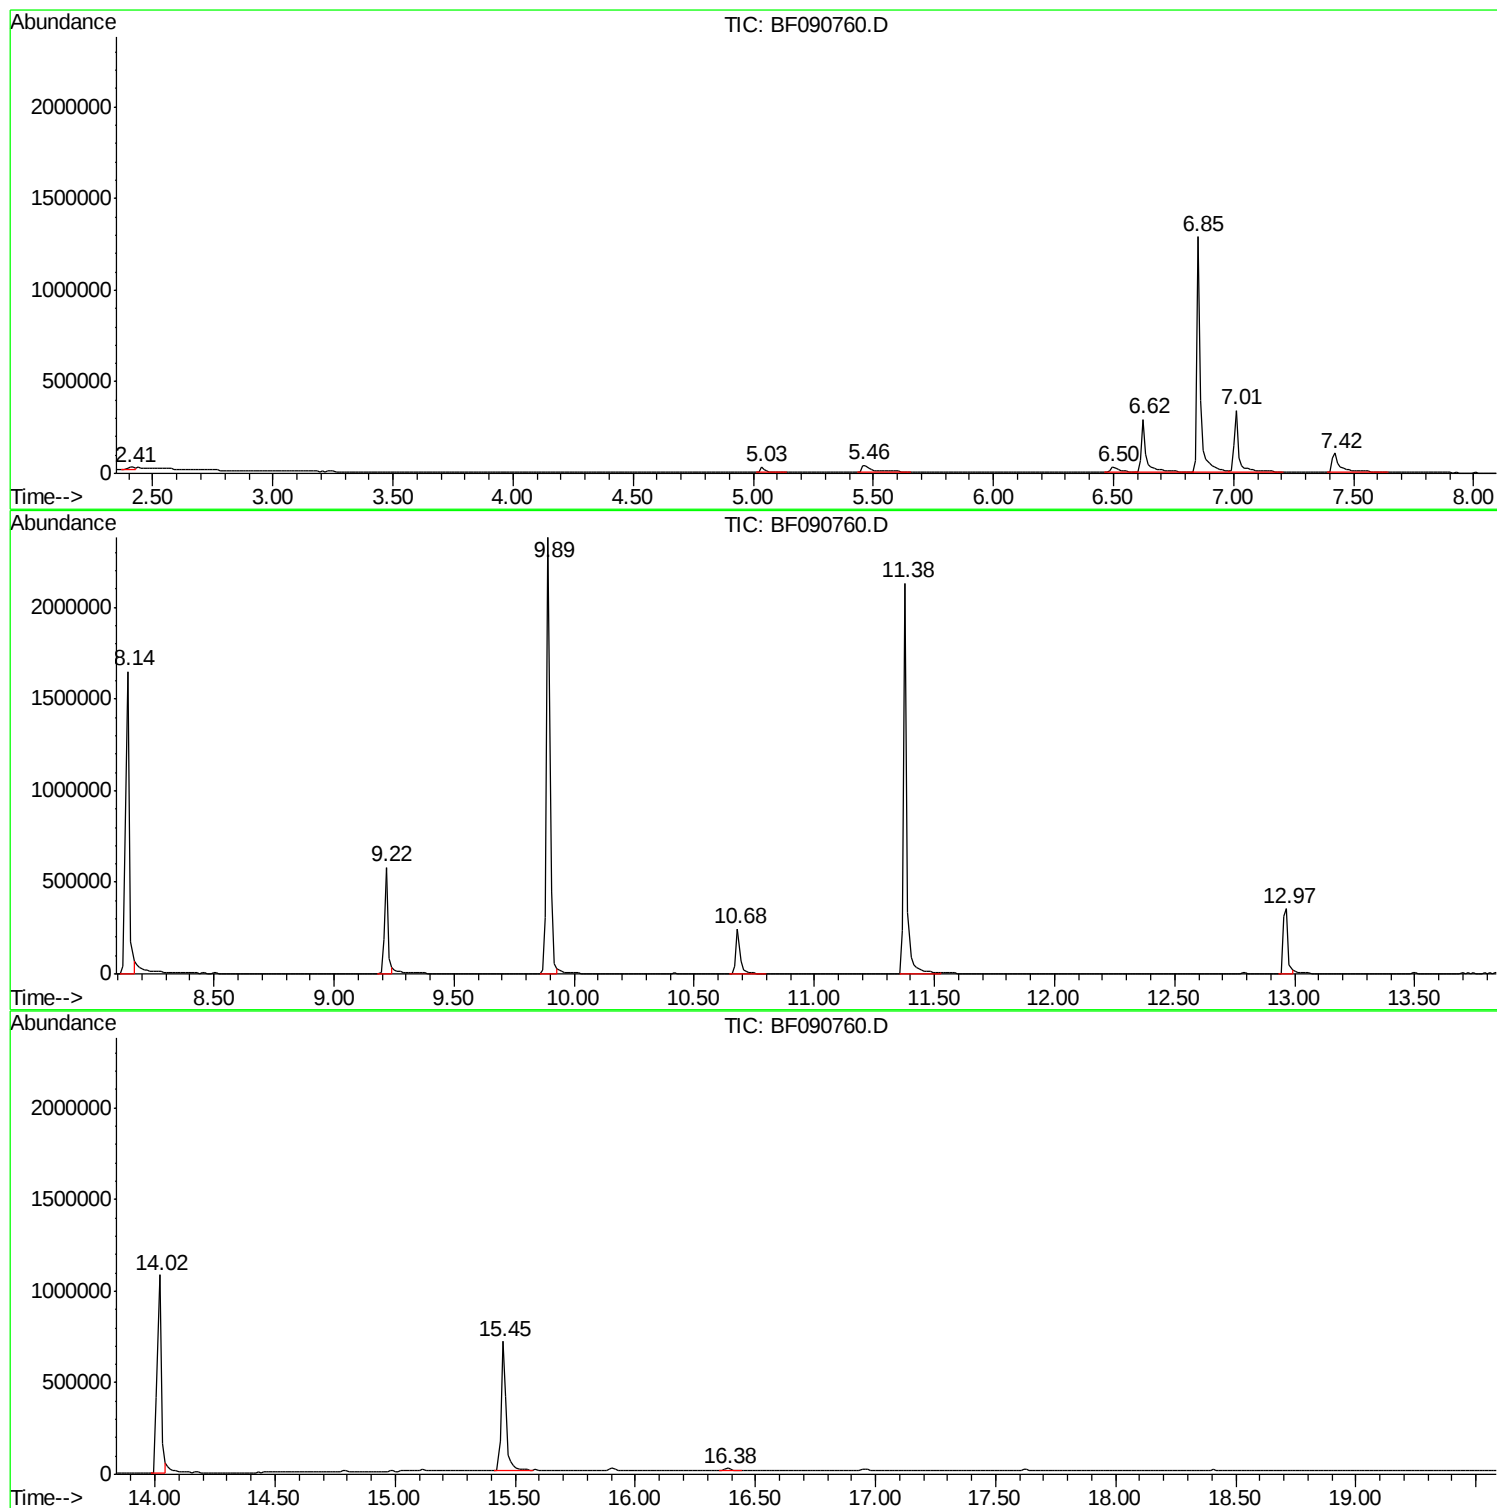

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102116\
Data File : BF090760.D
Acq On : 22 Oct 2016 14:15
Operator : UM/SJ
Sample : BLK-TEST
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BLK-TEST










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.62 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.62	6.06 ng	436221	1,4-Dichlorobenzene-d4	6.85

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2			4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
3			1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9
4			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5			Imidazole, 4,5-dicyano-1-methyl-	132	C6H4N4	019485-35-9	9

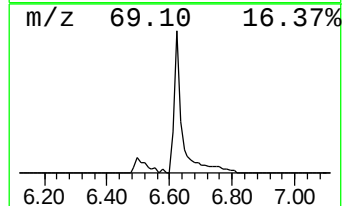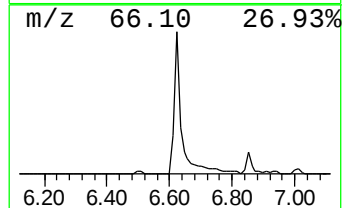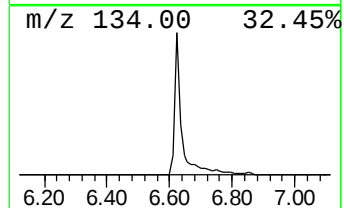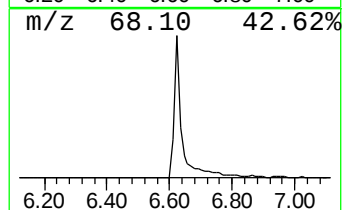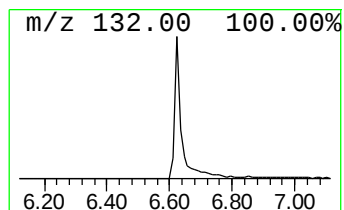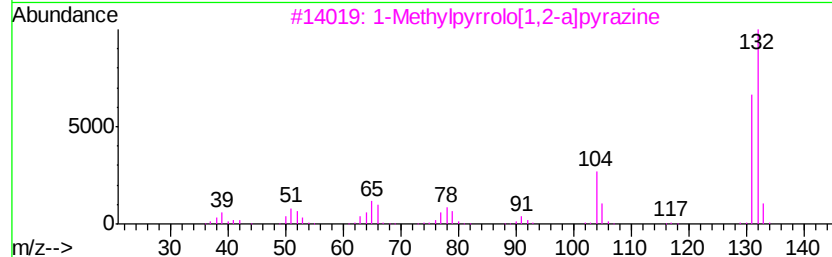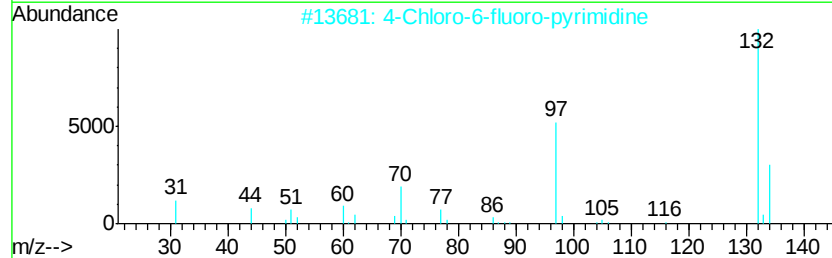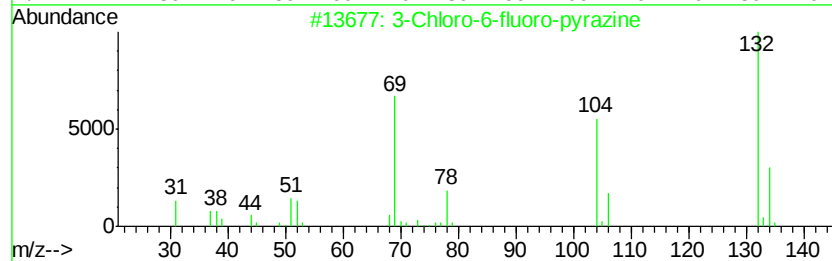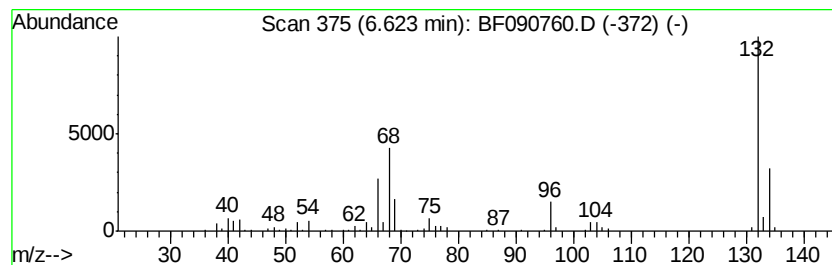

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
Data File : BF090760.D
Acq On : 22 Oct 2016 14:15
Operator : UM/SJ
Sample : BLK-TEST
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BLK-TEST

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.62	6.62	6.1	ng	436221	1	6.85	1438850	20.0