


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102116\
 Data File : BF090742.D
 Acq On : 22 Oct 2016 6:01
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 21 17:36:31 2016

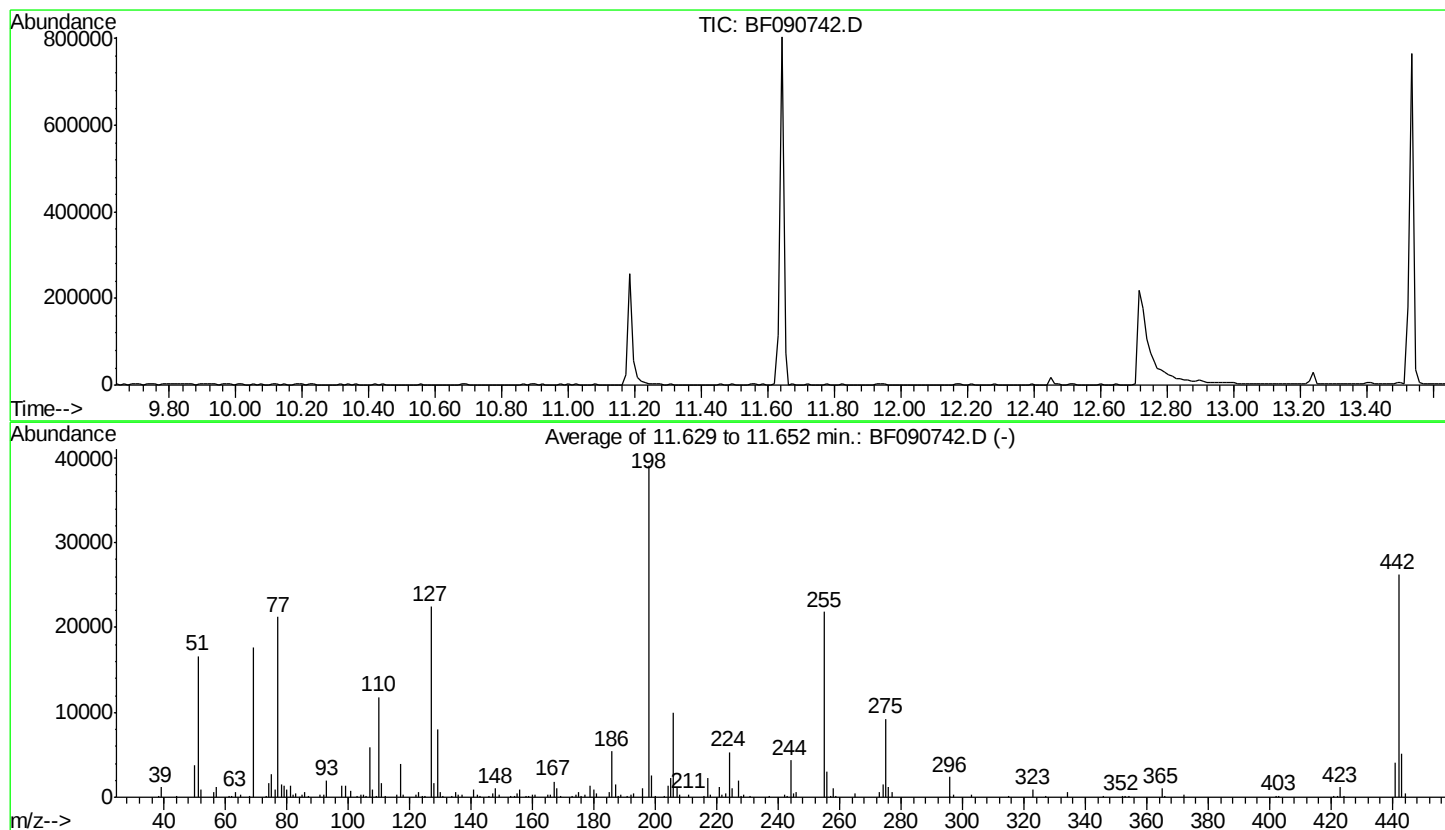

AutoFind: Scans 813, 814, 815; Background Corrected with Scan 810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	16671	PASS
68	69	0.00	2	1.1	192	PASS
69	198	0.00	100	45.0	17597	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.5	22473	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39091	PASS
199	198	5	9	6.7	2604	PASS
275	198	10	60	23.6	9214	PASS
365	198	1	100	2.5	993	PASS
441	442	0.01	24	15.4	4047	PASS
442	198	50	100	67.2	26252	PASS
443	442	15	24	19.3	5072	PASS