


Data Path : Z:\HPCHEM1\BNA F\Data\BF102117\
 Data File : BF099720.D
 Acq On : 21 Oct 2017 9:46
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 20 13:11:43 2017

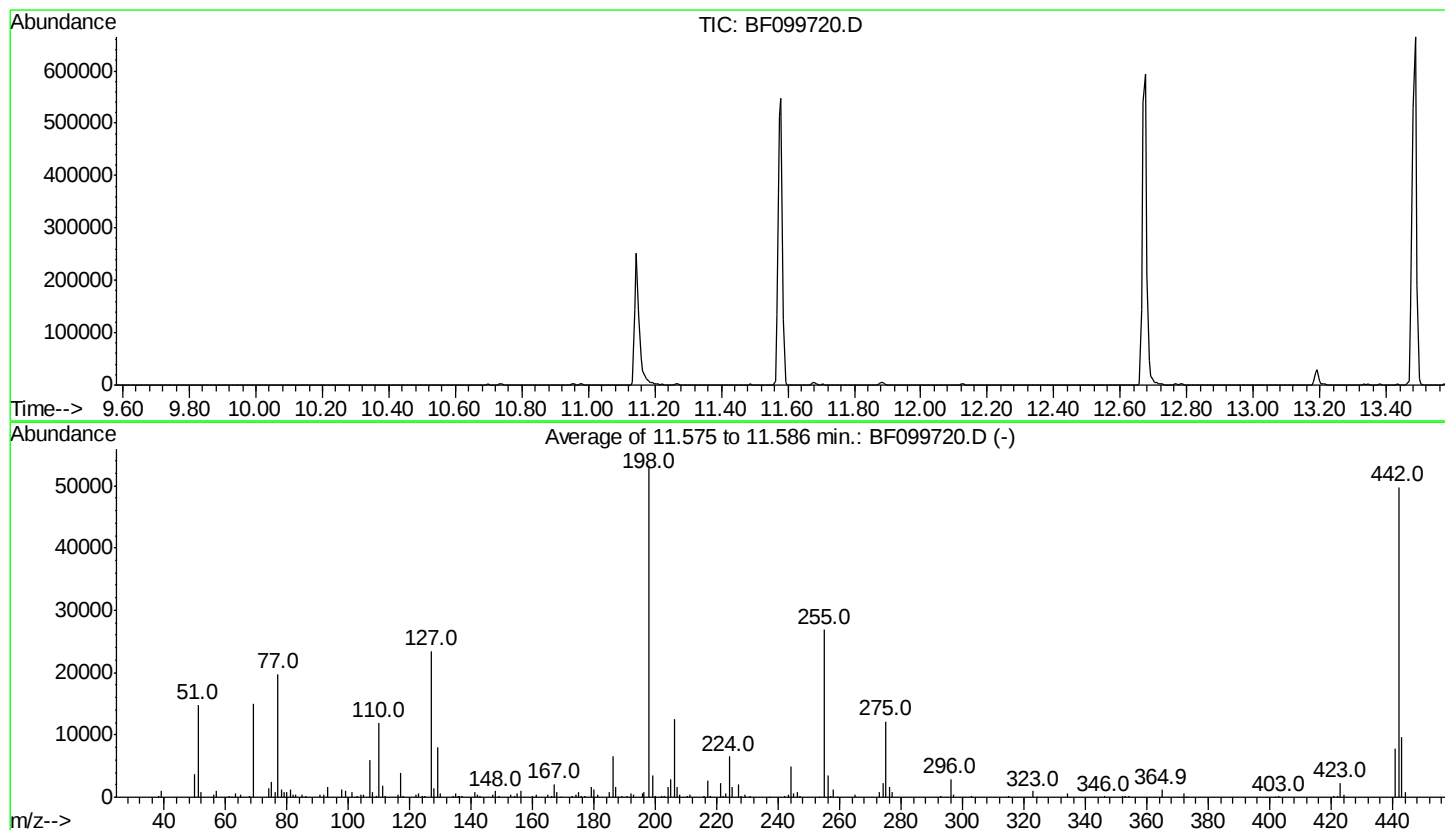

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	14832	PASS
68	69	0.00	2	2.0	293	PASS
69	198	0.00	100	28.0	14921	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.2	23511	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	53207	PASS
199	198	5	9	6.6	3537	PASS
275	198	10	60	22.8	12140	PASS
365	198	1	100	2.3	1204	PASS
441	442	0.01	24	15.6	7740	PASS
442	198	50	100	93.5	49730	PASS
443	442	15	24	19.5	9692	PASS