

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102122\
 Data File : BF130739.D
 Acq On : 21 Oct 2022 11:18
 Operator : CG\JU
 Sample : PB148422BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB148422BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130739.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.775	488	491	508	rBV	15113	35798	1.17%	0.210%
2	5.175	556	559	576	rBV	1842327	2053321	67.06%	12.023%
3	6.216	733	736	765	rBV	2104434	2403464	78.50%	14.073%
4	6.563	792	795	807	rBV	511886	482459	15.76%	2.825%
5	7.134	888	892	914	rBV	1398249	1383719	45.19%	8.102%
6	7.845	1009	1013	1033	rBV	587381	596030	19.47%	3.490%
7	8.922	1191	1196	1199	rBV	2848186	2684159	87.66%	15.717%
8	9.592	1306	1310	1322	rBV	721006	663152	21.66%	3.883%
9	10.380	1441	1444	1472	rBV	2007587	1918895	62.67%	11.236%
10	11.069	1558	1561	1572	rBV	712324	670486	21.90%	3.926%
11	12.657	1826	1831	1834	rBV	3443575	3061921	100.00%	17.929%
12	13.704	2006	2009	2021	rBV	592467	570938	18.65%	3.343%
13	15.080	2239	2243	2257	rBV	352732	481539	15.73%	2.820%
14	15.457	2303	2307	2310	rBV	24807	34962	1.14%	0.205%
15	15.886	2375	2380	2386	rVB2	21430	37464	1.22%	0.219%




Sum of corrected areas: 17078307

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102122\
Data File : BF130739.D
Acq On : 21 Oct 2022 11:18
Operator : CG\JU
Sample : PB148422BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148422BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

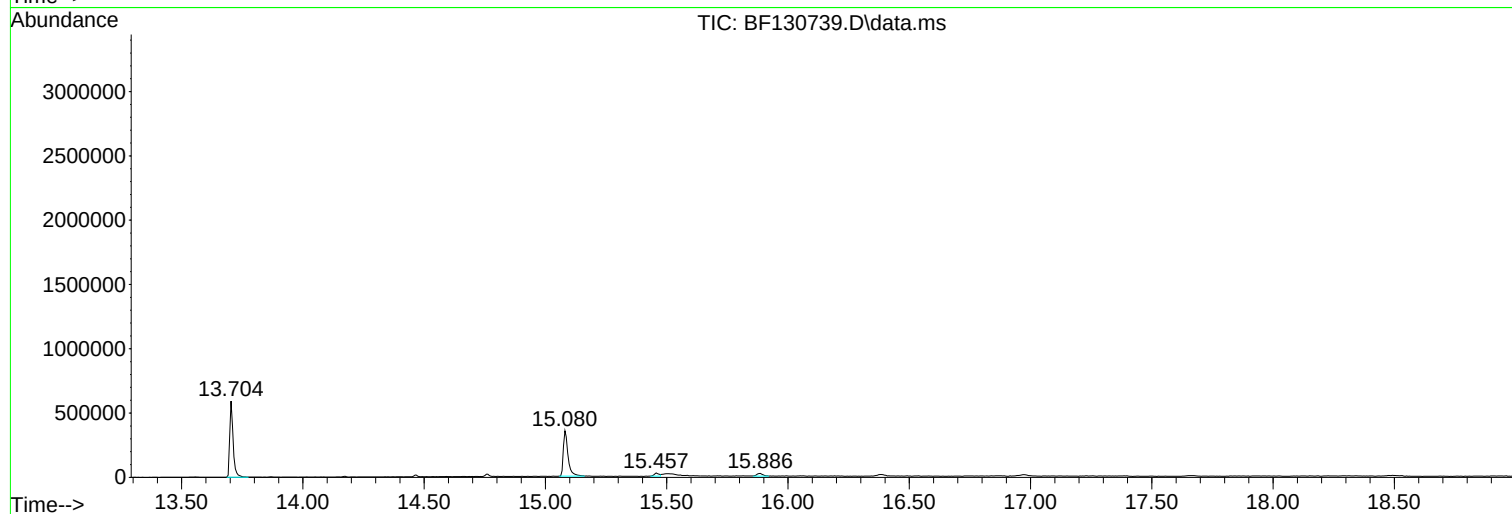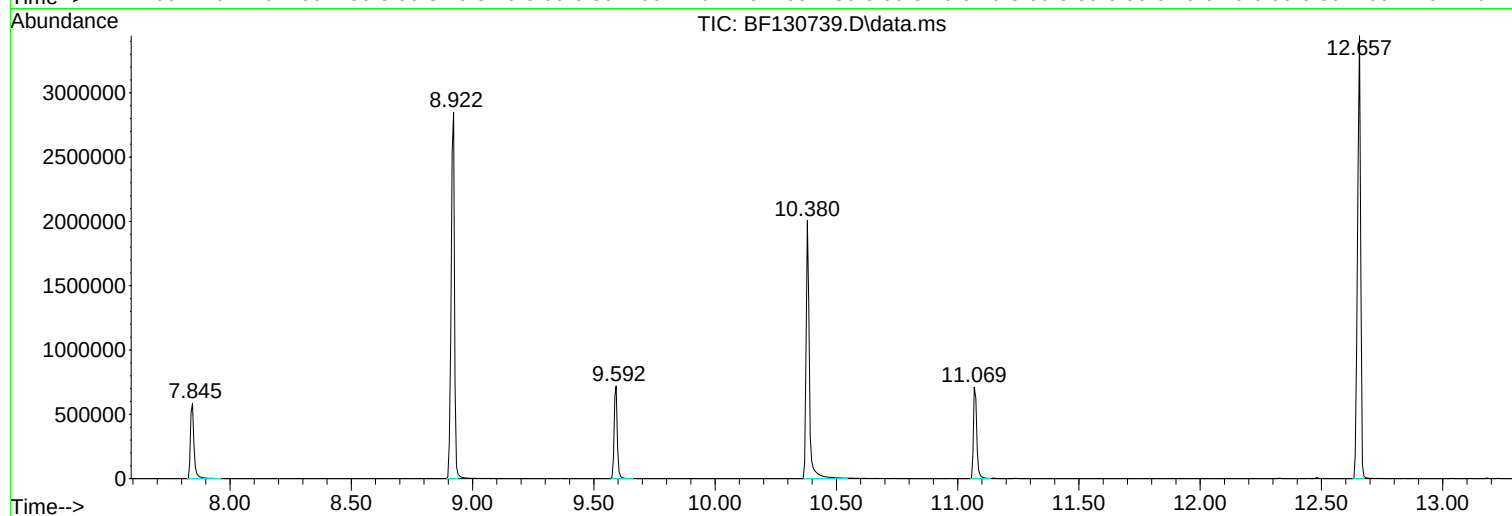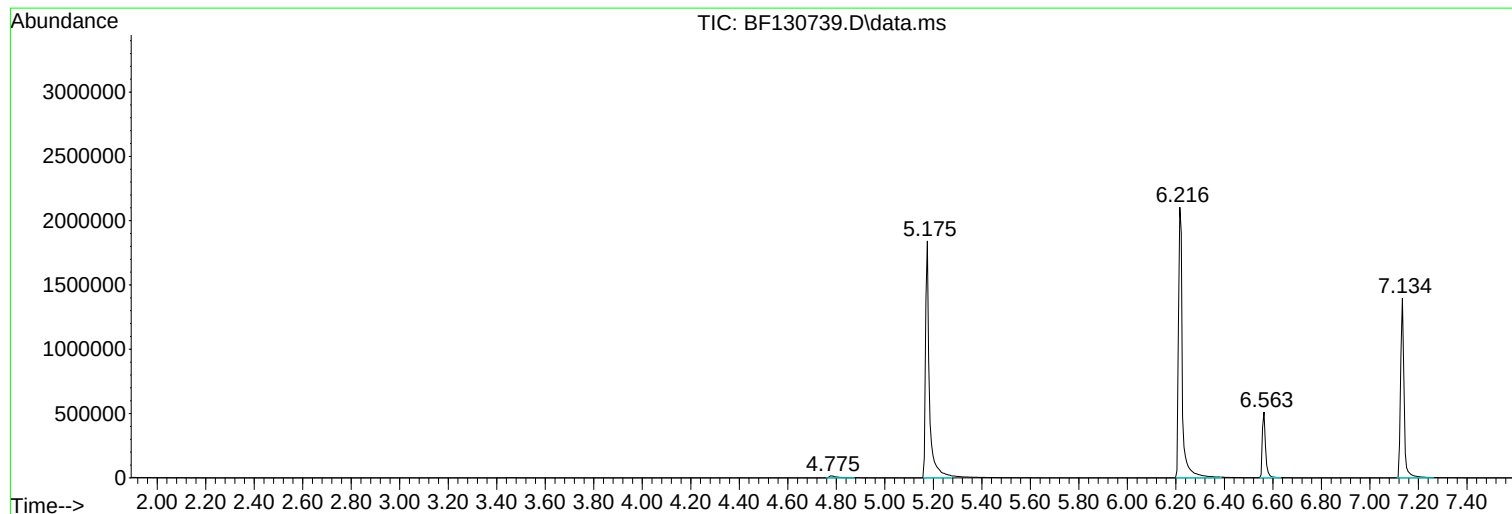

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102122\
Data File : BF130739.D
Acq On : 21 Oct 2022 11:18
Operator : CG\JU
Sample : PB148422BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148422BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102122\
Data File : BF130739.D
Acq On : 21 Oct 2022 11:18
Operator : CG\JU
Sample : PB148422BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148422BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------