
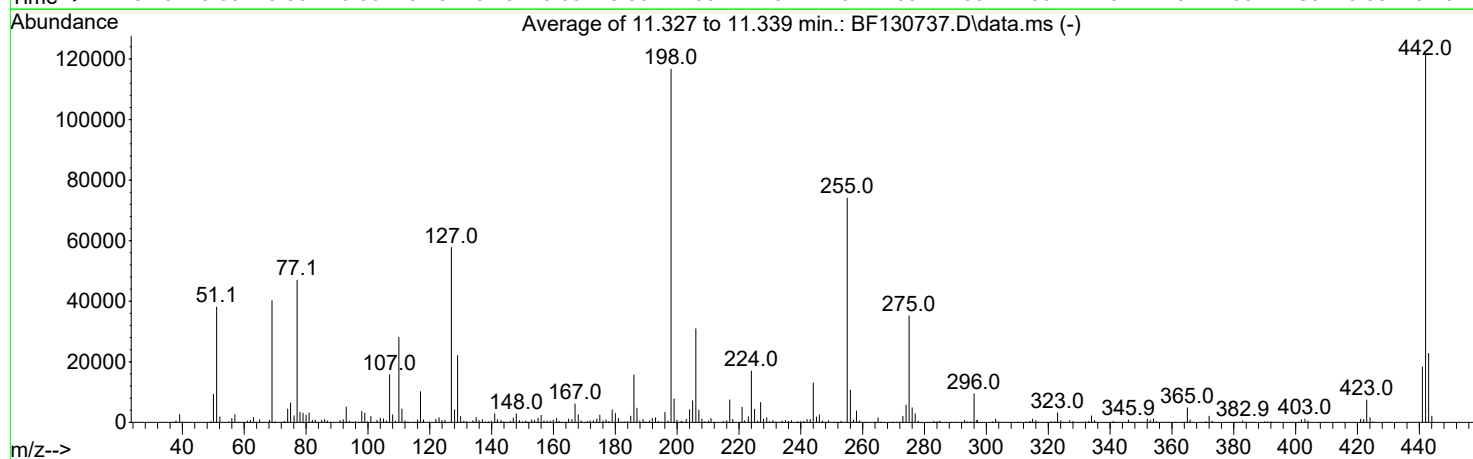


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102122\
 Data File : BF130737.D
 Acq On : 21 Oct 2022 09:11
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 21 06:12:36 2022

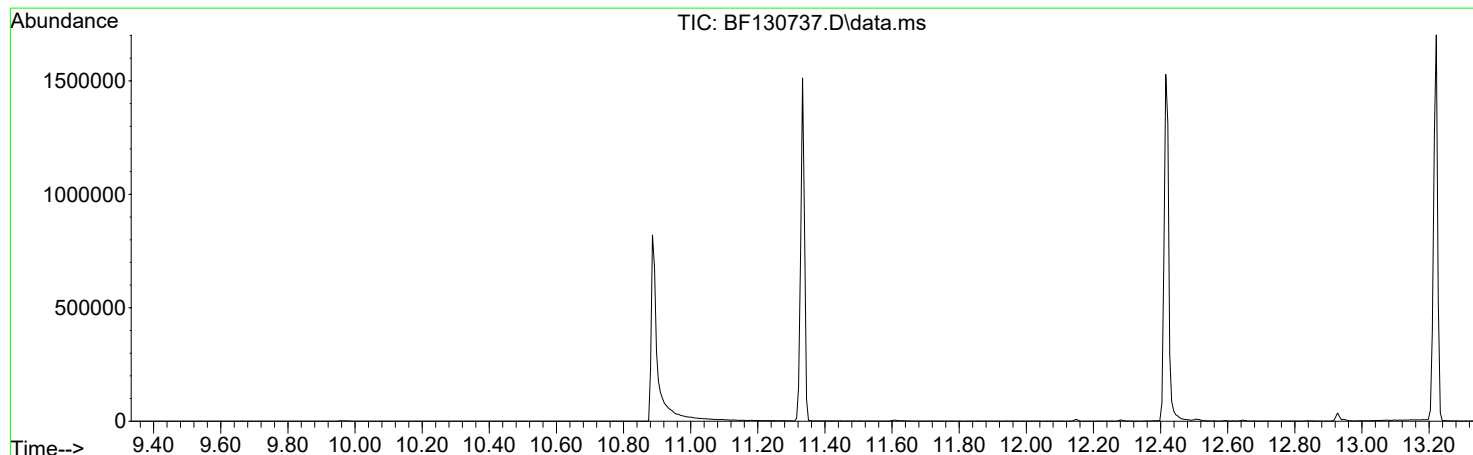




AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	38069	PASS
68	69	0.00	2	1.7	688	PASS
69	198	0.00	100	34.5	40205	PASS
70	69	0.00	2	0.5	197	PASS
127	198	10	80	49.5	57747	PASS
197	198	0.00	2	0.4	489	PASS
198	198	100	100	100.0	116629	PASS
199	198	5	9	6.7	7764	PASS
275	198	10	60	30.1	35155	PASS
365	198	1	100	4.1	4808	PASS
441	198	0.01	100	15.7	18290	PASS
442	442	50	100	100.0	121491	PASS
443	442	15	24	18.7	22762	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102122\
 Data File : BF130737.D
 Acq On : 21 Oct 2022 09:11
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 21 09:32:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 21 06:12:36 2022
 Response via : Initial Calibration

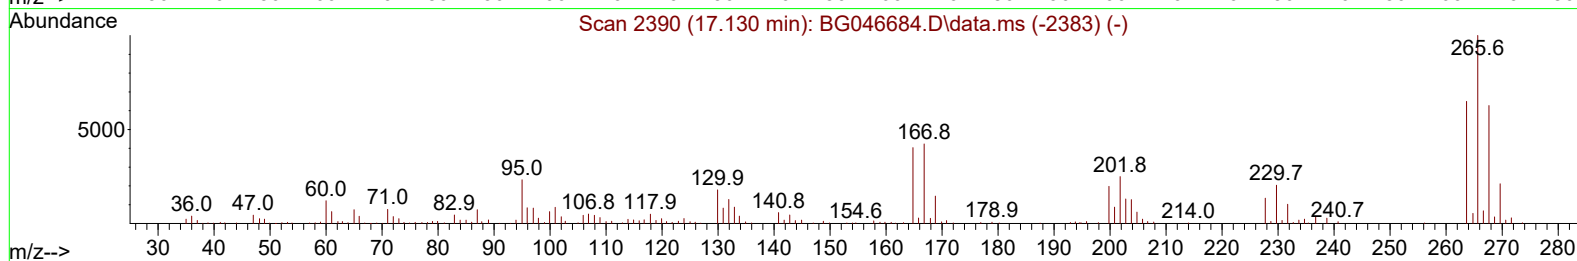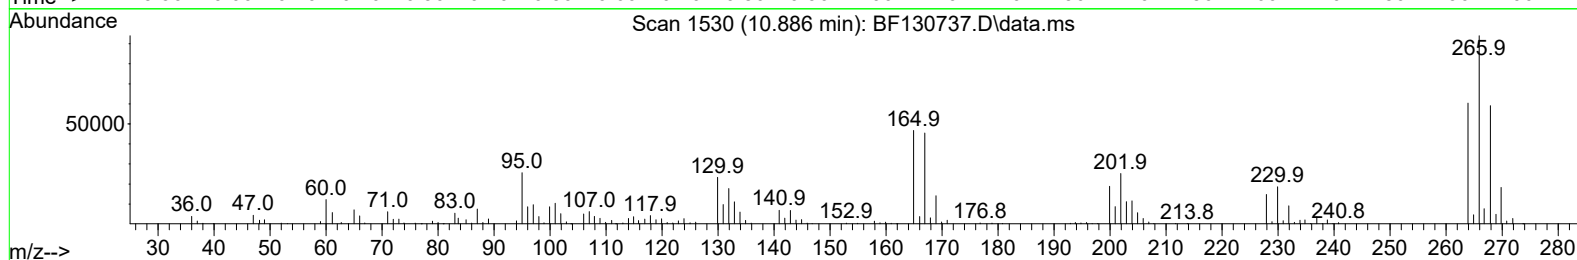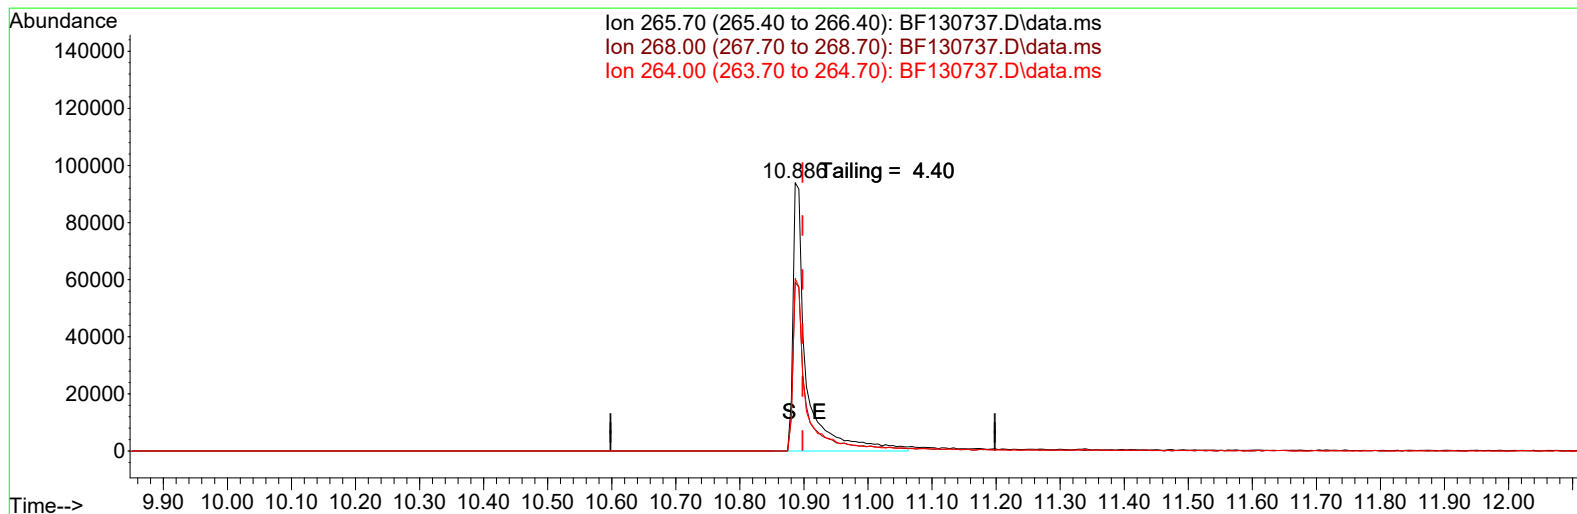

TIC: BF130737.D\data.ms

(70) Pentachlorophenol (C)

10.886min (-0.012) 5977.88 ng m




response 136877

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.86
264.00	67.00	64.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102122\
Data File : BF130737.D
Acq On : 21 Oct 2022 09:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 21 09:32:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 21 06:12:36 2022
Response via : Initial Calibration

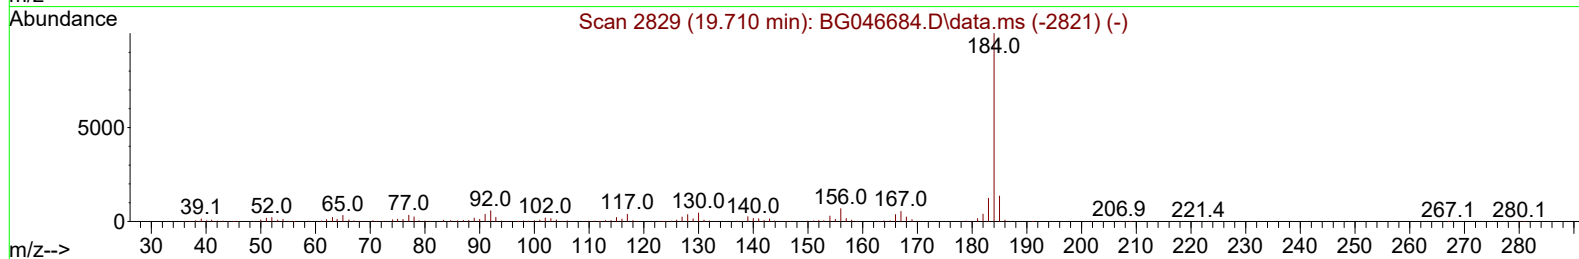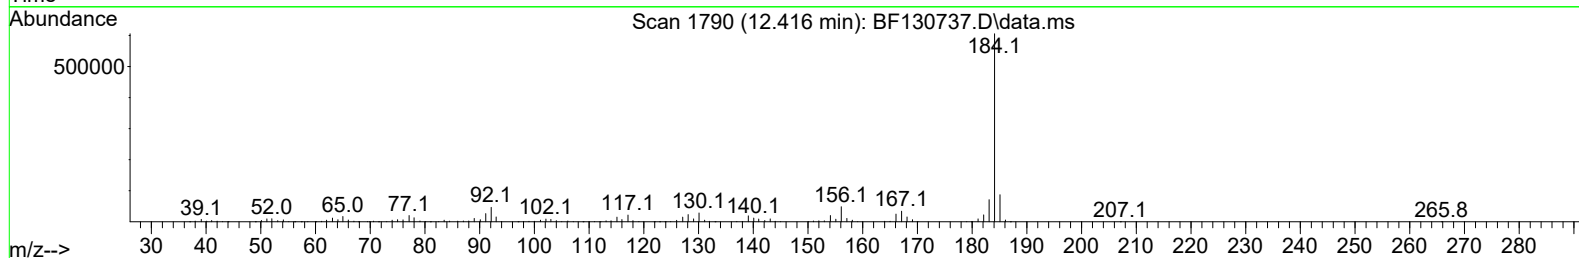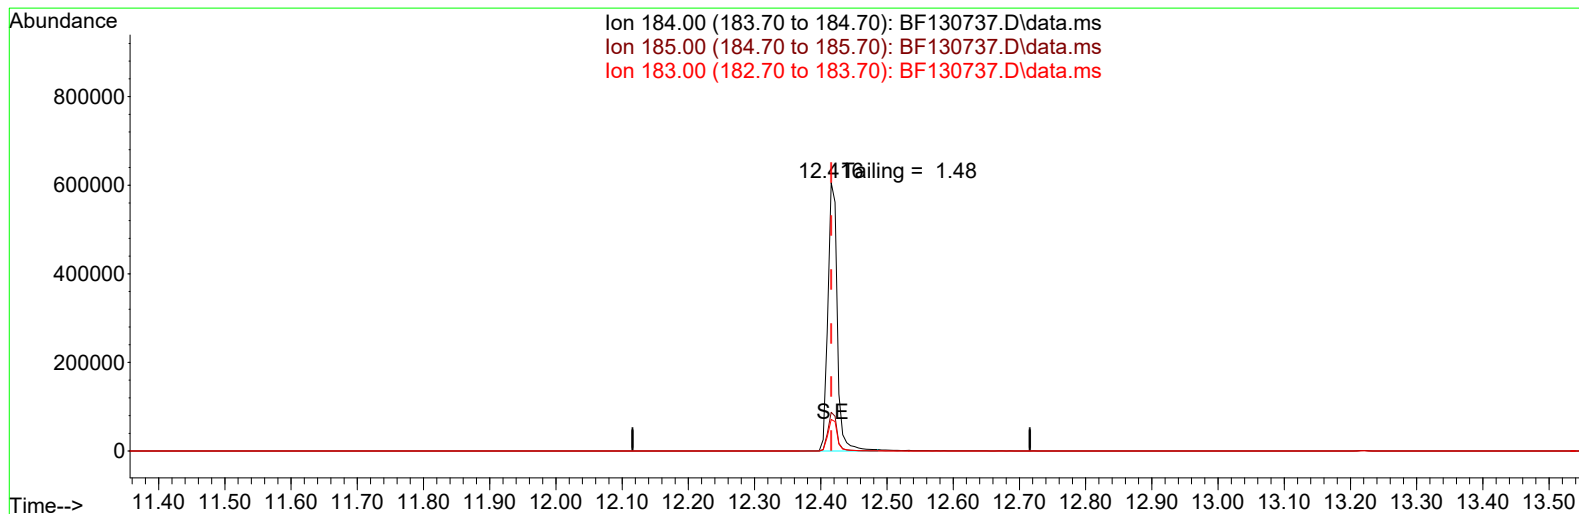

TIC: BF130737.D\data.ms

(77) Benzidine

12.416min (-0.000) -20.00 ng

response 604456

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.43
183.00	11.60	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/20/2022	BNA_F	BF130737.D
Compound Name	Response	Retention Time
DDT	276871	13.221
DDD	7654	12.947
DDE	2849	11.333
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10503	287374	3.65

Instrument :
BNA_F
ClientSampleId :
DFTPP